
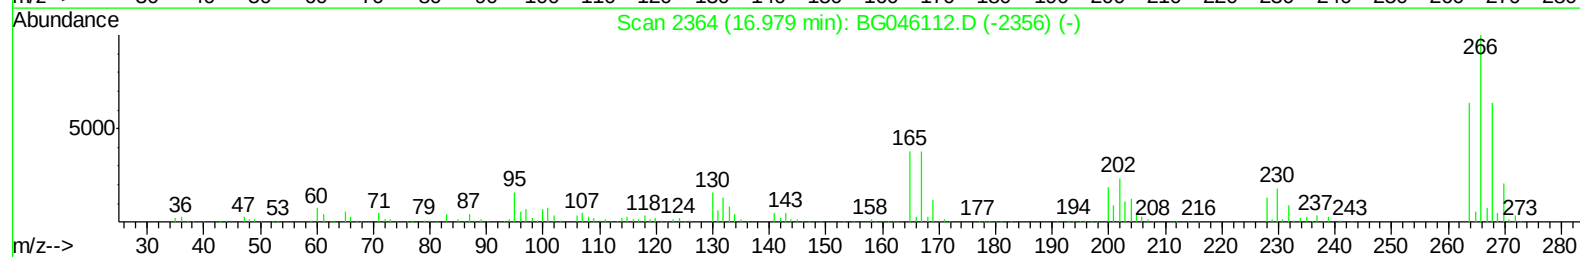
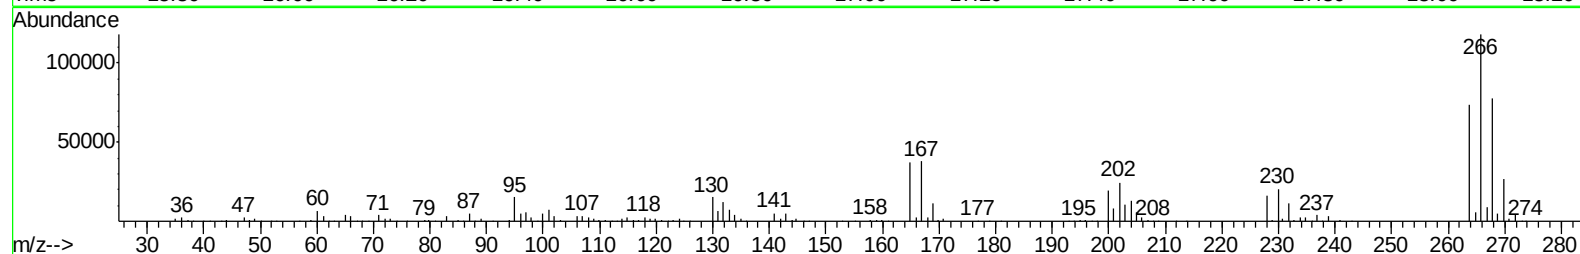


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG081420\
 Data File : BG046274.D
 Acq On : 14 Aug 2020 13:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 04:40:00 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 30 18:43:49 2020
 Response via : Initial Calibration

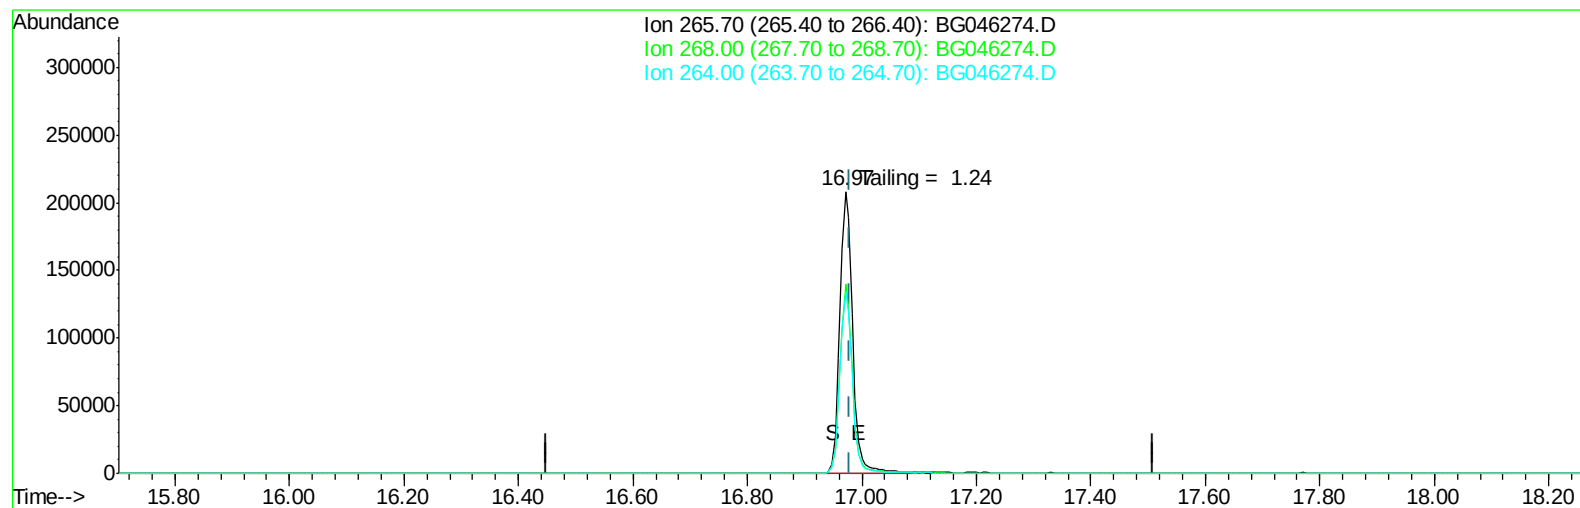

TIC: BG046274.D

(70) Pentachlorophenol (C)




16.971min (-0.008) 62535.94ng

response 327702

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	67.47
264.00	63.90	64.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG081420\
Data File : BG046274.D
Acq On : 14 Aug 2020 13:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 04:40:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 30 18:43:49 2020
Response via : Initial Calibration

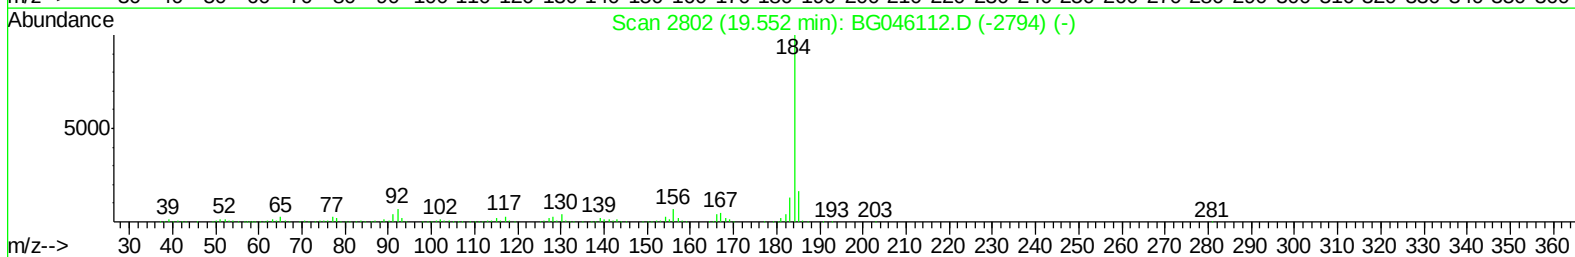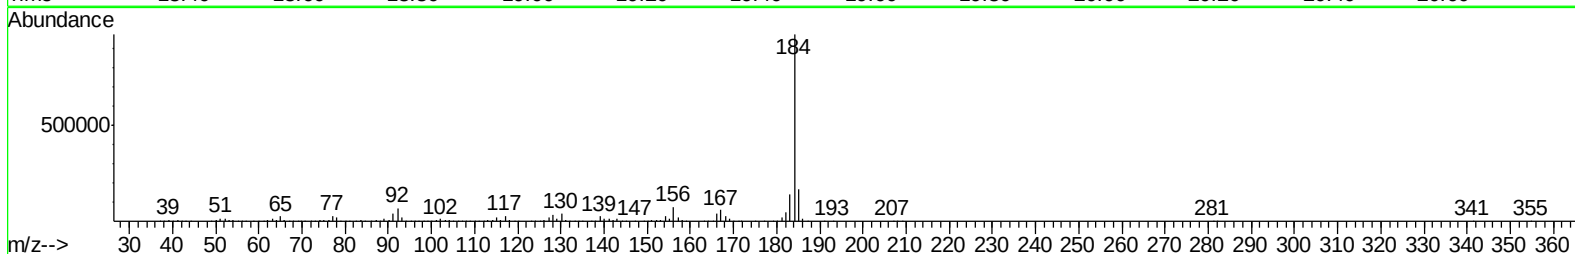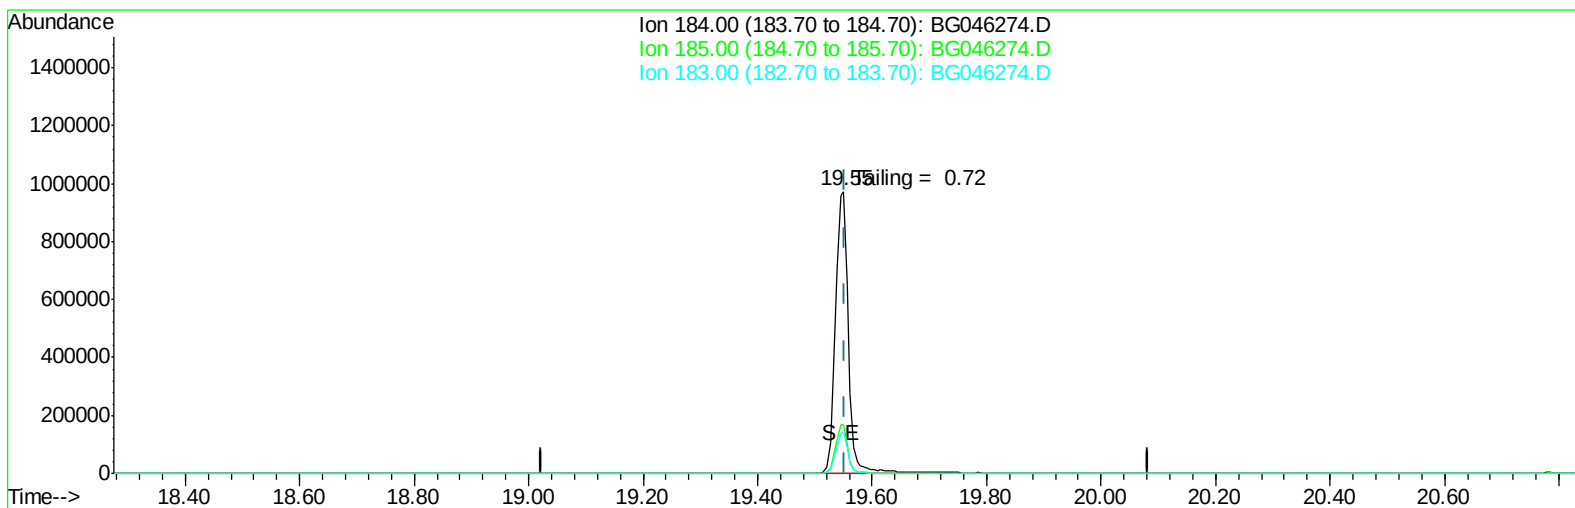

TIC: BG046274.D

(77) Benzidine

19.550min (-0.002) 44774.21ng

response 1533325

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	17.07
183.00	13.10	14.63
0.00	0.00	0.00