
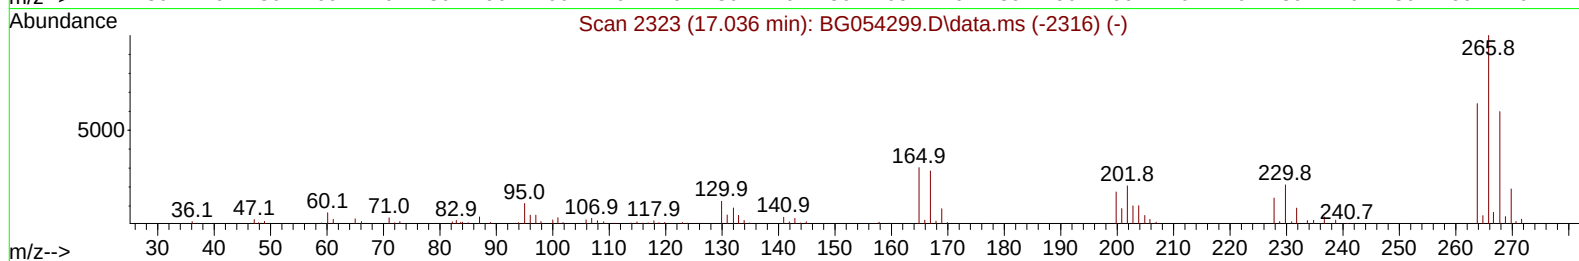
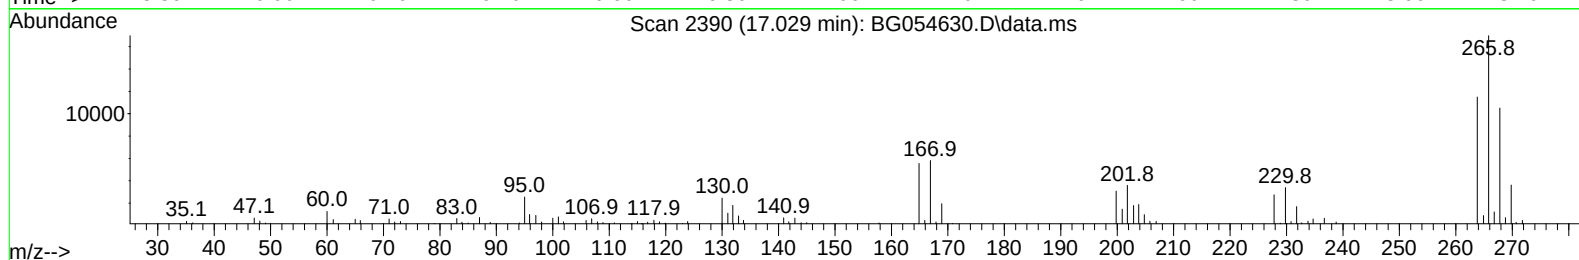


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081422\
Data File : BG054630.D
Acq On : 14 Aug 2022 12:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 13:26:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 13 00:32:40 2022
Response via : Initial Calibration

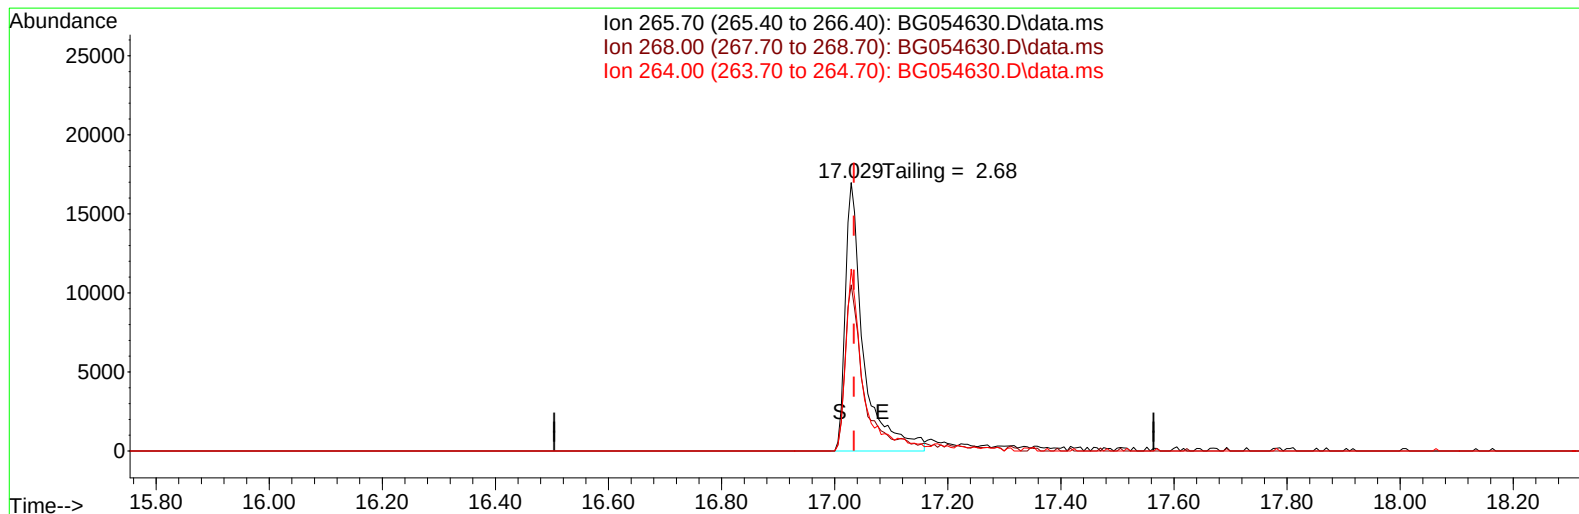

TIC: BG054630.D\data.ms

(70) Pentachlorophenol (C)




17.029min (-0.005) 33335.51 ng

response 37289

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	61.90
264.00	66.20	67.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081422\
Data File : BG054630.D
Acq On : 14 Aug 2022 12:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 13:26:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 13 00:32:40 2022
Response via : Initial Calibration

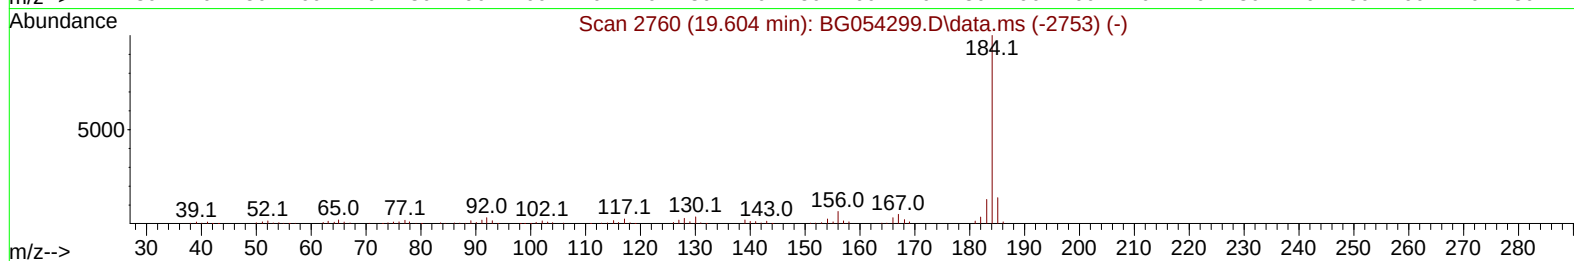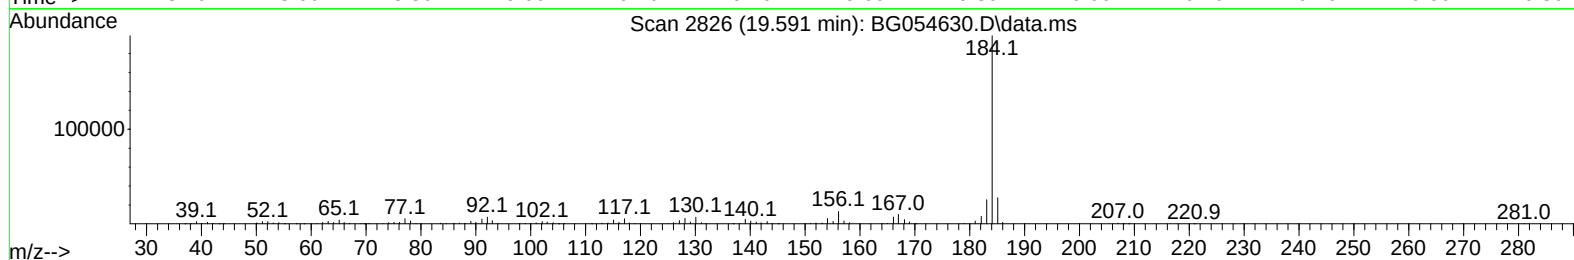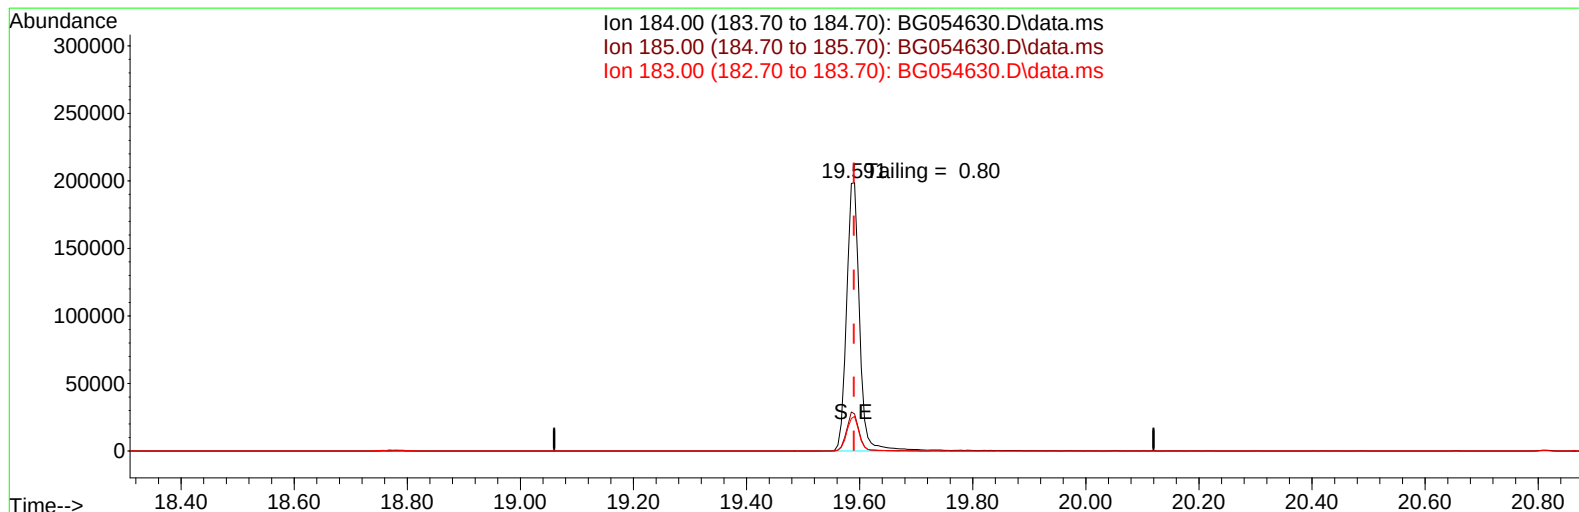

TIC: BG054630.D\data.ms

(77) Benzidine**19.591min (+ 0.001) 301340.21 ng****response 316535**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.85
183.00	11.10	12.88
0.00	0.00	0.00