


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081422\
 Data File : BG054630.D
 Acq On : 14 Aug 2022 12:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Aug 13 00:32:40 2022

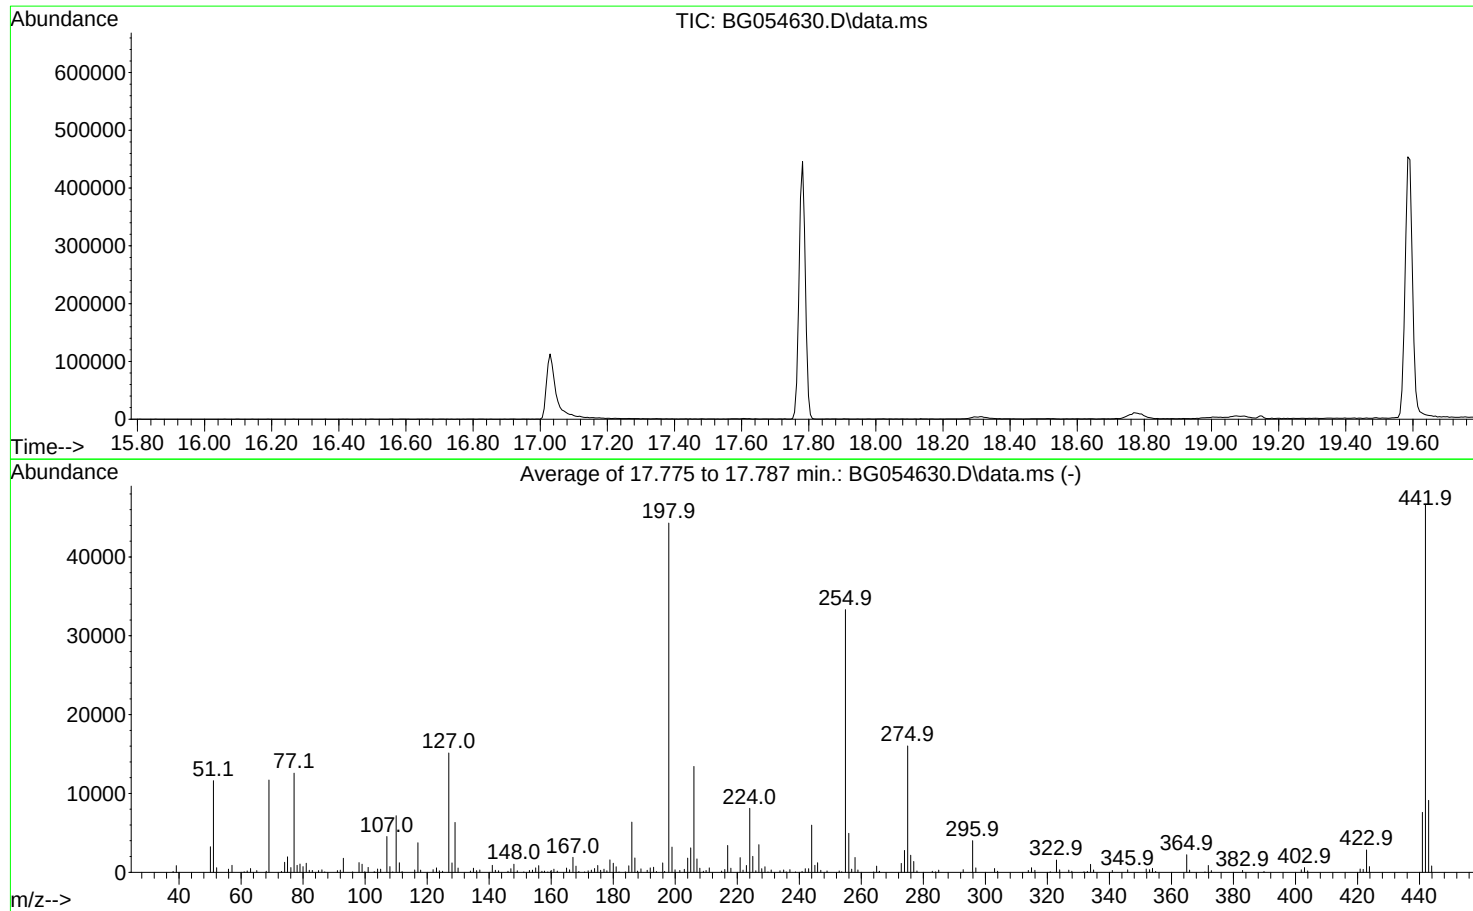




AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.2	11627	PASS
68	69	0.00	2	1.2	139	PASS
69	198	0.00	100	26.4	11695	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	34.2	15133	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	44304	PASS
199	198	5	9	7.2	3196	PASS
275	198	10	60	36.2	16034	PASS
365	198	1	100	5.0	2221	PASS
441	198	0.01	100	17.2	7607	PASS
442	442	50	100	100.0	46664	PASS
443	442	15	24	19.5	9120	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081422\
Data File : BG054630.D
Acq On : 14 Aug 2022 12:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 14 13:26:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 13 00:32:40 2022
Response via : Initial Calibration

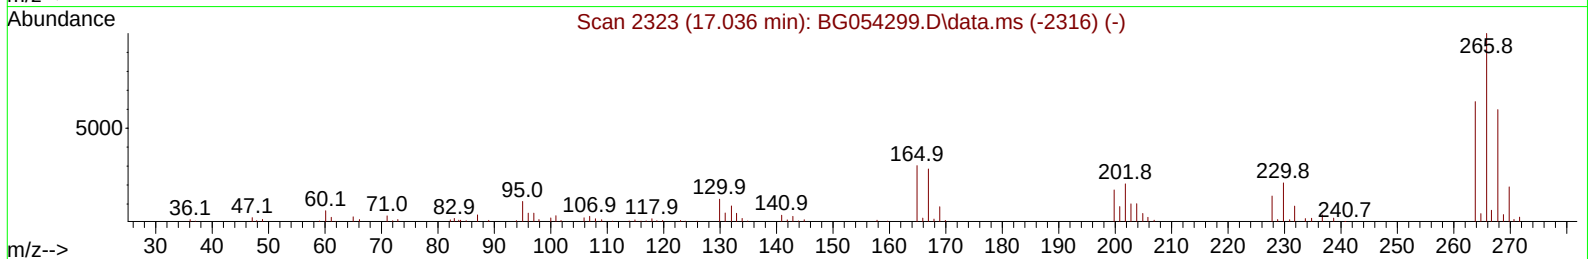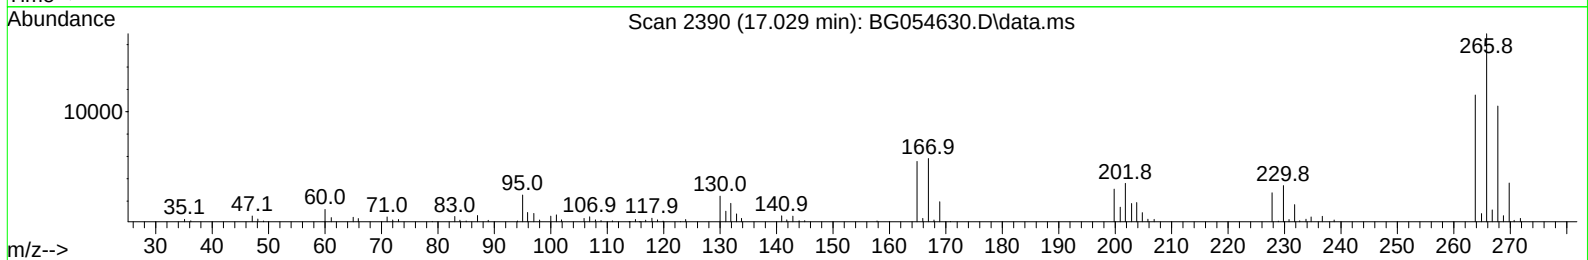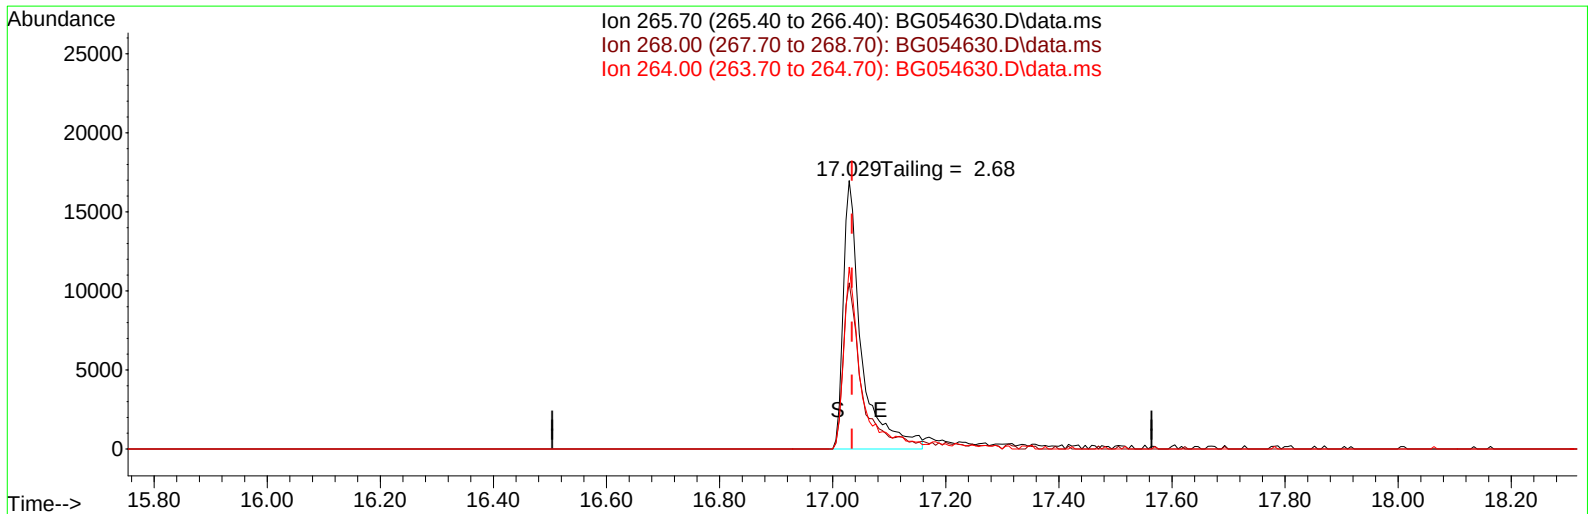

TIC: BG054630.D\data.ms

(70) Pentachlorophenol (C)

17.029min (-0.005) 33335.51 ng




response 37289

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	61.90
264.00	66.20	67.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081422\
Data File : BG054630.D
Acq On : 14 Aug 2022 12:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 14 13:26:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 13 00:32:40 2022
Response via : Initial Calibration

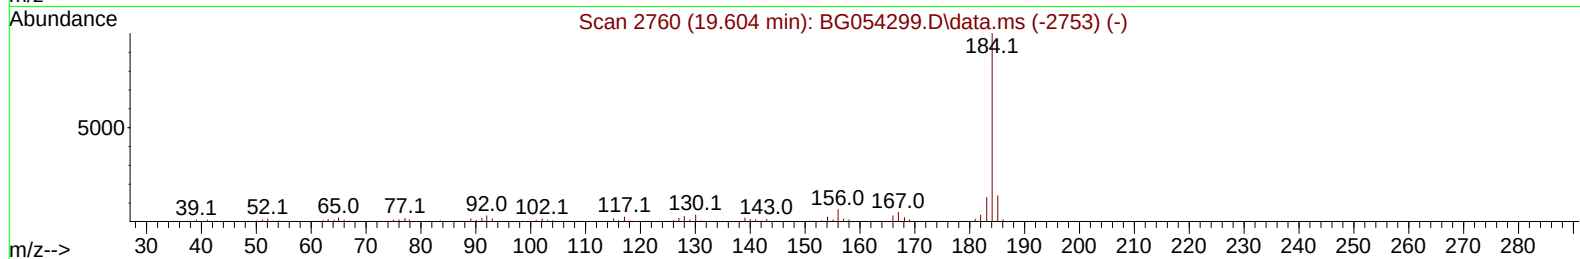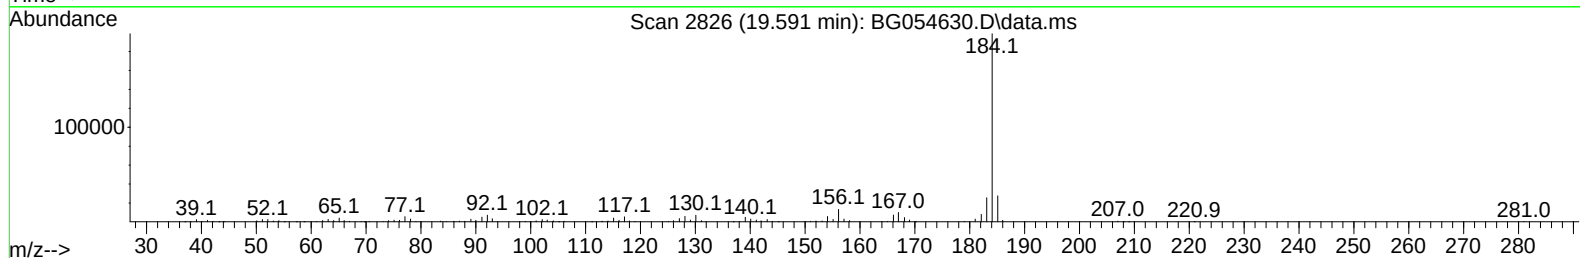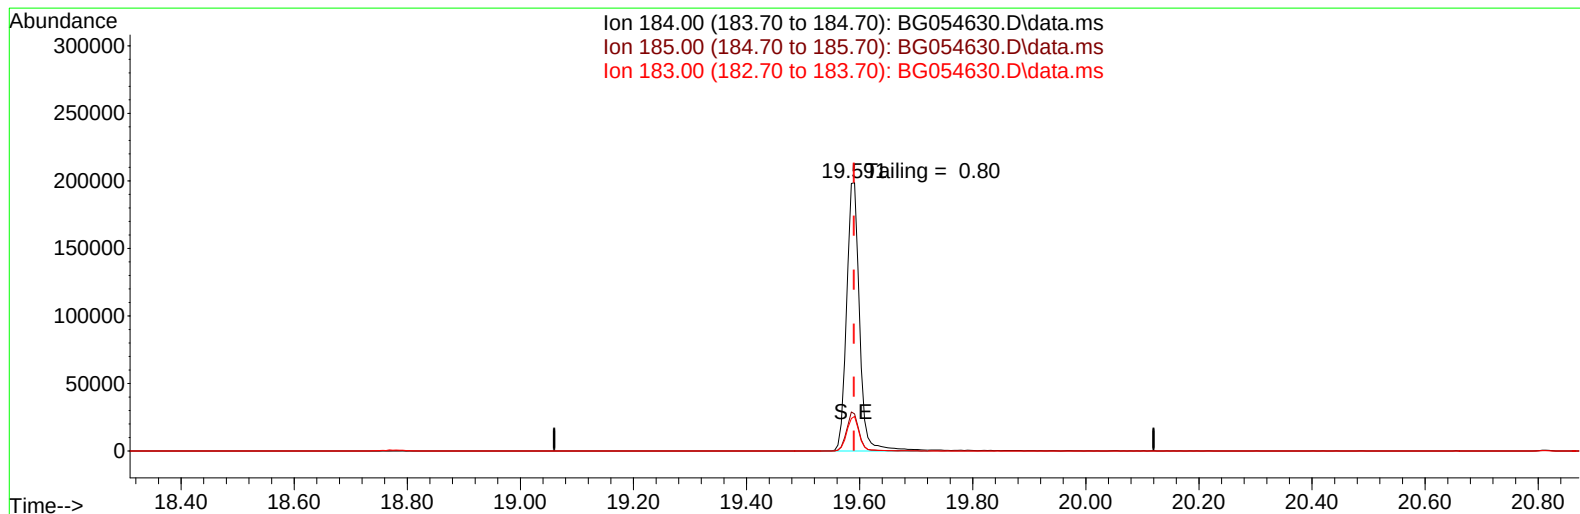

TIC: BG054630.D\data.ms

(77) Benzidine**19.591min (+ 0.001) 301340.21 ng****response 316535**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.85
183.00	11.10	12.88
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/14/2022	BNA_G	BG054630.D
Compound Name	Response	Retention Time
DDT	186045	20.813
DDD	3114	20.425
DDE	306	19.885
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3420	189465	1.81

Instrument :
BNA_G
ClientSampleId :
DFTPP