


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081424\
Data File : BG062389.D
Acq On : 14 Aug 2024 10:50
Operator : MA/JU
Sample : DFTPP412
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP412

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Title : SVOA CALIBRATION
Last Update : Wed Aug 14 15:31:21 2024

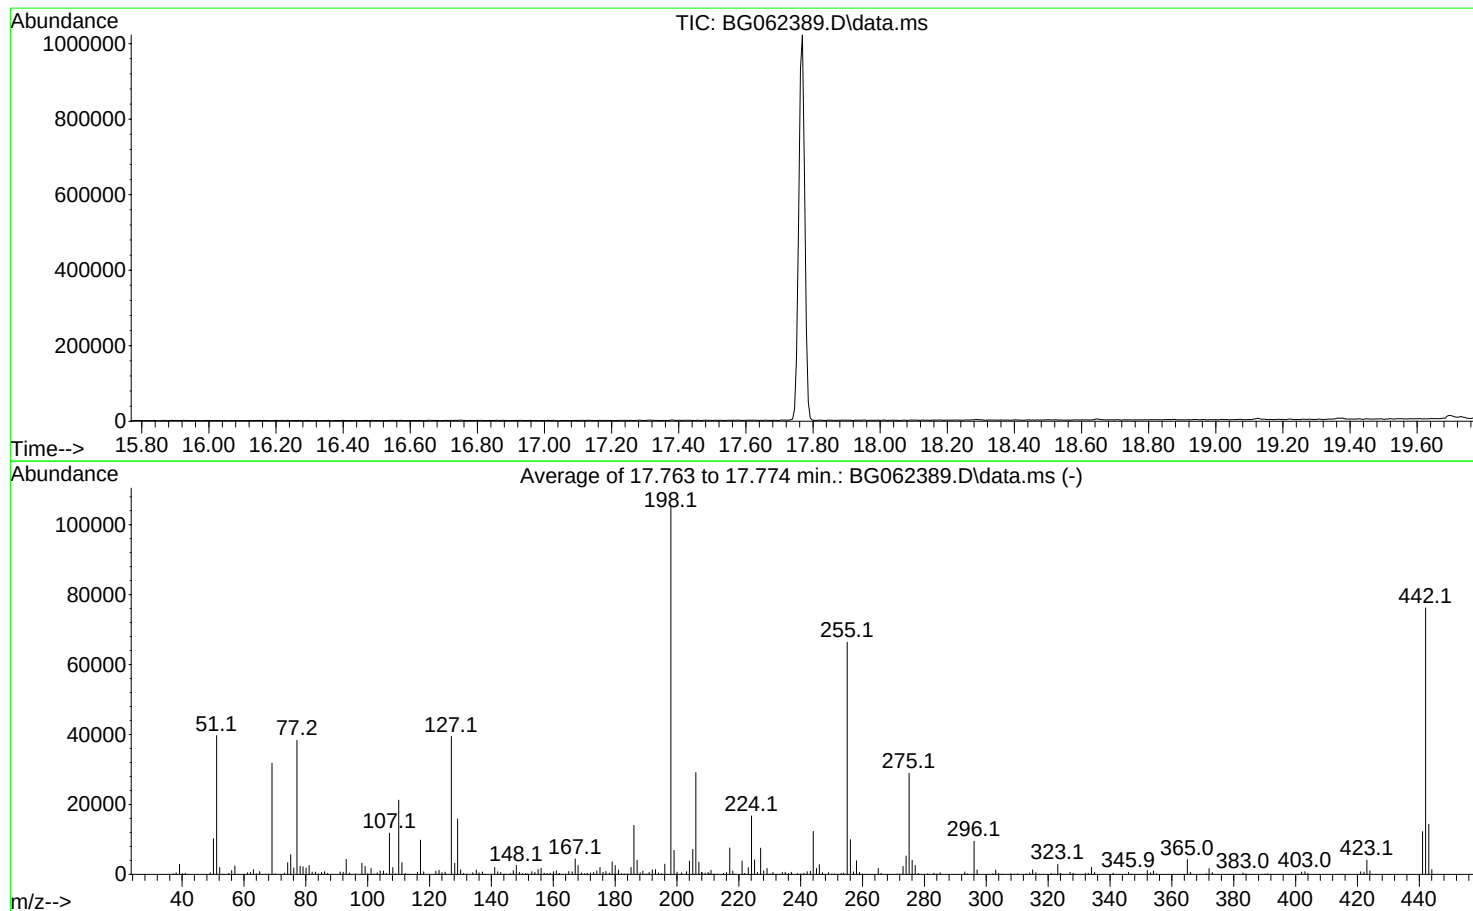

AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	39653	PASS
68	69	0.00	2	0.4	119	PASS
69	198	0.00	100	30.2	31803	PASS
70	69	0.00	2	0.5	166	PASS
127	198	10	80	37.5	39440	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	105197	PASS
199	198	5	9	6.5	6861	PASS
275	198	10	60	27.5	28923	PASS
365	198	1	100	4.0	4224	PASS
441	198	0.01	100	11.6	12232	PASS
442	198	50	100	72.4	76189	PASS
443	442	15	24	18.8	14312	PASS

m/z	Abundance
44.15	2020.0
83.75	159.0
167.05	363.0
207.15	226.0

Instrument :

BNA_G

ClientSampleId :

DFTPP412

m/z	Abundance
37.05	242.0
38.05	621.0
39.15	3224.0
40.15	281.0
41.05	265.0
44.15	1621.0
49.15	526.0
50.15	12451.0
51.15	48760.0
52.15	2336.0
53.05	187.0
55.05	349.0
56.05	1283.0
57.05	3063.0
58.15	205.0
61.15	625.0
62.15	685.0
63.05	1664.0
64.15	203.0
65.15	946.0
67.15	214.0
69.05	39216.0
70.05	256.0
73.15	468.0
74.15	4285.0
75.15	6472.0
76.05	2218.0
77.15	46048.0
78.15	3028.0
79.05	2419.0
80.05	2109.0
81.05	2840.0
82.05	902.0
83.05	720.0
84.15	198.0
85.15	516.0
86.15	791.0
87.05	441.0
88.15	174.0
91.05	775.0
92.05	626.0
93.05	5355.0
94.05	433.0
96.05	420.0
98.15	3565.0
99.15	2881.0
100.15	342.0
101.15	2193.0
102.05	161.0
103.05	599.0
104.05	1029.0
105.05	919.0
106.05	458.0
107.05	13505.0
108.05	2033.0
110.05	25144.0
111.05	3822.0
112.15	403.0
113.05	206.0
116.15	741.0
117.05	11192.0
118.15	876.0
122.05	996.0
123.05	1443.0
124.05	500.0
125.05	588.0
127.05	45504.0
128.15	3945.0
129.05	17888.0
130.05	1543.0
131.15	499.0
134.05	555.0
135.05	1655.0
135.95	444.0
137.05	856.0
141.05	2201.0
142.05	833.0
143.05	518.0
144.15	251.0
144.95	204.0
146.15	400.0
147.05	1301.0
148.05	2988.0
149.05	745.0
150.05	172.0
151.05	310.0
151.85	224.0
153.05	1085.0
154.05	805.0
155.05	1503.0
156.05	1917.0
157.05	414.0

Instrument :
BNA_G
ClientSampleId :
DFTPP412

157.95	484.0
159.05	258.0
160.05	674.0
161.05	991.0
162.05	356.0
164.05	208.0
165.05	960.0
166.15	823.0
167.15	5348.0
168.05	2804.0
169.05	378.0
171.05	341.0
172.05	421.0
173.05	549.0
174.05	1290.0
175.15	2127.0
176.15	519.0
176.95	918.0
178.15	415.0
179.05	3730.0
180.05	3036.0
181.15	1319.0
182.05	241.0
182.95	238.0
184.05	285.0
185.15	2011.0
186.15	15694.0
187.05	4276.0
188.15	597.0
188.95	845.0
190.15	214.0
190.95	657.0
192.05	1670.0
193.05	1529.0
194.05	591.0
195.15	222.0
195.95	2863.0
198.05	113576.0
199.05	7129.0
200.05	695.0
201.55	426.0
203.05	744.0
204.05	4262.0
205.15	6972.0
206.15	32152.0
207.15	3974.0
207.95	1174.0
209.05	448.0
210.15	558.0
211.05	1355.0
212.15	169.0
215.15	379.0
216.15	702.0
217.05	8235.0
218.05	1133.0
221.05	4011.0
223.05	2326.0
224.05	17464.0
225.15	3996.0
225.95	481.0
227.05	7587.0
228.05	1011.0
229.05	1697.0
230.15	242.0
231.05	498.0
234.05	554.0
234.95	655.0
236.05	442.0
237.05	726.0
239.05	175.0
240.15	361.0
241.15	546.0
242.15	769.0
243.15	921.0
244.05	12953.0
245.05	1768.0
246.05	3016.0
247.05	595.0
248.95	525.0
249.95	175.0
250.95	157.0
253.05	358.0
253.85	431.0
255.05	67416.0
256.05	10681.0
257.05	855.0
258.05	4055.0
259.05	544.0
260.05	169.0
265.05	1768.0
265.95	320.0
271.05	170.0
272.05	199.0
273.05	2491.0
274.05	5405.0
275.05	28856.0

Instrument :
BNA_G
ClientSampleId :
DFTPP412

276.05	4225.0
277.05	2287.0
277.95	350.0
281.05	201.0
283.05	292.0
284.05	264.0
285.05	412.0
293.05	909.0
293.95	152.0
296.05	9415.0
297.05	1268.0
302.05	209.0
303.05	1365.0
303.95	258.0
307.85	166.0
310.05	152.0
312.95	179.0
313.95	330.0
315.05	1189.0
316.05	421.0
320.95	347.0
322.15	181.0
323.05	2904.0
323.95	551.0
327.15	615.0
328.05	368.0
332.15	307.0
333.05	246.0
334.05	1955.0
335.05	510.0
340.95	342.0
345.85	523.0
352.15	1107.0
353.15	479.0
354.05	1009.0
364.95	3788.0
365.95	395.0
371.15	246.0
372.05	1406.0
373.05	385.0
382.95	232.0
389.95	178.0
390.95	197.0
391.75	157.0
401.95	477.0
402.95	627.0
403.85	452.0
421.05	655.0
422.15	553.0
423.05	3605.0
424.05	1010.0
441.05	10203.0
442.05	66080.0
443.05	12643.0
444.05	1245.0

Instrument :
BNA_G
ClientSampleId :
DFTPP412

m/z	Abundance
37.15	199.0
38.15	442.0
39.15	3504.0
40.15	309.0
41.05	266.0
44.15	2032.0
49.05	425.0
50.15	11853.0
51.15	45688.0
52.15	2405.0
55.15	409.0
56.05	1309.0
57.05	2677.0
61.15	507.0
62.05	721.0
63.05	1581.0
64.05	340.0
65.05	907.0
69.05	36584.0
70.15	242.0
73.15	424.0
74.15	3835.0
75.05	6462.0
76.15	2124.0
77.15	44280.0
78.15	2168.0
79.15	2564.0
80.15	2253.0
81.05	3042.0
82.05	680.0
83.15	815.0
85.05	685.0
86.05	1029.0
87.05	288.0
91.05	743.0
92.15	785.0
93.05	4836.0
94.15	448.0
95.95	200.0
98.15	3832.0
99.15	2384.0
99.95	262.0
101.05	1736.0
101.95	193.0
103.15	571.0
104.05	1266.0
105.15	1214.0
107.05	14350.0
108.15	2265.0
110.05	24344.0
111.05	4279.0
112.15	408.0
116.05	719.0
117.05	11462.0
118.05	920.0
119.95	177.0
122.05	1217.0
123.05	1168.0
124.05	415.0
125.05	755.0
127.05	45408.0
128.15	3688.0
129.05	18776.0
130.05	1639.0
131.05	242.0
132.05	237.0
133.95	523.0
135.15	1265.0
136.05	649.0
137.05	684.0
140.05	306.0
141.05	2374.0
142.05	796.0
143.05	734.0
146.05	355.0
147.05	1396.0
148.05	3087.0
149.05	581.0
149.95	199.0
150.25	179.0
151.15	302.0
151.75	321.0
153.05	833.0
154.05	487.0
155.15	1578.0
156.05	1941.0
157.15	384.0
158.15	424.0
158.85	474.0
160.05	954.0
161.05	1185.0
161.75	319.0

Instrument :
BNA_G
ClientSampleId :
DFTPP412

162.05	295.0
163.15	155.0
165.05	936.0
166.05	925.0
167.15	5683.0
168.05	2852.0
169.15	532.0
170.15	186.0
170.95	373.0
172.05	503.0
173.05	497.0
174.15	1052.0
175.05	2276.0
176.05	798.0
177.05	796.0
178.15	431.0
179.05	4651.0
180.05	2819.0
181.05	1562.0
182.05	250.0
183.85	394.0
185.15	2450.0
186.05	15966.0
187.15	5133.0
187.95	460.0
189.05	1193.0
189.95	179.0
191.05	654.0
192.05	1405.0
193.05	1659.0
194.05	410.0
195.05	291.0
196.05	3738.0
198.05	124120.0
199.05	8551.0
200.05	715.0
201.55	458.0
203.15	872.0
204.05	4561.0
205.05	8898.0
206.05	34104.0
207.15	4474.0
208.15	1372.0
209.05	347.0
210.05	730.0
210.95	1469.0
211.75	226.0
213.05	195.0
214.95	444.0
216.05	537.0
217.05	9069.0
218.05	1197.0
218.95	176.0
221.05	4605.0
223.05	2080.0
224.05	20040.0
225.05	5204.0
226.05	667.0
227.05	9265.0
228.05	1268.0
229.05	1967.0
230.05	193.0
231.05	643.0
233.15	190.0
234.05	708.0
235.05	875.0
236.05	222.0
236.95	582.0
238.95	450.0
240.05	258.0
240.95	286.0
242.05	960.0
243.15	1055.0
244.05	14209.0
245.15	1900.0
246.05	3192.0
247.05	446.0
247.95	163.0
249.05	542.0
250.15	182.0
250.95	156.0
251.95	328.0
253.15	446.0
253.85	341.0
255.05	79192.0
256.05	11155.0
257.05	924.0
258.05	4741.0
258.95	661.0
259.95	191.0
260.95	176.0
265.05	1954.0
266.05	247.0
272.05	278.0
273.15	2685.0
274.05	6271.0

Instrument :
BNA_G
ClientSampleId :
DFTPP412

275.05	34264.0
276.05	4762.0
276.95	3379.0
278.05	447.0
283.15	335.0
284.05	159.0
285.15	514.0
293.05	604.0
294.05	192.0
296.05	11097.0
297.05	1528.0
302.05	238.0
303.05	1600.0
303.95	353.0
305.15	163.0
307.95	191.0
309.05	151.0
310.05	197.0
313.95	440.0
314.95	1485.0
315.95	594.0
317.15	164.0
321.05	204.0
323.05	3068.0
324.15	562.0
327.05	727.0
327.95	373.0
332.15	290.0
333.05	293.0
334.05	2372.0
334.95	524.0
341.05	486.0
345.95	687.0
351.95	1440.0
353.15	524.0
354.05	1232.0
355.05	192.0
365.05	5278.0
366.05	905.0
371.05	295.0
372.05	2095.0
373.05	703.0
383.05	558.0
383.95	250.0
390.15	184.0
400.95	157.0
401.95	921.0
403.05	1009.0
403.95	332.0
415.15	162.0
421.05	869.0
422.05	817.0
423.05	4722.0
424.05	1244.0
441.05	15086.0
442.05	90472.0
443.05	17192.0
444.05	1606.0

Instrument :
BNA_G
ClientSampleId :
DFTPP412

m/z	Abundance
38.15	292.0
39.15	1871.0
41.15	240.0
44.05	2034.0
49.15	439.0
50.15	6358.0
51.15	24512.0
52.15	1119.0
55.15	208.0
56.05	740.0
57.15	1494.0
61.15	255.0
62.15	316.0
63.15	742.0
65.15	433.0
68.05	357.0
69.05	19608.0
73.05	269.0
74.15	1899.0
75.15	3980.0
76.05	1104.0
77.15	24760.0
78.05	1732.0
79.05	1462.0
80.05	1201.0
81.15	1649.0
82.15	442.0
83.05	393.0
84.15	253.0
85.05	394.0
86.15	548.0
87.15	222.0
91.15	532.0
92.05	402.0
93.15	2687.0
94.05	277.0
98.05	2270.0
99.05	1736.0
100.05	175.0
101.05	1121.0
103.05	278.0
104.05	683.0
105.05	695.0
106.05	375.0
107.05	7604.0
108.05	1571.0
108.95	371.0
110.05	14265.0
111.05	2034.0
116.05	395.0
117.05	6714.0
118.05	430.0
122.15	589.0
123.05	914.0
123.95	565.0
125.05	539.0
127.05	27408.0
128.05	1981.0
129.05	10811.0
130.05	733.0
130.95	239.0
131.95	151.0
133.95	299.0
135.15	810.0
136.05	303.0
137.15	524.0
137.95	156.0
141.05	1390.0
142.05	581.0
143.05	409.0
147.05	646.0
148.05	1595.0
149.15	305.0
149.85	151.0
150.95	195.0
153.05	480.0
154.05	303.0
155.05	1029.0
156.05	1410.0
156.95	260.0
157.95	249.0
159.05	321.0
160.05	694.0
160.95	853.0
162.05	196.0
163.95	170.0
165.05	624.0
166.05	437.0
167.05	3221.0
168.05	1929.0
169.05	315.0
170.15	242.0

Instrument :
BNA_G
ClientSampleId :
DFTPP412

170.85	190.0
172.05	372.0
173.05	470.0
174.05	586.0
175.15	1462.0
176.15	525.0
176.95	728.0
178.15	316.0
179.05	2393.0
180.05	1733.0
181.05	860.0
181.95	160.0
184.15	179.0
185.15	1404.0
186.05	10373.0
187.15	2631.0
188.15	353.0
189.05	746.0
191.05	326.0
191.95	798.0
192.95	1009.0
194.15	226.0
196.15	2145.0
198.05	77896.0
198.95	4902.0
200.05	456.0
201.45	380.0
203.05	680.0
204.05	2553.0
205.05	5530.0
206.05	21080.0
207.05	2824.0
207.95	583.0
209.15	358.0
210.05	448.0
210.45	406.0
211.05	608.0
215.15	150.0
215.95	381.0
217.05	5317.0
218.05	609.0
221.05	2936.0
221.95	949.0
223.05	1313.0
224.15	12552.0
225.05	3333.0
225.95	466.0
227.05	5652.0
228.05	773.0
229.15	1360.0
231.05	514.0
234.15	461.0
235.15	286.0
235.95	215.0
237.05	539.0
240.95	331.0
242.05	625.0
243.15	692.0
244.05	9694.0
245.05	1360.0
246.05	2203.0
247.05	394.0
249.05	442.0
252.95	203.0
253.95	390.0
255.05	52536.0
256.05	7967.0
257.15	495.0
258.05	2937.0
259.05	462.0
265.05	1402.0
266.05	211.0
271.25	180.0
273.05	1741.0
274.05	4178.0
275.05	23648.0
276.05	3268.0
277.05	2096.0
278.25	191.0
281.05	193.0
282.95	295.0
285.15	456.0
293.05	582.0
294.05	206.0
296.05	7847.0
297.05	1048.0
302.15	153.0
303.05	799.0
304.05	278.0
308.05	154.0
312.95	152.0
314.05	542.0
314.95	1106.0
316.05	499.0
321.05	307.0
322.05	208.0

Instrument :
BNA_G
ClientSampleId :
DFTPP412

323.15	2553.0
323.95	431.0
327.05	426.0
328.15	249.0
328.85	169.0
332.05	243.0
332.95	230.0
333.95	1672.0
335.05	564.0
341.05	314.0
346.05	507.0
347.05	244.0
352.05	675.0
352.95	446.0
354.15	742.0
355.05	287.0
364.95	3606.0
366.05	553.0
372.05	1408.0
373.05	391.0
382.95	433.0
383.95	151.0
391.05	159.0
402.05	465.0
403.05	699.0
404.05	244.0
421.05	694.0
422.05	560.0
423.05	3846.0
424.05	813.0
441.05	11407.0
442.05	72016.0
443.05	13100.0
444.05	1233.0

Instrument :
BNA_G
ClientSampleId :
DFTPP412