
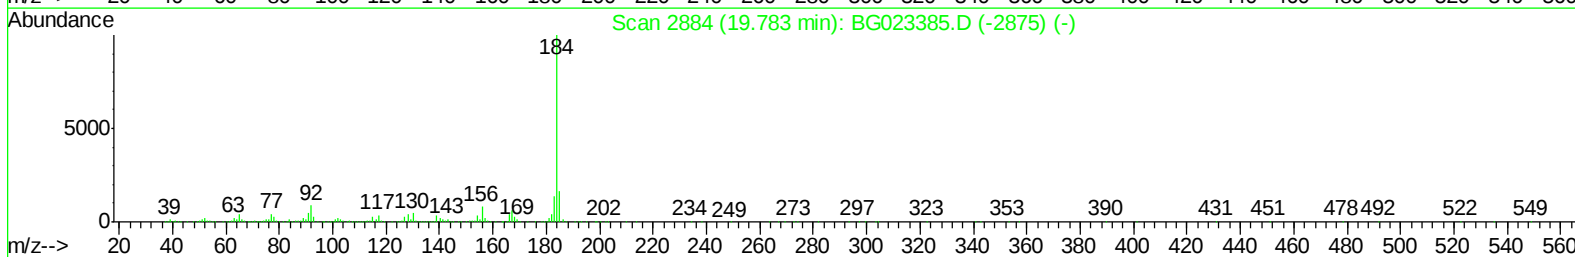
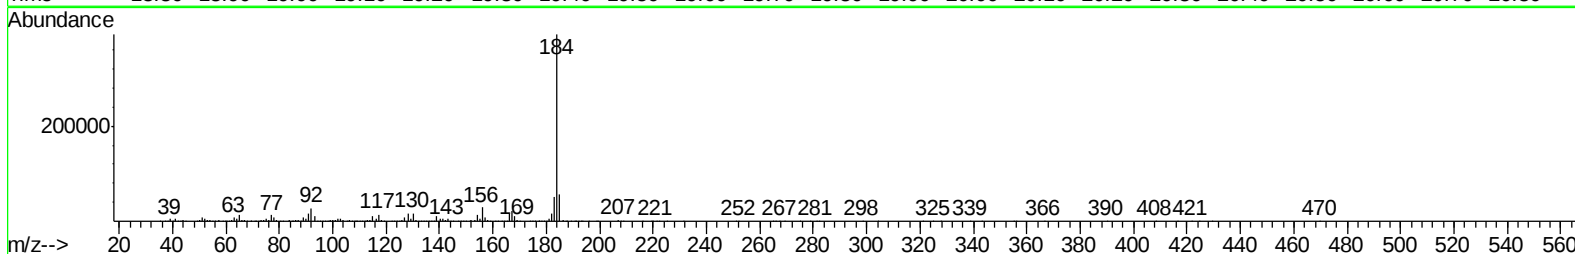


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081516\
Data File : BG023717.D
Acq On : 15 Aug 2016 9:25
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 04:29:43 2016
Quant Method : Z:\HPCHEM1\BNA_G\Methods\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 01 19:22:14 2016
Response via : Initial Calibration

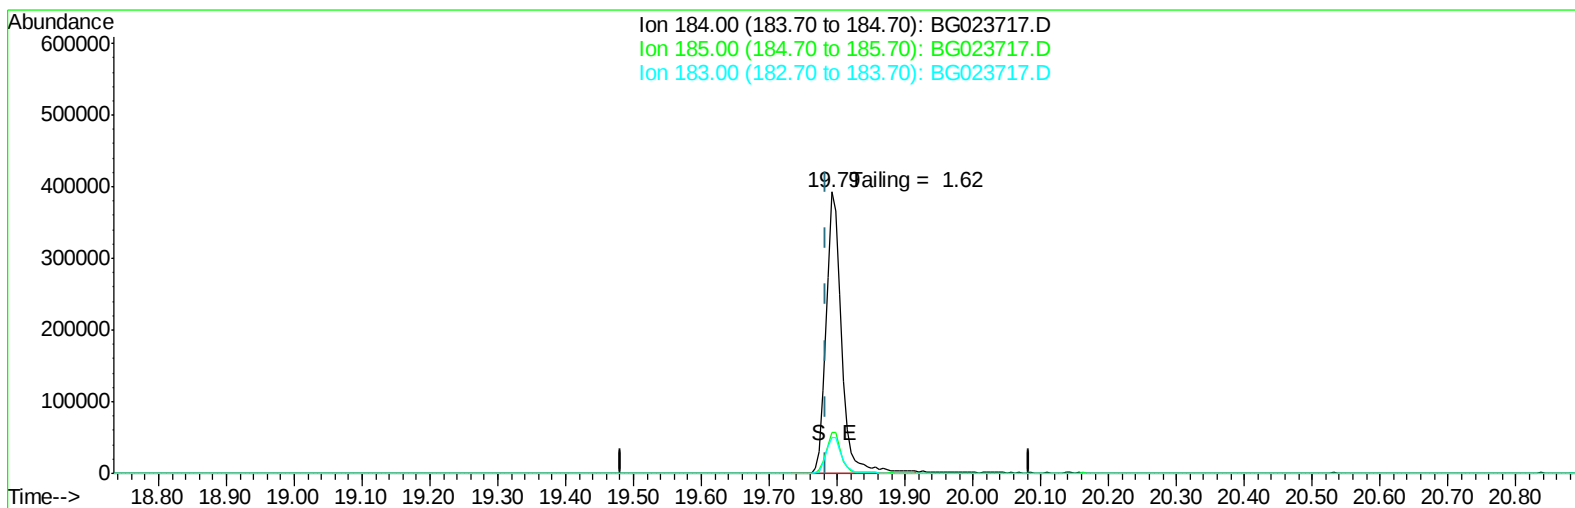

TIC: BG023717.D

(76) Benzidine




19.792min (+0.009) 42579.42ng

response 617864

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.57
183.00	13.40	12.78
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081516\
Data File : BG023717.D
Acq On : 15 Aug 2016 9:25
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 04:29:43 2016
Quant Method : Z:\HPCHEM1\BNA_G\Methods\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 01 19:22:14 2016
Response via : Initial Calibration

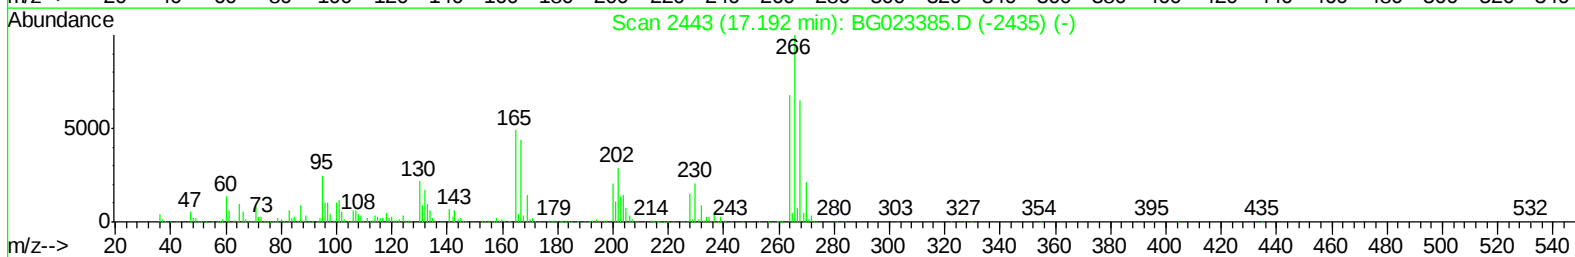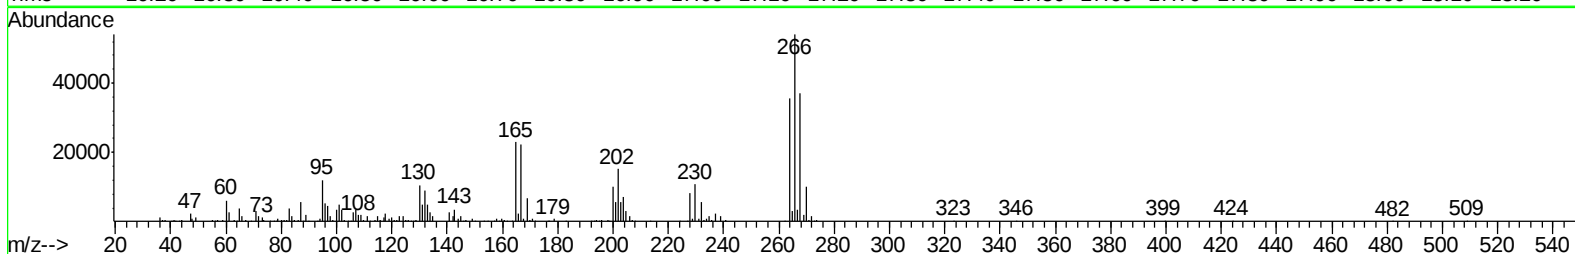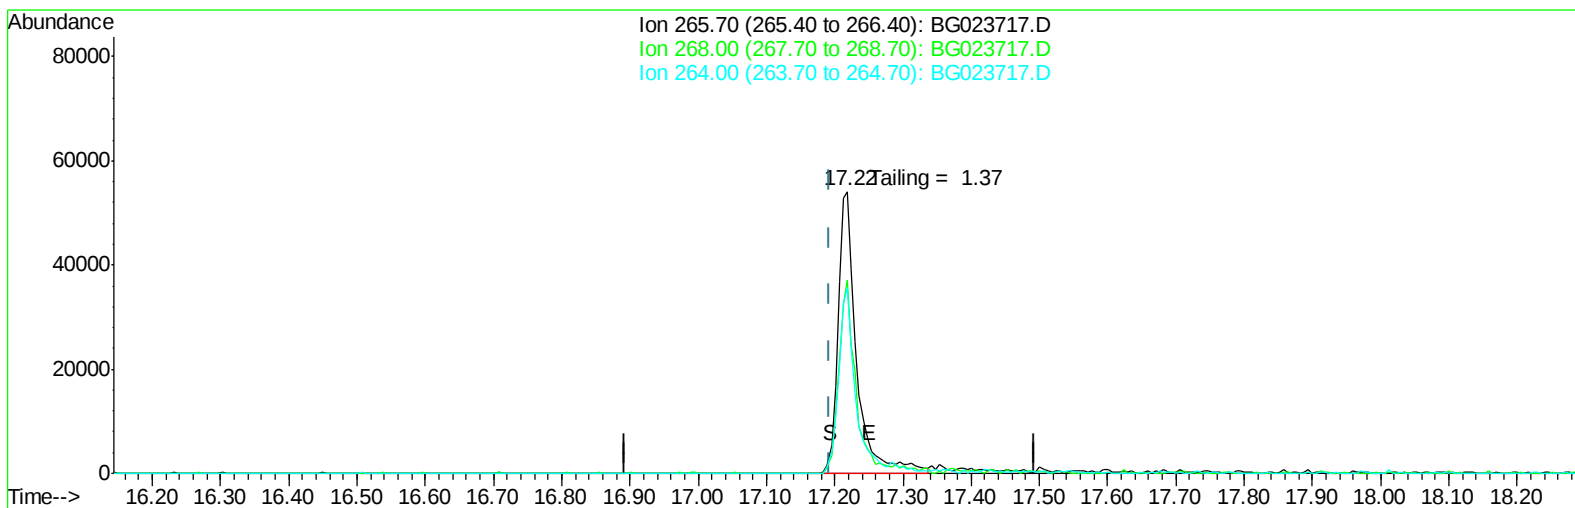

TIC: BG023717.D

(69) Pentachlorophenol (C)

17.219min (+0.026) 215982.56ng

response 99547

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	68.61
264.00	63.20	65.80
0.00	0.00	0.00