

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA G\DATA\BG081517\
 Data File : BG028361.D
 Acq On : 16 Aug 2017 2:38
 Operator : SJ/JU
 Sample : I4672-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampled :
 C0AH4

Manual Integrations
 APPROVED

Sohil
 8/16/2017 6:40:27 PM

Quant Time: Aug 16 04:57:12 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
 Quant Title : SVOA CALIBRATION
 OLast Update : Wed Aug 16 04:06:35 2017
 Response via : Initial Calibration

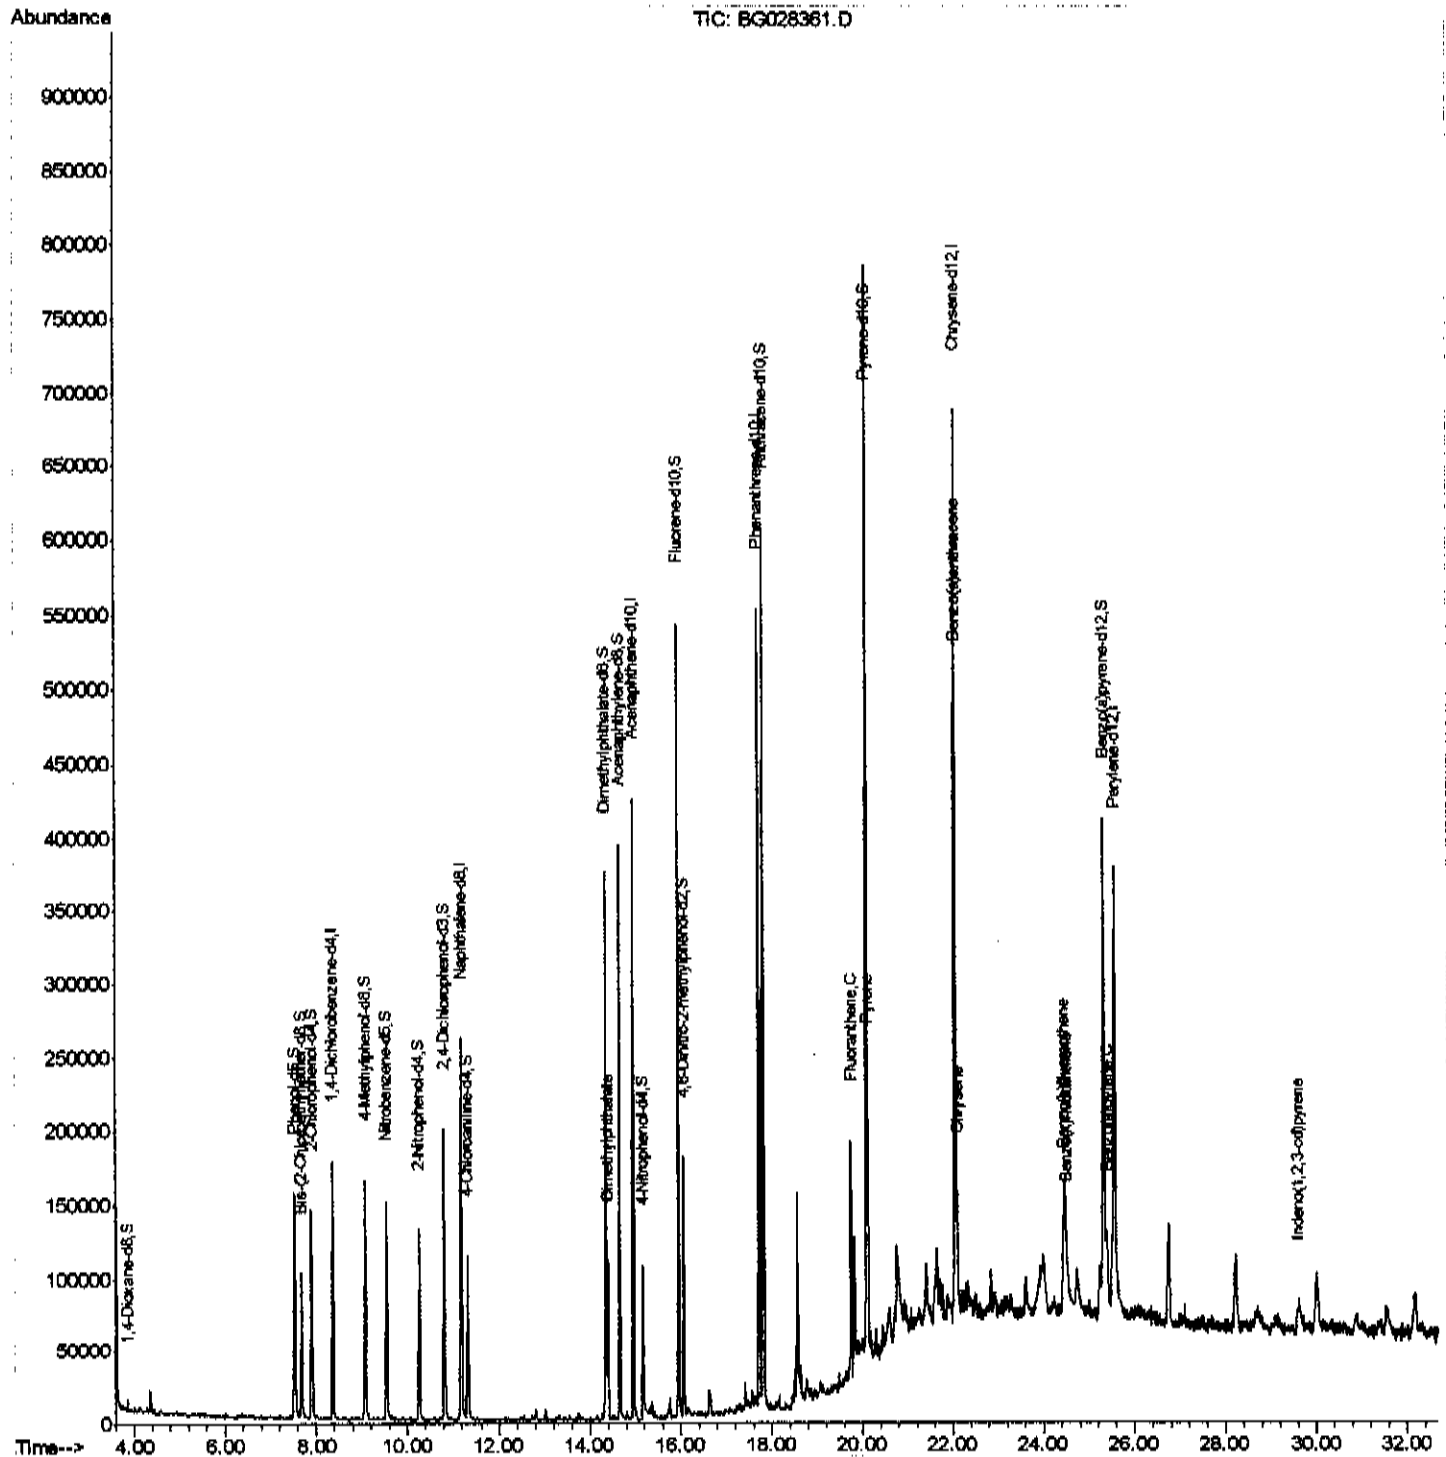

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA G\DATA\BG081517\
 Data File : BG028361.D
 Acq On : 16 Aug 2017 2:38
 Operator : SJ/JU
 Sample : I4672-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampled :
 C0AH4

Manual Integrations
 APPROVED

Sohil
 8/16/2017 6:40:27 PM

Quant Time: Aug 16 04:09:34 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 16 04:06:35 2017
 Response via : Initial Calibration

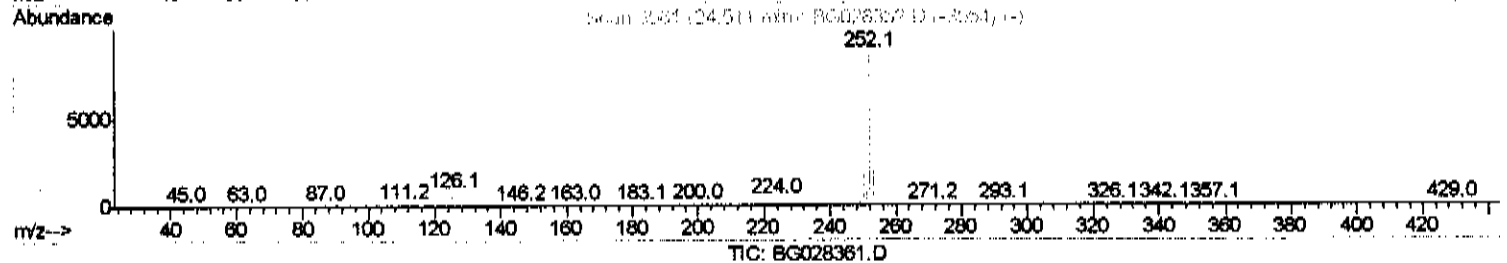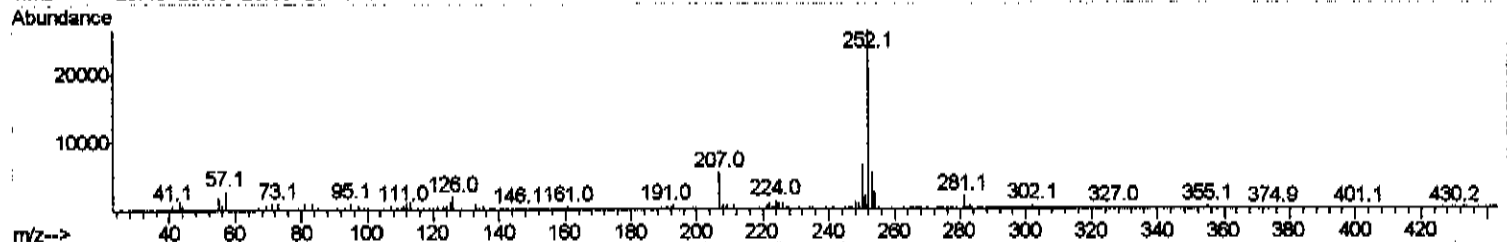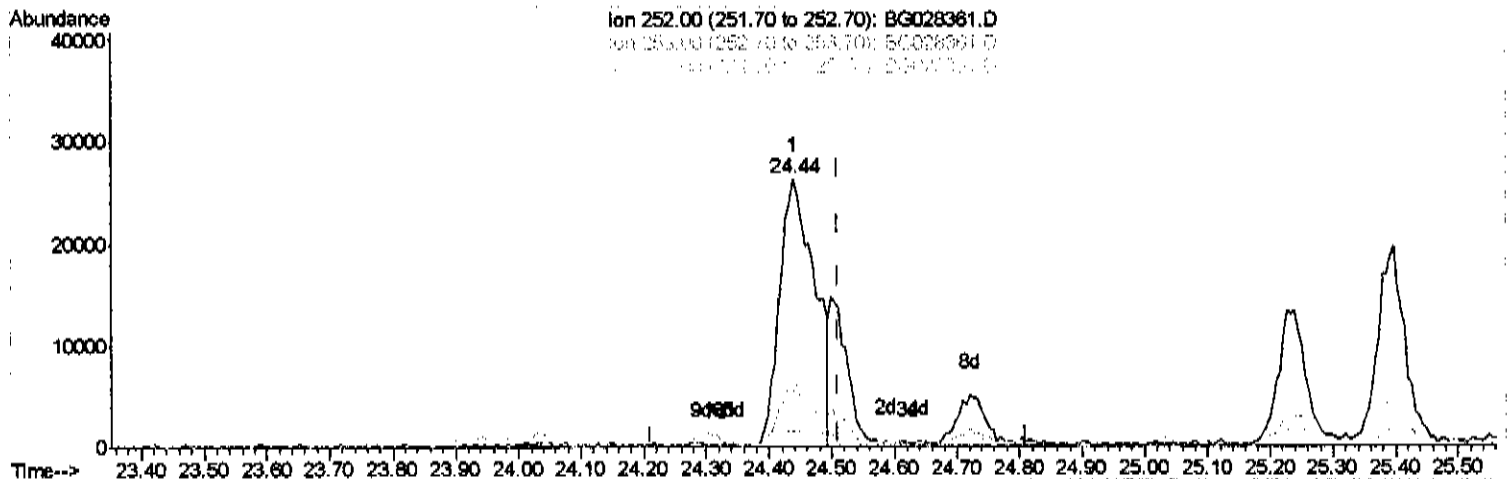

(86) Benzo(k)fluoranthene

24.439min (-0.072) 4.66ng/ul

response 101504

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	21.05
125.00	5.10	5.46
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA G\DATA\BG081517\
 Data File : BG028361.D
 Acq On : 16 Aug 2017 2:38
 Operator : SJ/JU
 Sample : I4672-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampled :
 C0AH4

Manual Integrations
 APPROVED

Sohil
 8/16/2017 6:40:27 PM

Quant Time: Aug 16 04:09:34 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 16 04:06:35 2017
 Response via : Initial Calibration

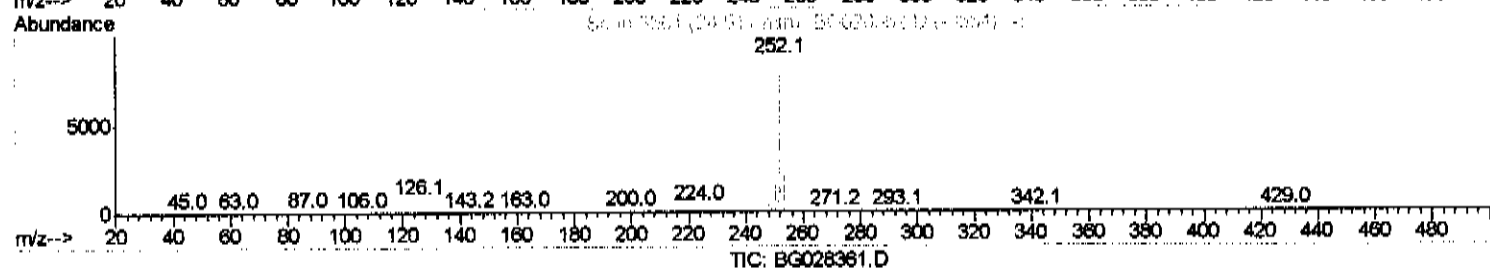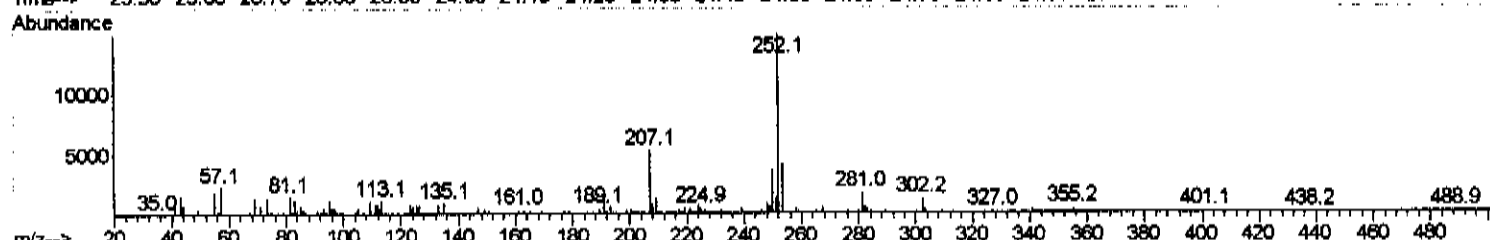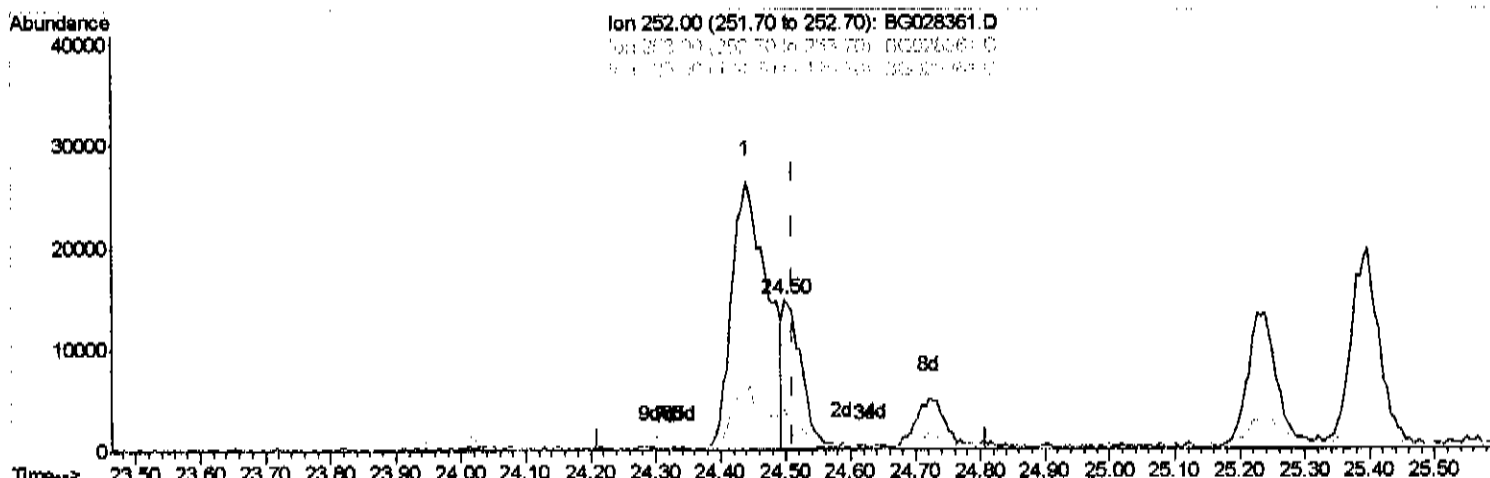

(66) Benzo(k)fluoranthene

24.498min (-0.013) 1.33ng/ul m

response 28965

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	27.57
125.00	5.10	5.93
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Instrument :
BNA_G
ClientSampled :
COAH4

Manual Integrations
APPROVED

Sohil
8/16/2017 6:40:27 PM

Data Path : Z:\HPCHEM1\BNA G\DATA\BG081517\
Data File : BG028361.D
Acq On : 16 Aug 2017 2:38
Operator : SJ/JU
Sample : I4672-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Aug 16 04:57:12 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 16 04:06:35 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.36	152	48282	20.00	ng/ul	0.00
18) Naphthalene-d8	11.18	136	216342	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.96	164	148924	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.71	188	345603	20.00	ng/ul	0.00
75) Chrysene-d12	22.05	240	394198	20.00	ng/ul	0.00
83) Perylene-d12	25.57	264	372833	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.85	96	3096	2.99	ng/uL	0.01
5) Phenol-d5	7.51	99	88024	16.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.67	67	55432	16.51	ng/ul	0.00
9) 2-Chlorophenol-d4	7.89	132	63543	19.00	ng/ul	0.00
13) 4-Methylphenol-d8	9.06	113	67293	15.18	ng/ul	0.00
19) Nitrobenzene-d5	9.53	128	34137	20.18	ng/ul	0.00
22) 2-Nitrophenol-d4	10.25	143	39593	21.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.80	165	76798	20.01	ng/ul	0.00
29) 4-Chloroaniline-d4	11.31	131	64941	15.20	ng/ul	0.00
43) Dimethylphthalate-d6	14.35	166	258007	19.48	ng/ul	0.00
46) Acenaphthylene-d8	14.66	160	304232	20.37	ng/ul	0.00
51) 4-Nitrophenol-d4	15.17	143	32024	15.21	ng/ul	0.00
57) Fluorene-d10	15.95	176	228928	19.27	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.07	200	41486	18.48	ng/ul	0.00
70) Anthracene-d10	17.81	188	367131	22.15	ng/ul	0.00
76) Pvrene-d10	20.09	212	432351	21.39	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.32	264	384125	22.01	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.40	163	67590	5.542	ng/ul	98
74) Fluoranthene	19.75	202	107333	5.078	ng/ul	99
77) Pvrene	20.11	202	94523	4.019	ng/ul	98
80) Benzo(a)anthracene	22.03	228	67277	2.954	ng/ul	97
82) Chrysene	22.10	228	64082	3.124	ng/ul	95
85) Benzo(b)fluoranthene	24.44	252	101504	4.550	ng/ul	98
86) Benzo(k)fluoranthene	24.50	252	28965m	1.329	ng/ul	98
88) Benzo(a)pyrene	25.40	252	58164	2.693	ng/ul#	98
89) Indeno(1,2,3-cd)pyrene	29.60	276	37545	1.484	ng/ul#	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed