

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081517\
 Data File : BG028346.D
 Acq On : 15 Aug 2017 16:41
 Operator : SJ/JU
 Sample : I4672-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AH5

Manual Integrations
 APPROVED

Sohil
 8/16/2017 6:39:52 PM

Quant Time: Aug 16 03:38:53 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 16 01:22:31 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.36	152	48343	20.00	ng/ul	0.00
18) Naphthalene-d8	11.18	136	231457	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.97	164	168755	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.71	188	403451m	20.00	ng/ul	0.00
75) Chrysene-d12	22.05	240	428225	20.00	ng/ul	0.00
83) Perylene-d12	25.57	264	379827	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.84	96	3045	2.93	ng/uL	0.00
5) Phenol-d5	7.51	99	89444	16.85	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.67	67	55857	16.61	ng/ul	0.00
9) 2-Chlorophenol-d4	7.89	132	64920	19.38	ng/ul	0.00
13) 4-Methylphenol-d8	9.06	113	75191	16.94	ng/ul	0.00
19) Nitrobenzene-d5	9.53	128	35322	19.52	ng/ul	0.00
22) 2-Nitrophenol-d4	10.25	143	42372	21.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.80	165	77475	18.87	ng/ul	0.00
29) 4-Chloroaniline-d4	11.31	131	94408	20.66	ng/ul	0.00
43) Dimethylphthalate-d6	14.36	166	276131	18.40	ng/ul	0.00
46) Acenaphthylene-d8	14.66	160	324279	19.16	ng/ul	0.00
51) 4-Nitrophenol-d4	15.17	143	33691	14.12	ng/ul	0.01
57) Fluorene-d10	15.95	176	241588	17.94	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.07	200	41852m	15.97	ng/ul	0.00
70) Anthracene-d10	17.81	188	393091	20.32	ng/ul	0.00
76) Pyrene-d10	20.09	212	457625	20.84	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.32	264	384220	21.61	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	14.40	163	63408	4.588	ng/ul#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG081517\
Data File : BG028346.D
Acq On : 15 Aug 2017 16:41
Operator : SJ/JU
Sample : I4672-07
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
C0AH5

Quant Time: Aug 16 03:38:53 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 16 01:22:31 2017
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
8/16/2017 6:39:52 PM

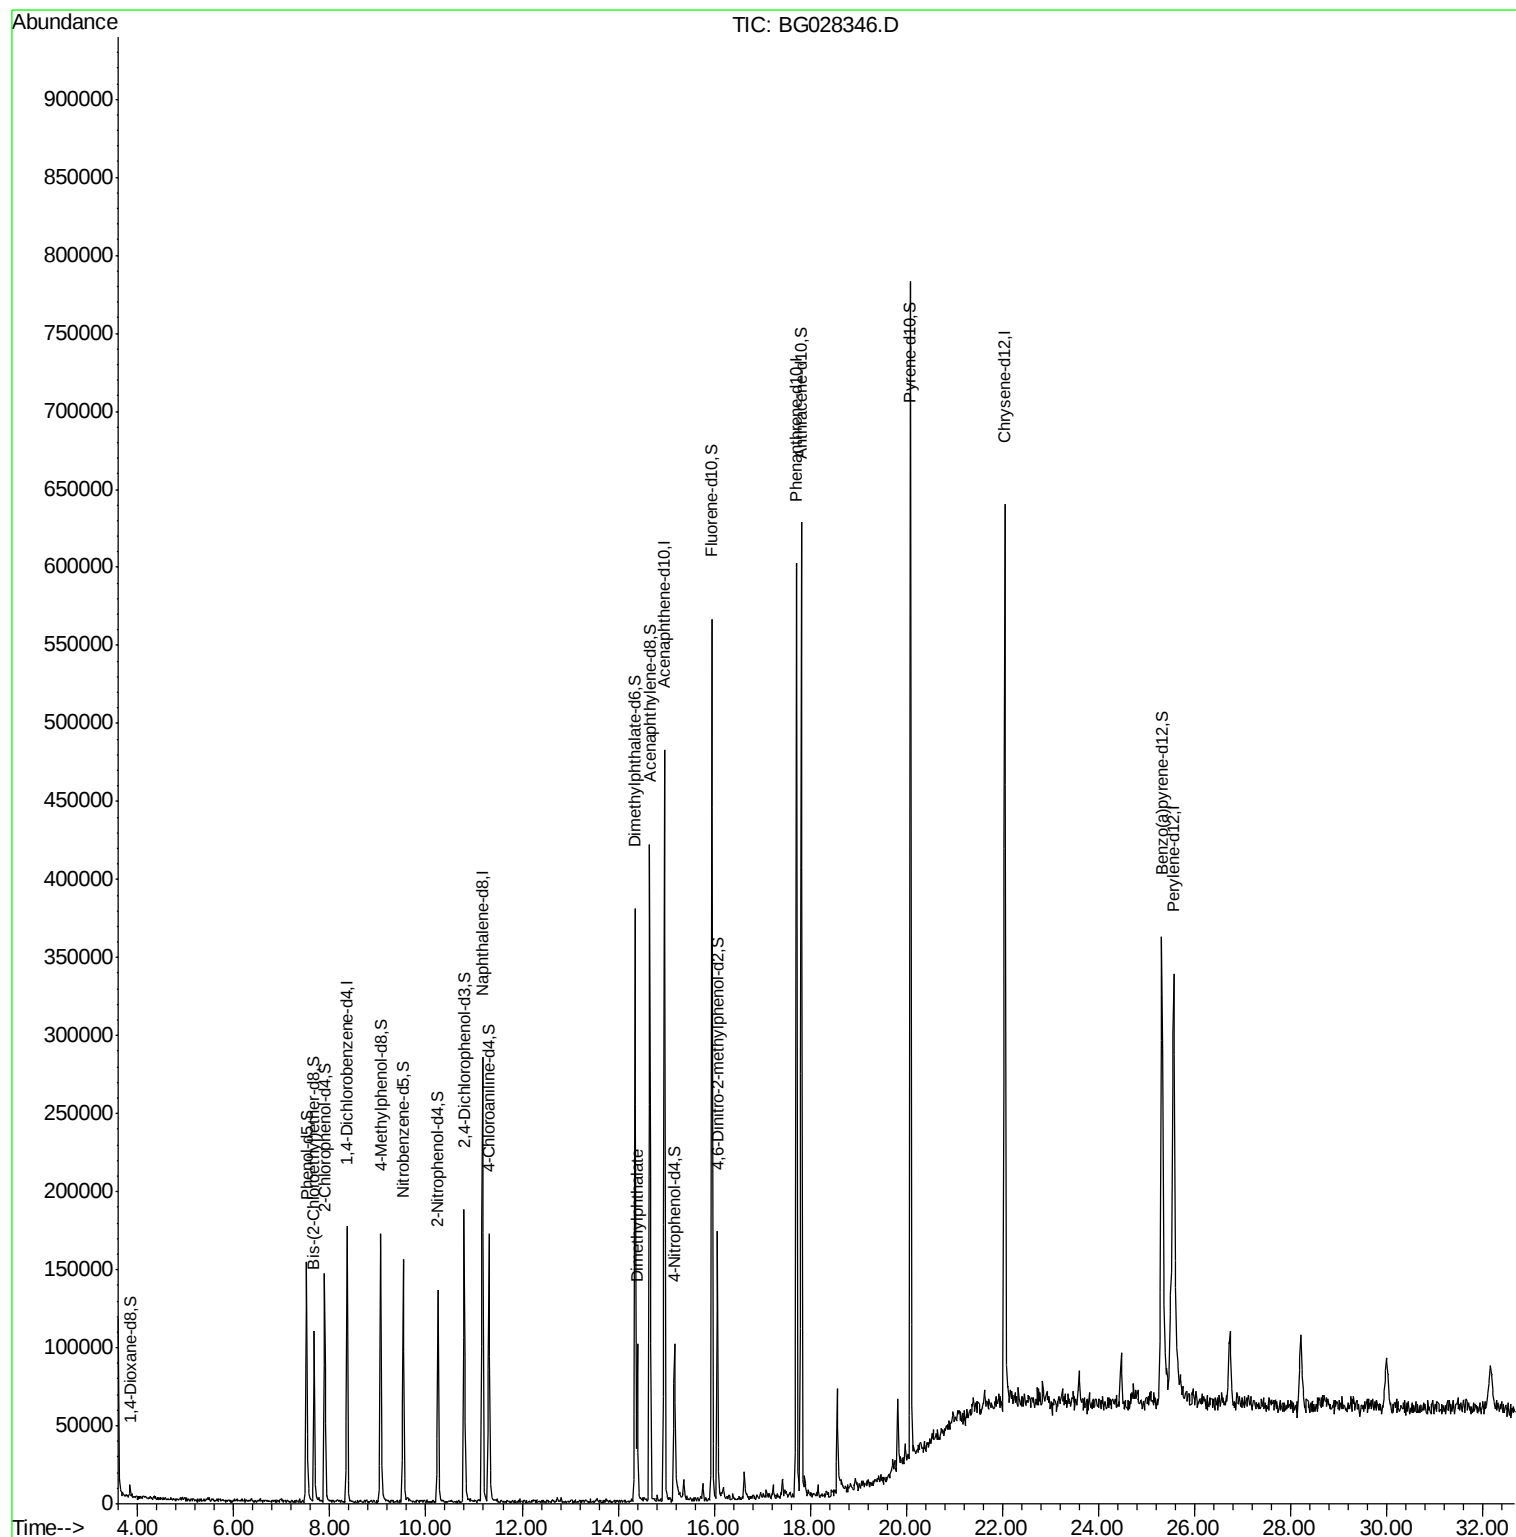

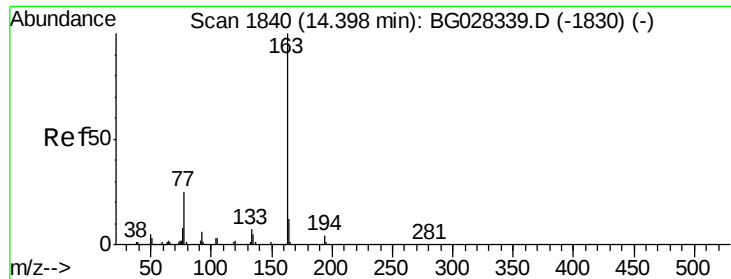

#44
 Dimethylphthalate
 Concen: 4.588 ng/ul
 RT: 14.40 min Scan# 1840
 Delta R.T. 0.00 min
 Lab File: BG028346.D
 Acq: 15 Aug 2017 16:41

Instrument :
 BNA_G
 ClientSampleId :
 C0AH5

Tgt Ion:	163	Resp:	63408
Ion Ratio	Lower	Upper	
163	100		
194	4.9	3.4	5.0
164	13.7	9.0	13.4#

Manual Integrations
 APPROVED

Sohil
 8/16/2017 6:39:52 PM

