




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
Data File : BG062453.D
Acq On : 16 Aug 2024 21:47
Operator : MA/JU
Sample : P3555-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCXW1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/17/2024
Supervised By :mohammad ahmed 08/17/2024

Quant Time: Aug 16 23:02:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 14 15:31:21 2024
Response via : Initial Calibration

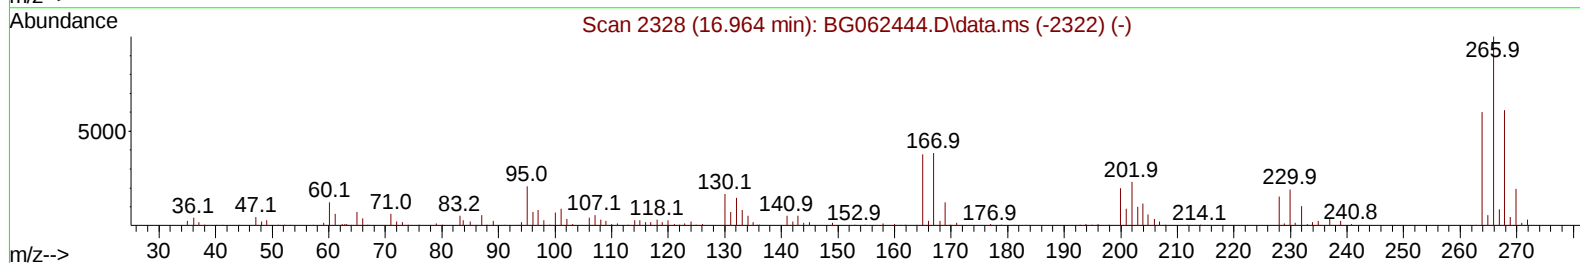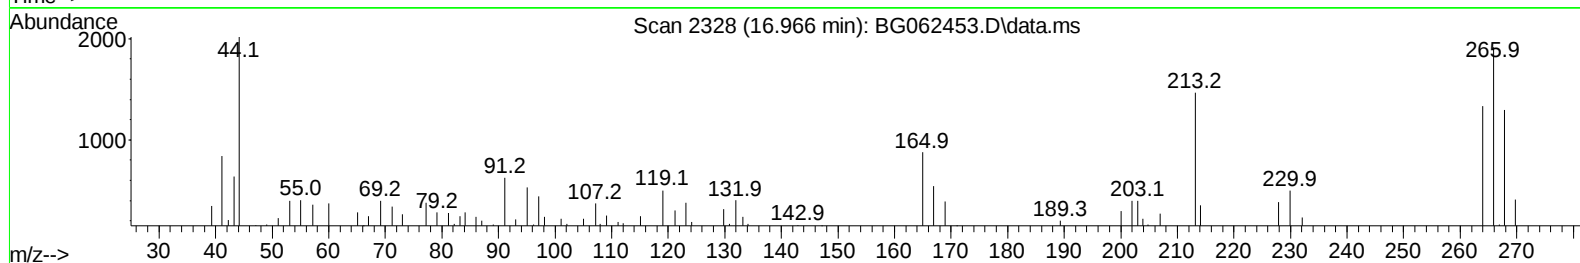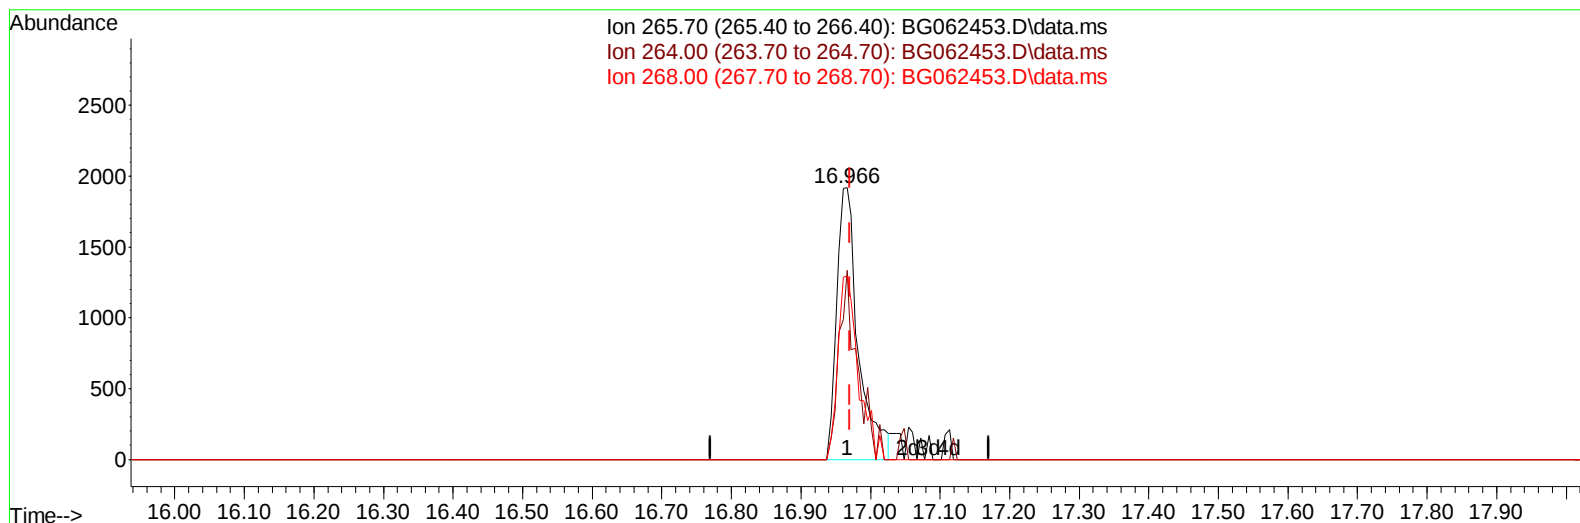

TIC: BG062453.D\data.ms

(71) Pentachlorophenol (C)

16.966min (-0.004) 1.27 ng/u1

response 4137

Ion	Exp%	Act%
265.70	100.00	100.00
264.00	61.80	69.64
268.00	62.60	67.50
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
Data File : BG062453.D
Acq On : 16 Aug 2024 21:47
Operator : MA/JU
Sample : P3555-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCXW1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/17/2024
Supervised By :mohammad ahmed 08/17/2024

Quant Time: Aug 16 23:02:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 14 15:31:21 2024
Response via : Initial Calibration

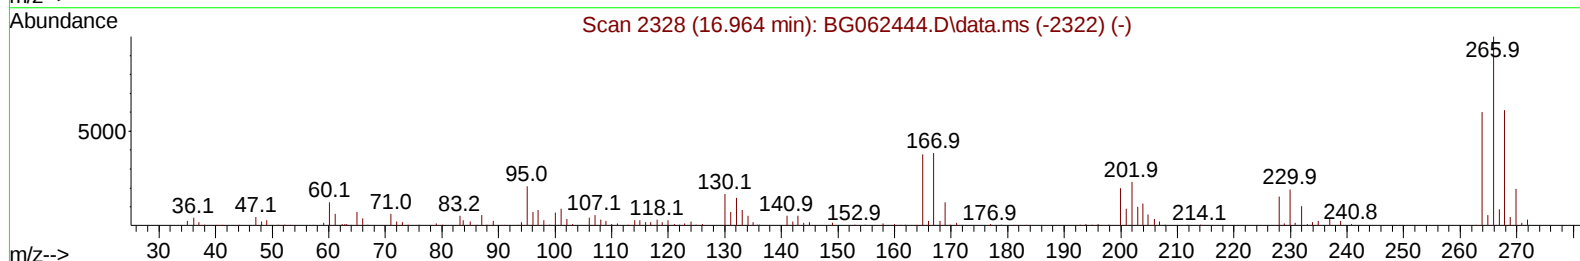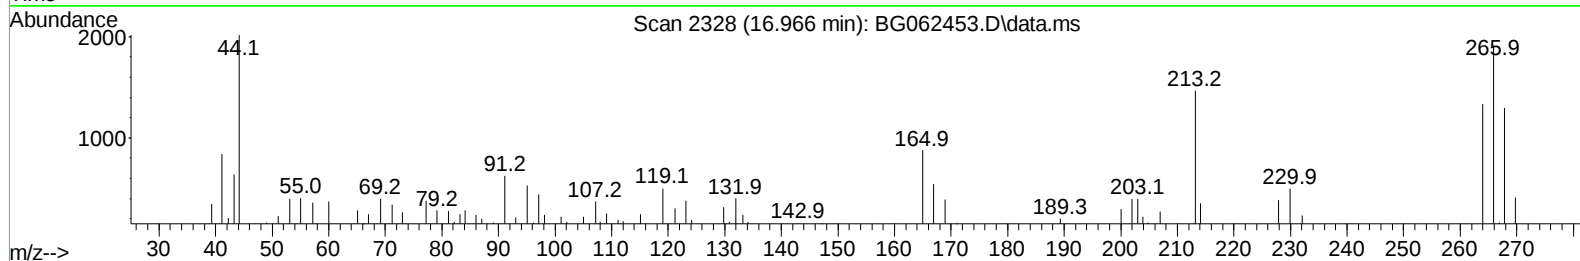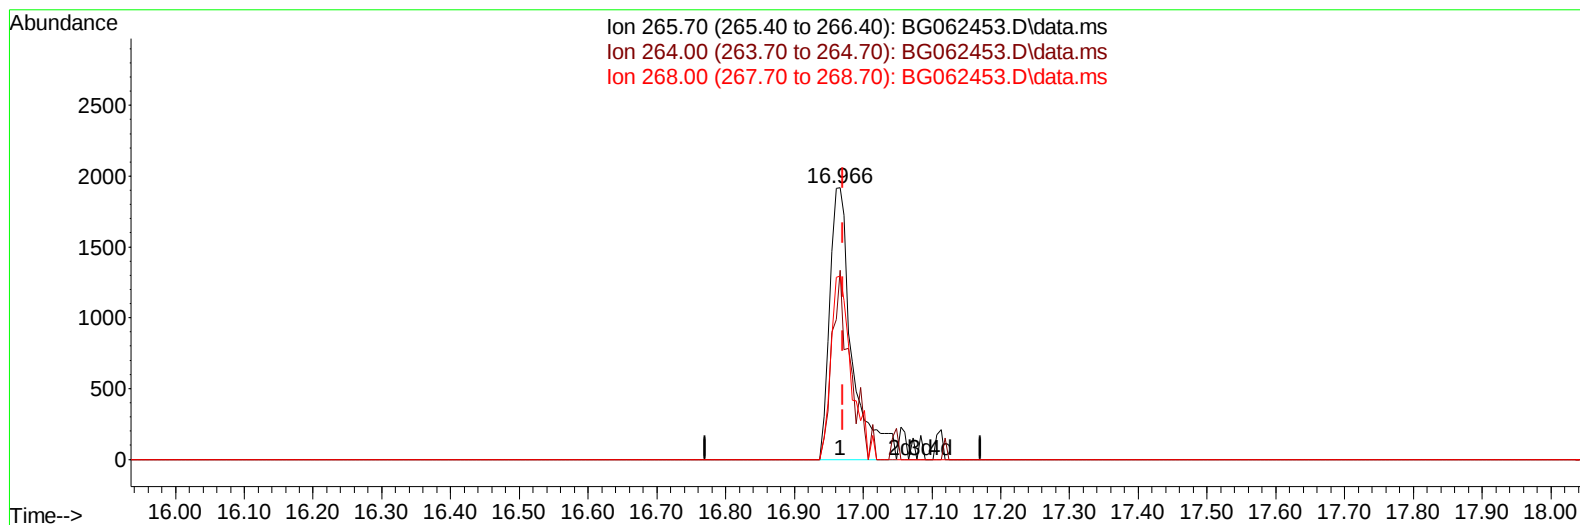

TIC: BG062453.D\data.ms

(71) Pentachlorophenol (C)

16.966min (-0.004) 1.33 ng/u1 m

response 4330

Ion	Exp%	Act%
265.70	100.00	100.00
264.00	61.80	69.64
268.00	62.60	67.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
 Data File : BG062453.D
 Acq On : 16 Aug 2024 21:47
 Operator : MA/JU
 Sample : P3555-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCXW1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/17/2024
 Supervised By :mohammad ahmed 08/17/2024

Quant Time: Aug 16 23:22:31 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 14 15:31:21 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.955	152		58059	20.000	ng/ul	0.00
20) Naphthalene-d8	10.751	136		262201	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.576	164		200106	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.313	188		425487	20.000	ng/ul	0.00
79) Chrysene-d12	21.554	240		419173	20.000	ng/ul	0.00
88) Perylene-d12	24.644	264		493308	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.426	96		3715	2.429	ng/uL	0.00
4) Pyridine-d5	0.000	84		0d	0.000	ng/ul	
7) Phenol-d5	7.115	99		69437	12.022	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.285	67		43589	11.981	ng/ul	0.00
11) 2-Chlorophenol-d4	7.485	132		53308	13.511	ng/ul	0.00
15) 4-Methylphenol-d8	8.654	113		48643	10.047	ng/ul	0.00
21) Nitrobenzene-d5	9.107	128		25741	15.308	ng/ul	0.00
24) 2-Nitrophenol-d4	9.829	143		28465	17.017	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.364	165		57907	13.592	ng/ul	0.00
31) 4-Chloroaniline-d4	10.881	131		4030	0.596	ng/ul	0.00
46) Dimethylphthalate-d6	13.976	166		183625	11.797	ng/ul	0.00
49) Acenaphthylene-d8	14.270	160		211779	12.288	ng/ul	0.00
54) 4-Nitrophenol-d4	14.758	143		26599	10.712	ng/ul	0.00
60) Fluorene-d10	15.562	176		171395	12.209	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.674	200		21954	11.356	ng/ul	0.00
73) Anthracene-d10	17.413	188		245392	12.006	ng/ul	0.00
81) Pyrene-d10	19.692	212		325784	13.271	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.427	264		327466	12.508	ng/ul	-0.02
Target Compounds							
71) Pentachlorophenol	16.966	266		4330m	1.334	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
Data File : BG062453.D
Acq On : 16 Aug 2024 21:47
Operator : MA/JU
Sample : P3555-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCXW1

Manual IntegrationsAPPROVED

Quant Time: Aug 16 23:22:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 14 15:31:21 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/17/2024
Supervised By :mohammad ahmed 08/17/2024

