

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
 Data File : BG062419.D
 Acq On : 15 Aug 2024 17:21
 Operator : MA/JU
 Sample : P3502-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCXT9

Quant Time: Aug 15 18:34:26 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 14 15:31:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.955	152	75773	20.000	ng/ul	0.00
20) Naphthalene-d8	10.751	136	349252	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.575	164	269180	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.313	188	582062	20.000	ng/ul	0.00
79) Chrysene-d12	21.554	240	574203	20.000	ng/ul	0.00
88) Perylene-d12	24.650	264	658857	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.414	96	2819	1.412	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.115	99	71066	9.428	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.285	67	42105	8.868	ng/ul	0.00
11) 2-Chlorophenol-d4	7.491	132	51457	9.993	ng/ul	0.00
15) 4-Methylphenol-d8	8.648	113	38840	6.147	ng/ul	0.00
21) Nitrobenzene-d5	9.106	128	25658	11.456	ng/ul	0.00
24) 2-Nitrophenol-d4	9.829	143	29293	13.147	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	62810	11.068	ng/ul	0.00
31) 4-Chloroaniline-d4	10.875	131	36861	4.096	ng/ul	0.00
46) Dimethylphthalate-d6	13.982	166	220471	10.530	ng/ul	0.00
49) Acenaphthylene-d8	14.270	160	241270	10.407	ng/ul	0.00
54) 4-Nitrophenol-d4	14.752	143	30971	9.272	ng/ul	0.00
60) Fluorene-d10	15.568	176	204910	10.851	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.674	200	25332	9.579	ng/ul	0.00
73) Anthracene-d10	17.413	188	281700	10.075	ng/ul	0.00
81) Pyrene-d10	19.698	212	361604	10.753	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.433	264	289040	8.266	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.777	105	14938	1.443	ng/ul	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
Data File : BG062419.D
Acq On : 15 Aug 2024 17:21
Operator : MA/JU
Sample : P3502-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCXT9

Quant Time: Aug 15 18:34:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 14 15:31:21 2024
Response via : Initial Calibration

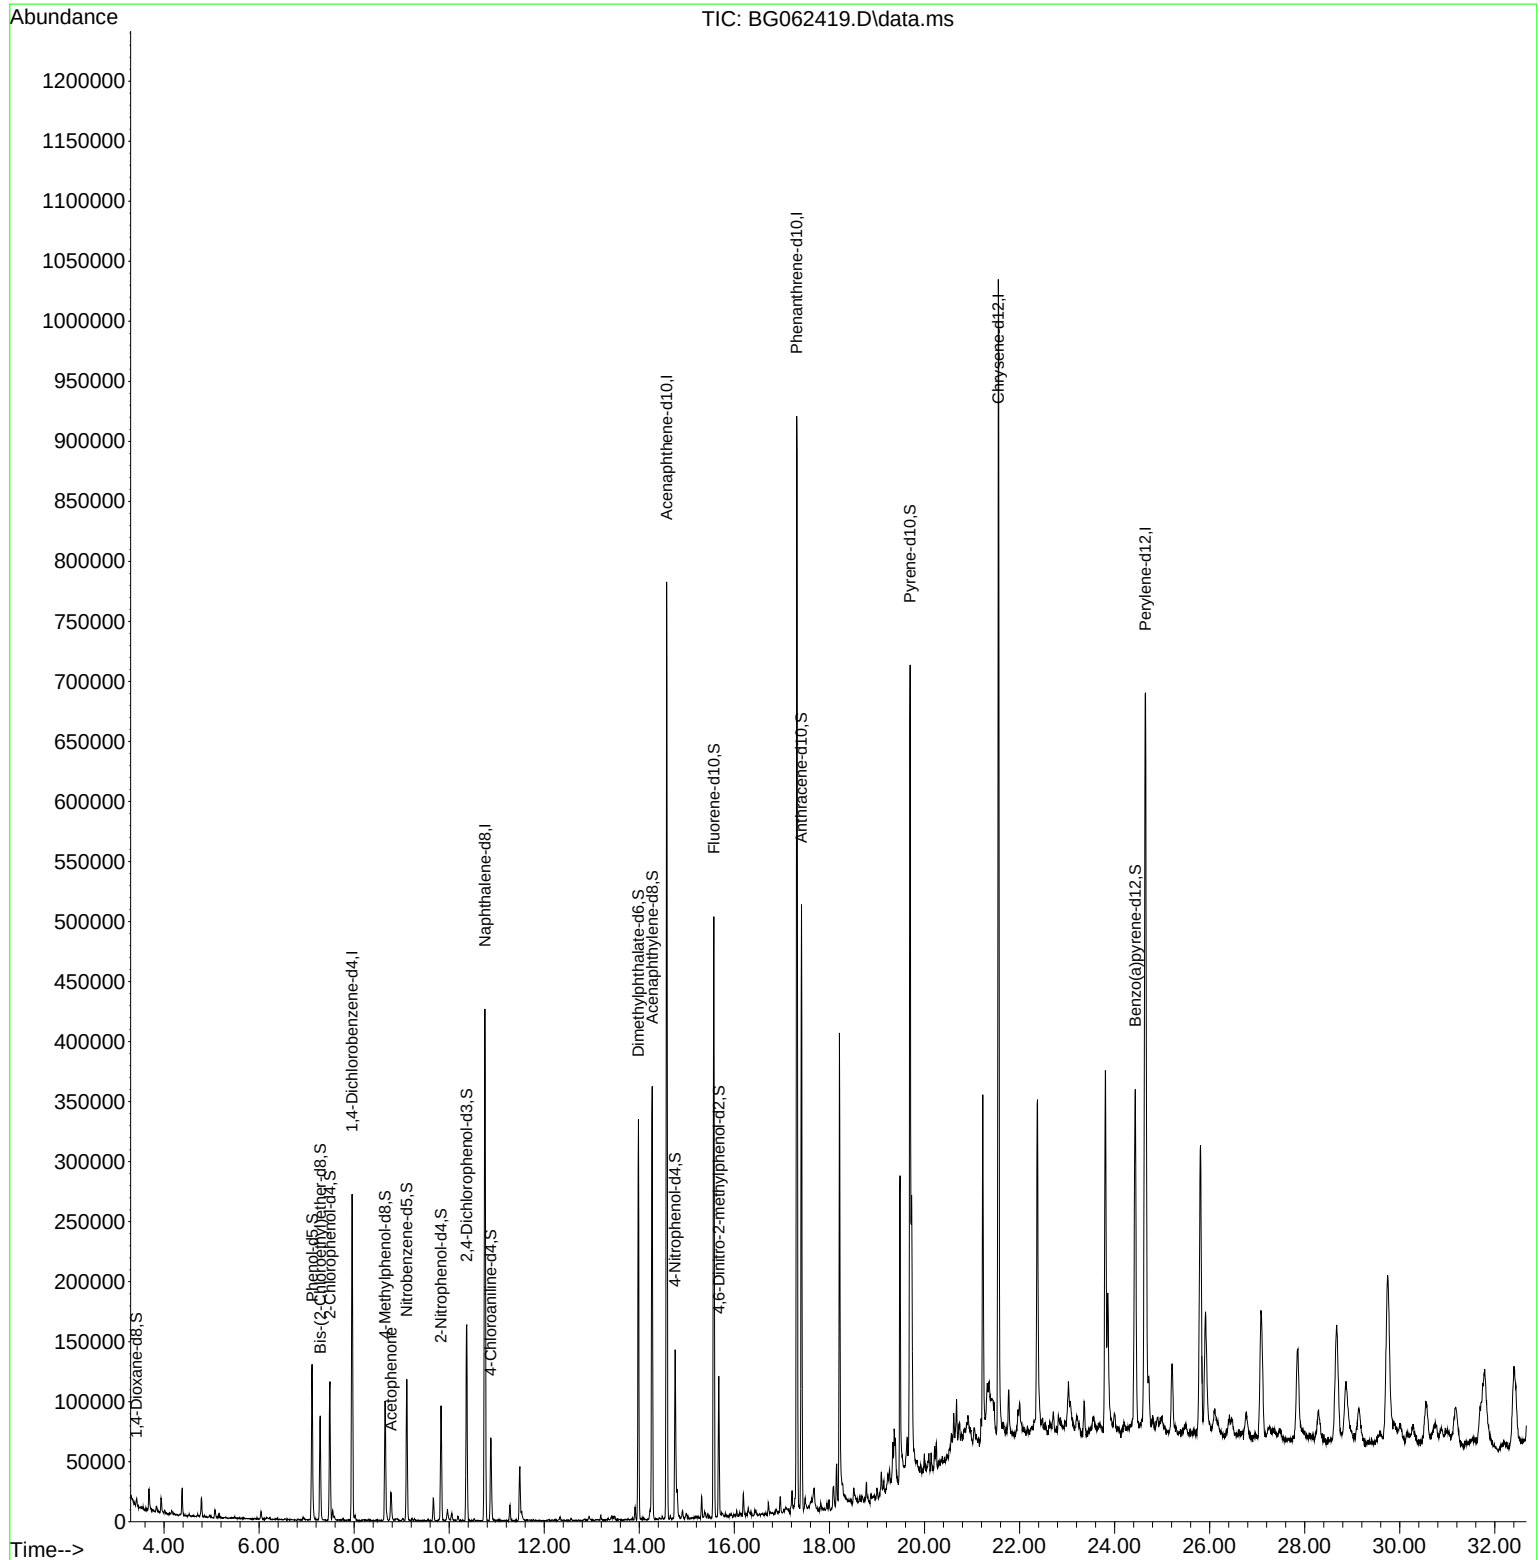

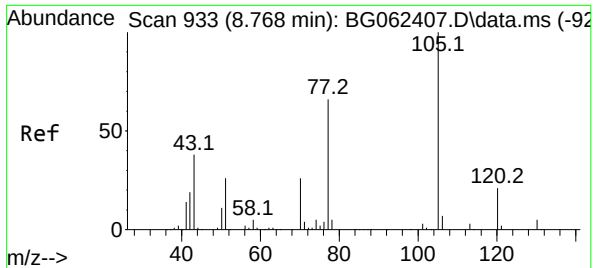

#16
 Acetophenone
 Concen: 1.443 ng/ul
 RT: 8.777 min Scan# 91
 Delta R.T. 0.002 min
 Lab File: BG062419.D
 Acq: 15 Aug 2024 17:21

Instrument :
 BNA_G
 ClientSampleId :
 DCXT9

Tgt Ion:	105	Resp:	14938
Ion	Ratio	Lower	Upper
105	100		
77	70.3	64.6	97.0
51	36.2	27.8	41.8

