

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
 Data File : BG062421.D
 Acq On : 15 Aug 2024 18:44
 Operator : MA/JU
 Sample : PB162649BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK649

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062421.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.418	18	22	28	rVB	15090	23787	1.02%	0.105%
2	3.823	87	91	105	rBV	227283	368767	15.79%	1.621%
3	4.164	145	149	156	rVB3	4174	7432	0.32%	0.033%
4	7.113	644	651	662	rBV	302624	516582	22.13%	2.271%
5	7.283	674	680	690	rVB	212978	358449	15.35%	1.576%
6	7.489	706	715	726	rVB	277861	459913	19.70%	2.021%
7	7.959	785	795	803	rBV	264802	442673	18.96%	1.946%
8	8.652	906	913	921	rBV	365880	610611	26.15%	2.684%
9	9.110	982	991	1001	rBV	278596	485269	20.78%	2.133%
10	9.832	1106	1114	1123	rBV	227517	401178	17.18%	1.763%
11	10.367	1197	1205	1214	rBV	382046	650317	27.85%	2.858%
12	10.749	1263	1270	1282	rVB	402190	715614	30.65%	3.145%
13	10.878	1284	1292	1302	rVV	354603	624677	26.76%	2.746%
14	11.530	1397	1403	1407	rBV3	1439	2372	0.10%	0.010%
15	12.335	1535	1540	1545	rVB2	5217	8578	0.37%	0.038%
16	13.980	1814	1820	1827	rBV	685348	992632	42.52%	4.363%
17	14.268	1862	1869	1878	rBV	793595	1239775	53.10%	5.449%
18	14.573	1913	1921	1930	rVB	708543	1112730	47.66%	4.891%
19	14.755	1944	1952	1966	rBV	337234	537841	23.04%	2.364%
20	15.566	2083	2090	2101	rBV	1064451	1585058	67.89%	6.967%
21	15.672	2101	2108	2118	rBV	291362	441388	18.91%	1.940%
22	15.807	2128	2131	2136	rVB5	2998	4545	0.19%	0.020%
23	16.347	2219	2223	2228	rVB3	4445	5732	0.25%	0.025%
24	17.105	2348	2352	2354	rBV2	2407	3816	0.16%	0.017%
25	17.316	2381	2388	2396	rBV	901065	1339583	57.38%	5.888%
26	17.416	2398	2405	2412	rVB	1108748	1705247	73.04%	7.495%
27	17.663	2440	2447	2453	rVB7	5656	15235	0.65%	0.067%
28	17.998	2498	2504	2506	rVB4	2176	3469	0.15%	0.015%
29	18.027	2506	2509	2513	rBV5	1790	3147	0.13%	0.014%
30	18.809	2637	2642	2643	rBV4	2669	3079	0.13%	0.014%
31	18.873	2649	2653	2655	rBV4	1880	2666	0.11%	0.012%
32	19.090	2686	2690	2692	rBV4	2753	2568	0.11%	0.011%
33	19.261	2715	2719	2723	rBV3	15296	20527	0.88%	0.090%
34	19.331	2727	2731	2735	rVV	13151	17798	0.76%	0.078%
35	19.402	2741	2743	2748	rVB6	3851	3502	0.15%	0.015%
36	19.560	2767	2770	2771	rBV3	2755	3432	0.15%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
Data File : BG062421.D
Acq On : 15 Aug 2024 18:44
Operator : MA/JU
Sample : PB162649BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK649

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Title : SVOA CALIBRATION

37	19.631	2779	2782	2785	rBV5	9452	14014	0.60%	0.062%
38	19.696	2787	2793	2813	rVB	1464585	2334718	100.00%	10.262%
39	20.042	2850	2852	2857	rBV6	2517	3585	0.15%	0.016%
40	20.671	2957	2959	2964	rVB6	7883	9025	0.39%	0.040%
41	21.558	3103	3110	3123	rVB2	938048	1496010	64.08%	6.575%
42	23.032	3357	3361	3368	rVB2	23035	37975	1.63%	0.167%
43	23.802	3486	3492	3499	rBV4	29962	70526	3.02%	0.310%
44	24.436	3589	3600	3612	rBV2	783957	2164810	92.72%	9.515%
45	24.648	3625	3636	3645	rBV	610287	1650587	70.70%	7.255%
46	25.805	3827	3833	3843	rVB2	42852	113181	4.85%	0.497%
47	27.103	4046	4054	4065	rVB5	39432	131495	5.63%	0.578%
48	28.801	4341	4343	4345	rBV3	6173	5380	0.23%	0.024%




Sum of corrected areas: 22751295

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
Data File : BG062421.D
Acq On : 15 Aug 2024 18:44
Operator : MA/JU
Sample : PB162649BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK649

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

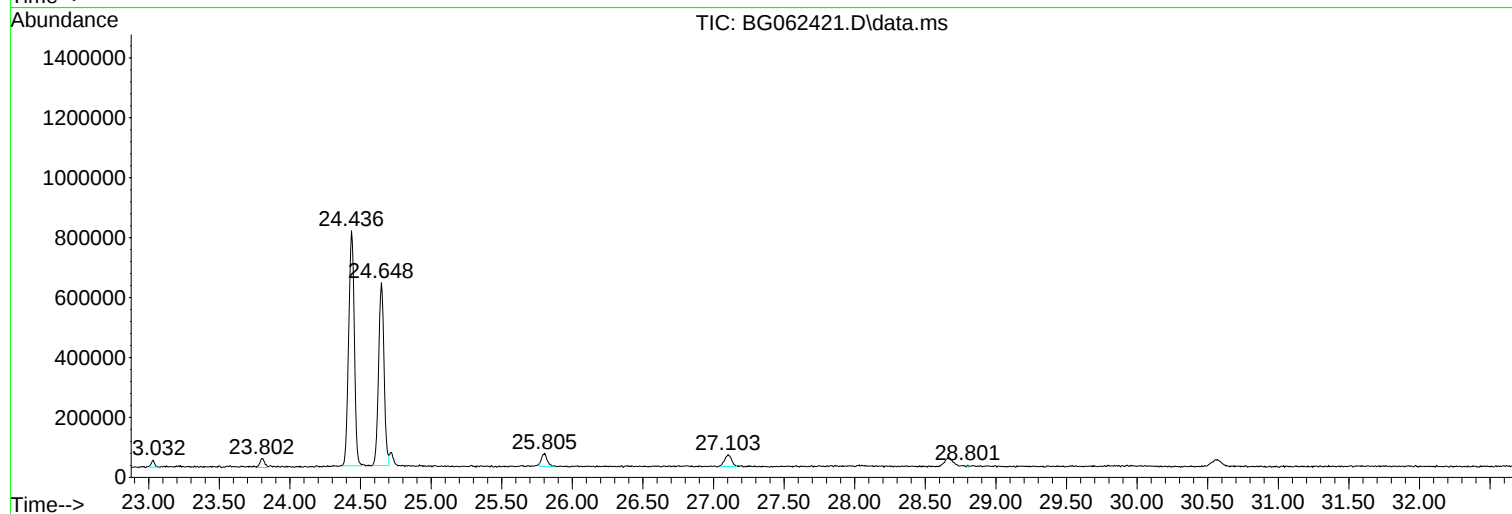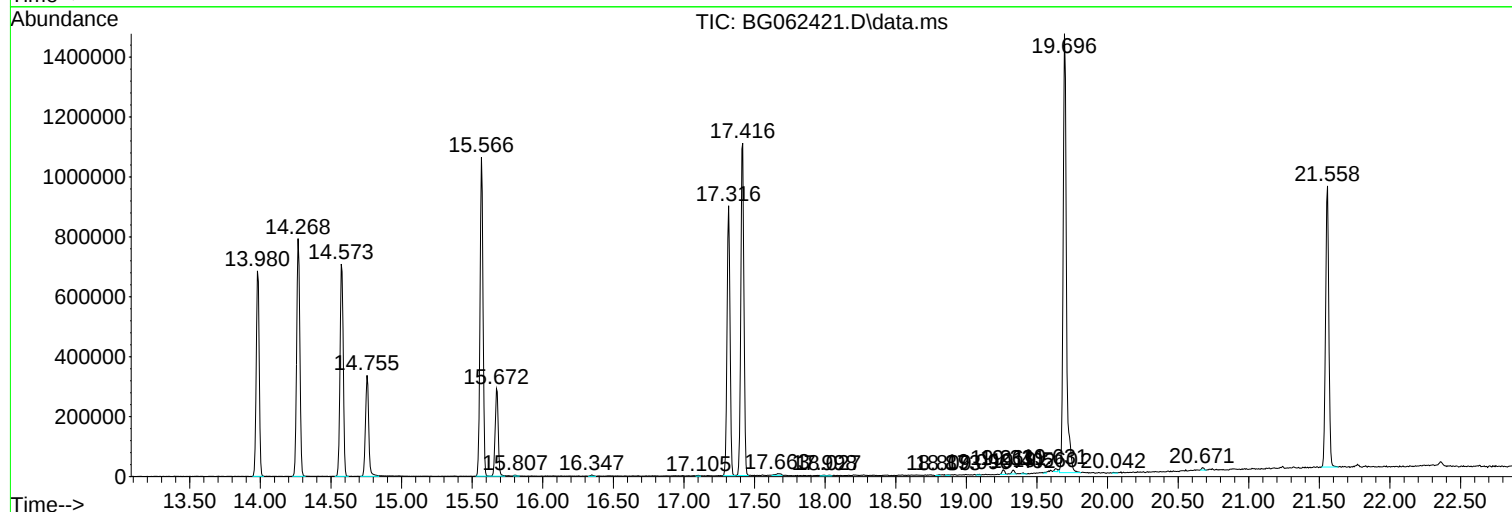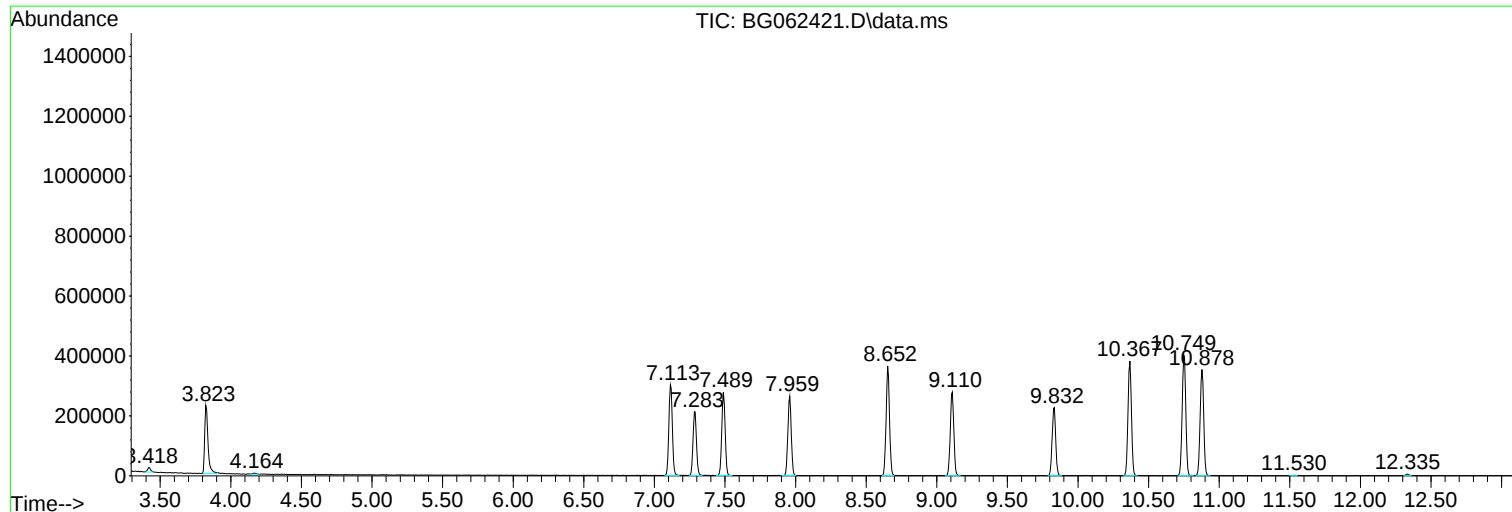

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
Data File : BG062421.D
Acq On : 15 Aug 2024 18:44
Operator : MA/JU
Sample : PB162649BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK649

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
Data File : BG062421.D
Acq On : 15 Aug 2024 18:44
Operator : MA/JU
Sample : PB162649BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK649

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------