

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
 Data File : BG062437.D
 Acq On : 16 Aug 2024 9:01
 Operator : MA/JU
 Sample : PB162719BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK719

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062437.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.412	17	21	28	rVB2	12176	19423	1.14%	0.116%
2	3.817	85	90	105	rVB	161929	268881	15.77%	1.607%
3	4.158	143	148	154	rBV5	2511	5042	0.30%	0.030%
4	5.697	406	410	414	rVB4	1065	2052	0.12%	0.012%
5	7.107	643	650	660	rBV	245454	401313	23.54%	2.398%
6	7.277	672	679	687	rBV	170960	277246	16.26%	1.657%
7	7.483	704	714	721	rBV	209289	353058	20.71%	2.109%
8	7.953	786	794	803	rBV	159011	264761	15.53%	1.582%
9	8.646	905	912	920	rBV	296734	500162	29.34%	2.988%
10	9.104	982	990	1004	rVB	214047	381593	22.38%	2.280%
11	9.827	1102	1113	1124	rVB	172677	310273	18.20%	1.854%
12	10.361	1197	1204	1214	rBV	307542	532488	31.24%	3.182%
13	10.743	1261	1269	1277	rBV	254052	460233	27.00%	2.750%
14	10.872	1284	1291	1302	rVB	290446	517385	30.35%	3.091%
15	11.518	1396	1401	1406	rBV2	1292	2044	0.12%	0.012%
16	12.329	1533	1539	1546	rVB	4197	6564	0.39%	0.039%
17	13.980	1812	1820	1827	rBV	552928	780566	45.79%	4.664%
18	14.268	1861	1869	1879	rBV	627385	980127	57.49%	5.856%
19	14.415	1888	1894	1900	rVB	982	1762	0.10%	0.011%
20	14.573	1910	1921	1930	rBV	468882	701384	41.14%	4.191%
21	14.755	1945	1952	1964	rBV	254745	403025	23.64%	2.408%
22	15.566	2083	2090	2102	rVB	823163	1246782	73.14%	7.449%
23	15.672	2102	2108	2118	rVB	228825	324588	19.04%	1.939%
24	15.801	2127	2130	2135	rVB2	2787	2967	0.17%	0.018%
25	16.347	2219	2223	2229	rVB5	2461	3222	0.19%	0.019%
26	17.093	2345	2350	2353	rBV2	1382	2685	0.16%	0.016%
27	17.311	2381	2387	2396	rVB	551275	802061	47.05%	4.792%
28	17.411	2396	2404	2416	rBV	893372	1304996	76.55%	7.797%
29	17.669	2445	2448	2449	rBV2	2661	2268	0.13%	0.014%
30	18.209	2536	2540	2545	rBV4	5013	7376	0.43%	0.044%
31	19.267	2715	2720	2725	rVV4	11283	18356	1.08%	0.110%
32	19.331	2727	2731	2739	rVB2	10968	19603	1.15%	0.117%
33	19.484	2753	2757	2761	rBV5	2694	5476	0.32%	0.033%
34	19.578	2771	2773	2775	rBV3	2376	2926	0.17%	0.017%
35	19.637	2780	2783	2787	rVV5	7716	13611	0.80%	0.081%
36	19.696	2787	2793	2797	rVV	1122617	1642215	96.33%	9.812%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
Data File : BG062437.D
Acq On : 16 Aug 2024 9:01
Operator : MA/JU
Sample : PB162719BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK719

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Title : SVOA CALIBRATION

37	19.731	2797	2799	2808	rVB	128595	164360	9.64%	0.982%
38	19.901	2826	2828	2830	rBV3	2039	2338	0.14%	0.014%
39	20.060	2852	2855	2856	rVB3	2922	1901	0.11%	0.011%
40	20.113	2862	2864	2866	rBV3	2003	2039	0.12%	0.012%
41	20.218	2879	2882	2885	rBV4	2081	3522	0.21%	0.021%
42	20.418	2914	2916	2918	rBV3	2332	1826	0.11%	0.011%
43	20.671	2957	2959	2965	rVB5	6772	6958	0.41%	0.042%
44	20.741	2968	2971	2974	rVV5	5003	6305	0.37%	0.038%
45	20.818	2982	2984	2988	rVB4	3777	3284	0.19%	0.020%
46	20.859	2988	2991	2992	rBV2	3256	2918	0.17%	0.017%
47	21.235	3051	3055	3060	rBV4	12887	20720	1.22%	0.124%
48	21.552	3101	3109	3116	rBV2	574173	970203	56.91%	5.797%
49	21.763	3142	3145	3153	rVB2	16594	24659	1.45%	0.147%
50	22.357	3242	3246	3251	rVB2	20996	32292	1.89%	0.193%
51	23.021	3355	3359	3366	rVB2	28085	48915	2.87%	0.292%
52	23.326	3409	3411	3416	rVB6	4922	4856	0.28%	0.029%
53	23.549	3447	3449	3450	rBV2	4283	2411	0.14%	0.014%
54	23.796	3486	3491	3498	rVB4	28536	62279	3.65%	0.372%
55	24.054	3533	3535	3538	rBV3	5123	4952	0.29%	0.030%
56	24.430	3589	3599	3611	rBV2	638295	1704725	100.00%	10.185%
57	24.642	3625	3635	3644	rBV	384726	1021191	59.90%	6.101%
58	25.100	3711	3713	3715	rBV3	4902	3540	0.21%	0.021%
59	25.787	3825	3830	3840	rVB6	24897	72120	4.23%	0.431%




Sum of corrected areas: 16736828

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
Data File : BG062437.D
Acq On : 16 Aug 2024 9:01
Operator : MA/JU
Sample : PB162719BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK719

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

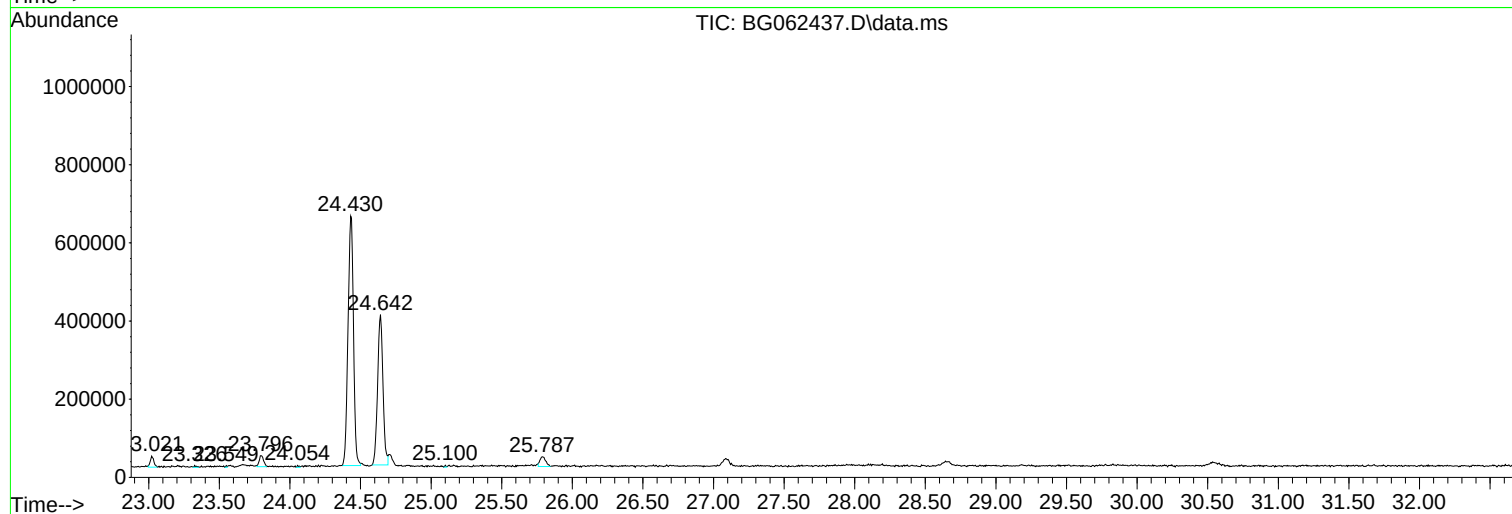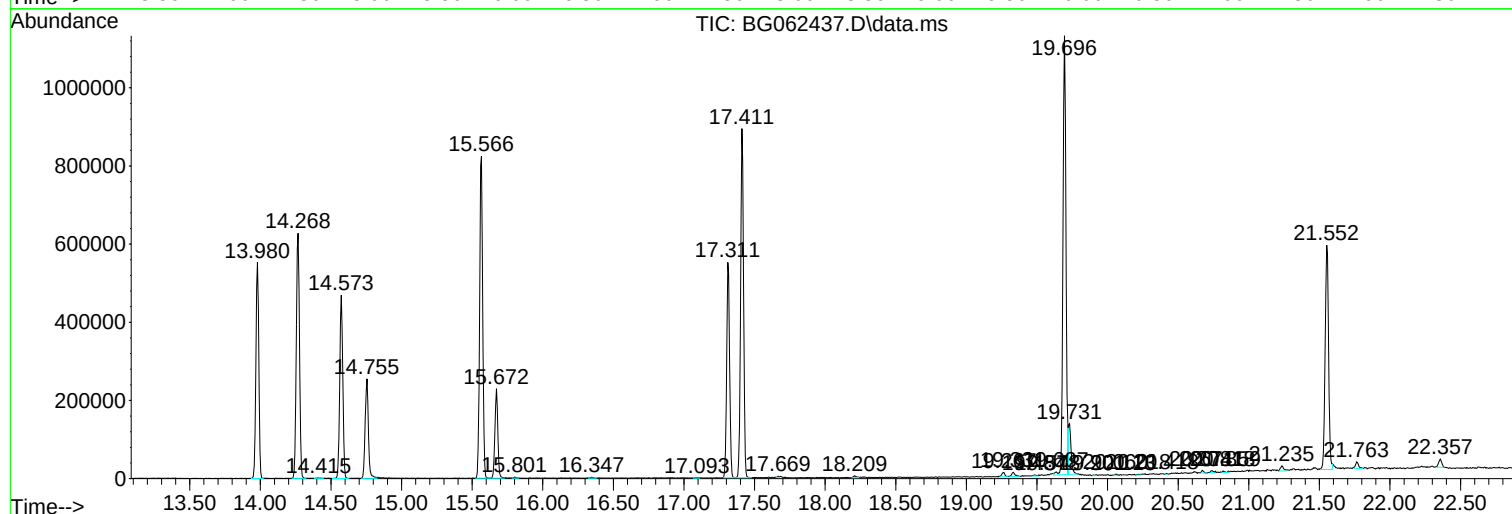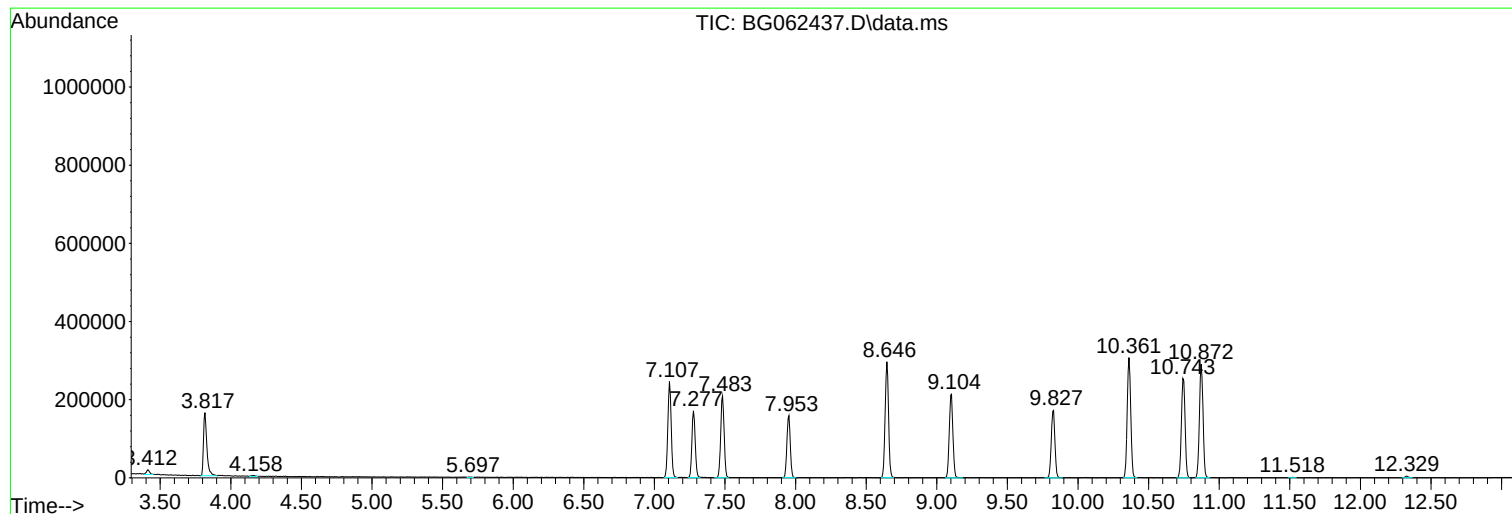

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
Data File : BG062437.D
Acq On : 16 Aug 2024 9:01
Operator : MA/JU
Sample : PB162719BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK719

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
Data File : BG062437.D
Acq On : 16 Aug 2024 9:01
Operator : MA/JU
Sample : PB162719BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK719

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc