

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
 Data File : BG062445.D
 Acq On : 16 Aug 2024 15:30
 Operator : MA/JU
 Sample : PB162719BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK719

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062445.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.417	18	22	30	rVB3	17996	28017	1.33%	0.141%
2	3.581	48	50	53	rBV3	1830	2186	0.10%	0.011%
3	3.822	86	91	107	rBV	232058	386324	18.35%	1.950%
4	4.163	146	149	155	rVV4	3964	6430	0.31%	0.032%
5	4.216	157	158	167	rVB5	3228	5496	0.26%	0.028%
6	7.112	645	651	662	rBV	273185	460246	21.86%	2.323%
7	7.282	673	680	690	rBV	190947	317192	15.07%	1.601%
8	7.488	708	715	726	rVB	244137	409244	19.44%	2.066%
9	7.958	787	795	802	rBV	196003	324367	15.41%	1.637%
10	8.651	906	913	922	rBV	334599	564112	26.80%	2.848%
11	9.109	983	991	1001	rBV	253553	439194	20.86%	2.217%
12	9.832	1106	1114	1122	rVB	206742	362187	17.21%	1.828%
13	10.366	1195	1205	1214	rBV	338499	580890	27.60%	2.932%
14	10.748	1261	1270	1279	rBV	306342	547029	25.99%	2.761%
15	10.877	1285	1292	1301	rBV	328219	578593	27.49%	2.921%
16	12.334	1536	1540	1545	rVB2	4493	7608	0.36%	0.038%
17	13.979	1814	1820	1827	rBV	613147	902561	42.88%	4.556%
18	14.267	1862	1869	1878	rBV	710762	1113835	52.91%	5.622%
19	14.578	1914	1922	1929	rVB	568462	867985	41.23%	4.381%
20	14.755	1946	1952	1972	rVB	302895	473723	22.50%	2.391%
21	15.565	2083	2090	2098	rBV	936264	1431469	68.00%	7.226%
22	15.671	2102	2108	2118	rBV	261244	401238	19.06%	2.025%
23	15.800	2126	2130	2135	rBV2	3050	4857	0.23%	0.025%
24	16.076	2174	2177	2182	rBV3	1200	2194	0.10%	0.011%
25	16.347	2220	2223	2227	rVB2	2779	3517	0.17%	0.018%
26	17.316	2381	2388	2397	rBV	708149	1041112	49.46%	5.255%
27	17.416	2397	2405	2417	rVB	1042266	1528263	72.60%	7.714%
28	17.703	2449	2454	2459	rVB3	4068	5752	0.27%	0.029%
29	17.985	2498	2502	2506	rVB3	2396	3100	0.15%	0.016%
30	18.209	2537	2540	2547	rVB5	3242	5492	0.26%	0.028%
31	18.643	2609	2614	2618	rBV2	53916	61895	2.94%	0.312%
32	18.755	2631	2633	2639	rVV4	1787	2198	0.10%	0.011%
33	19.013	2675	2677	2682	rBV5	1600	2370	0.11%	0.012%
34	19.102	2688	2692	2694	rBV4	2342	2777	0.13%	0.014%
35	19.266	2713	2720	2724	rBV3	16870	26624	1.26%	0.134%
36	19.331	2726	2731	2736	rBV2	13118	19285	0.92%	0.097%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
 Data File : BG062445.D
 Acq On : 16 Aug 2024 15:30
 Operator : MA/JU
 Sample : PB162719BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK719

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
 Title : SVOA CALIBRATION

37	19.542	2765	2767	2768	rBV2	2946	2138	0.10%	0.011%
38	19.642	2779	2784	2787	rBV5	11894	21002	1.00%	0.106%
39	19.701	2787	2794	2807	rVB	1299585	2105014	100.00%	10.626%
40	19.989	2840	2843	2844	rBV3	3148	3355	0.16%	0.017%
41	20.241	2885	2886	2890	rBV4	2710	3284	0.16%	0.017%
42	20.617	2948	2950	2953	rBV3	3138	2541	0.12%	0.013%
43	20.676	2957	2960	2963	rVB5	9797	11509	0.55%	0.058%
44	20.746	2969	2972	2974	rBV4	5453	5485	0.26%	0.028%
45	21.557	3103	3110	3118	rBV2	739569	1175251	55.83%	5.933%
46	21.774	3143	3147	3154	rVB8	9376	14142	0.67%	0.071%
47	22.356	3244	3246	3254	rVB7	13530	21351	1.01%	0.108%
48	23.026	3357	3360	3365	rVB4	19243	26322	1.25%	0.133%
49	23.801	3487	3492	3500	rVB4	25394	54016	2.57%	0.273%
50	24.441	3590	3601	3614	rBV2	748338	1970499	93.61%	9.947%
51	24.647	3626	3636	3645	rBV2	466572	1290951	61.33%	6.517%
52	25.804	3826	3833	3840	rVB3	30172	83067	3.95%	0.419%
53	27.103	4044	4054	4063	rVB5	29219	101033	4.80%	0.510%




Sum of corrected areas: 19810322

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
Data File : BG062445.D
Acq On : 16 Aug 2024 15:30
Operator : MA/JU
Sample : PB162719BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK719

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

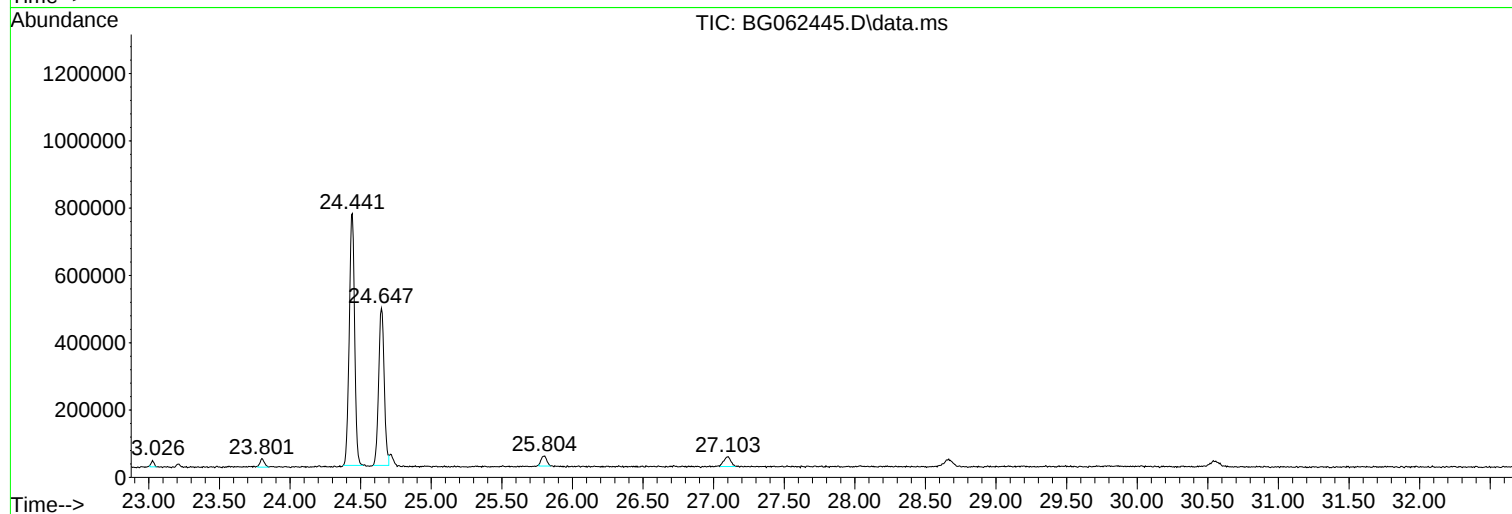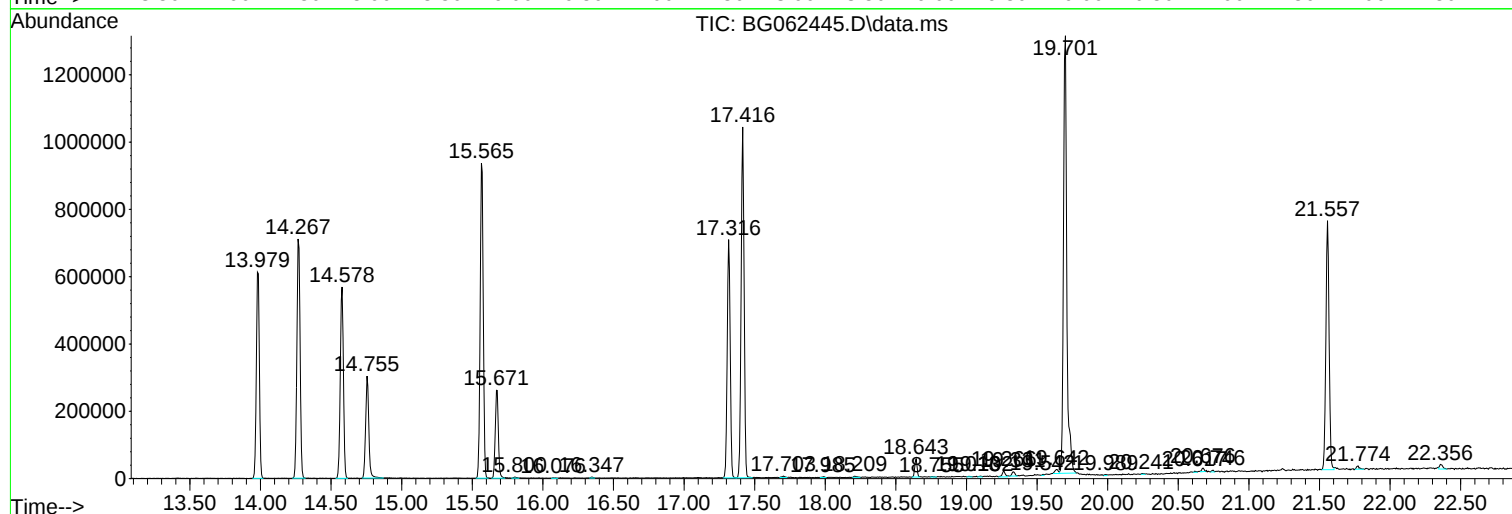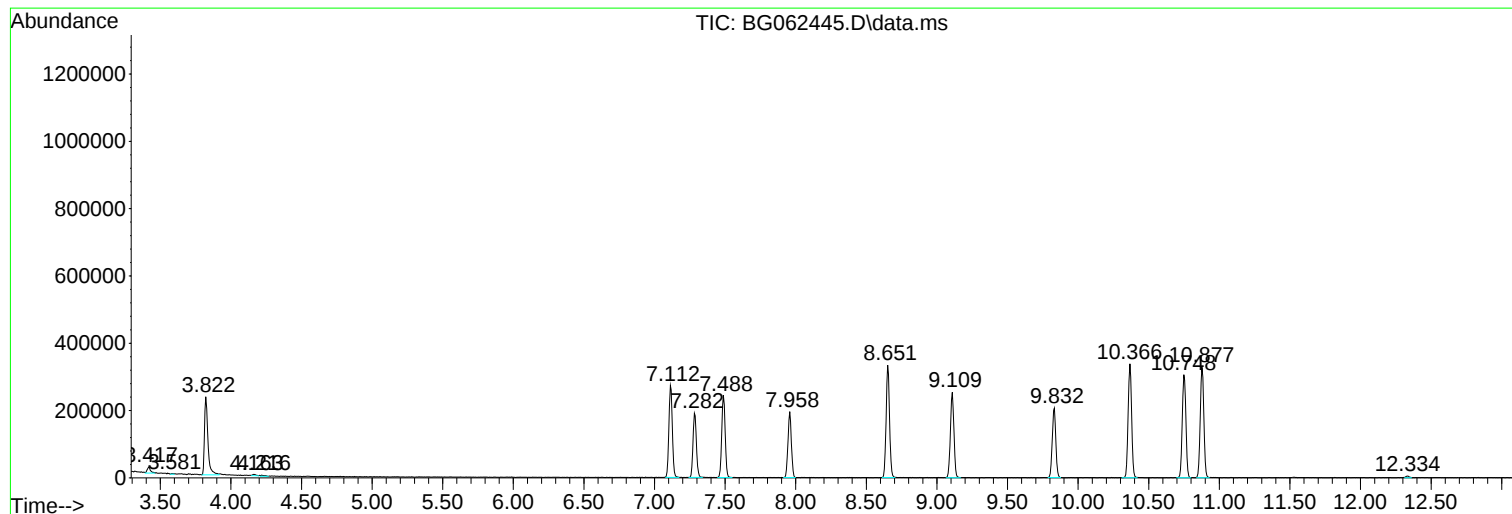

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
Data File : BG062445.D
Acq On : 16 Aug 2024 15:30
Operator : MA/JU
Sample : PB162719BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK719

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
Data File : BG062445.D
Acq On : 16 Aug 2024 15:30
Operator : MA/JU
Sample : PB162719BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK719

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc