

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
 Data File : BG062457.D
 Acq On : 17 Aug 2024 00:31
 Operator : MA/JU
 Sample : PB162801BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK801

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062457.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.423	19	23	28	rVB	18922	25617	1.16%	0.114%
2	3.828	87	92	108	rBV	258698	427423	19.38%	1.897%
3	4.163	146	149	152	rVB3	4314	5685	0.26%	0.025%
4	7.118	644	652	660	rBV	358685	603917	27.38%	2.680%
5	7.282	673	680	691	rBV	239890	397736	18.03%	1.765%
6	7.488	707	715	724	rVB	322109	538345	24.41%	2.389%
7	7.958	788	795	803	rBV	301309	506325	22.96%	2.247%
8	8.651	906	913	923	rBV	346667	596657	27.05%	2.648%
9	9.109	981	991	1002	rBV	267106	470564	21.34%	2.088%
10	9.826	1107	1113	1123	rVB	221671	394114	17.87%	1.749%
11	10.366	1197	1205	1217	rVB	368403	644071	29.20%	2.858%
12	10.748	1262	1270	1278	rBV	394613	698497	31.67%	3.100%
13	10.877	1284	1292	1302	rBV	343351	598961	27.16%	2.658%
14	11.530	1397	1403	1407	rBV5	1972	2887	0.13%	0.013%
15	12.328	1534	1539	1545	rBV	6065	8873	0.40%	0.039%
16	13.979	1812	1820	1827	rBV	676588	971668	44.06%	4.312%
17	14.267	1862	1869	1876	rBV	785777	1226958	55.63%	5.445%
18	14.572	1914	1921	1929	rVB	729319	1124117	50.97%	4.988%
19	14.755	1946	1952	1964	rBV	327589	525972	23.85%	2.334%
20	15.565	2083	2090	2097	rBV	1003550	1504377	68.21%	6.676%
21	15.671	2102	2108	2116	rBV	299155	432559	19.61%	1.920%
22	15.806	2127	2131	2134	rBV2	2731	3757	0.17%	0.017%
23	15.882	2142	2144	2150	rVB2	1695	2357	0.11%	0.010%
24	16.347	2219	2223	2229	rBV5	3588	6515	0.30%	0.029%
25	16.758	2292	2293	2298	rBV3	1810	2863	0.13%	0.013%
26	16.875	2311	2313	2317	rBV3	1839	2620	0.12%	0.012%
27	17.098	2348	2351	2352	rBV3	1963	2221	0.10%	0.010%
28	17.316	2380	2388	2395	rBV	884893	1336060	60.58%	5.929%
29	17.410	2398	2404	2414	rVV2	1081964	1671368	75.78%	7.417%
30	17.815	2471	2473	2475	rBV2	2419	2409	0.11%	0.011%
31	17.991	2495	2503	2505	rVB5	3338	6804	0.31%	0.030%
32	18.038	2508	2511	2514	rVB4	2765	3734	0.17%	0.017%
33	18.185	2531	2536	2537	rBV4	1714	2719	0.12%	0.012%
34	18.209	2537	2540	2545	rVB7	3396	4477	0.20%	0.020%
35	18.279	2550	2552	2555	rVB4	3218	3264	0.15%	0.014%
36	18.579	2599	2603	2605	rVB5	2430	3069	0.14%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
 Data File : BG062457.D
 Acq On : 17 Aug 2024 00:31
 Operator : MA/JU
 Sample : PB162801BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK801

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
 Title : SVOA CALIBRATION

37	18.608	2605	2608	2609	rBV3	2737	2424	0.11%	0.011%
38	18.643	2610	2614	2616	rVV5	2443	2822	0.13%	0.013%
39	18.873	2651	2653	2655	rBV3	2664	2348	0.11%	0.010%
40	18.914	2658	2660	2664	rVV5	2069	2619	0.12%	0.012%
41	19.055	2681	2684	2685	rBV3	3022	2459	0.11%	0.011%
42	19.266	2716	2720	2723	rVV3	15892	23035	1.04%	0.102%
43	19.331	2726	2731	2735	rBV	16082	22598	1.02%	0.100%
44	19.395	2740	2742	2746	rBV5	3567	5552	0.25%	0.025%
45	19.442	2748	2750	2752	rBV3	3066	2753	0.12%	0.012%
46	19.601	2771	2777	2779	rBV2	12719	24138	1.09%	0.107%
47	19.695	2787	2793	2798	rBV	1376379	2205559	100.00%	9.787%
48	19.906	2827	2829	2831	rBV3	3189	3040	0.14%	0.013%
49	20.100	2860	2862	2865	rBV4	3005	2750	0.12%	0.012%
50	20.130	2865	2867	2869	rBV3	3377	3373	0.15%	0.015%
51	20.323	2898	2900	2901	rBV2	3382	2329	0.11%	0.010%
52	20.670	2957	2959	2963	rVB5	8074	8950	0.41%	0.040%
53	21.557	3102	3110	3120	rBV2	926102	1531305	69.43%	6.795%
54	24.430	3589	3599	3613	rVB2	787003	2106496	95.51%	9.348%
55	24.647	3625	3636	3653	rVB	593016	1726320	78.27%	7.661%
56	25.781	3821	3829	3840	rBV5	28949	94413	4.28%	0.419%




Sum of corrected areas: 22534843

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
Data File : BG062457.D
Acq On : 17 Aug 2024 00:31
Operator : MA/JU
Sample : PB162801BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK801

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

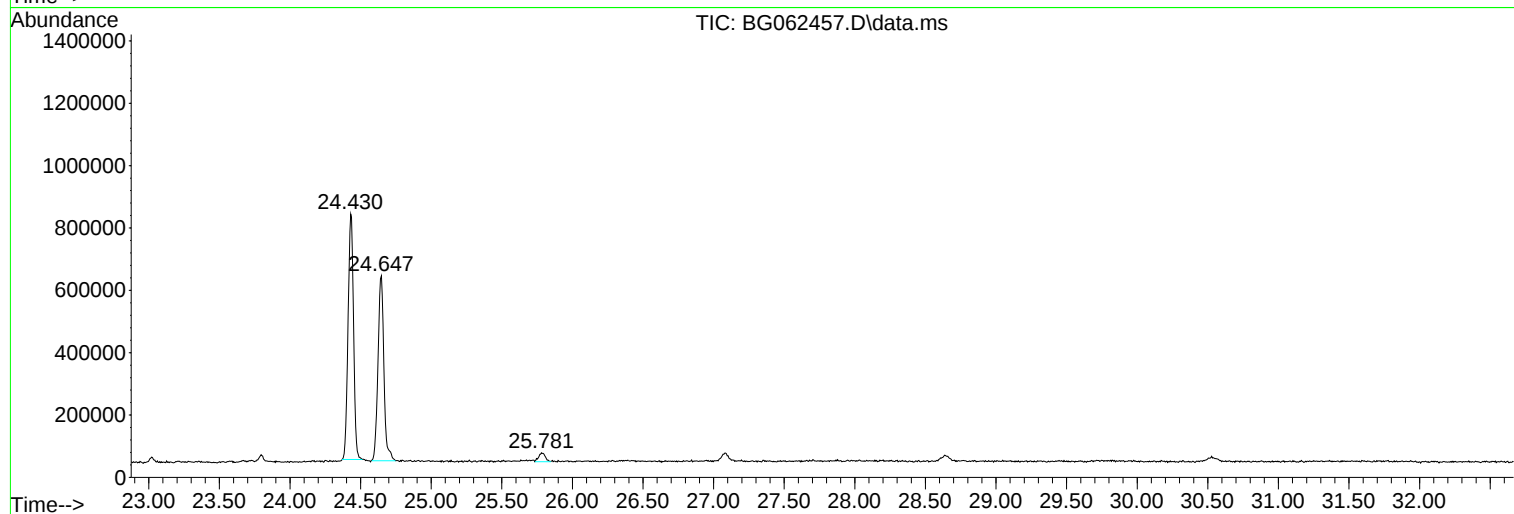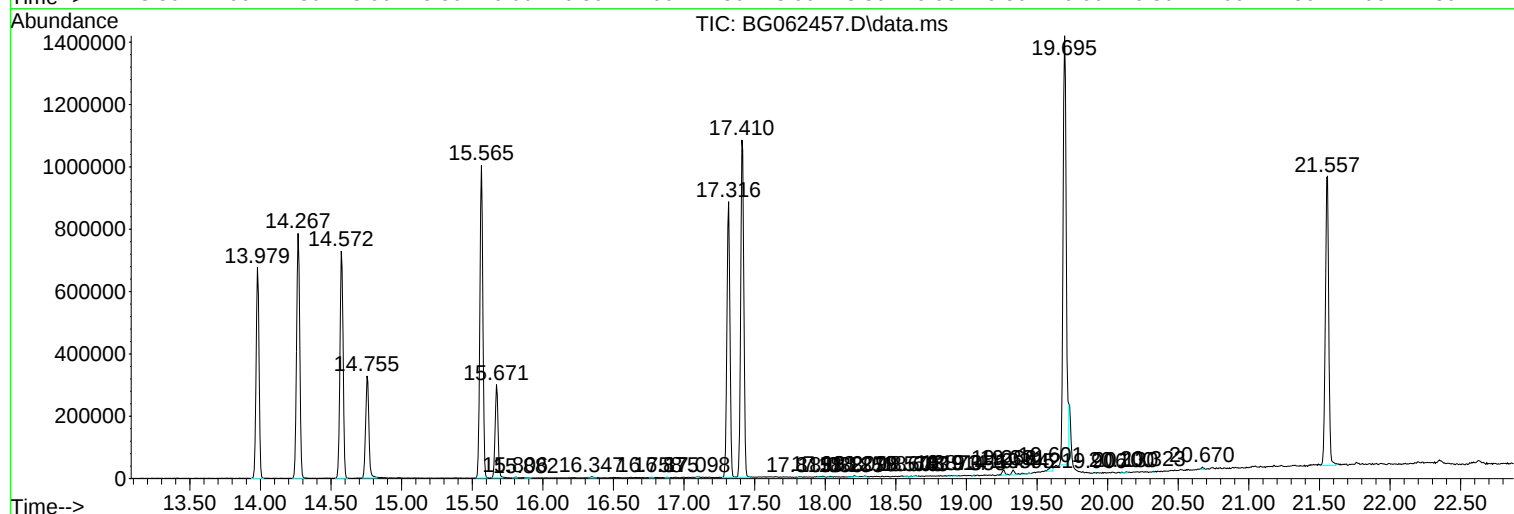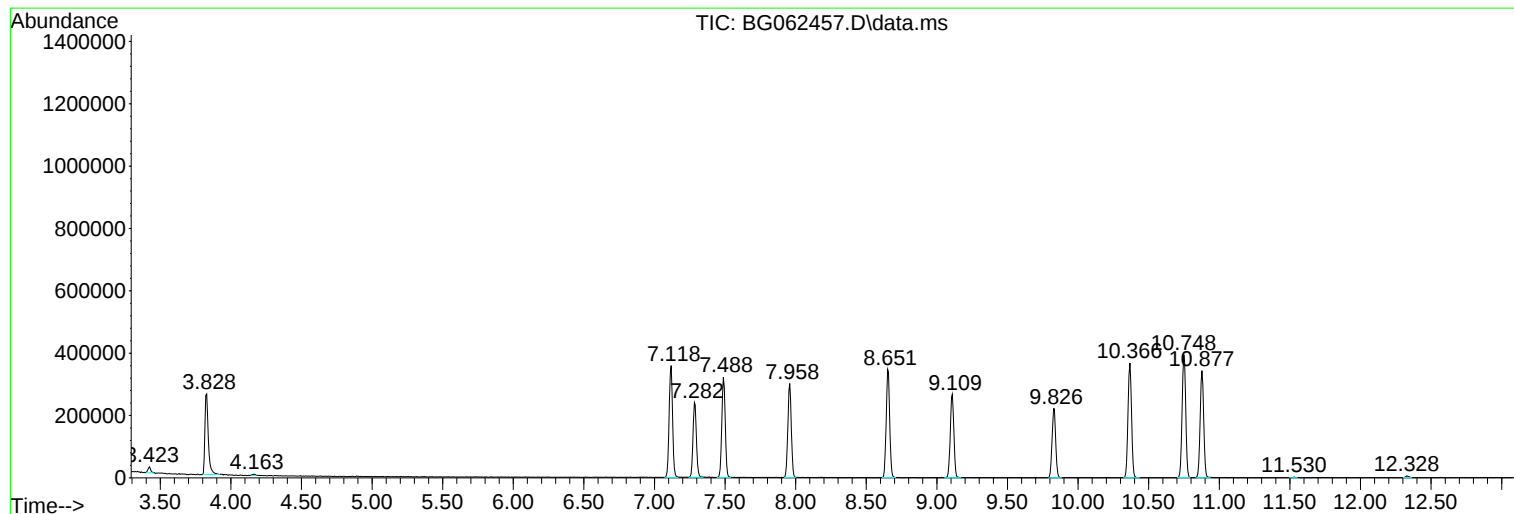

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
Data File : BG062457.D
Acq On : 17 Aug 2024 00:31
Operator : MA/JU
Sample : PB162801BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK801

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081524\
Data File : BG062457.D
Acq On : 17 Aug 2024 00:31
Operator : MA/JU
Sample : PB162801BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK801

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc