
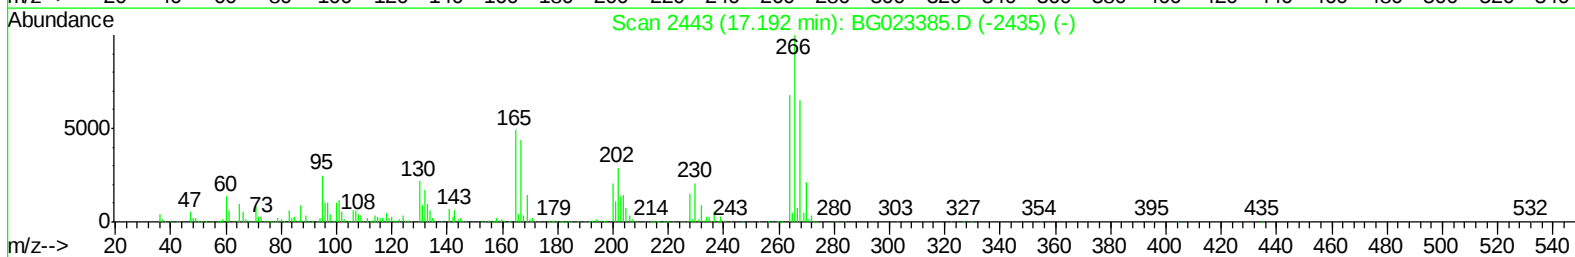
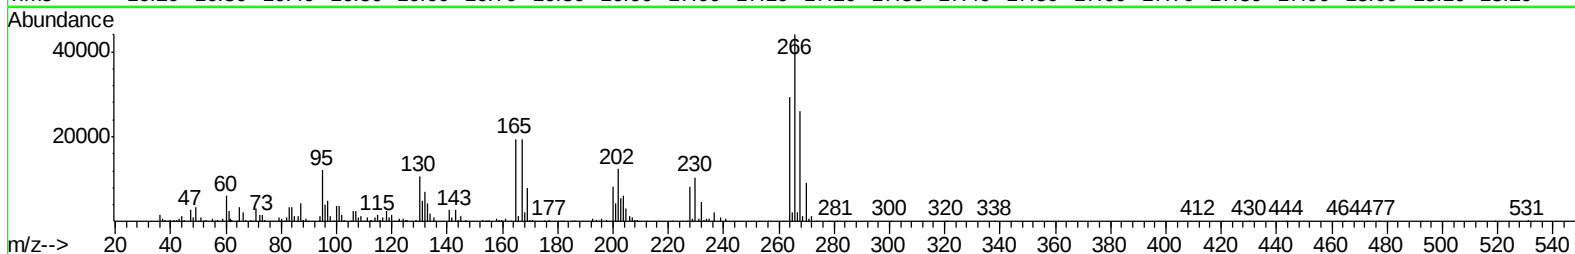


Data Path : Z:\HPCHEM1\BNA_G\Data\BG081616\
Data File : BG023729.D
Acq On : 16 Aug 2016 15:11
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 05:19:20 2016
Quant Method : Z:\HPCHEM1\BNA_G\Methods\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 01 19:22:14 2016
Response via : Initial Calibration

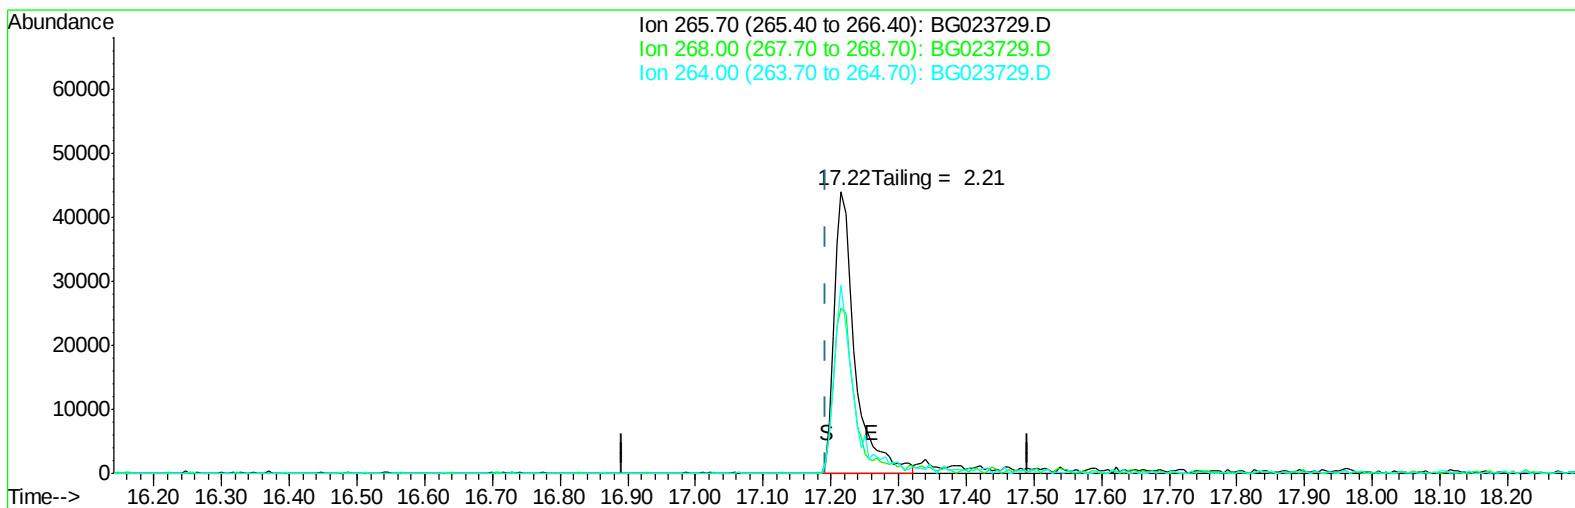

TIC: BG023729.D

(69) Pentachlorophenol (C)




17.216min (+0.023) 11637.21ng

response 90403

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	58.76
264.00	63.20	66.72
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG081616\
Data File : BG023729.D
Acq On : 16 Aug 2016 15:11
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 05:19:20 2016
Quant Method : Z:\HPCHEM1\BNA_G\Methods\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 01 19:22:14 2016
Response via : Initial Calibration

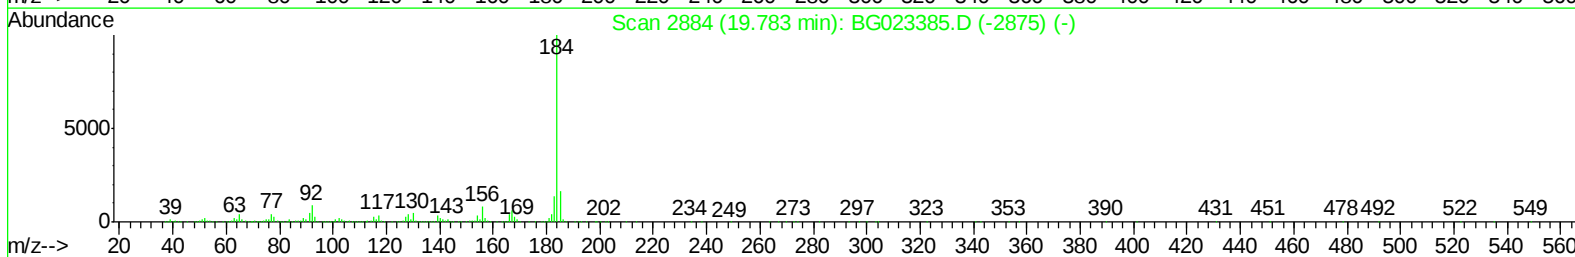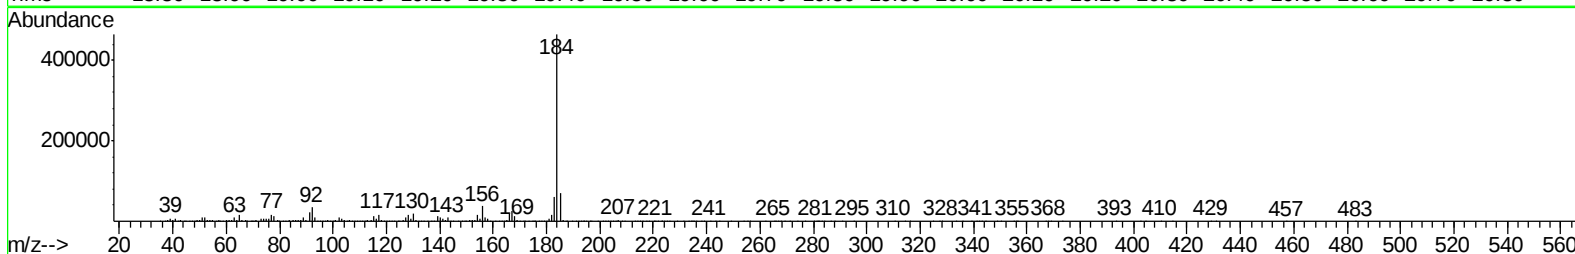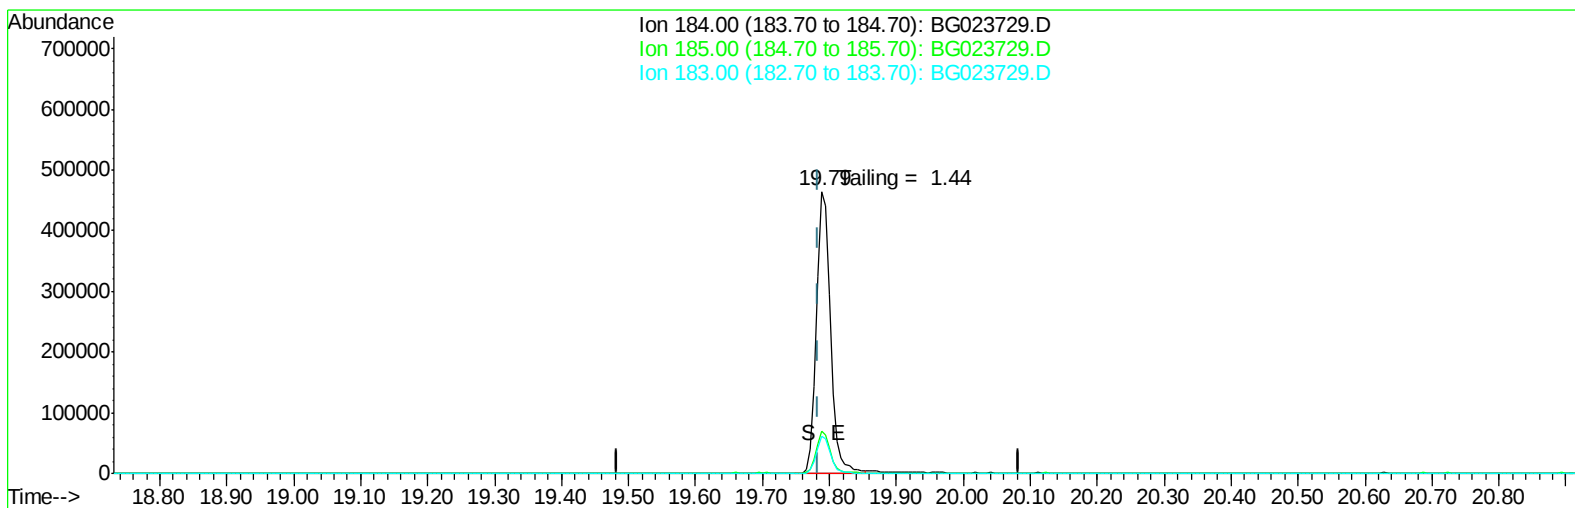

TIC: BG023729.D

(76) Benzidine

19.789min (+0.006) 6745.90ng

response 708850

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.85
183.00	13.40	13.03
0.00	0.00	0.00