


Data Path : Z:\HPCHEM1\BNA\_G\DATA\BG081616\  
 Data File : BG023729.D  
 Acq On : 16 Aug 2016 15:11  
 Operator : UM/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_G\Methods\8270-BG080116.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Aug 01 19:22:14 2016

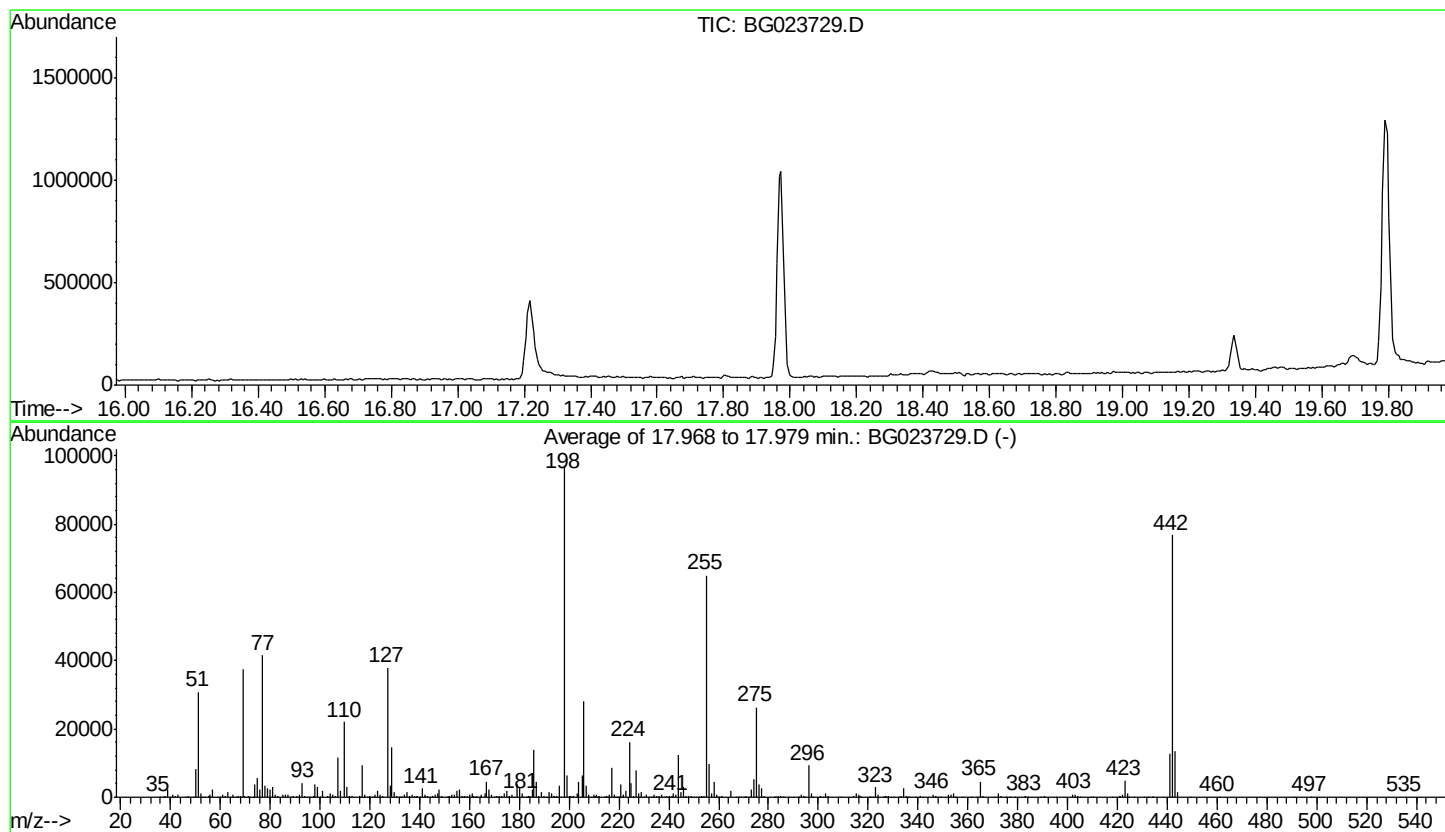

AutoFind: Scans 2575, 2576, 2577; Background Corrected with Scan 2568

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 31.7      | 30812   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.0       | 392     | PASS             |
| 69          | 198          | 0.00         | 100          | 38.8      | 37647   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.8       | 303     | PASS             |
| 127         | 198          | 10           | 80           | 39.2      | 38056   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 97128   | PASS             |
| 199         | 198          | 5            | 9            | 6.6       | 6422    | PASS             |
| 275         | 198          | 10           | 60           | 27.1      | 26344   | PASS             |
| 365         | 198          | 1            | 100          | 4.8       | 4673    | PASS             |
| 441         | 442          | 0.01         | 24           | 16.6      | 12715   | PASS             |
| 442         | 198          | 50           | 100          | 79.0      | 76696   | PASS             |
| 443         | 442          | 15           | 24           | 17.7      | 13544   | PASS             |