

Data Path : Z:\HPCHEM1\BNA G\DATA\BG081617\
 Data File : BG028370.D
 Acq On : 16 Aug 2017 14:13
 Operator : SJ/JU
 Sample : PB101604BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Aug 17 06:52:49 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 17 06:52:43 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.35	152	32249	20.00	ng/ul	0.00
18) Naphthalene-d8	11.17	136	142875	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.96	164	112574	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.81	188	515455	20.00	ng/ul	0.10
75) Chrysene-d12	22.03	240	347040	20.00	ng/ul	0.00
83) Perylene-d12	25.54	264	332663	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.83	96	4132	5.97	ng/uL	0.00
5) Phenol-d5	7.50	99	93366	26.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.66	67	59592	26.57	ng/ul	0.01
9) 2-Chlorophenol-d4	7.88	132	68297	30.57	ng/ul	0.00
13) 4-Methylphenol-d8	9.05	113	81110	27.40	ng/ul	0.00
19) Nitrobenzene-d5	9.52	128	35395	31.68	ng/ul	0.00
22) 2-Nitrophenol-d4	10.24	143	44334	36.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.78	165	82898	32.71	ng/ul	0.00
29) 4-Chloroaniline-d4	11.30	131	107292	38.03	ng/ul	0.00
43) Dimethylphthalate-d6	14.35	166	354409	35.40	ng/ul	0.00
46) Acenaphthylene-d8	14.65	160	362313	32.09	ng/ul	0.00
51) 4-Nitrophenol-d4	15.16	143	49987	31.40	ng/ul	0.00
57) Fluorene-d10	15.94	176	289472	32.23	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.13	200	870	0.26	ng/ul	0.07
70) Anthracene-d10	17.81	188	515455	20.85	ng/ul	0.00
76) Pyrene-d10	20.08	212	565717	31.79	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.30	264	523280	33.60	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	9.04	70	2632	1.097	ng/ul# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG081617\
Data File : BG028370.D
Acq On : 16 Aug 2017 14:13
Operator : SJ/JU
Sample : PB101604BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Aug 17 06:52:49 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 17 06:52:43 2017
Response via : Initial Calibration

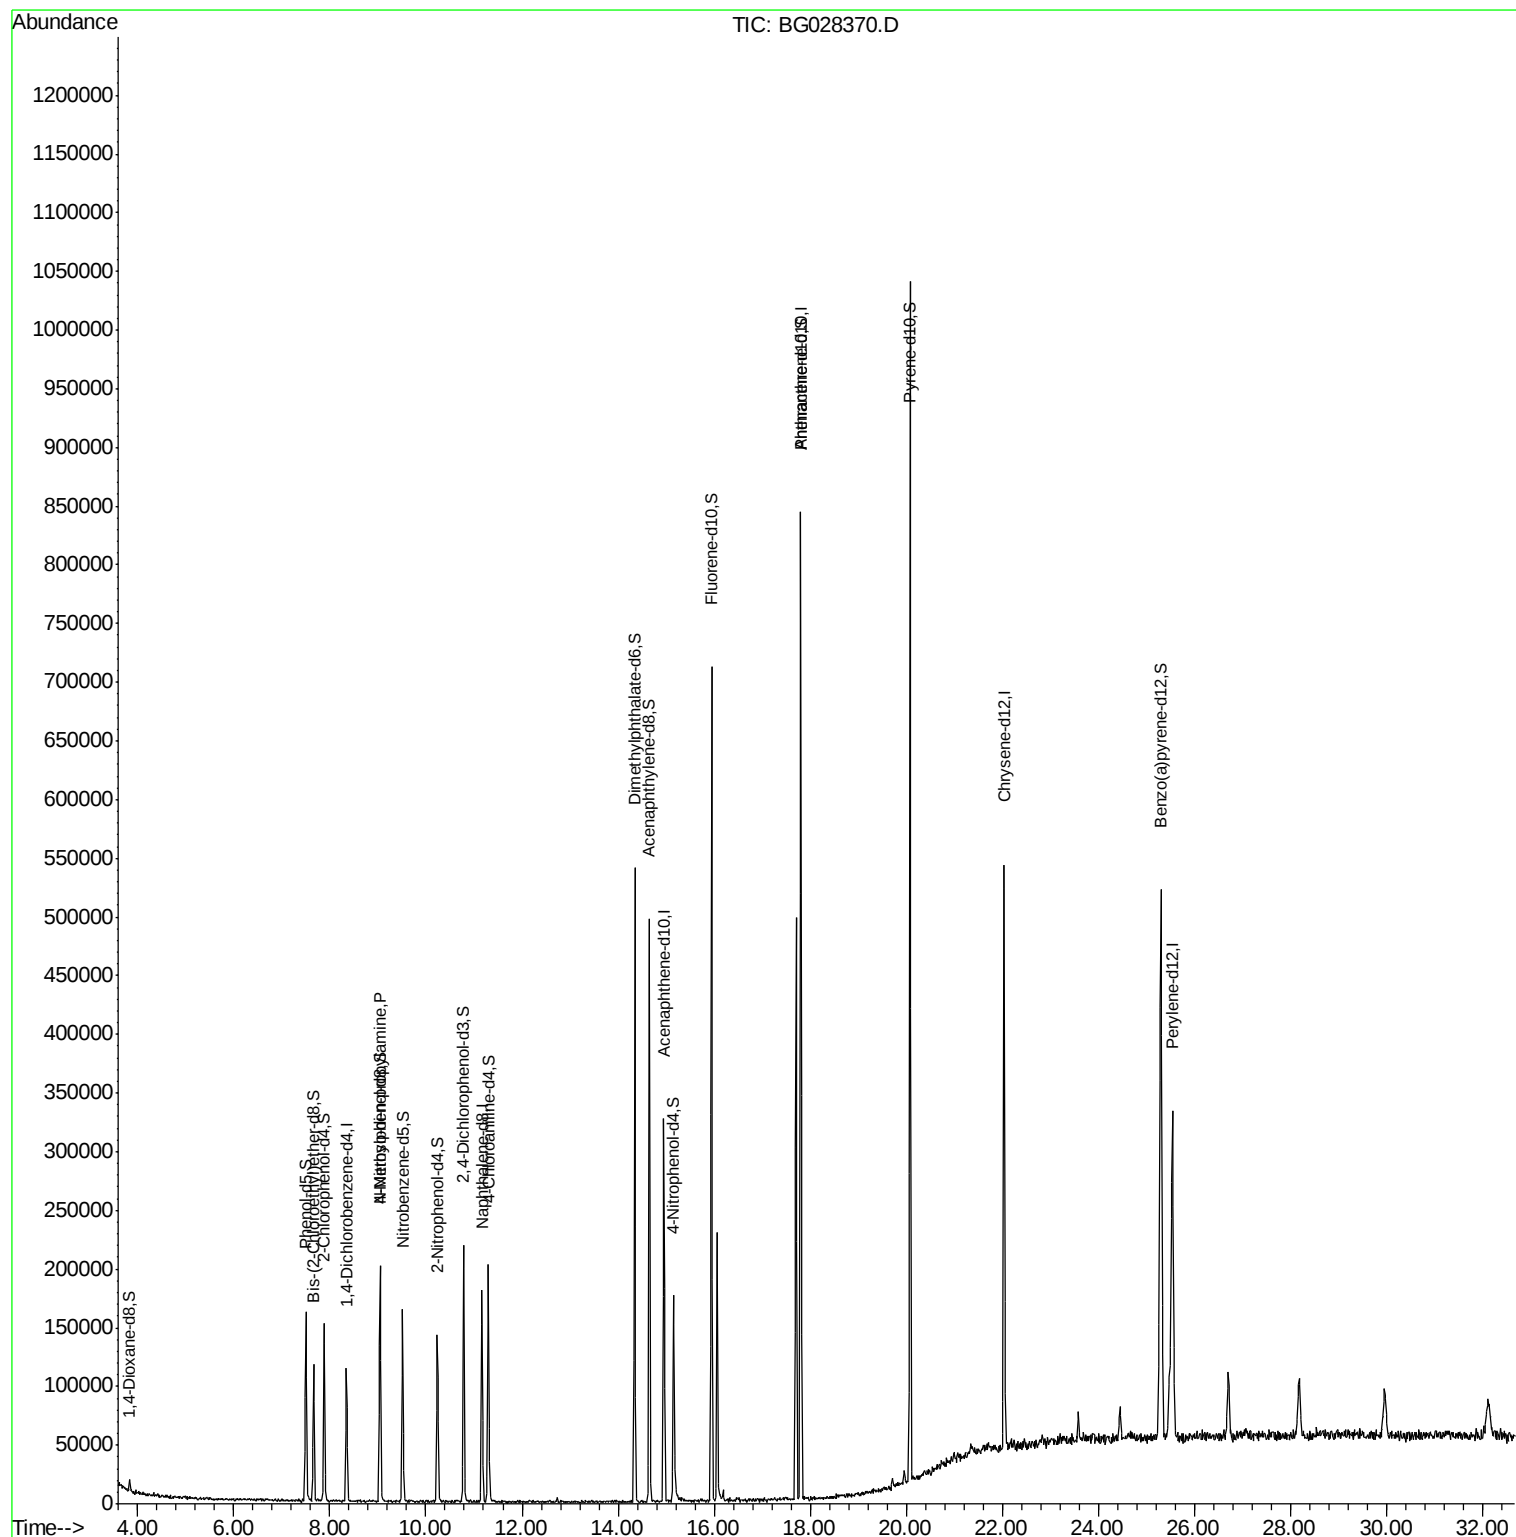

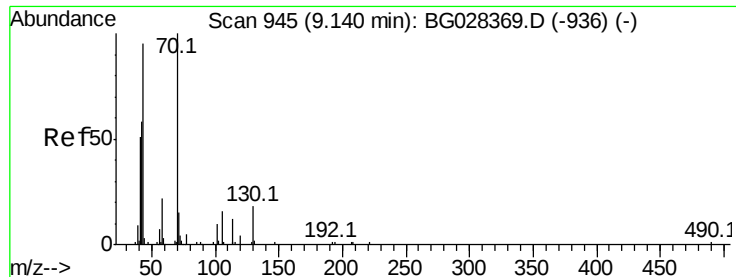

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.097 ng/ul
 RT: 9.04 min Scan# 928
 Delta R.T. -0.10 min
 Lab File: BG028370.D
 Acq: 16 Aug 2017 14:13

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ion	Ratio	Lower	Upper
70	100			
42	312.9	59.0	88.6#	
101	0.0	6.6	9.8#	
130	0.0	15.6	23.4#	

