
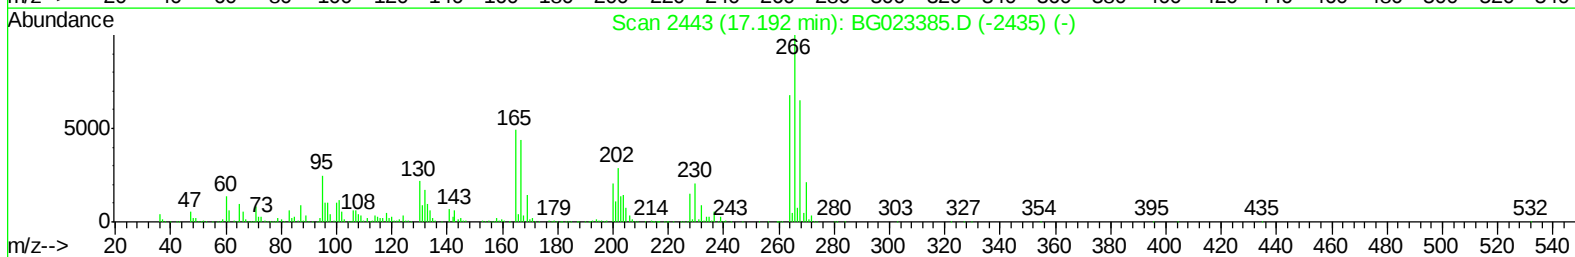
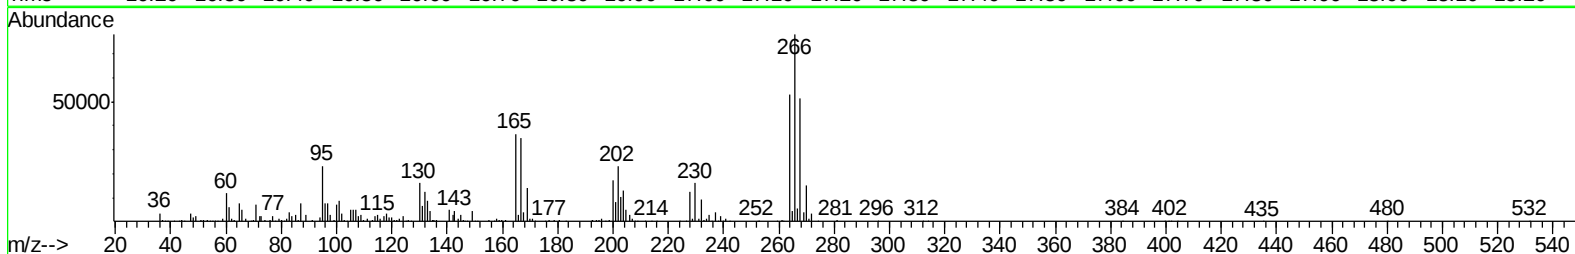


Data Path : Z:\HPCHEM1\BNA G\DATA\BG081716\
Data File : BG023744.D
Acq On : 17 Aug 2016 9:01
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 16:53:52 2016
Quant Method : Z:\HPCHEM1\BNA G\Methods\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 01 19:22:14 2016
Response via : Initial Calibration

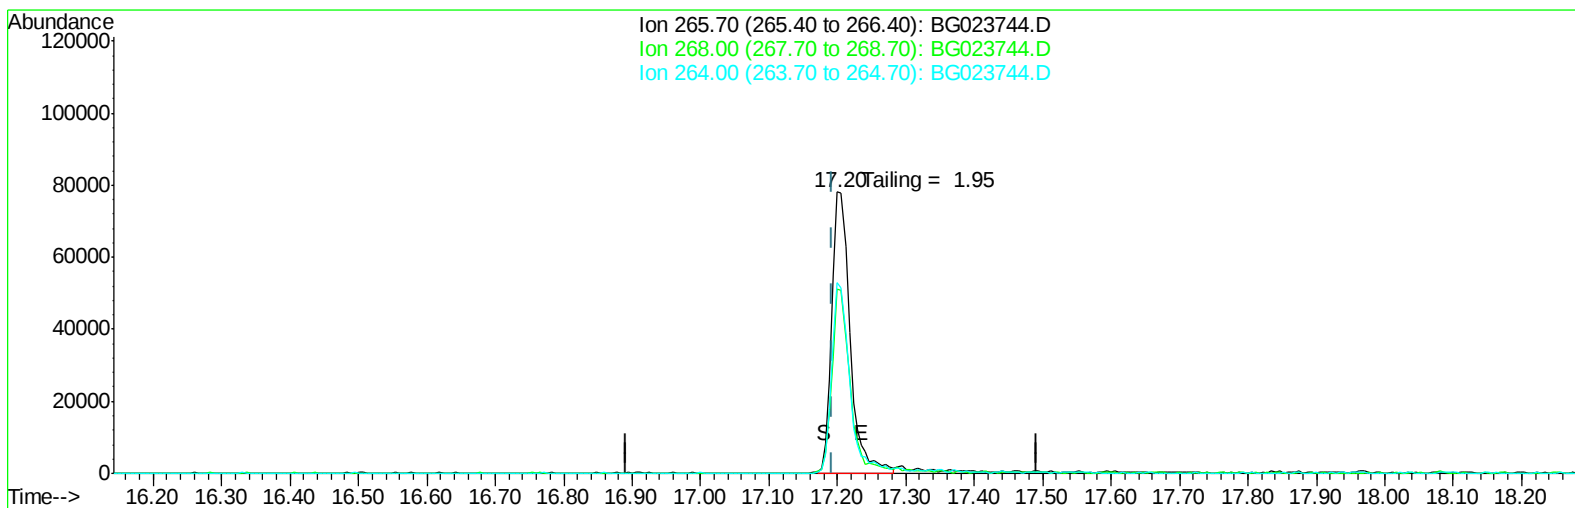

TIC: BG023744.D

(69) Pentachlorophenol (C)




17.200min (+0.007) 38894.05ng

response 145435

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	65.66
264.00	63.20	67.88
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG081716\
 Data File : BG023744.D
 Acq On : 17 Aug 2016 9:01
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 16:53:52 2016
 Quant Method : Z:\HPCHEM1\BNA G\Methods\8270-BG080116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 01 19:22:14 2016
 Response via : Initial Calibration

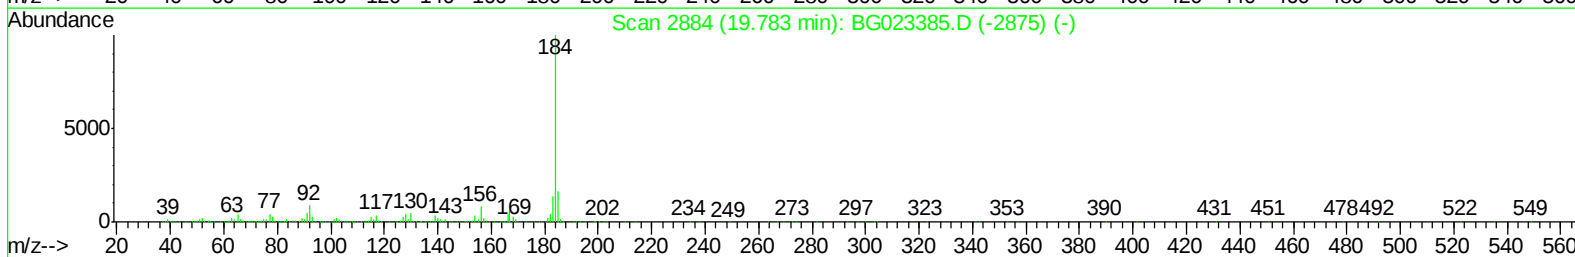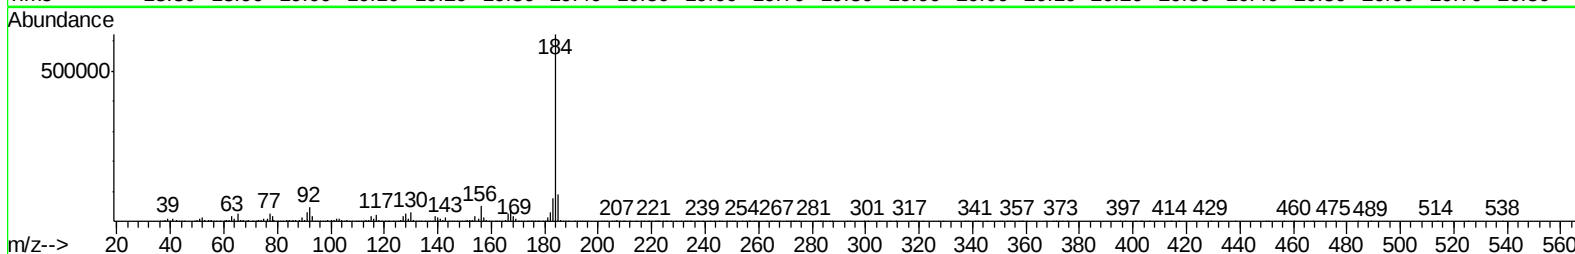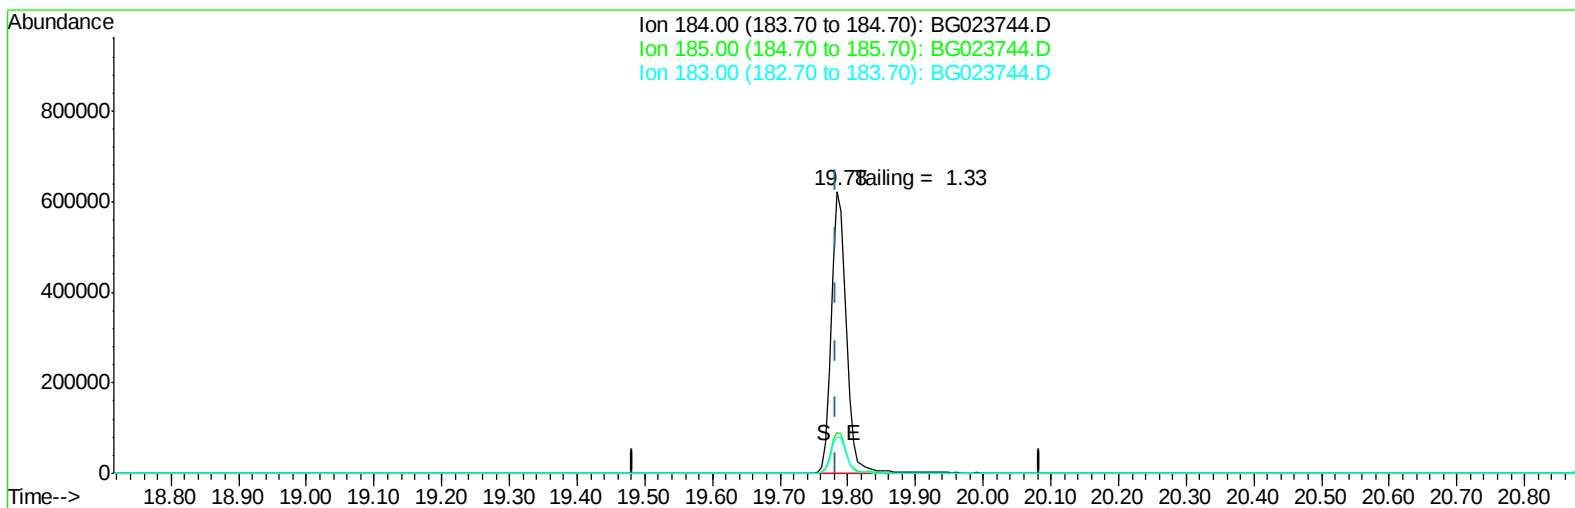

TIC: BG023744.D

(76) Benzidine

19.785min (+0.002) 13956.31ng

response 936549

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.57
183.00	13.40	12.57
0.00	0.00	0.00