


Data Path : Z:\HPCHEM1\BNA G\DATA\BG081716\
 Data File : BG023744.D
 Acq On : 17 Aug 2016 9:01
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\Methods\8270-BG080116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 01 19:22:14 2016

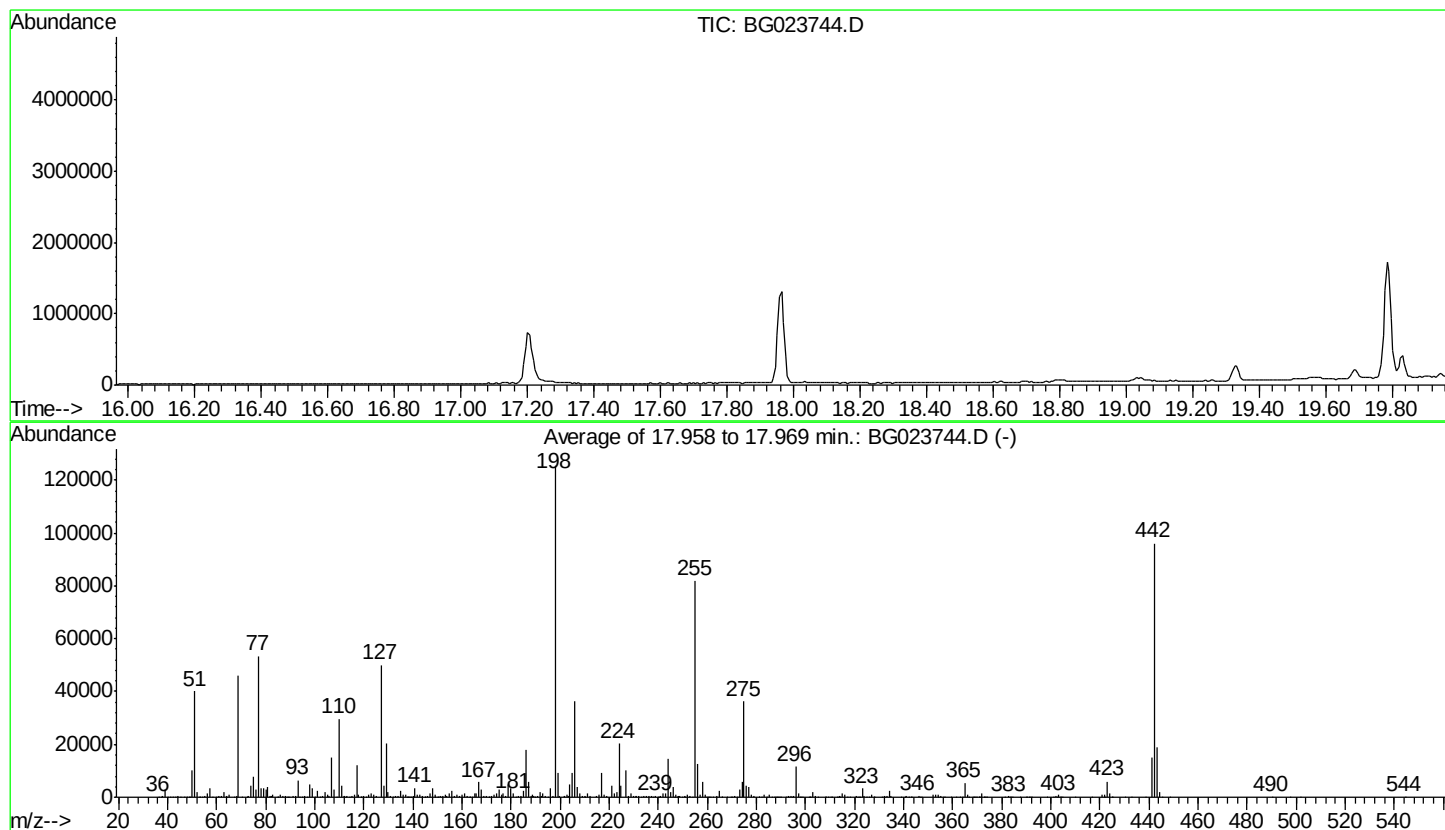

AutoFind: Scans 2574, 2575, 2576; Background Corrected with Scan 2566

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.9	39997	PASS
68	69	0.00	2	0.7	327	PASS
69	198	0.00	100	36.7	46015	PASS
70	69	0.00	2	0.2	97	PASS
127	198	10	80	39.8	49958	PASS
197	198	0.00	2	0.5	566	PASS
198	198	100	100	100.0	125488	PASS
199	198	5	9	7.3	9193	PASS
275	198	10	60	28.9	36317	PASS
365	198	1	100	4.3	5365	PASS
441	442	0.01	24	15.5	14928	PASS
442	198	50	100	76.6	96120	PASS
443	442	15	24	19.5	18722	PASS