

Data File : BG042275.D
Acq On : 17 Aug 2019 1:01
Operator : HP/JU
Sample : K4265-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
REACTOR-4-B-(0-3.4)

Quant Time: Aug 17 05:38:17 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG072719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 08:57:26 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	59280	20.00	ng	-0.03
21) Naphthalene-d8	10.83	136	219454	20.00	ng	-0.04
39) Acenaphthene-d10	14.67	164	161652	20.00	ng	-0.03
64) Phenanthrene-d10	17.43	188	397381	20.00	ng	-0.03
76) Chrysene-d12	21.70	240	465900	20.00	ng	-0.03
87) Perylene-d12	24.96	264	545466	20.00	ng	-0.05

System Monitoring Compounds						
5) 2-Fluorophenol	5.57	112	375716	123.31	ng	-0.02
7) Phenol-d6	7.17	99	444536	108.22	ng	-0.02
23) Nitrobenzene-d5	9.18	82	325484	102.07	ng	-0.03
42) 2,4,6-Tribromophenol	16.16	330	346471	188.69	ng	-0.03
45) 2-Fluorobiphenyl	13.29	172	1008013	109.98	ng	-0.04
79) Terphenyl-d14	20.04	244	1974781	96.99	ng	-0.03


Target Compounds				Qvalue		
2) 1,4-Dioxane	3.14	88	15983	11.145	ng	# 1
19) n-Nitroso-di-n-propylamine	9.18	70	42212	14.155	ng	# 62
51) 2,6-Dinitrotoluene	14.67	165	21192	9.180	ng	# 27
57) 2,4-Dinitrotoluene	14.67	165	21192	6.675	ng	# 28
65) 4,6-Dinitro-2-methylphenol	16.16	198	736	7.177	ng	# 9
67) 4-Bromophenyl-phenylether	16.16	248	24216	4.947	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BG042275.D
Acq On : 17 Aug 2019 1:01
Operator : HP/JU
Sample : K4265-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
REACTOR-4-B-(0-3.4)

Quant Time: Aug 17 05:38:17 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG072719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 08:57:26 2019
Response via : Initial Calibration

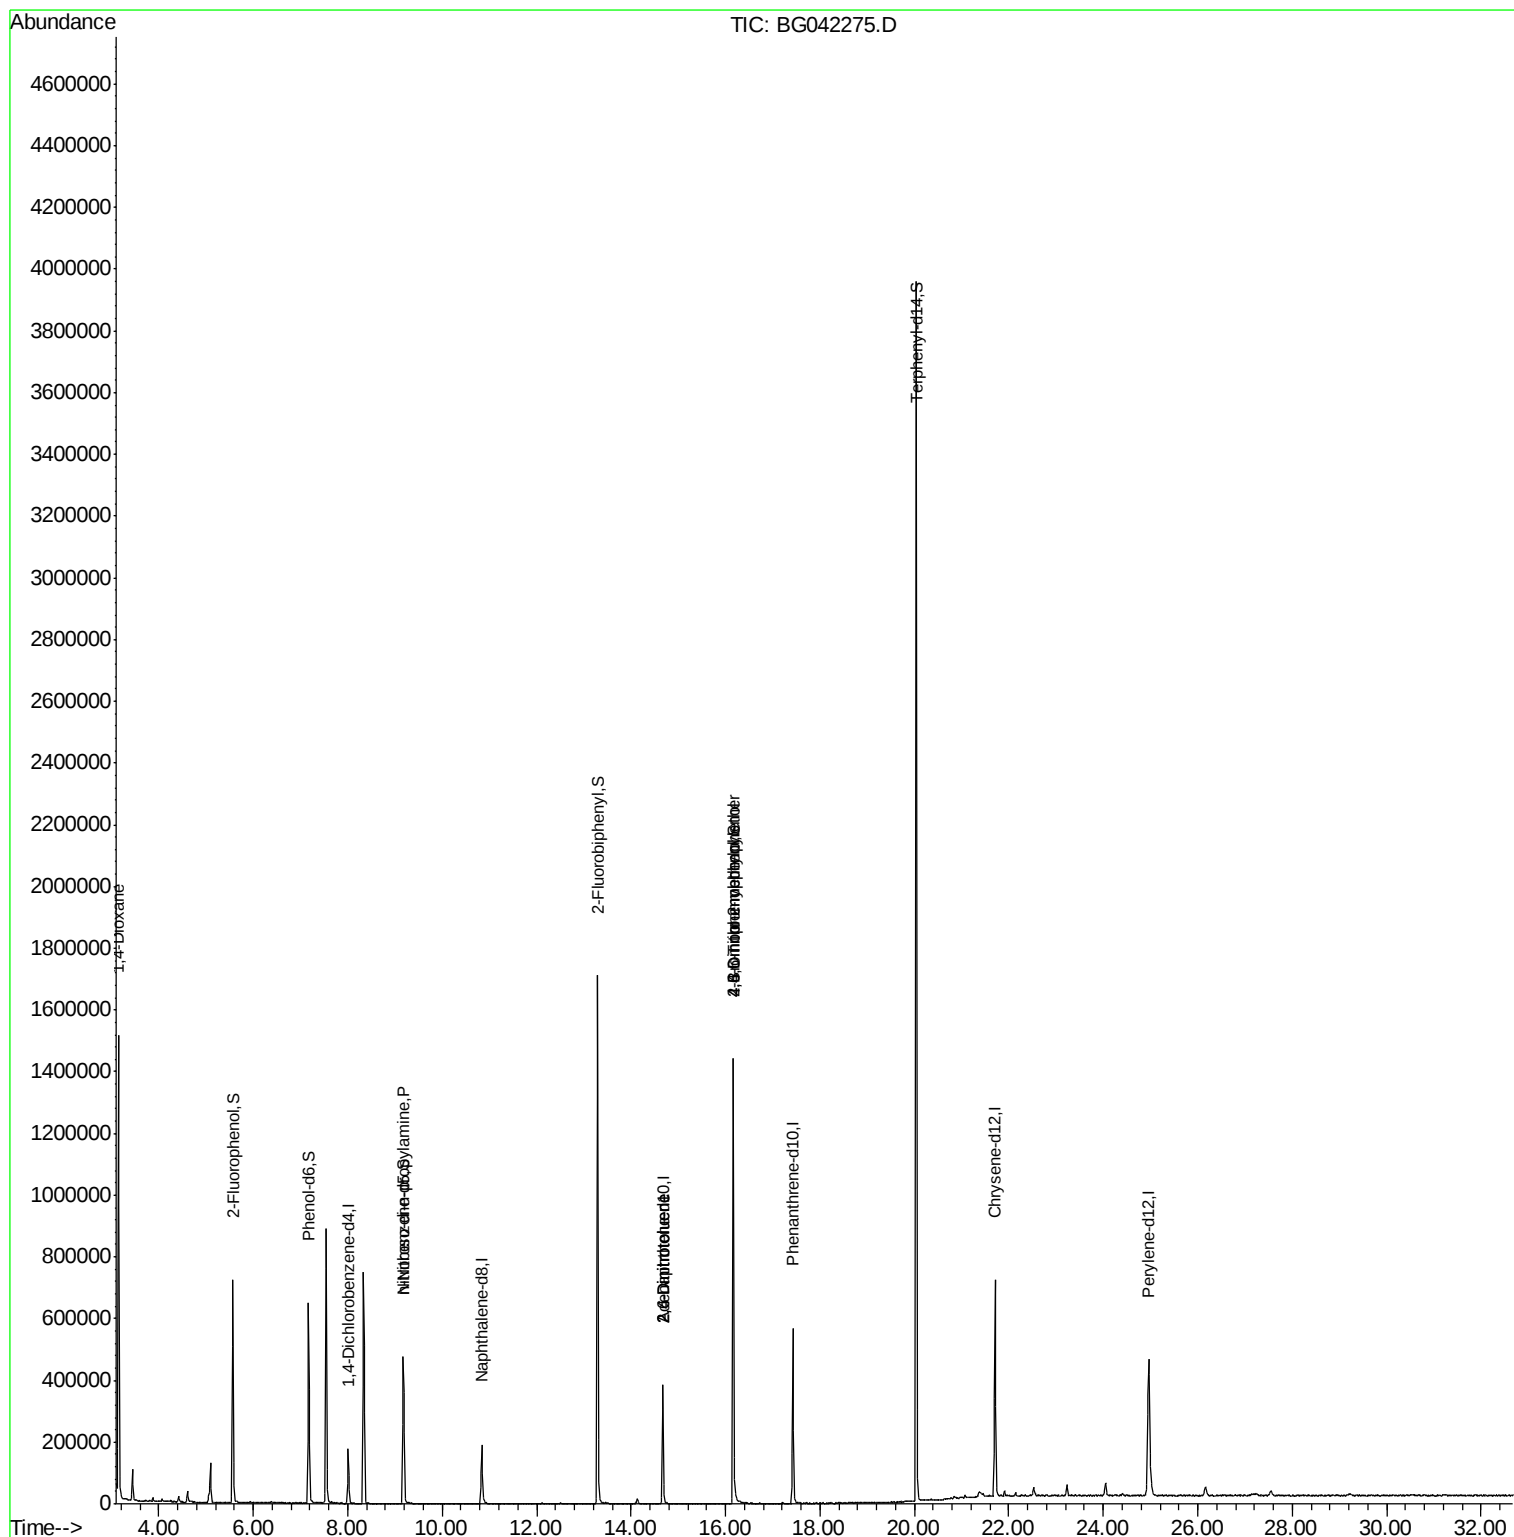



#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.01 min Scan# 838

Delta R.T. -0.03 min

Lab File: BG042275.D

Acq: 17 Aug 2019 1:01

Instrument :

BNA_G

ClientSampleId :

REACTOR-4-B-(0-3.4)


Tgt Ion:152 Resp: 59280

Ion Ratio Lower Upper

152 100

150 159.5 126.9 190.3




115 50.9 45.0 67.6

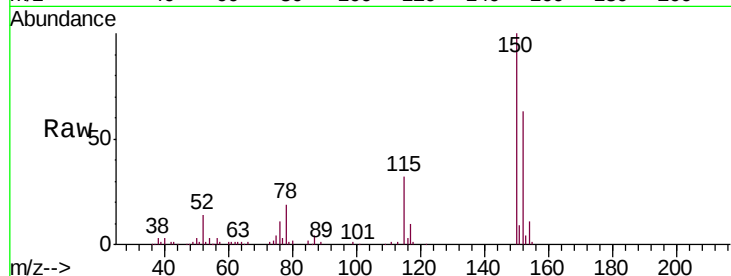

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

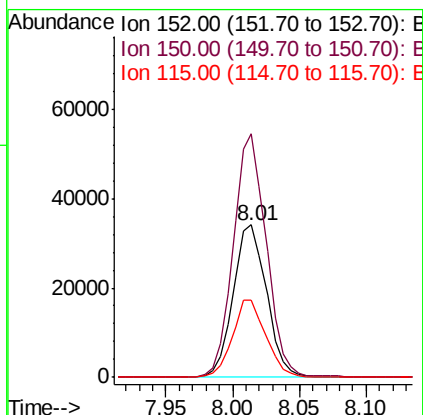

#2

1,4-Dioxane

Concen: 11.145 ng

RT: 3.14 min Scan# 9

Delta R.T. -0.33 min

Lab File: BG042275.D

Acq: 17 Aug 2019 1:01


Tgt Ion: 88 Resp: 15983

Ion Ratio Lower Upper

88 100

58 23.0 76.2 114.2#



43 1850.8 27.2 40.8#




Abundance Ion 88.00 (87.70 to 88.70): BGC

Ion 58.00 (57.70 to 58.70): BGC

Ion 43.00 (42.70 to 43.70): BGC

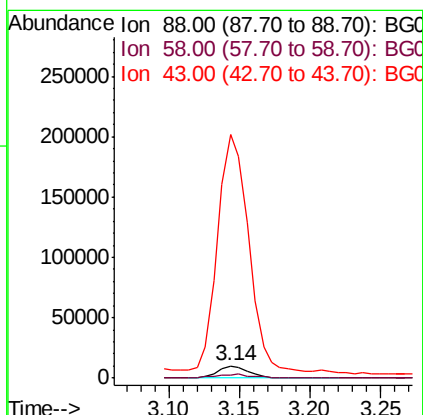



#5

2-Fluorophenol

Concen: 123.313 ng

RT: 5.57 min Scan# 422

Delta R.T. -0.02 min

Lab File: BG042275.D

Acq: 17 Aug 2019 1:01

Instrument :

BNA_G

ClientSampleId :

REACTOR-4-B-(0-3.4)


Tgt Ion: 112 Resp: 375716

Ion Ratio Lower Upper

112 100

64 54.4 55.4 83.2#




63 27.9 29.1 43.7#



Abundance Ion 112.00 (111.70 to 112.70): BGC

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

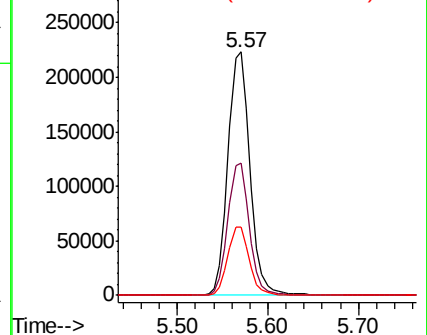

#7

Phenol-d6

Concen: 108.222 ng

RT: 7.17 min Scan# 695

Delta R.T. -0.02 min

Lab File: BG042275.D

Acq: 17 Aug 2019 1:01


Tgt Ion: 99 Resp: 444536

Ion Ratio Lower Upper

99 100

42 14.2 17.6 26.4#



71 31.2 27.8 41.6




Abundance Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC




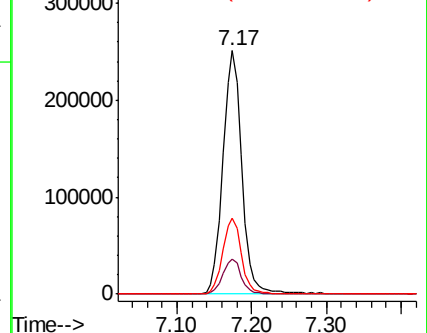




#19
n-Nitroso-di-n-propylamine
Concen: 14.155 ng
RT: 9.18 min Scan# 1036
Delta R.T. 0.32 min
Lab File: BG042275.D
Acq: 17 Aug 2019 1:01




Instrument :
BNA_G
ClientSampleId :
REACTOR-4-B-(0-3.4)


Tgt Ion: 70 Resp: 42212
Ion Ratio Lower Upper
70 100
42 37.5 55.8 83.6#
101 0.0 8.1 12.1#
130 2.5 17.3 25.9#

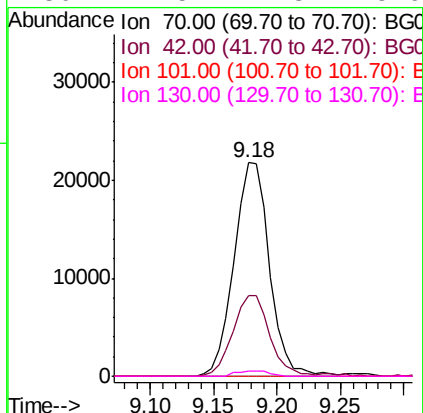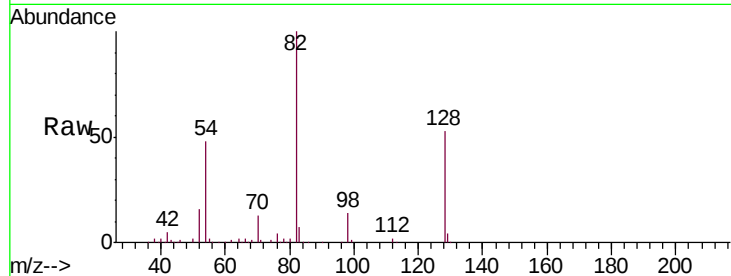

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.83 min Scan# 1318
Delta R.T. -0.04 min
Lab File: BG042275.D
Acq: 17 Aug 2019 1:01

Tgt Ion: 136 Resp: 219454
Ion Ratio Lower Upper
136 100
137 10.8 9.2 13.8
54 6.4 8.7 13.1#
68 4.8 5.5 8.3#


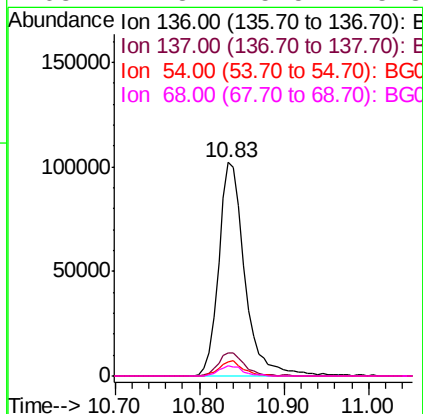

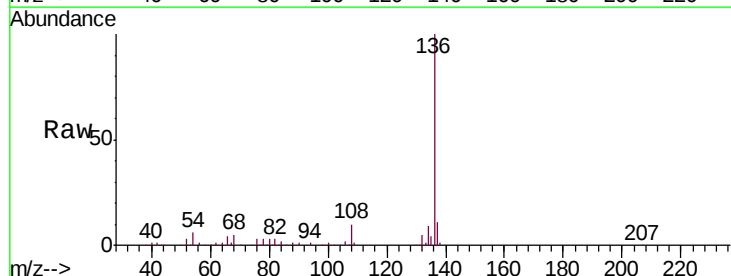




#23
 Nitrobenzene-d5
 Concen: 102.065 ng
 RT: 9.18 min Scan# 1037
 Delta R.T. -0.03 min
 Lab File: BG042275.D
 Acq: 17 Aug 2019 1:01




Instrument :
 BNA_G
 ClientSampleId :
 REACTOR-4-B-(0-3.4)


Tgt Ion: 82 Resp: 325484
 Ion Ratio Lower Upper
 82 100
 128 50.7 35.1 52.7
 54 45.6 48.7 73.1#

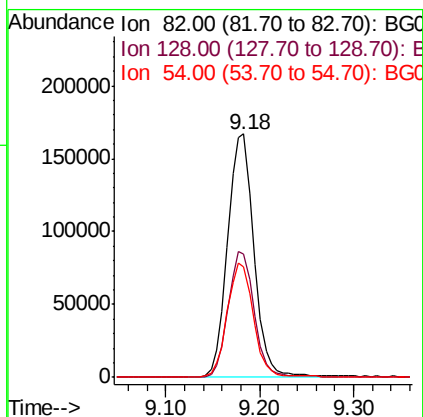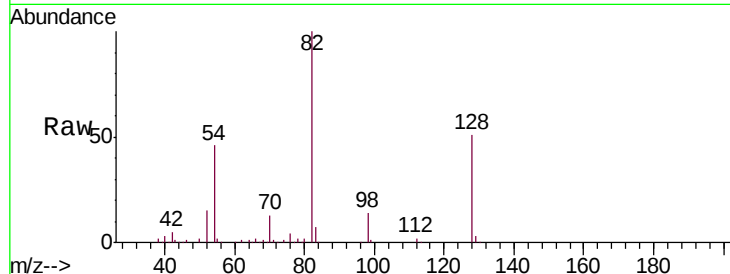

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.67 min Scan# 1971
 Delta R.T. -0.03 min
 Lab File: BG042275.D
 Acq: 17 Aug 2019 1:01

Tgt Ion: 164 Resp: 161652
 Ion Ratio Lower Upper
 164 100
 162 100.0 79.6 119.4
 160 43.9 35.4 53.0

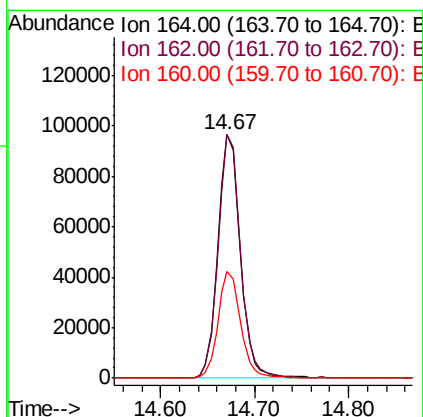



#42

2,4,6-Tribromophenol

Concen: 188.695 ng

RT: 16.16 min Scan# 2225

Delta R.T. -0.03 min

Lab File: BG042275.D

Acq: 17 Aug 2019 1:01

Instrument :

BNA_G

ClientSampleId :

REACTOR-4-B-(0-3.4)


Tgt Ion:330 Resp: 346471

Ion Ratio Lower Upper




330 100

332 96.4 77.4 116.0

141 28.6 31.9 47.9#

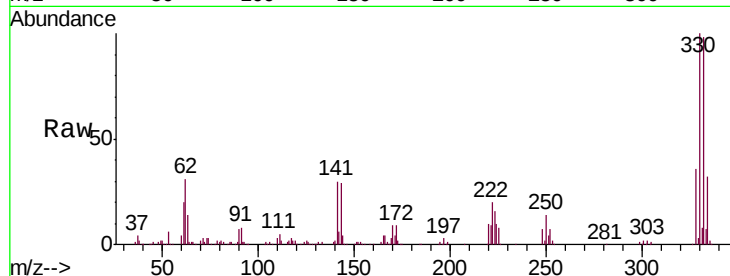

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

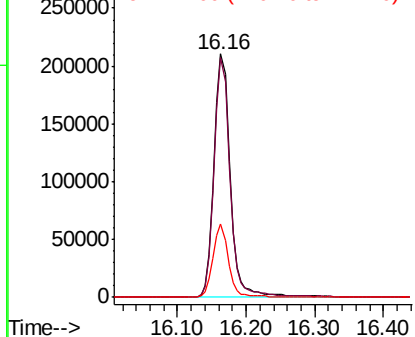

#45

2-Fluorobiphenyl

Concen: 109.980 ng

RT: 13.29 min Scan# 1736

Delta R.T. -0.04 min

Lab File: BG042275.D

Acq: 17 Aug 2019 1:01


Tgt Ion:172 Resp: 1008013

Ion Ratio Lower Upper



172 100


171 38.4 35.0 52.4

170 25.1 23.5 35.3



Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E




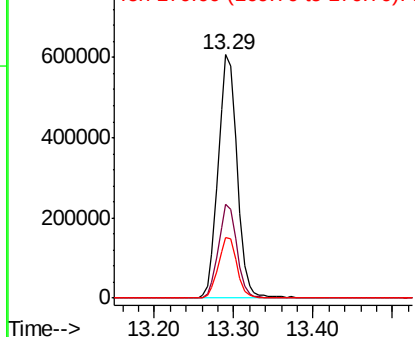


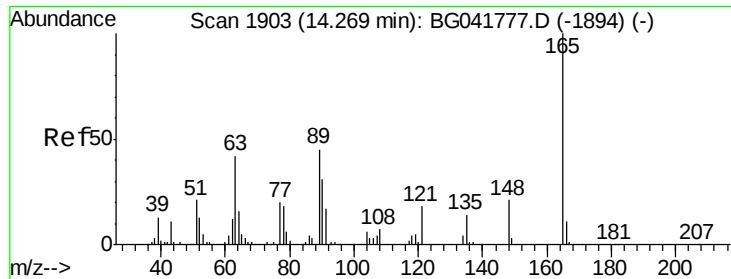

#51
 2,6-Dinitrotoluene
 Concen: 9.180 ng
 RT: 14.67 min Scan# 1971
 Delta R.T. 0.40 min
 Lab File: BG042275.D
 Acq: 17 Aug 2019 1:01




Instrument :
 BNA_G
 ClientSampleId :
 REACTOR-4-B-(0-3.4)


Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.7	42.4	63.6#
89	0.0	42.1	63.1#

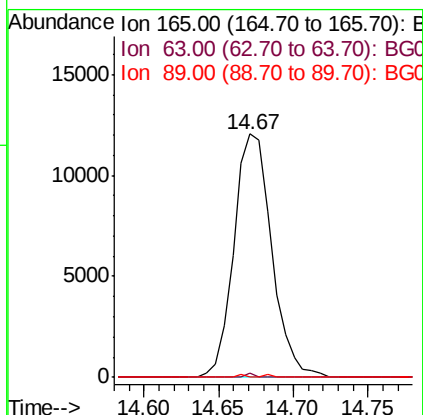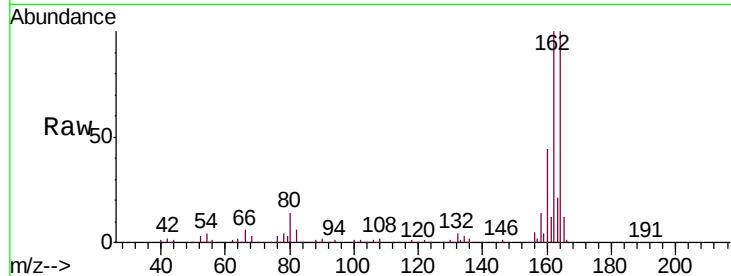

#57
 2,4-Dinitrotoluene
 Concen: 6.675 ng
 RT: 14.67 min Scan# 1971
 Delta R.T. -0.38 min
 Lab File: BG042275.D
 Acq: 17 Aug 2019 1:01

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.7	31.7	47.5#
89	0.0	50.2	75.4#
182	0.0	2.6	4.0#

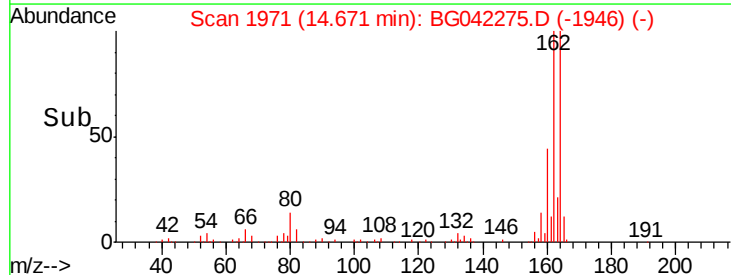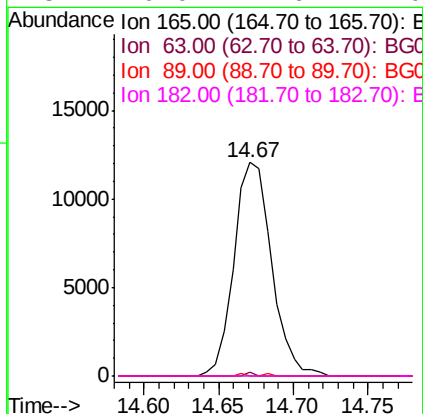



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.43 min Scan# 2440

Delta R.T. -0.03 min

Lab File: BG042275.D

Acq: 17 Aug 2019 1:01

Instrument :

BNA_G

ClientSampleId :

REACTOR-4-B-(0-3.4)


Tgt Ion:188 Resp: 397381

Ion Ratio Lower Upper

188 100

94 6.3 6.9 10.3#




80 6.9 8.0 12.0#



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

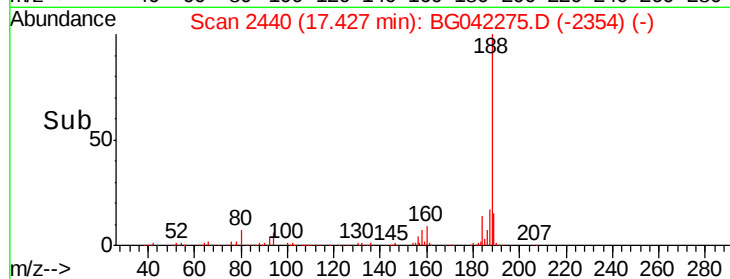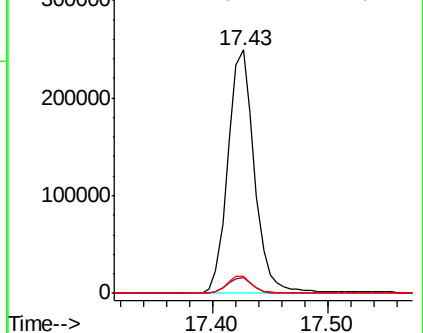

#65

4,6-Dinitro-2-methylphenol

Concen: 7.177 ng

RT: 16.16 min Scan# 2225

Delta R.T. 0.34 min

Lab File: BG042275.D

Acq: 17 Aug 2019 1:01


Tgt Ion:198 Resp: 736

Ion Ratio Lower Upper

198 100

51 72.2 22.3 62.3#



105 122.8 18.0 58.0#




Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BGC

Ion 105.00 (104.70 to 105.70): E

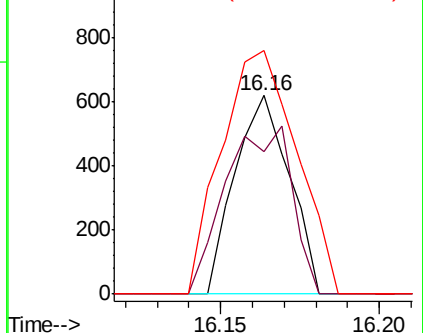


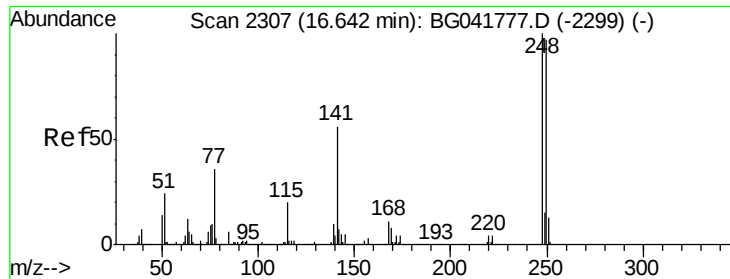

#67
 4-Bromophenyl-phenylether
 Concen: 4.947 ng
 RT: 16.16 min Scan# 2225
 Delta R.T. -0.48 min
 Lab File: BG042275.D
 Acq: 17 Aug 2019 1:01

Instrument :
 BNA_G
 ClientSampleId :
 REACTOR-4-B-(0-3.4)

Tgt Ion	Ratio	Lower	Upper
248	100		
250	197.3	78.1	117.1#
141	413.6	49.6	74.4#






Abundance

Ion 248.00 (247.70 to 248.70): E


Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

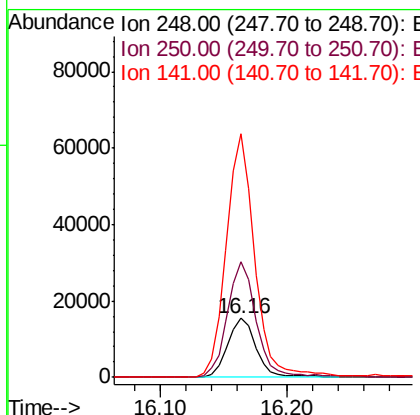

#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.70 min Scan# 3168
 Delta R.T. -0.03 min
 Lab File: BG042275.D
 Acq: 17 Aug 2019 1:01

Tgt Ion	Ratio	Lower	Upper
240	100		
120	7.7	8.0	12.0#
236	26.1	22.6	33.8






Abundance

Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

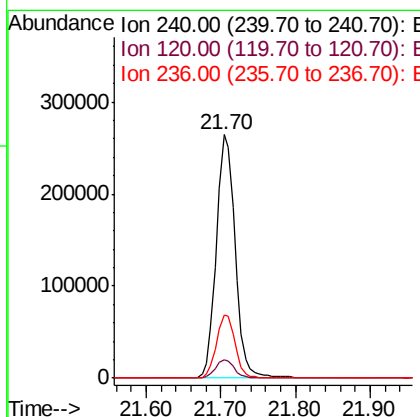



#79

Terphenyl-d14

Concen: 96.991 ng

RT: 20.04 min Scan# 2885

Delta R.T. -0.03 min

Lab File: BG042275.D

Acq: 17 Aug 2019 1:01

Instrument :

BNA_G

ClientSampleId :

REACTOR-4-B-(0-3.4)


Tgt Ion:244 Resp: 1974781

Ion Ratio Lower Upper

244 100

212 8.7 9.7 14.5#




122 10.1 12.5 18.7#



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

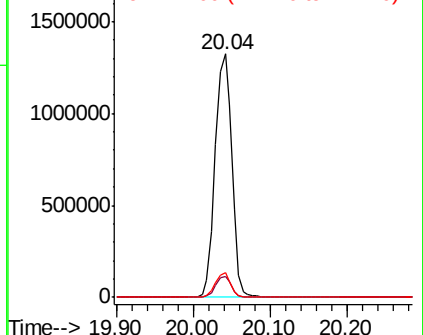

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.96 min Scan# 3723

Delta R.T. -0.05 min

Lab File: BG042275.D

Acq: 17 Aug 2019 1:01


Tgt Ion:264 Resp: 545466

Ion Ratio Lower Upper

264 100

260 23.6 19.5 29.3

265 21.8 18.0 27.0



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

