

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081719\
 Data File : BG042275.D
 Acq On : 17 Aug 2019 1:01
 Operator : HP/JU
 Sample : K4265-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 REACTOR-4-B-(0-3.4)

Quant Time: Aug 17 05:41:38 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG072719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 31 08:57:26 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	59280	20.00	ng	-0.03
21) Naphthalene-d8	10.83	136	219454	20.00	ng	-0.04
39) Acenaphthene-d10	14.67	164	161652	20.00	ng	-0.03
64) Phenanthrene-d10	17.43	188	397381	20.00	ng	-0.03
76) Chrysene-d12	21.70	240	465900	20.00	ng	-0.03
87) Perylene-d12	24.96	264	545466	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.57	112	375716	123.31	ng	-0.02
7) Phenol-d6	7.17	99	444536	108.22	ng	-0.02
23) Nitrobenzene-d5	9.18	82	325484	102.07	ng	-0.03
42) 2,4,6-Tribromophenol	16.16	330	346471	188.69	ng	-0.03
45) 2-Fluorobiphenyl	13.29	172	1008013	109.98	ng	-0.04
79) Terphenyl-d14	20.04	244	1974781	96.99	ng	-0.03


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081719\
Data File : BG042275.D
Acq On : 17 Aug 2019 1:01
Operator : HP/JU
Sample : K4265-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
REACTOR-4-B-(0-3.4)

Quant Time: Aug 17 05:41:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG072719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 08:57:26 2019
Response via : Initial Calibration

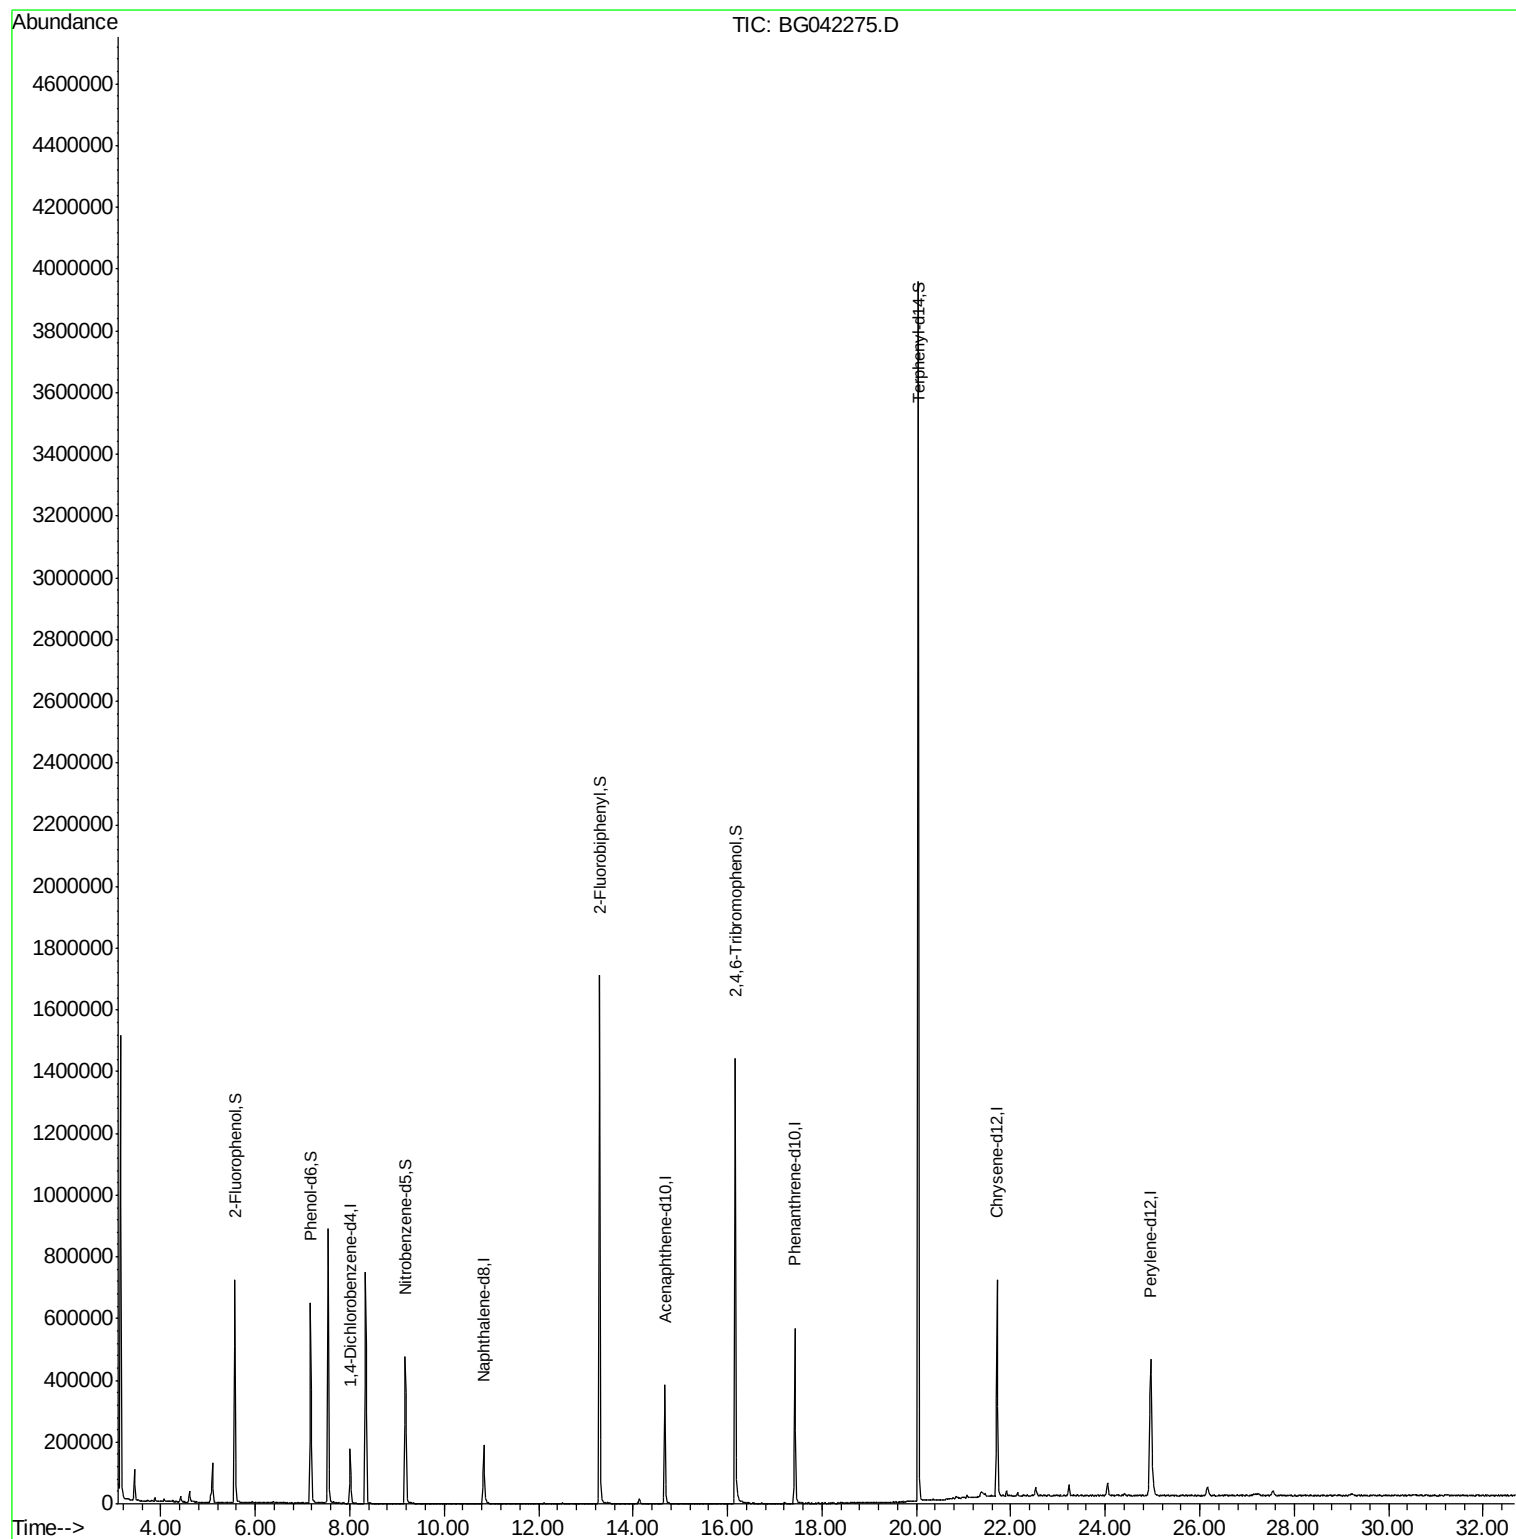




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.01 min Scan# 838
Delta R.T. -0.03 min
Lab File: BG042275.D
Acq: 17 Aug 2019 1:01

Instrument :
BNA_G
ClientSampleId :
REACTOR-4-B-(0-3.4)

Tot Ion	Ratio	Lower	Upper
152	100		
150	159.5	126.9	190.3
115	50.9	45.0	67.6

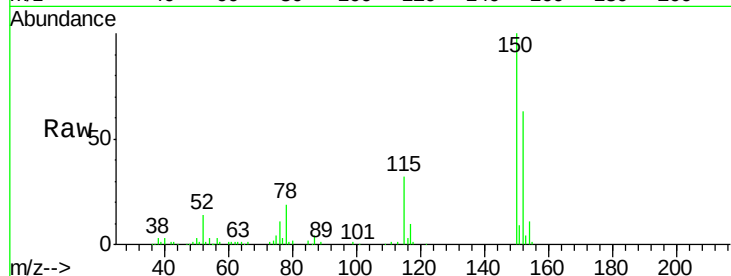


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

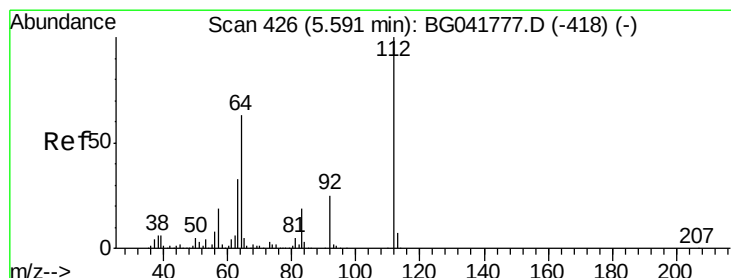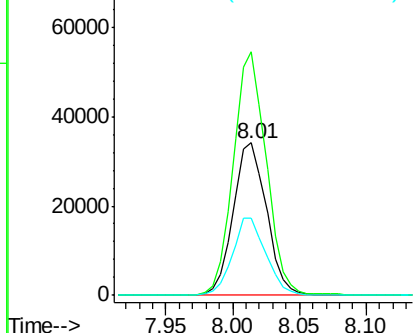



#5




2-Fluorophenol
Concen: 123.313 ng
RT: 5.57 min Scan# 422
Delta R.T. -0.02 min
Lab File: BG042275.D
Acq: 17 Aug 2019 1:01

Tgt Ion	Ratio	Lower	Upper
112	100		
64	54.4	55.4	83.2#
63	27.9	29.1	43.7#

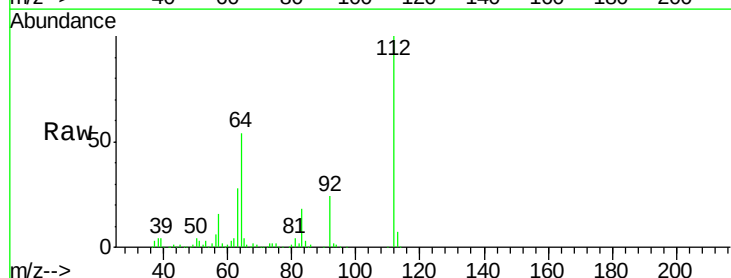

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

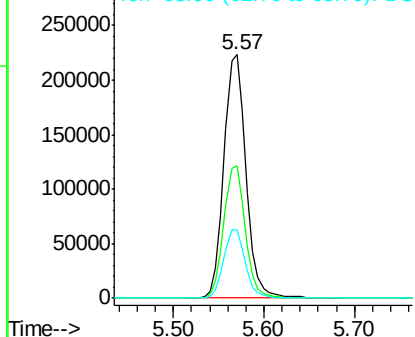

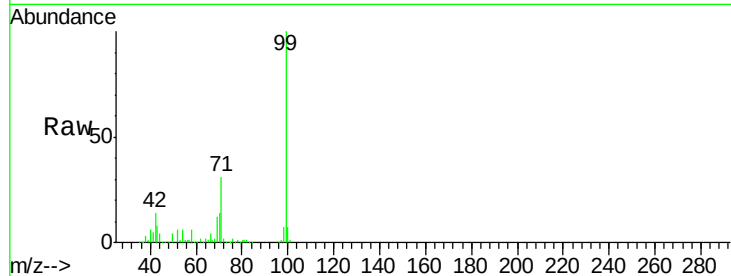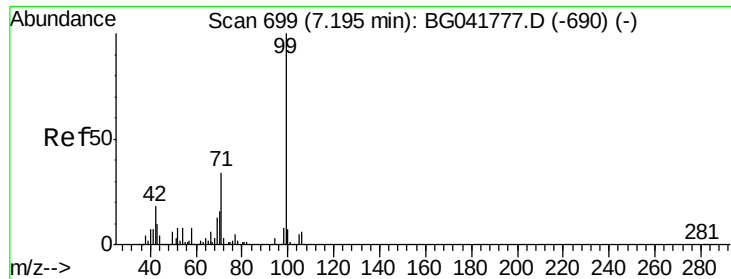

#7

Phenol-d6

Concen: 108.222 ng

RT: 7.17 min Scan# 695

Delta R.T. -0.02 min

Lab File: BG042275.D

Acq: 17 Aug 2019 1:01

Instrument :

BNA_G

ClientSampleId :

REACTOR-4-B-(0-3.4)





Tot Ion: 99 Resp: 444536

Ion Ratio Lower Upper

99 100

42 14.2 17.6 26.4#

71 31.2 27.8 41.6

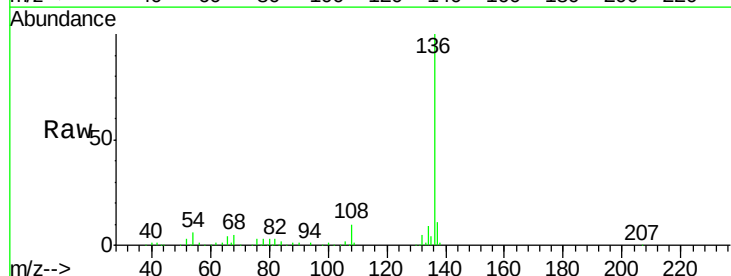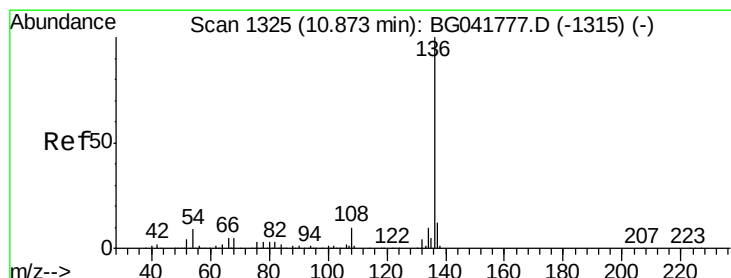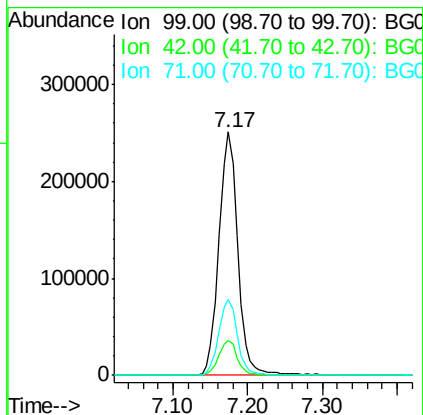

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.83 min Scan# 1318

Delta R.T. -0.04 min

Lab File: BG042275.D

Acq: 17 Aug 2019 1:01

Tgt Ion: 136 Resp: 219454


Ion Ratio Lower Upper


136 100

137 10.8 9.2 13.8

54 6.4 8.7 13.1#

68 4.8 5.5 8.3#




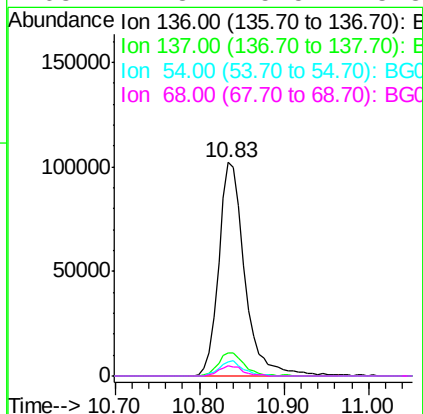




#23
Nitrobenzene-d5
Concen: 102.065 ng
RT: 9.18 min Scan# 1037
Delta R.T. -0.03 min
Lab File: BG042275.D
Acq: 17 Aug 2019 1:01




Instrument :
BNA_G
ClientSampleId :
REACTOR-4-B-(0-3.4)


Tot Ion: 82 Resp: 325484
Ion Ratio Lower Upper
82 100
128 50.7 35.1 52.7
54 45.6 48.7 73.1#

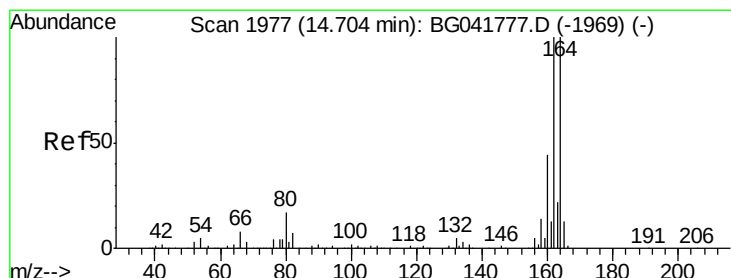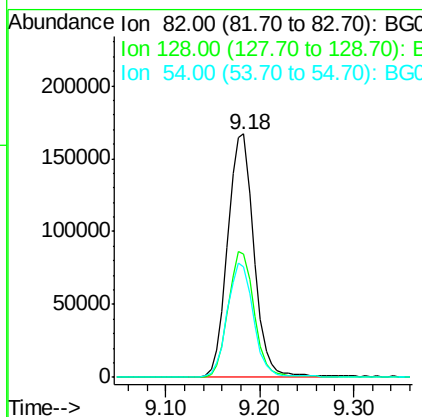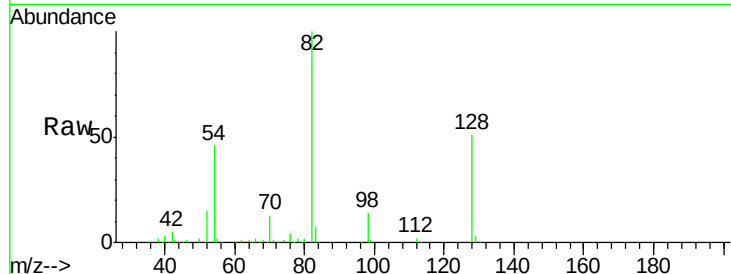

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.67 min Scan# 1971
Delta R.T. -0.03 min
Lab File: BG042275.D
Acq: 17 Aug 2019 1:01

Tgt Ion:164 Resp: 161652
Ion Ratio Lower Upper
164 100
162 100.0 79.6 119.4
160 43.9 35.4 53.0

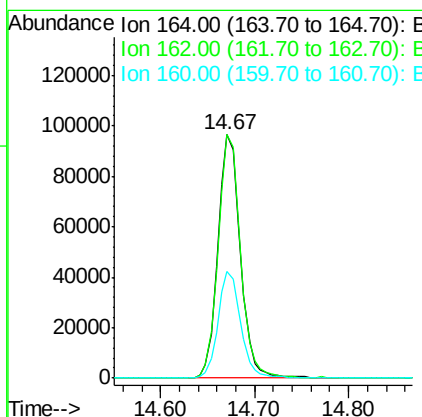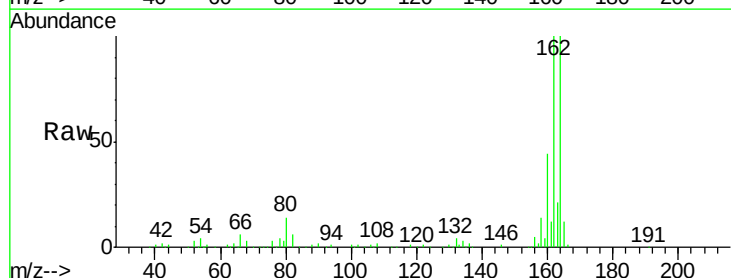

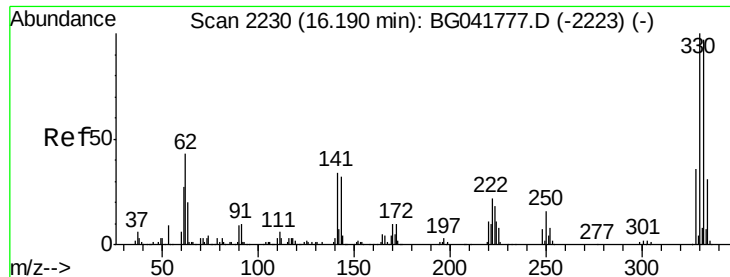

#42

2,4,6-Tribromophenol

Concen: 188.695 ng

RT: 16.16 min Scan# 2225

Delta R.T. -0.03 min

Lab File: BG042275.D

Acq: 17 Aug 2019 1:01

Instrument :

BNA_G

ClientSampleId :

REACTOR-4-B-(0-3.4)


Tot Ion:330 Resp: 346471

Ion Ratio Lower Upper

330 100

332 96.4 77.4 116.0




141 28.6 31.9 47.9#

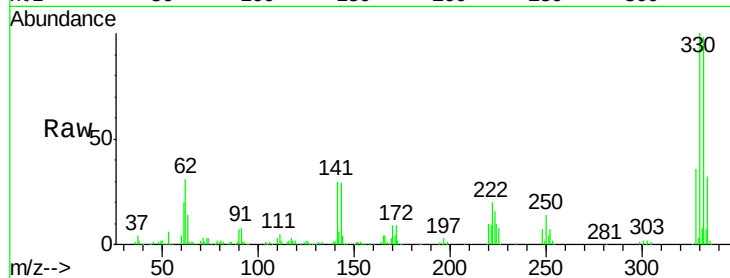

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

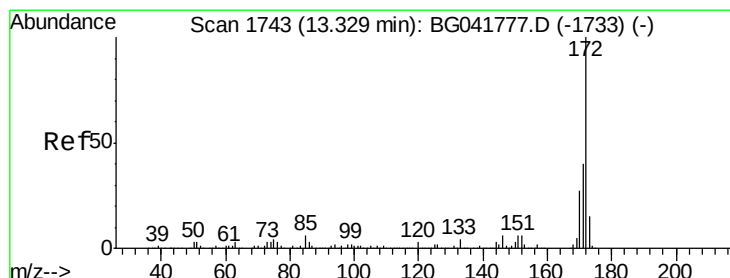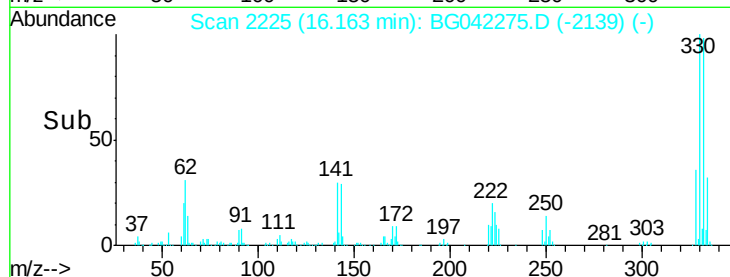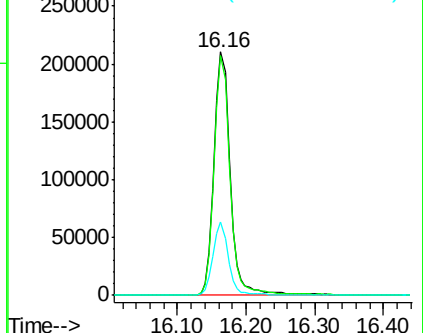

#45

2-Fluorobiphenyl

Concen: 109.980 ng

RT: 13.29 min Scan# 1736

Delta R.T. -0.04 min

Lab File: BG042275.D

Acq: 17 Aug 2019 1:01


Tgt Ion:172 Resp: 1008013

Ion Ratio Lower Upper

172 100

171 38.4 35.0 52.4



170 25.1 23.5 35.3

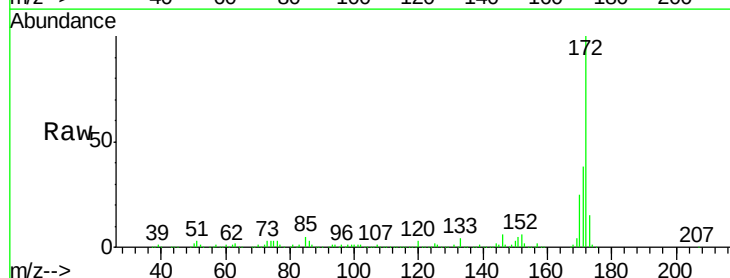


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



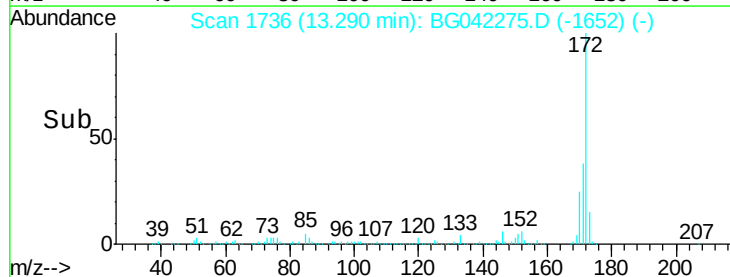
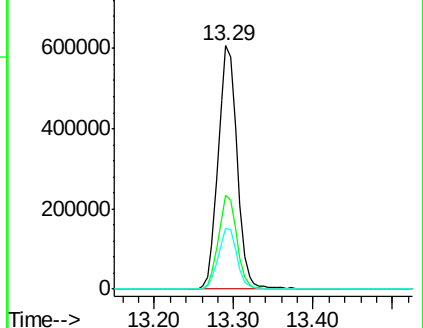


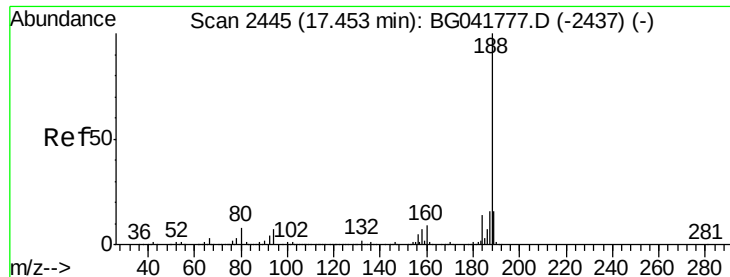

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.43 min Scan# 2440
Delta R.T. -0.03 min
Lab File: BG042275.D
Acq: 17 Aug 2019 1:01




Instrument :
BNA_G
ClientSampleId :
REACTOR-4-B-(0-3.4)


Tot Ion:188 Resp: 397381
Ion Ratio Lower Upper
188 100
94 6.3 6.9 10.3#
80 6.9 8.0 12.0#

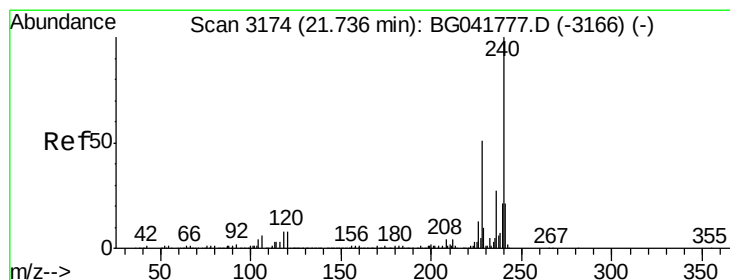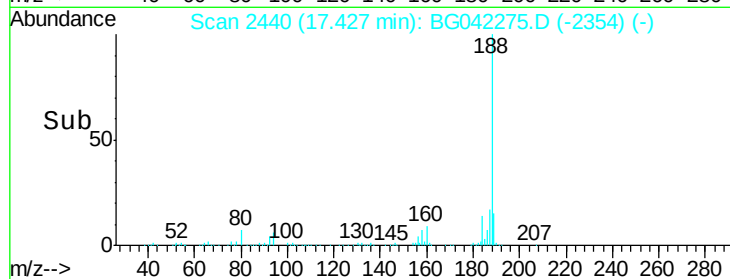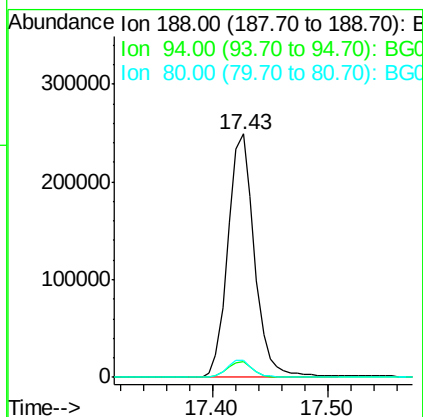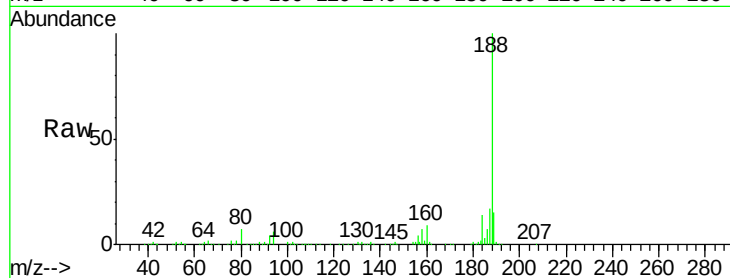

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.70 min Scan# 3168
Delta R.T. -0.03 min
Lab File: BG042275.D
Acq: 17 Aug 2019 1:01

Tgt Ion:240 Resp: 465900
Ion Ratio Lower Upper
240 100
120 7.7 8.0 12.0#
236 26.1 22.6 33.8

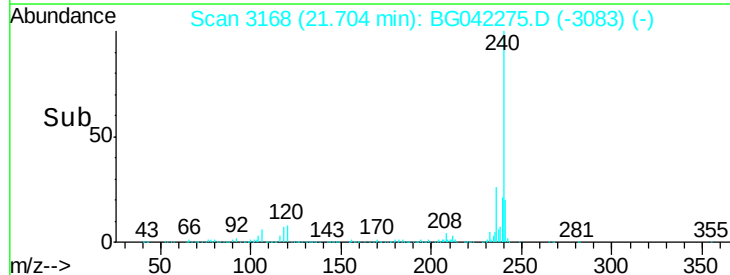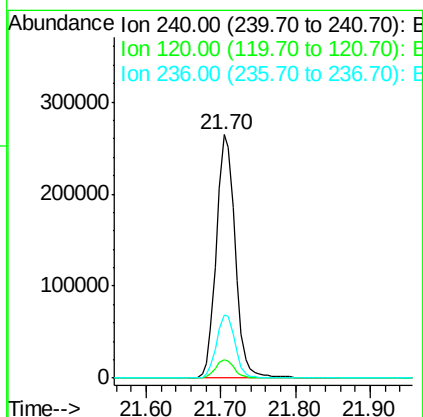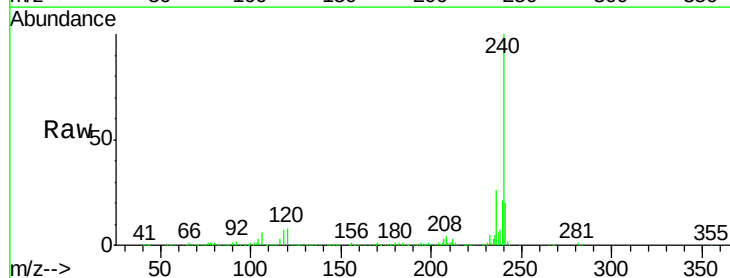



#79

Terphenyl-d14

Concen: 96.991 ng

RT: 20.04 min Scan# 2885

Delta R.T. -0.03 min

Lab File: BG042275.D

Acq: 17 Aug 2019 1:01

Instrument :

BNA_G

ClientSampleId :

REACTOR-4-B-(0-3.4)


Tot Ion:244 Resp: 1974781

Ion Ratio Lower Upper

244 100

212 8.7 9.7 14.5#




122 10.1 12.5 18.7#

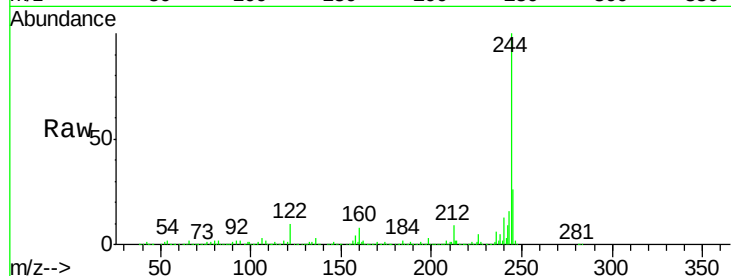

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

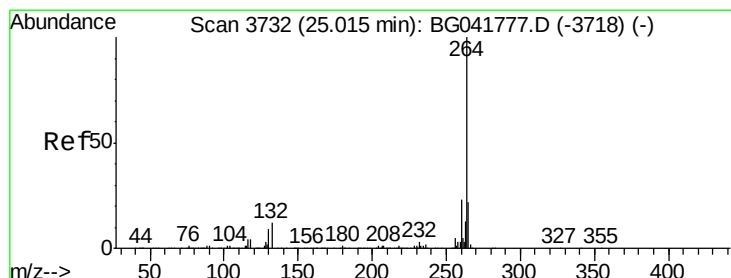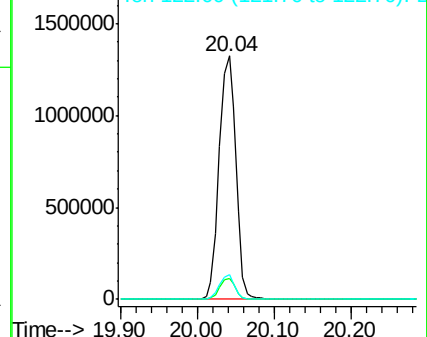

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.96 min Scan# 3723

Delta R.T. -0.05 min

Lab File: BG042275.D

Acq: 17 Aug 2019 1:01


Tgt Ion:264 Resp: 545466

Ion Ratio Lower Upper

264 100

260 23.6 19.5 29.3

265 21.8 18.0 27.0

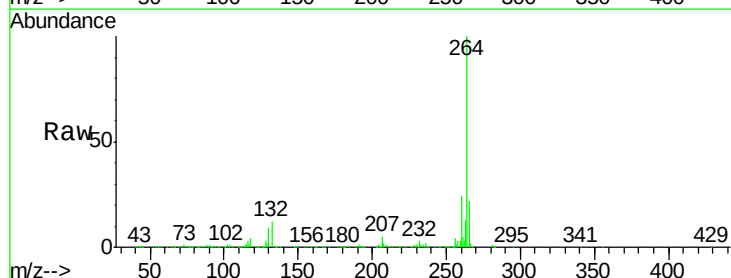

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

