


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081719\
 Data File : BG042298.D
 Acq On : 17 Aug 2019 22:30
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG072719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 19 06:42:36 2019

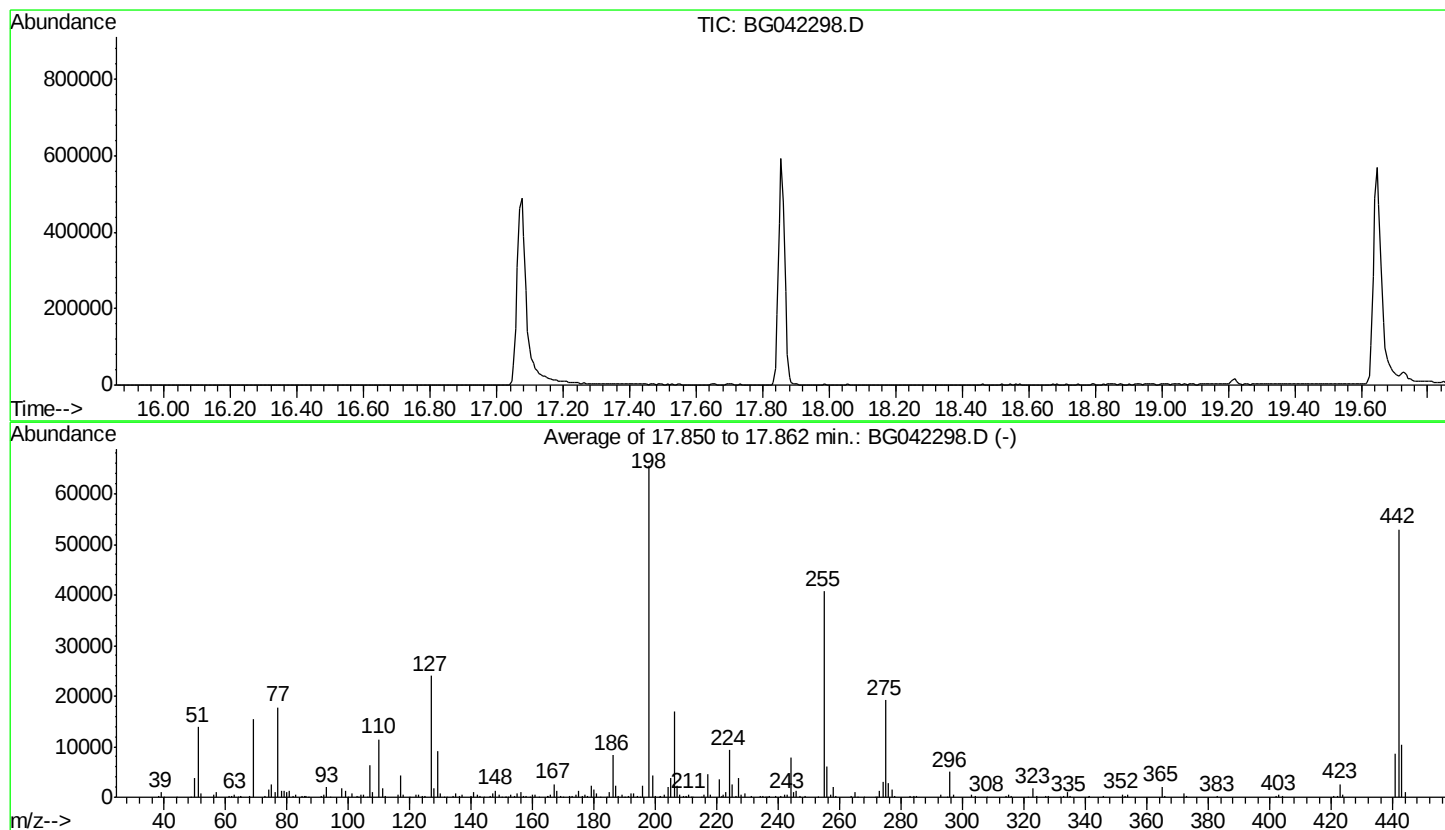

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.2	13877	PASS
68	69	0.00	2	1.9	297	PASS
69	198	0.00	100	23.6	15454	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	36.5	23946	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	65584	PASS
199	198	5	9	6.7	4418	PASS
275	198	10	60	29.3	19235	PASS
365	198	1	100	3.3	2136	PASS
441	198	0.01	100	13.0	8556	PASS
442	198	50	100	80.8	53000	PASS
443	442	15	24	19.4	10298	PASS