

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081722\
 Data File : BG054642.D
 Acq On : 17 Aug 2022 16:09
 Operator : CG/JU
 Sample : SSTD01036
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD010436

Quant Time: Aug 18 02:22:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 18 02:20:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.166	152	36110	20.000	ng/u1	0.00
20) Naphthalene-d8	10.992	136	152818	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.800	164	99163	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.543	188	218606	20.000	ng/u1	0.00
79) Chrysene-d12	21.844	240	213207	20.000	ng/u1	0.00
88) Perylene-d12	25.228	264	216697	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.513	96	3803	5.011	ng/uL	0.00
4) Pyridine-d5	3.942	84	26659	12.915	ng/u1	0.00
7) Phenol-d5	7.297	99	30505	11.792	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.479	67	20571	13.182	ng/u1	0.00
11) 2-Chlorophenol-d4	7.690	132	21893	10.613	ng/u1	0.00
15) 4-Methylphenol-d8	8.859	113	22917	10.390	ng/u1	0.00
21) Nitrobenzene-d5	9.335	128	9034	7.964	ng/u1	0.00
24) 2-Nitrophenol-d4	10.064	143	7603	6.308	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.599	165	22628	8.486	ng/u1	0.00
31) 4-Chloroaniline-d4	11.121	131	33055	9.813	ng/u1	0.00
46) Dimethylphthalate-d6	14.194	166	69395	8.896	ng/u1	0.00
49) Acenaphthylene-d8	14.494	160	84474	9.958	ng/u1	0.00
54) 4-Nitrophenol-d4	14.964	143	8562	8.016	ng/u1	0.00
60) Fluorene-d10	15.787	176	63366	9.043	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.892	200	5480	4.595	ng/u1	0.00
73) Anthracene-d10	17.643	188	98951	10.023	ng/u1	0.00
81) Pyrene-d10	19.923	212	111872	10.064	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.993	264	105484	9.644	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.554	88	4508	5.443	ng/uL	89
5) Pyridine	3.959	79	27406	12.802	ng/u1	94
6) Benzaldehyde	7.297	77	16141	12.253	ng/u1	100
8) Phenol	7.326	94	31218	11.565	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.579	93	26150	12.789	ng/u1	94
12) 2-Chlorophenol	7.720	128	23879	11.337	ng/u1	98
13) 2-Methylphenol	8.595	108	23347	11.142	ng/u1	93
14) 2,2'-oxybis(1-Chloropr...	8.695	45	43306	14.259	ng/u1	97
16) Acetophenone	8.989	105	38983	11.428	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.971	70	20823	11.974	ng/u1	99
18) 4-Methylphenol	8.924	108	24687	11.013	ng/u1	98
19) Hexachloroethane	9.265	117	9888	11.079	ng/u1	92
22) Nitrobenzene	9.376	77	24848	9.197	ng/u1	97
23) Isophorone	9.899	82	54325	10.371	ng/u1	99
25) 2-Nitrophenol	10.093	139	9023	7.140	ng/u1	94
26) 2,4-Dimethylphenol	10.140	107	27613	10.006	ng/u1	97
27) Bis(2-Chloroethoxy)met...	10.387	93	34578	11.725	ng/u1	96
29) 2,4-Dichlorophenol	10.628	162	22358	8.385	ng/u1	98
30) Naphthalene	11.045	128	82316	10.859	ng/u1	99
32) 4-Chloroaniline	11.145	127	34619	10.364	ng/u1	93
33) Hexachlorobutadiene	11.321	225	16441	6.312	ng/u1	99
34) Caprolactam	11.897	113	6392	8.033	ng/u1	89
35) 4-Chloro-3-methylphenol	12.244	107	23285	9.080	ng/u1	97
36) 2-Methylnaphthalene	12.637	142	55617	9.918	ng/u1	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081722\
 Data File : BG054642.D
 Acq On : 17 Aug 2022 16:09
 Operator : CG/JU
 Sample : SSTD01036
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD010436

Quant Time: Aug 18 02:22:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 18 02:20:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.855	142	55200	9.870	ng/ul	95
39) 1,2,4,5-Tetrachloroben...	12.996	216	30942	7.677	ng/ul	99
40) Hexachlorocyclopentadiene	12.978	237	17837	7.891	ng/ul	98
41) 2,4,6-Trichlorophenol	13.231	196	16952	8.103	ng/ul	96
42) 2,4,5-Trichlorophenol	13.301	196	18957	8.016	ng/ul	99
43) 1,1'-Biphenyl	13.636	154	74906	10.899	ng/ul	98
44) 2-Chloronaphthalene	13.683	162	56508	9.901	ng/ul	98
45) 2-Nitroaniline	13.877	65	10907	7.596	ng/ul	95
47) Dimethylphthalate	14.241	163	70876	9.453	ng/ul	99
48) 2,6-Dinitrotoluene	14.365	165	9241	6.128	ng/ul	98
50) Acenaphthylene	14.523	152	94425	10.841	ng/ul	98
51) 3-Nitroaniline	14.694	138	9100	7.434	ng/ul	94
52) Acenaphthene	14.864	153	61865	10.636	ng/ul	98
53) 2,4-Dinitrophenol	14.894	184	3973	5.687	ng/ul	94
55) 4-Nitrophenol	14.976	109	7580	7.239	ng/ul	97
56) Dibenzofuran	15.193	168	86685	9.740	ng/ul	98
57) 2,4-Dinitrotoluene	15.146	165	12783	5.844	ng/ul	100
58) 2,3,4,6-Tetrachlorophenol	15.411	232	14360	6.988	ng/ul	99
59) Diethylphthalate	15.604	149	69053	9.393	ng/ul	99
61) Fluorene	15.845	166	70773	9.764	ng/ul	95
62) 4-Chlorophenyl-phenyle...	15.834	204	35792	7.766	ng/ul	99
63) 4-Nitroaniline	15.845	138	8547	7.261	ng/ul	90
66) 4,6-Dinitro-2-methylph...	15.904	198	5537	4.837	ng/ul	95
67) N-Nitrosodiphenylamine	16.045	169	61120	11.436	ng/ul	96
68) 4-Bromophenyl-phenylether	16.727	248	22983	8.464	ng/ul	98
69) Hexachlorobenzene	16.838	284	26441	8.308	ng/ul	98
70) Atrazine	16.985	200	22395	8.531	ng/ul	96
71) Pentachlorophenol	17.185	266	11774	8.728	ng/ul	97
72) Phenanthrene	17.584	178	113472	10.477	ng/ul	99
74) Anthracene	17.679	178	115164	10.551	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.601	216	32454	8.716	ng/uL	97
76) Pentachlorobenzene	15.111	250	31367	9.160	ng/uL	98
77) Carbazole	17.943	167	101201	11.246	ng/ul	99
78) Di-n-butylphthalate	18.501	149	114609	11.186	ng/ul	99
80) Fluoranthene	19.588	202	138193	11.136	ng/ul	100
82) Pyrene	19.952	202	142371	11.539	ng/ul	98
83) Butylbenzylphthalate	20.840	149	43355	11.660	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.733	252	46059	10.439	ng/ul	96
85) Benzo(a)anthracene	21.821	228	136560	10.391	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.727	149	67758	12.471	ng/ul	100
87) Chrysene	21.891	228	131311	10.415	ng/ul	99
89) Di-n-octyl phthalate	23.008	149	109808	11.799	ng/ul	100
90) Benzo(b)fluoranthene	24.142	252	137519	10.277	ng/ul	98
91) Benzo(k)fluoranthene	24.218	252	129287	10.091	ng/ul	97
93) Benzo(a)pyrene	25.070	252	134724	10.452	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	29.118	276	158329	10.210	ng/ul	99
95) Dibenzo(a,h)anthracene	29.194	278	133471	10.227	ng/ul	98
96) Benzo(g,h,i)perylene	30.323	276	130353	9.956	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :

BNA G

ClientSampleId :

SSTD010436


Quant Time: Aug 18 02:22:42 2022


Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081722.M

Quant Title : SVOA CALIBRATION

QLast Update : Thu Aug 18 02:20:33 2022


Response via : Initial Calibration








#2
1,4-Dioxane
Concen: 5.443 ng/uL
RT: 3.554 min Scan# 41
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Instrument :
BNA_G
ClientSampleId :
SSTD010436







Tgt Ion: 88	Resp: 4508
Ion Ratio	Lower Upper
88	100
43	36.6 28.3 42.5
58	92.5 63.4 95.2



#5
Pyridine
Concen: 12.802 ng/uL
RT: 3.959 min Scan# 114
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion: 79	Resp: 27406
Ion Ratio	Lower Upper
79	100
52	85.4 74.2 111.2
51	39.3 31.9 47.9


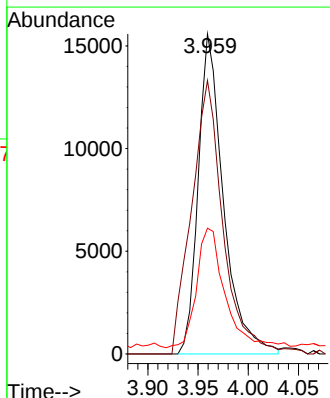






#6
Benzaldehyde
Concen: 12.253 ng/ul
RT: 7.297 min Scan# 682
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion: 77 Resp: 16141
Ion Ratio Lower Upper
77 100
105 91.5 73.6 110.4
106 89.5 71.5 107.3



#8
Phenol
Concen: 11.565 ng/ul
RT: 7.326 min Scan# 687
Delta R.T. -0.004 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion: 94 Resp: 31218
Ion Ratio Lower Upper
94 100
65 30.3 24.0 36.0
66 35.9 29.0 43.6









#10
 Bis(2-Chloroethyl)ether
 Concen: 12.789 ng/ul
 RT: 7.579 min Scan# 710
 Delta R.T. 0.002 min
 Lab File: BG054642.D
 Acq: 17 Aug 2022 16:09




Instrument :
 BNA_G
 ClientSampleId :
 SSTD010436


Tgt Ion:	93	Resp:	26150
Ion	Ratio	Lower	Upper
93	100		
63	86.3	63.2	94.8
95	33.0	25.5	38.3



#12
 2-Chlorophenol
 Concen: 11.337 ng/ul
 RT: 7.720 min Scan# 754
 Delta R.T. -0.004 min
 Lab File: BG054642.D
 Acq: 17 Aug 2022 16:09

Tgt Ion:	128	Resp:	23879
Ion	Ratio	Lower	Upper
128	100		
64	50.1	41.4	62.0
130	33.8	26.0	39.0









#13
2-Methylphenol
Concen: 11.142 ng/ul
RT: 8.595 min Scan# 90
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion:108 Resp: 23347
Ion Ratio Lower Upper
108 100
107 95.6 71.4 107.2

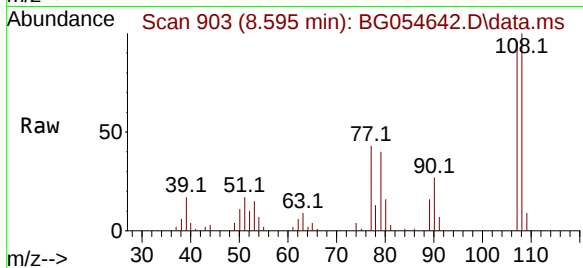

#14
2,2'-oxybis(1-Chloropropane)
Concen: 14.259 ng/ul
RT: 8.695 min Scan# 920
Delta R.T. 0.007 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion: 45 Resp: 43306
Ion Ratio Lower Upper
45 100
77 11.0 9.9 14.9
79 9.3 6.6 9.8




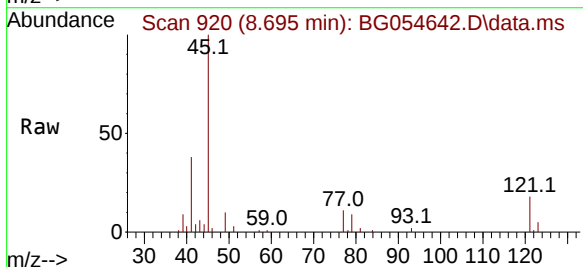




#16
Acetophenone
Concen: 11.428 ng/ul
RT: 8.989 min Scan# 91
Delta R.T. -0.004 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion:105 Resp: 38983
Ion Ratio Lower Upper
105 100
77 80.1 63.0 94.6
51 31.0 23.8 35.6



#17
N-Nitroso-di-n-propylamine
Concen: 11.974 ng/ul
RT: 8.971 min Scan# 967
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion: 70 Resp: 20823
Ion Ratio Lower Upper
70 100
42 60.9 49.6 74.4
101 7.7 6.6 10.0
130 19.0 15.7 23.5









#18
4-Methylphenol
Concen: 11.013 ng/ul
RT: 8.924 min Scan# 91
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion:108 Resp: 24687
Ion Ratio Lower Upper
108 100
107 118.1 92.5 138.7



#19
Hexachloroethane
Concen: 11.079 ng/ul
RT: 9.265 min Scan# 1017
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion:117 Resp: 9888
Ion Ratio Lower Upper
117 100
201 107.4 92.7 139.1
199 64.7 57.5 86.3



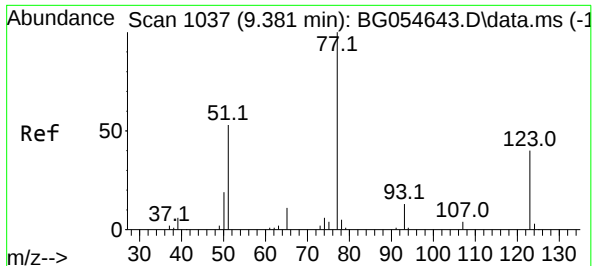

#22

Nitrobenzene

Concen: 9.197 ng/ul

RT: 9.376 min Scan# 1036

Delta R.T. -0.004 min

Lab File: BG054642.D

Acq: 17 Aug 2022 16:09

Instrument :

BNA_G

ClientSampleId :

SSTD010436





Tgt Ion: 77 Resp: 24848

Ion Ratio Lower Upper

77 100

123 41.7 31.6 47.4

65 12.6 9.0 13.6

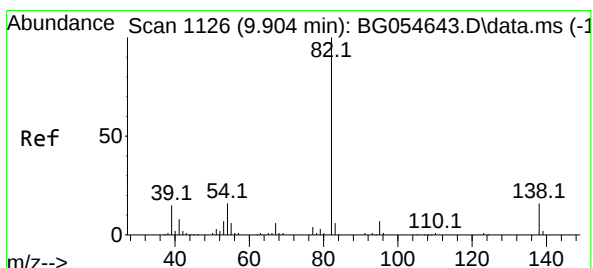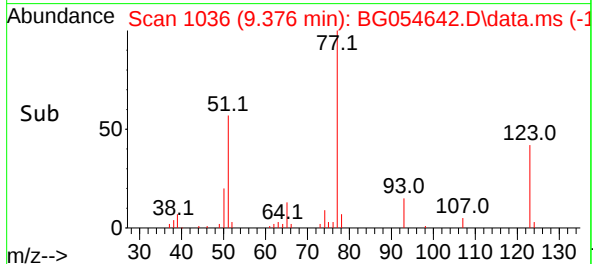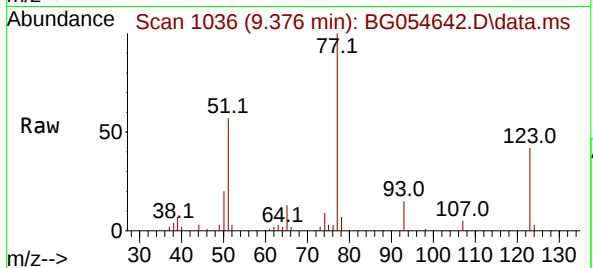

#23

Isophorone

Concen: 10.371 ng/ul

RT: 9.899 min Scan# 1125

Delta R.T. -0.004 min

Lab File: BG054642.D

Acq: 17 Aug 2022 16:09




Tgt Ion: 82 Resp: 54325


Ion Ratio Lower Upper

82 100

95 6.0 5.4 8.0

138 16.8 13.2 19.8


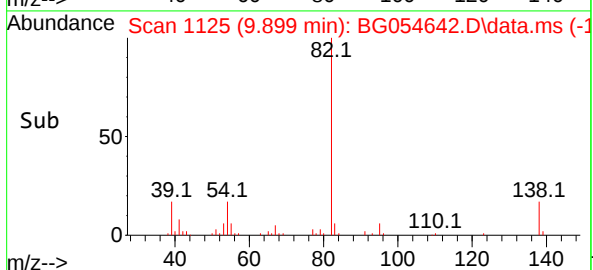

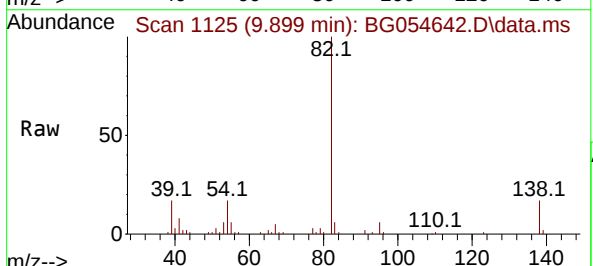




#25
2-Nitrophenol
Concen: 7.140 ng/ul
RT: 10.093 min Scan# 1158
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion:139 Resp: 9023
Ion Ratio Lower Upper
139 100
65 45.2 40.8 61.2
109 29.8 24.2 36.2

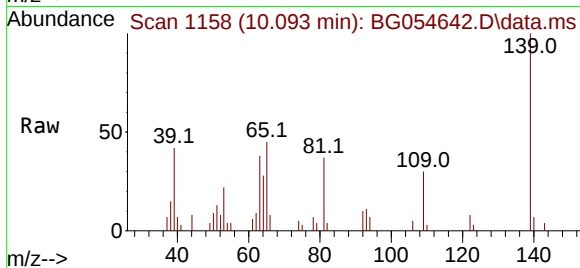

#26
2,4-Dimethylphenol
Concen: 10.006 ng/ul
RT: 10.140 min Scan# 1166
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion:107 Resp: 27613
Ion Ratio Lower Upper
107 100
121 50.6 42.1 63.1
122 85.7 70.6 105.8




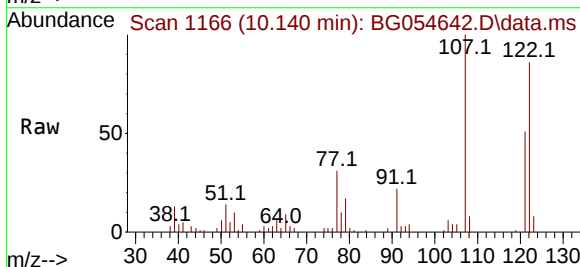




#27
 Bis(2-Chloroethoxy)methane
 Concen: 11.725 ng/ul
 RT: 10.387 min Scan# 1208
 Delta R.T. 0.002 min
 Lab File: BG054642.D
 Acq: 17 Aug 2022 16:09




Instrument :
 BNA_G
 ClientSampleId :
 SSTD010436


Tgt Ion: 93 Resp: 34578
 Ion Ratio Lower Upper
 93 100
 95 30.4 26.0 39.0
 123 10.1 9.0 13.6

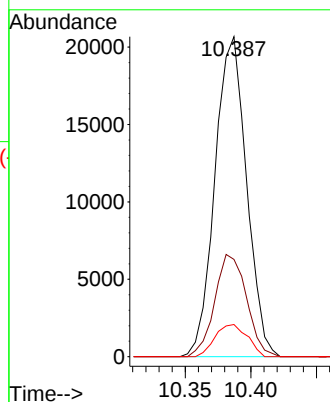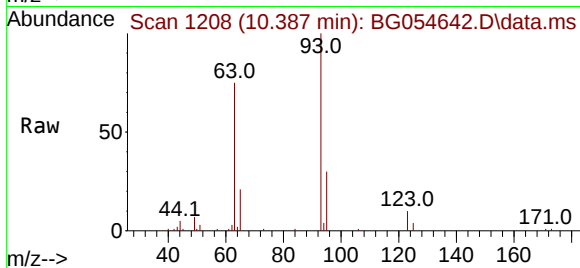

#29
 2,4-Dichlorophenol
 Concen: 8.385 ng/ul
 RT: 10.628 min Scan# 1249
 Delta R.T. 0.002 min
 Lab File: BG054642.D
 Acq: 17 Aug 2022 16:09

Tgt Ion:162 Resp: 22358
 Ion Ratio Lower Upper
 162 100
 164 68.0 55.7 83.5
 98 35.9 29.1 43.7




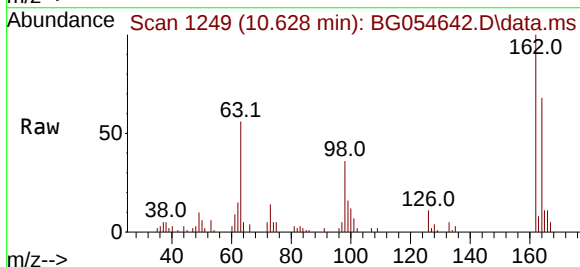




#30
Naphthalene
Concen: 10.859 ng/ul
RT: 11.045 min Scan# 11045
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion:128 Resp: 82316
Ion Ratio Lower Upper
128 100
129 11.2 8.9 13.3
127 13.7 10.7 16.1



#32
4-Chloroaniline
Concen: 10.364 ng/ul
RT: 11.145 min Scan# 1337
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion:127 Resp: 34619
Ion Ratio Lower Upper
127 100
129 34.1 24.4 36.6









#33
Hexachlorobutadiene
Concen: 6.312 ng/ul
RT: 11.321 min Scan# 11
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion:225 Resp: 16441
Ion Ratio Lower Upper
225 100
223 64.0 51.5 77.3
227 65.1 53.1 79.7

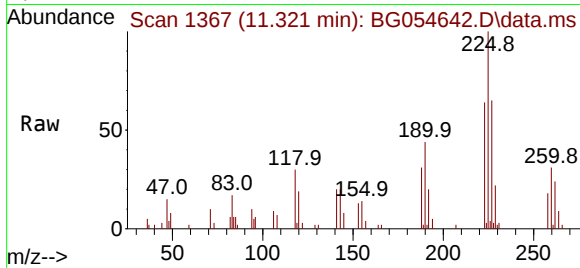

#34
Caprolactam
Concen: 8.033 ng/ul
RT: 11.897 min Scan# 1465
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion:113 Resp: 6392
Ion Ratio Lower Upper
113 100
55 200.7 171.4 257.0
56 126.8 116.2 174.4




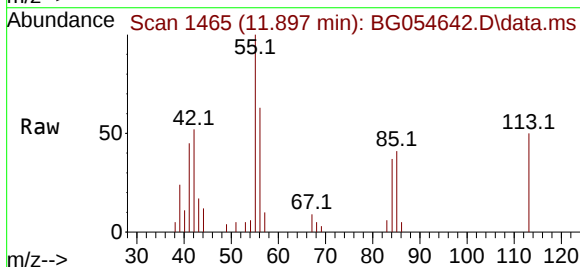




#35
4-Chloro-3-methylphenol
Concen: 9.080 ng/ul
RT: 12.244 min Scan# 1524
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion	Ratio	Lower	Upper
107	100		
144	24.7	21.2	31.8
142	77.3	63.4	95.0

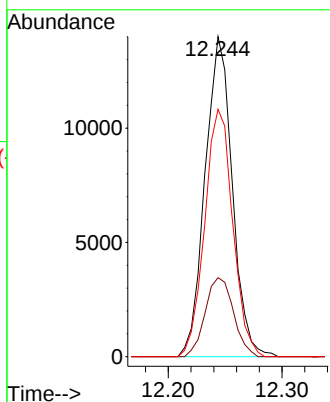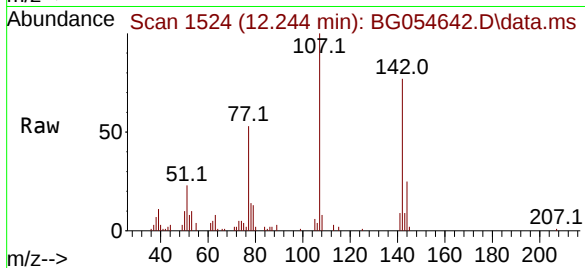

#36
2-Methylnaphthalene
Concen: 9.918 ng/ul
RT: 12.637 min Scan# 1591
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion	Ratio	Lower	Upper
142	100		
141	91.2	73.0	109.6



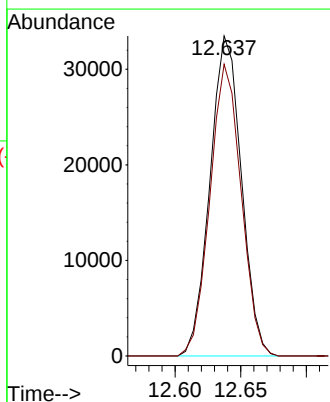
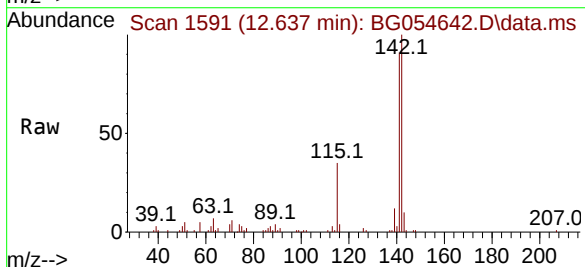


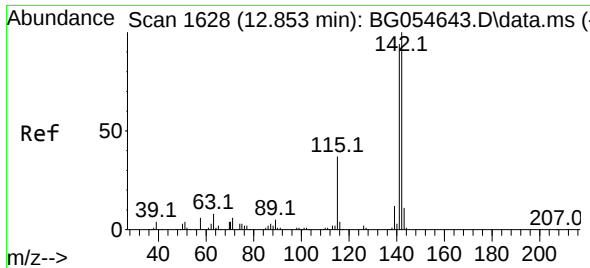

#37
1-Methylnaphthalene
Concen: 9.870 ng/ul
RT: 12.855 min Scan# 1
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion:142 Resp: 55200
Ion Ratio Lower Upper
142 100
141 98.7 75.0 112.4
116 4.4 3.3 4.9

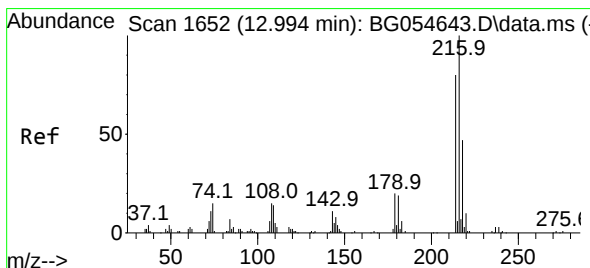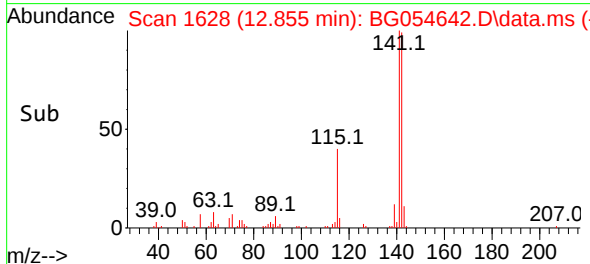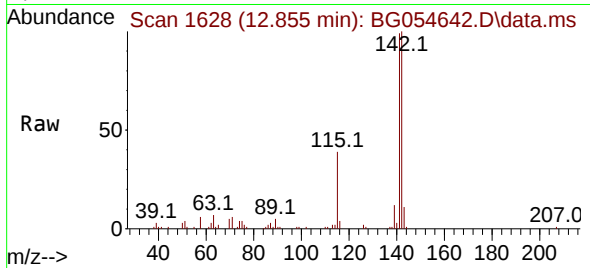

#39
1,2,4,5-Tetrachlorobenzene
Concen: 7.677 ng/ul
RT: 12.996 min Scan# 1652
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion:216 Resp: 30942
Ion Ratio Lower Upper
216 100
214 79.1 63.7 95.5
179 21.4 15.8 23.6
108 15.8 12.1 18.1


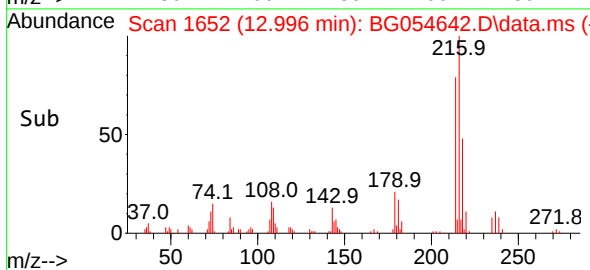

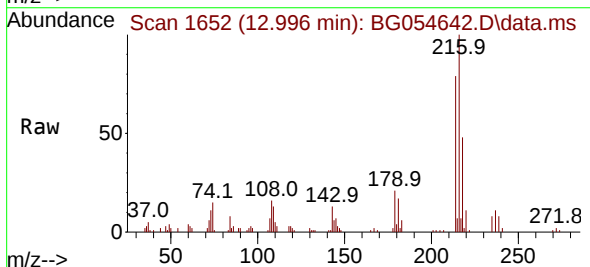




#40
Hexachlorocyclopentadiene
Concen: 7.891 ng/ul
RT: 12.978 min Scan# 1649
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion:237 Resp: 17837
Ion Ratio Lower Upper
237 100
235 62.5 50.9 76.3
272 11.5 11.3 16.9



#41
2,4,6-Trichlorophenol
Concen: 8.103 ng/ul
RT: 13.231 min Scan# 1692
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion:196 Resp: 16952
Ion Ratio Lower Upper
196 100
198 101.4 77.5 116.3
200 29.8 23.4 35.2









#42
2,4,5-Trichlorophenol
Concen: 8.016 ng/ul
RT: 13.301 min Scan# 1704
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion:196 Resp: 18957
Ion Ratio Lower Upper
196 100
198 98.8 78.2 117.2
200 31.9 25.4 38.0



#43
1,1'-Biphenyl
Concen: 10.899 ng/ul
RT: 13.636 min Scan# 1761
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion:154 Resp: 74906
Ion Ratio Lower Upper
154 100
153 41.0 33.8 50.6
76 14.0 11.0 16.6



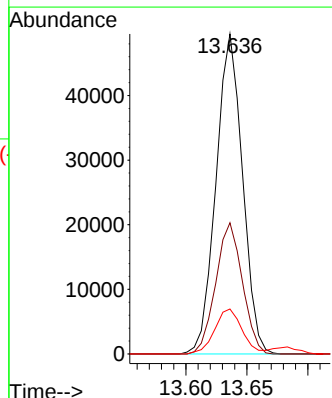





#44
2-Chloronaphthalene
Concen: 9.901 ng/ul
RT: 13.683 min Scan# 1769
Delta R.T. 0.007 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion:162 Resp: 56508
Ion Ratio Lower Upper
162 100
164 34.9 26.0 39.0
127 38.9 31.4 47.0



#45
2-Nitroaniline
Concen: 7.596 ng/ul
RT: 13.877 min Scan# 1802
Delta R.T. 0.007 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion: 65 Resp: 10907
Ion Ratio Lower Upper
65 100
92 65.6 55.3 82.9
138 104.2 78.8 118.2









#47
Dimethylphthalate
Concen: 9.453 ng/ul
RT: 14.241 min Scan# 1864
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion:163 Resp: 70876
Ion Ratio Lower Upper
163 100
194 4.0 3.0 4.6
164 10.4 8.7 13.1



#48
2,6-Dinitrotoluene
Concen: 6.128 ng/ul
RT: 14.365 min Scan# 1885
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion:165 Resp: 9241
Ion Ratio Lower Upper
165 100
89 59.4 48.7 73.1
121 22.9 18.2 27.2









#50
Acenaphthylene
Concen: 10.841 ng/ul
RT: 14.523 min Scan# 1912
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion:152 Resp: 94425
Ion Ratio Lower Upper
152 100
151 21.8 16.9 25.3
153 14.2 10.5 15.7

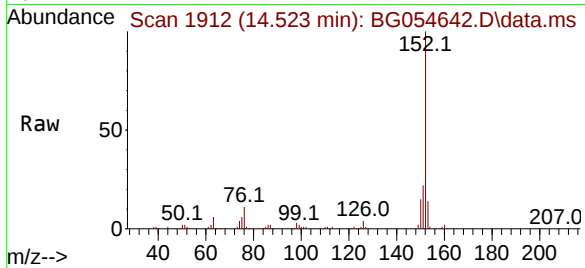

#51
3-Nitroaniline
Concen: 7.434 ng/ul
RT: 14.694 min Scan# 1941
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion:138 Resp: 9100
Ion Ratio Lower Upper
138 100
108 17.9 12.8 19.2
92 124.3 93.7 140.5




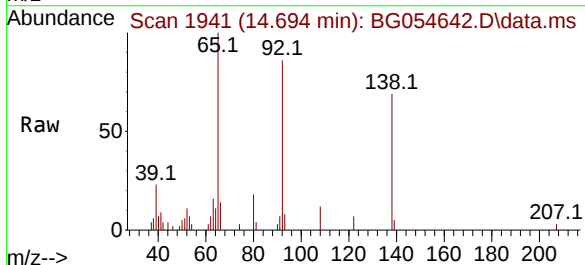




#52
Acenaphthene
Concen: 10.636 ng/ul
RT: 14.864 min Scan# 1969
Delta R.T. 0.007 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion:153 Resp: 61865
Ion Ratio Lower Upper
153 100
152 47.8 36.9 55.3
154 84.0 68.2 102.2

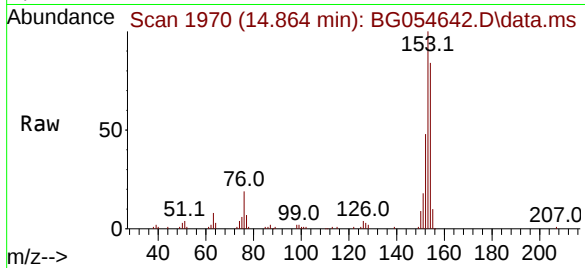

#53
2,4-Dinitrophenol
Concen: 5.687 ng/ul
RT: 14.894 min Scan# 1975
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion:184 Resp: 3973
Ion Ratio Lower Upper
184 100
63 52.9 42.0 63.0
154 52.3 48.9 73.3




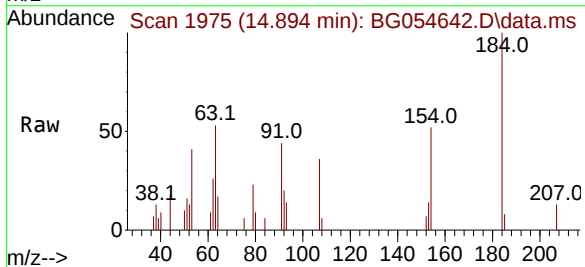




#55
4-Nitrophenol
Concen: 7.239 ng/ul
RT: 14.976 min Scan# 1989
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion:109 Resp: 7580
Ion Ratio Lower Upper
109 100
139 138.9 105.4 158.0
65 137.4 110.2 165.4

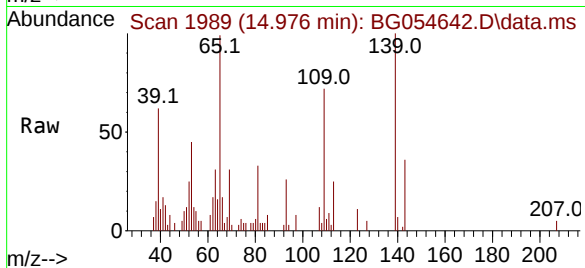

#56
Dibenzofuran
Concen: 9.740 ng/ul
RT: 15.193 min Scan# 2026
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion:168 Resp: 86685
Ion Ratio Lower Upper
168 100
139 37.9 29.4 44.2




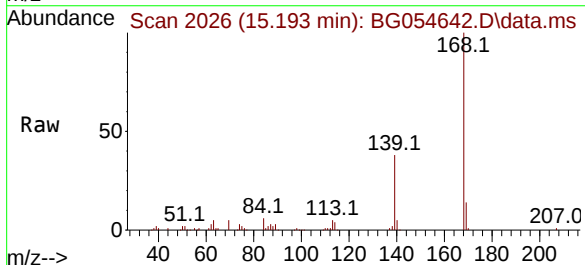




#57
2,4-Dinitrotoluene
Concen: 5.844 ng/ul
RT: 15.146 min Scan# 2018
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion:165 Resp: 12783
Ion Ratio Lower Upper
165 100
63 43.6 35.0 52.4
182 2.7 2.1 3.1

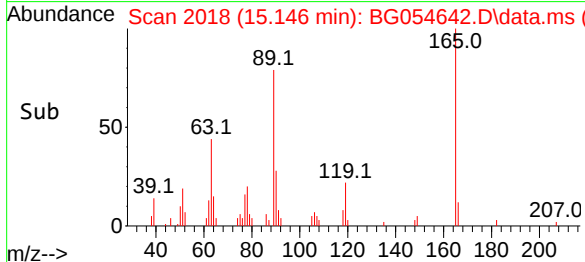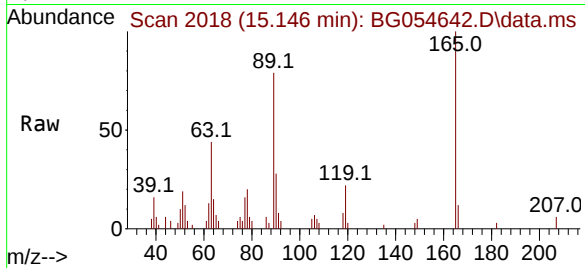

#58
2,3,4,6-Tetrachlorophenol
Concen: 6.988 ng/ul
RT: 15.411 min Scan# 2063
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion:232 Resp: 14360
Ion Ratio Lower Upper
232 100
131 43.1 33.8 50.8
130 2.3 2.0 3.0
166 30.8 24.4 36.6


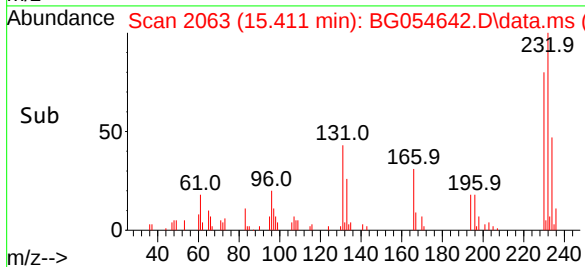
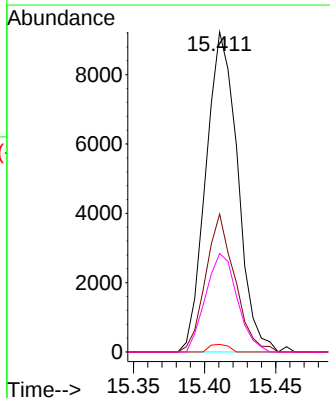
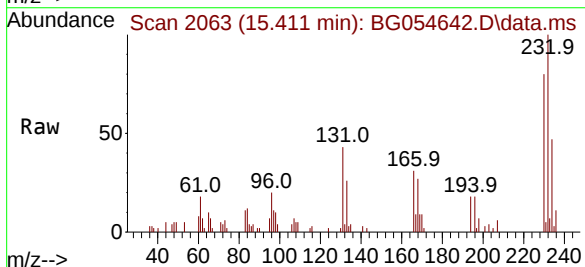




#59
Diethylphthalate
Concen: 9.393 ng/ul
RT: 15.604 min Scan# 2096
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion:149 Resp: 69053
Ion Ratio Lower Upper
149 100
177 22.5 18.4 27.6
150 13.0 9.8 14.8

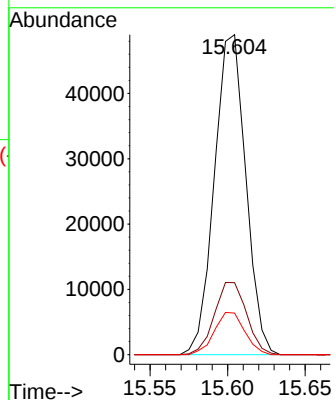

#61
Fluorene
Concen: 9.764 ng/ul
RT: 15.845 min Scan# 2137
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion:166 Resp: 70773
Ion Ratio Lower Upper
166 100
165 96.3 81.3 121.9
167 13.4 11.0 16.4



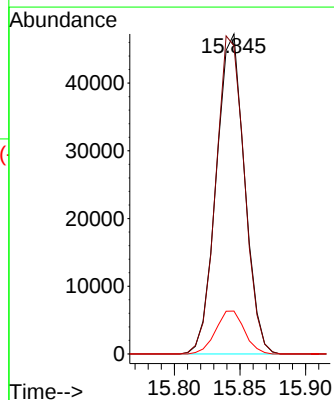





#62
4-Chlorophenyl-phenylether
Concen: 7.766 ng/ul
RT: 15.834 min Scan# 2135
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion:204 Resp: 35792
Ion Ratio Lower Upper
204 100
206 31.1 25.7 38.5
141 54.4 43.9 65.9

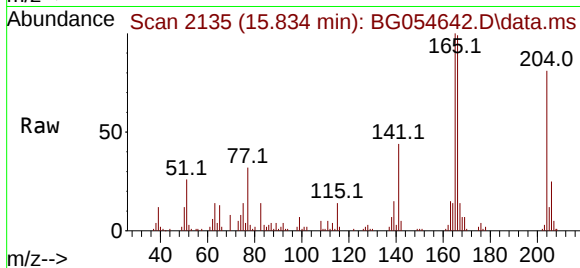

#63
4-Nitroaniline
Concen: 7.261 ng/ul
RT: 15.845 min Scan# 2137
Delta R.T. -0.004 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion:138 Resp: 8547
Ion Ratio Lower Upper
138 100
92 46.2 40.5 60.7
108 69.7 64.5 96.7




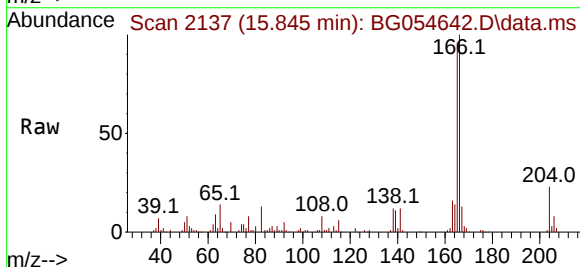




#66
 4,6-Dinitro-2-methylphenol
 Concen: 4.837 ng/ul
 RT: 15.904 min Scan# 2147
 Delta R.T. 0.002 min
 Lab File: BG054642.D
 Acq: 17 Aug 2022 16:09




Instrument :
 BNA_G
 ClientSampleId :
 SSTD010436


Tgt Ion:198 Resp: 5537
 Ion Ratio Lower Upper
 198 100
 182 5.2 4.0 6.0
 77 22.2 20.2 30.2



#67
 N-Nitrosodiphenylamine
 Concen: 11.436 ng/ul
 RT: 16.045 min Scan# 2171
 Delta R.T. 0.002 min
 Lab File: BG054642.D
 Acq: 17 Aug 2022 16:09

Tgt Ion:169 Resp: 61120
 Ion Ratio Lower Upper
 169 100
 168 69.6 53.8 80.8
 167 39.8 29.4 44.0









#68
4-Bromophenyl-phenylether
Concen: 8.464 ng/ul
RT: 16.727 min Scan# 21
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion:248 Resp: 22983
Ion Ratio Lower Upper
248 100
250 94.9 79.1 118.7
141 65.5 52.5 78.7

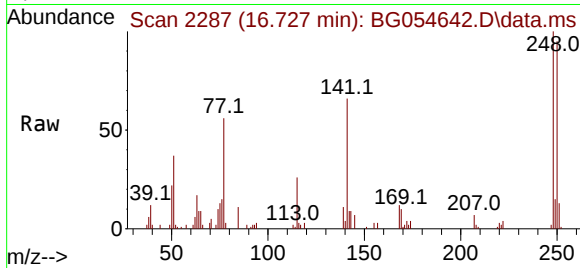

#69
Hexachlorobenzene
Concen: 8.308 ng/ul
RT: 16.838 min Scan# 2306
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion:284 Resp: 26441
Ion Ratio Lower Upper
284 100
142 31.5 23.7 35.5
249 30.0 24.2 36.2




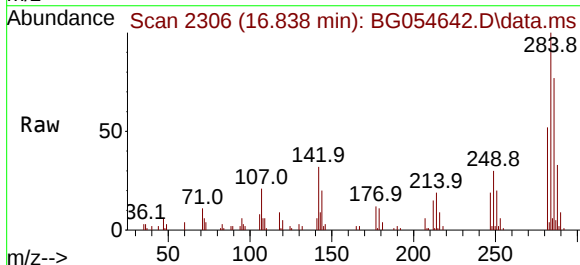




#70
 Atrazine
 Concen: 8.531 ng/ul
 RT: 16.985 min Scan# 21
 Delta R.T. 0.002 min
 Lab File: BG054642.D
 Acq: 17 Aug 2022 16:09




Instrument :
 BNA_G
 ClientSampleId :
 SST010436


Tgt Ion:200 Resp: 22395
 Ion Ratio Lower Upper
 200 100
 173 23.9 21.3 31.9
 215 45.7 38.8 58.2



#71
 Pentachlorophenol
 Concen: 8.728 ng/ul
 RT: 17.185 min Scan# 2365
 Delta R.T. 0.002 min
 Lab File: BG054642.D
 Acq: 17 Aug 2022 16:09

Tgt Ion:266 Resp: 11774
 Ion Ratio Lower Upper
 266 100
 264 64.8 53.8 80.8
 268 64.3 52.8 79.2





#72

Phenanthrene

Concen: 10.477 ng/u1

RT: 17.584 min Scan# 2433

Delta R.T. 0.002 min

Lab File: BG054642.D

Acq: 17 Aug 2022 16:09

Instrument :

BNA_G

ClientSampleId :

SSTD010436





Tgt Ion:178 Resp: 113472

Ion Ratio Lower Upper

178 100

179 16.3 12.8 19.2

176 20.3 15.6 23.4



#74

Anthracene

Concen: 10.551 ng/u1

RT: 17.679 min Scan# 2449

Delta R.T. 0.002 min

Lab File: BG054642.D

Acq: 17 Aug 2022 16:09




Tgt Ion:178 Resp: 115164


Ion Ratio Lower Upper

178 100

179 15.4 12.5 18.7

176 19.3 15.9 23.9









#75
1,2,3,4-Tetrachlorobenzene
Concen: 8.716 ng/uL
RT: 13.601 min Scan# 1755
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion:216 Resp: 32454
Ion Ratio Lower Upper
216 100
214 78.4 61.9 92.9
218 46.0 39.5 59.3



#76
Pentachlorobenzene
Concen: 9.160 ng/uL
RT: 15.111 min Scan# 2012
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion:250 Resp: 31367
Ion Ratio Lower Upper
250 100
248 62.1 49.1 73.7
252 65.8 50.6 76.0









#77
 Carbazole
 Concen: 11.246 ng/ul
 RT: 17.943 min Scan# 2494
 Delta R.T. 0.002 min
 Lab File: BG054642.D
 Acq: 17 Aug 2022 16:09




Instrument :
 BNA_G
 ClientSampleId :
 SSTD010436


Tgt Ion:167 Resp: 101201
 Ion Ratio Lower Upper
 167 100
 166 22.6 17.8 26.6
 139 12.5 9.9 14.9



#78
 Di-n-butylphthalate
 Concen: 11.186 ng/ul
 RT: 18.501 min Scan# 2589
 Delta R.T. 0.007 min
 Lab File: BG054642.D
 Acq: 17 Aug 2022 16:09

Tgt Ion:149 Resp: 114609
 Ion Ratio Lower Upper
 149 100
 150 10.0 7.7 11.5
 104 5.1 4.2 6.4









#80
Fluoranthene
Concen: 11.136 ng/ul
RT: 19.588 min Scan# 21
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion:202 Resp: 138193
Ion Ratio Lower Upper
202 100
101 10.0 8.0 12.0
100 8.7 6.7 10.1



#82
Pyrene
Concen: 11.539 ng/ul
RT: 19.952 min Scan# 2836
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion:202 Resp: 142371
Ion Ratio Lower Upper
202 100
101 11.9 10.1 15.1
100 11.2 8.4 12.6





#83

Butylbenzylphthalate

Concen: 11.660 ng/ul

RT: 20.840 min Scan# 2986

Delta R.T. 0.007 min

Lab File: BG054642.D

Acq: 17 Aug 2022 16:09

Instrument :

BNA_G

ClientSampleId :

SSTD010436





Tgt Ion:149 Resp: 43355

Ion Ratio Lower Upper

149 100

91 71.0 59.1 88.7

206 21.9 16.8 25.2

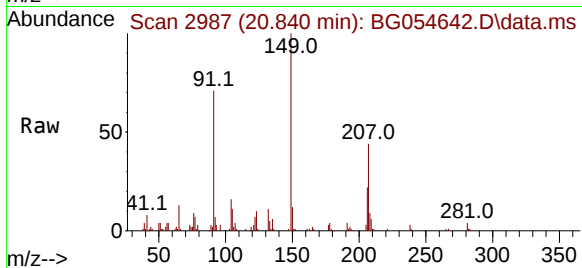

#84

3,3'-Dichlorobenzidine

Concen: 10.439 ng/ul

RT: 21.733 min Scan# 3139

Delta R.T. 0.007 min

Lab File: BG054642.D

Acq: 17 Aug 2022 16:09




Tgt Ion:252 Resp: 46059


Ion Ratio Lower Upper

252 100

254 64.2 49.1 73.7

126 9.4 8.3 12.5




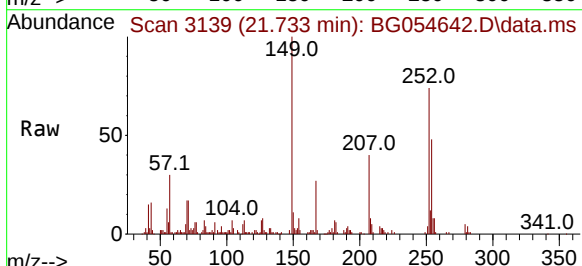




#85
Benzo(a)anthracene
Concen: 10.391 ng/ul
RT: 21.821 min Scan# 3154
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion:228 Resp: 136560
Ion Ratio Lower Upper
228 100
229 19.5 15.8 23.6
226 26.9 22.2 33.4

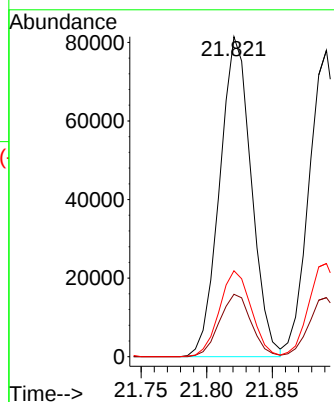

#86
Bis(2-ethylhexyl)phthalate
Concen: 12.471 ng/ul
RT: 21.727 min Scan# 3138
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion:149 Resp: 67758
Ion Ratio Lower Upper
149 100
167 27.0 21.5 32.3
279 3.8 3.4 5.0



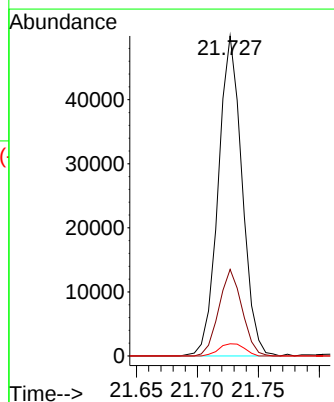



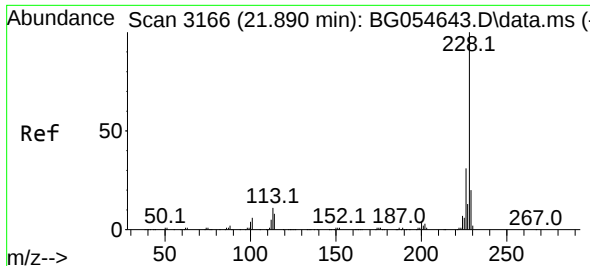

#87
Chrysene
Concen: 10.415 ng/ul
RT: 21.891 min Scan# 3166
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion:228 Resp: 131311
Ion Ratio Lower Upper
228 100
226 30.4 24.6 36.8
229 19.3 16.0 24.0

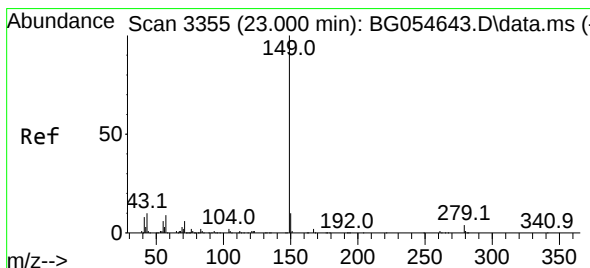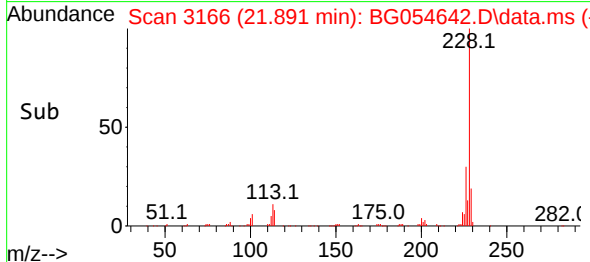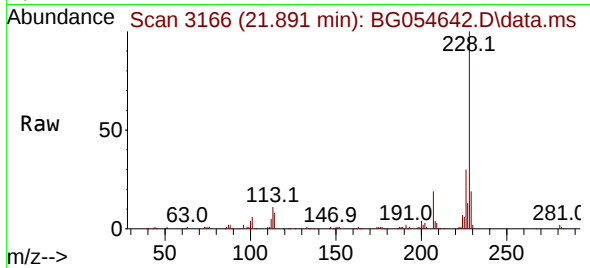

#89
Di-n-octyl phthalate
Concen: 11.799 ng/ul
RT: 23.008 min Scan# 3356
Delta R.T. 0.007 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion:149 Resp: 109808


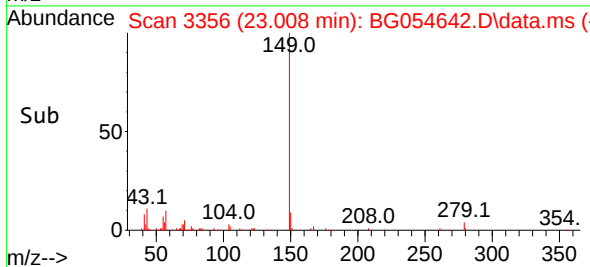

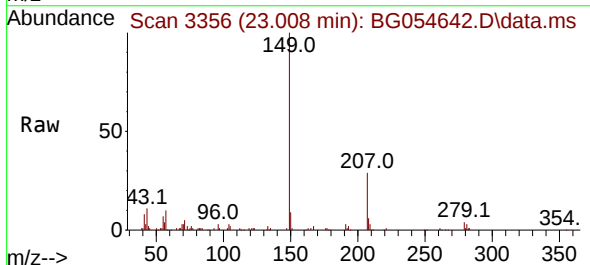




#90
Benzo(b)fluoranthene
Concen: 10.277 ng/ul
RT: 24.142 min Scan# 3549
Delta R.T. 0.002 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion:252 Resp: 137519
Ion Ratio Lower Upper
252 100
253 20.9 17.7 26.5
125 9.0 7.4 11.0

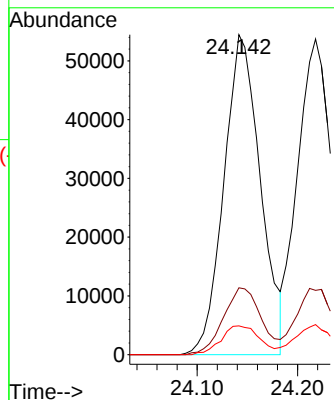

#91
Benzo(k)fluoranthene
Concen: 10.091 ng/ul
RT: 24.218 min Scan# 3562
Delta R.T. 0.007 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion:252 Resp: 129287
Ion Ratio Lower Upper
252 100
253 20.4 18.1 27.1
125 9.5 7.6 11.4



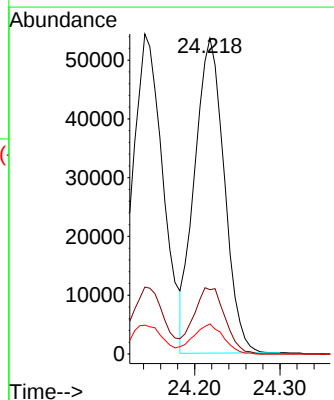





#93
Benzo(a)pyrene
Concen: 10.452 ng/ul
RT: 25.070 min Scan# 31
Delta R.T. 0.013 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09




Instrument :
BNA_G
ClientSampleId :
SSTD010436


Tgt Ion:252 Resp: 134724
Ion Ratio Lower Upper
252 100
253 20.7 17.0 25.4
125 9.5 9.0 13.6



#94
Indeno(1,2,3-cd)pyrene
Concen: 10.210 ng/ul
RT: 29.118 min Scan# 4396
Delta R.T. 0.013 min
Lab File: BG054642.D
Acq: 17 Aug 2022 16:09

Tgt Ion:276 Resp: 158329
Ion Ratio Lower Upper
276 100
138 17.6 14.5 21.7
277 23.2 18.3 27.5





#95

Dibenzo(a,h)anthracene

Concen: 10.227 ng/ul

RT: 29.194 min Scan# 4409

Delta R.T. 0.007 min

Lab File: BG054642.D

Acq: 17 Aug 2022 16:09

Instrument :

BNA_G

ClientSampleId :

SSTD010436





Tgt Ion:278 Resp: 133471

Ion Ratio Lower Upper

278 100

139 13.5 11.2 16.8

279 23.4 19.6 29.4



#96

Benzo(g,h,i)perylene

Concen: 9.956 ng/ul

RT: 30.323 min Scan# 4601

Delta R.T. 0.002 min

Lab File: BG054642.D

Acq: 17 Aug 2022 16:09

Tgt Ion:276 Resp: 130353

Ion Ratio Lower Upper

276 100

138 19.0 15.4 23.2

277 22.1 19.5 29.3

