


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081722\
 Data File : BG054640.D
 Acq On : 17 Aug 2022 14:47
 Operator : CG/JU
 Sample : DFTPP482
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP482

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 18 12:03:10 2022

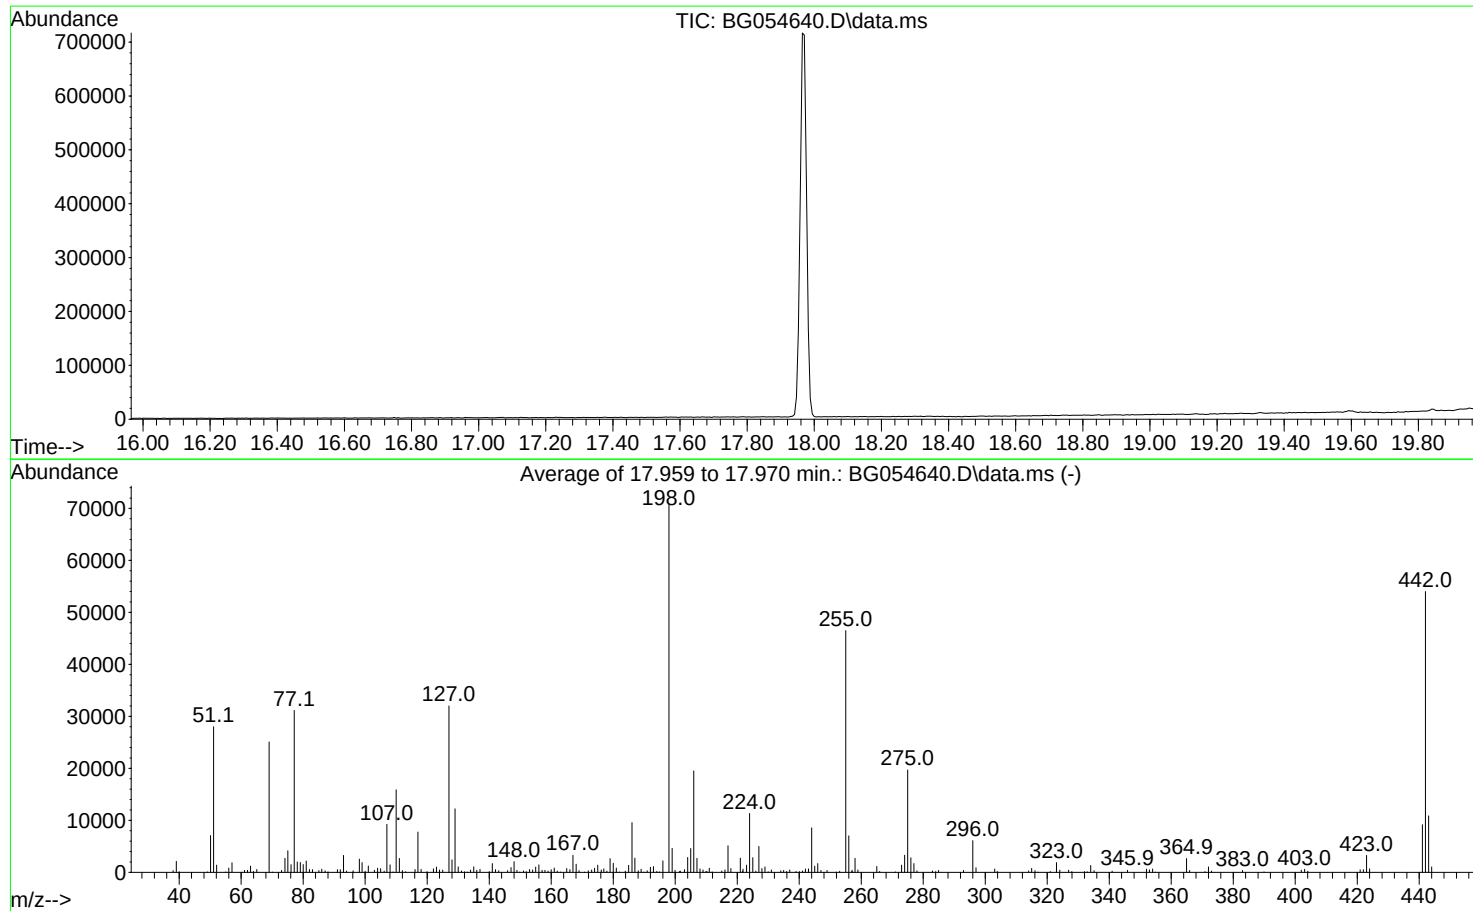

AutoFind: Scans 2548, 2549, 2550; Background Corrected with Scan 2542

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	27992	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.4	25080	PASS
70	69	0.00	2	0.2	59	PASS
127	198	10	80	45.2	31987	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	70771	PASS
199	198	5	9	6.5	4598	PASS
275	198	10	60	27.8	19691	PASS
365	198	1	100	3.7	2651	PASS
441	198	0.01	100	12.9	9155	PASS
442	442	50	100	100.0	54003	PASS
443	442	15	24	20.1	10854	PASS