


Data Path : Z:\HPCHEM1\BNA G\Data\BG081915\
Data File : BG018482.D
Acq On : 19 Aug 2015 20:13
Operator : UM/MA
Sample : C3302-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampled :
C0551

Quant Time: Aug 20 04:19:42 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 20 01:31:35 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

apatel
8/20/2015 8:35:58 AM

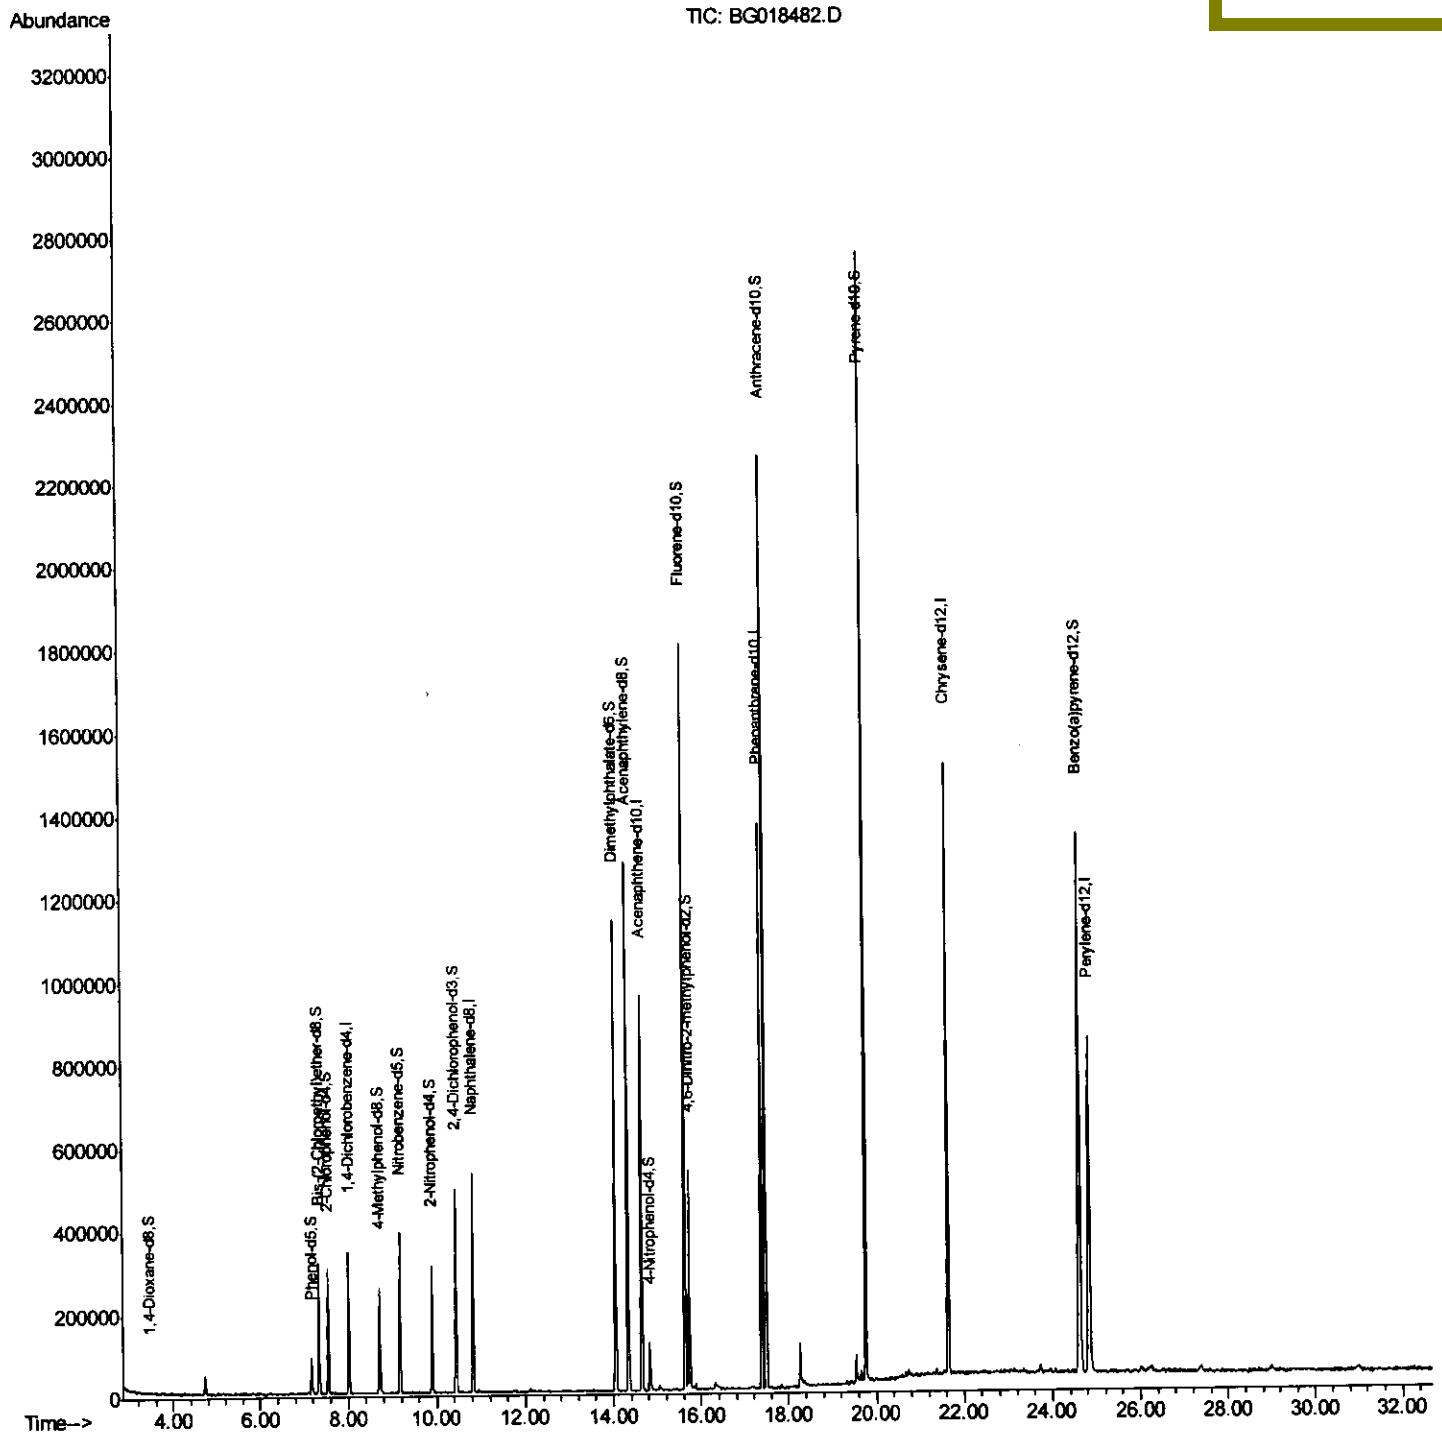

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA G\Data\BG081915\
 Data File : BG018482.D
 Acq On : 19 Aug 2015 20:13
 Operator : UM/MA
 Sample : G3302-13
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0551

Quant Time: Aug 20 01:32:43 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 20 01:31:35 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 8/20/2015 8:35:58 AM

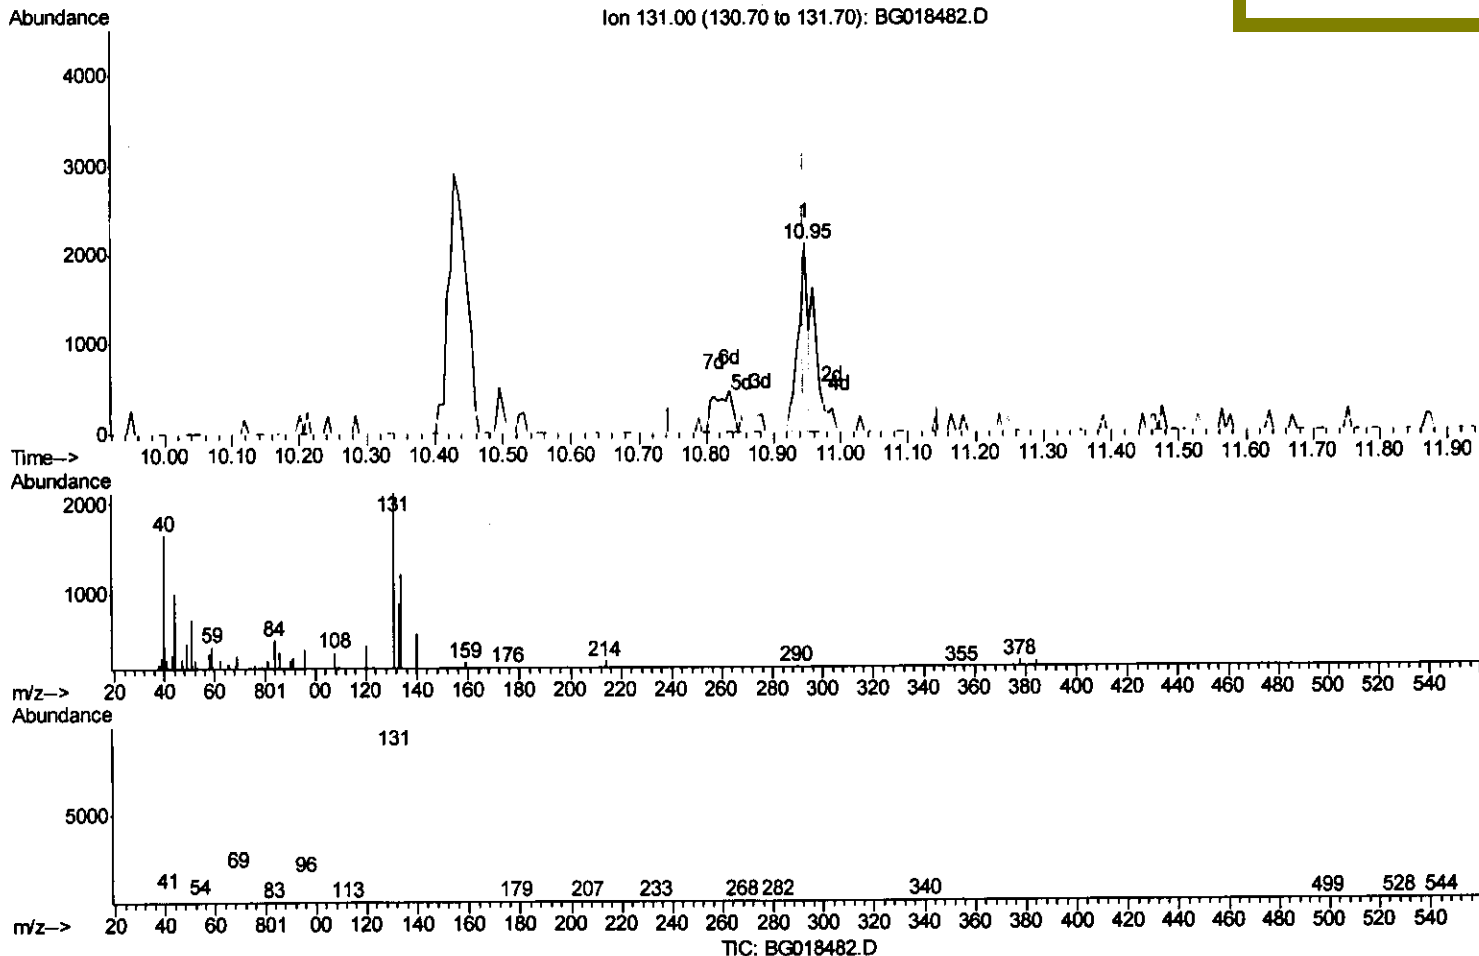

(29) 4-Chloroaniline-d4 (S)

10.947min (+0.001) 0.25ng/ul

response 2167

Ion	Exp%	Act%
131.00	100	100
133.00	32.00	41.27#
69.00	18.90	14.42#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA G\Data\BG081915\
 Data File : BG018482.D
 Acq On : 19 Aug 2015 20:13
 Operator : UM/MA
 Sample : G3302-13
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0551

Quant Time: Aug 20 01:32:43 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 20 01:31:35 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 8/20/2015 8:35:58 AM

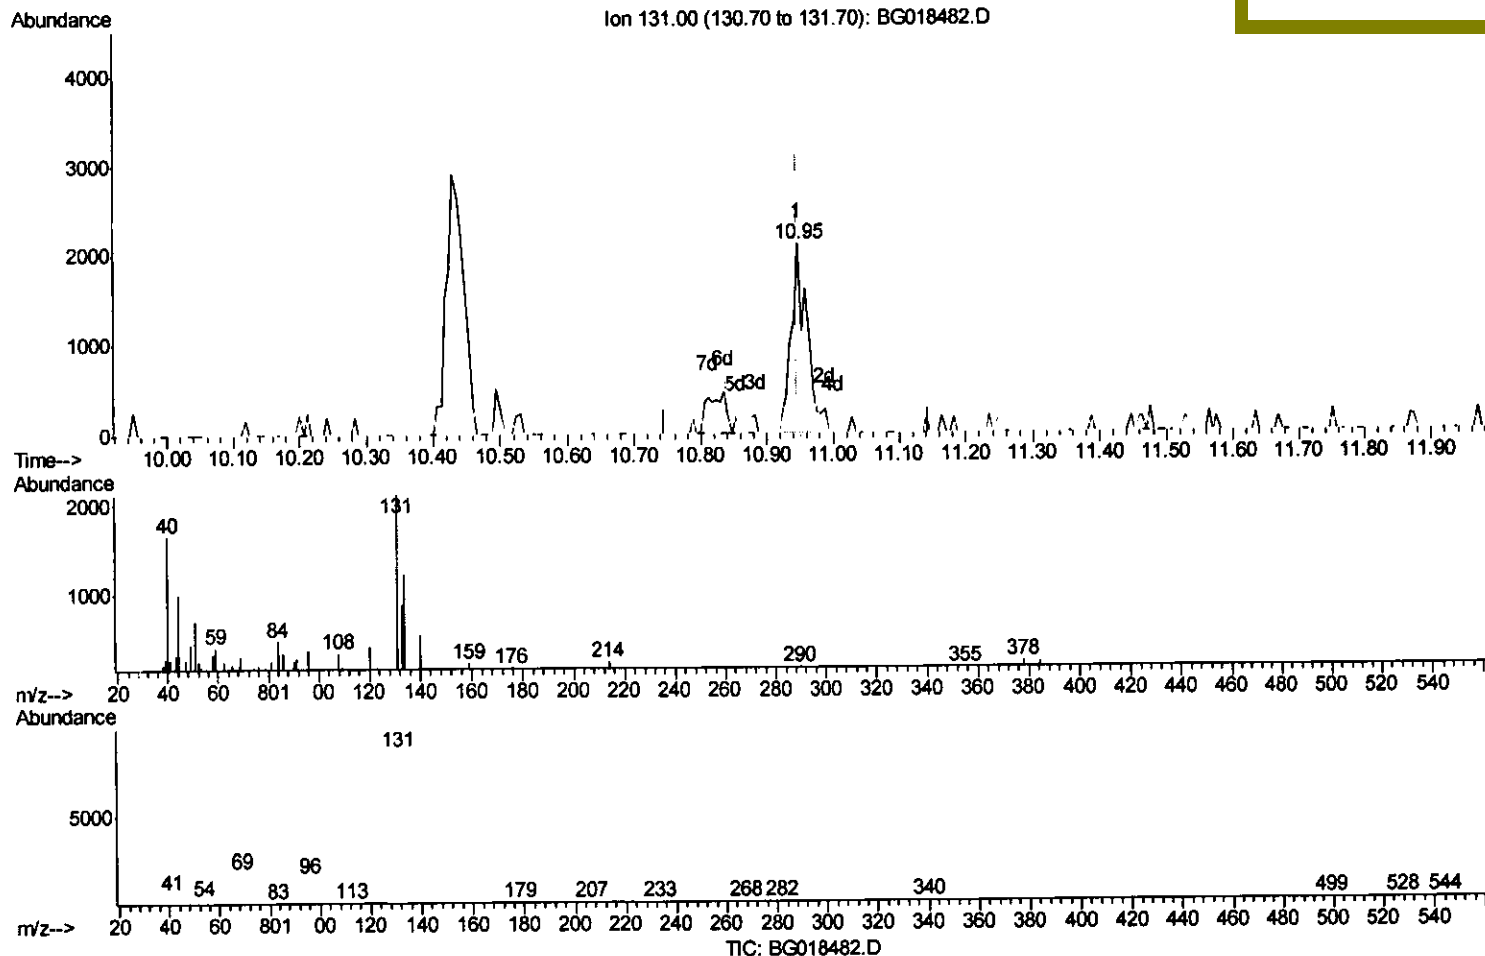

(29) 4-Chloroaniline-d4 (S)

10.947min (+0.001) 0.39ng/ul m

response 3412

Ion Exp% Act%

131.00 100 100

133.00 32.00 41.27#

69.00 18.90 14.42#

0.00 0.00 0.00

M.A
 8/20/15

Data Path : Z:\HPCHEM1\BNA G\Data\BG081915\
 Data File : BG018482.D
 Acq On : 19 Aug 2015 20:13
 Operator : UM/MA
 Sample : G3302-13
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 Client Sample ID :
 C0551

Quant Time: Aug 20 04:19:42 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 20 01:31:35 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 8/20/2015 8:35:58 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	99515	20.00	ng/ul	0.00
18) Naphthalene-d8	10.82	136	460374	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.64	164	314865	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.38	188	814768	20.00	ng/ul	0.00
78) Chrysene-d12	21.64	240	816622	20.00	ng/ul	0.00
86) Perylene-d12	24.84	264	801505	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.45	96	3014	1.34	ng/uL	0.00
5) Phenol-d5	7.17	99	54264	6.01	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	150107	26.82	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	148732	21.50	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	108302	14.27	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	100756	28.08	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	103709	28.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	195593	25.21	ng/ul	0.00
29) 4-Chloroaniline-d4	10.95	131	3412m	0.39	ng/ul	0.00
44) Dimethylphthalate-d6	14.04	166	784600	29.62	ng/ul	0.00
47) Acenaphthylene-d8	14.33	160	932892	27.97	ng/ul	0.00
52) 4-Nitrophenol-d4	14.82	143	31748	6.66	ng/ul	-0.01
58) Fluorene-d10	15.63	176	698893	30.29	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.74	200	111774	27.89	ng/ul	0.00
71) Anthracene-d10	17.48	188	1221193	31.34	ng/ul	0.00
79) Pyrene-d10	19.77	212	1348394	31.83	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.62	264	1294141	30.41	ng/ul	0.00

M.A
 8/20/15

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed