

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081920\
 Data File : BG046429.D
 Acq On : 22 Aug 2020 1:28
 Operator : CG/JU
 Sample : SSTDC0020
 Misc :
 ALS Vial : 93 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Aug 22 02:26:50 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG081320PAH.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 22 00:58:34 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.94	152	86998	20.00	ng/ul	0.00
2) Naphthalene-d8	10.74	136	358973	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.57	164	232585	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.31	188	519430	20.00	ng/ul	0.00
18) Chrysene-d12	21.56	240	514711	20.00	ng/ul	0.00
23) Perylene-d12	24.68	264	512738	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 2,4-Dichlorophenol-d3	10.36	165	125934	20.37	ng/ul	0.00
7) Acenaphthylene-d8	14.26	160	423327	19.78	ng/ul	0.00
10) Fluorene-d10	15.56	176	320391	19.53	ng/ul	0.00
15) Anthracene-d10	17.41	188	465443	19.33	ng/ul	0.00
19) Pyrene-d10	19.70	212	528339	19.94	ng/ul	0.00
26) Benzo(a)pyrene-d12	24.46	264	562220	20.09	ng/ul	0.00
Target Compounds				Qvalue		
4) Naphthalene	10.79	128	364541	19.523	ng/ul	100
5) 2-Methylnaphthalene	12.40	142	281716	19.791	ng/ul	99
8) Acenaphthylene	14.29	152	434354	19.959	ng/ul	99
9) Acenaphthene	14.63	153	303437	19.526	ng/ul	99
11) Fluorene	15.62	166	351231	19.330	ng/ul	99
13) Pentachlorophenol	16.97	266	73990	17.223	ng/ul	98
14) Phenanthrene	17.35	178	555037	19.423	ng/ul	100
16) Anthracene	17.45	178	562032	19.493	ng/ul	99
17) Fluoranthene	19.36	202	670730	21.050	ng/ul	99
20) Pyrene	19.73	202	670511	19.846	ng/ul	98
21) Benzo(a)anthracene	21.54	228	663283	19.806	ng/ul	100
22) Chrysene	21.61	228	640815	19.794	ng/ul	100
24) Benzo(b)fluoranthene	23.69	252	689688	20.341	ng/ul	98
25) Benzo(k)fluoranthene	23.75	252	673971	20.038	ng/ul	99
27) Benzo(a)pyrene	24.53	252	597611	19.198	ng/ul	100
28) Indeno(1,2,3-cd)pyrene	28.20	276	627234	16.093	ng/ul	98
29) Dibenzo(a,h)anthracene	28.25	278	553512	17.515	ng/ul	98
30) Benzo(g,h,i)perylene	29.29	276	471797	14.464	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081920\
Data File : BG046429.D
Acq On : 22 Aug 2020 1:28
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 93 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Aug 22 02:26:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG081320PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 22 00:58:34 2020
Response via : Initial Calibration

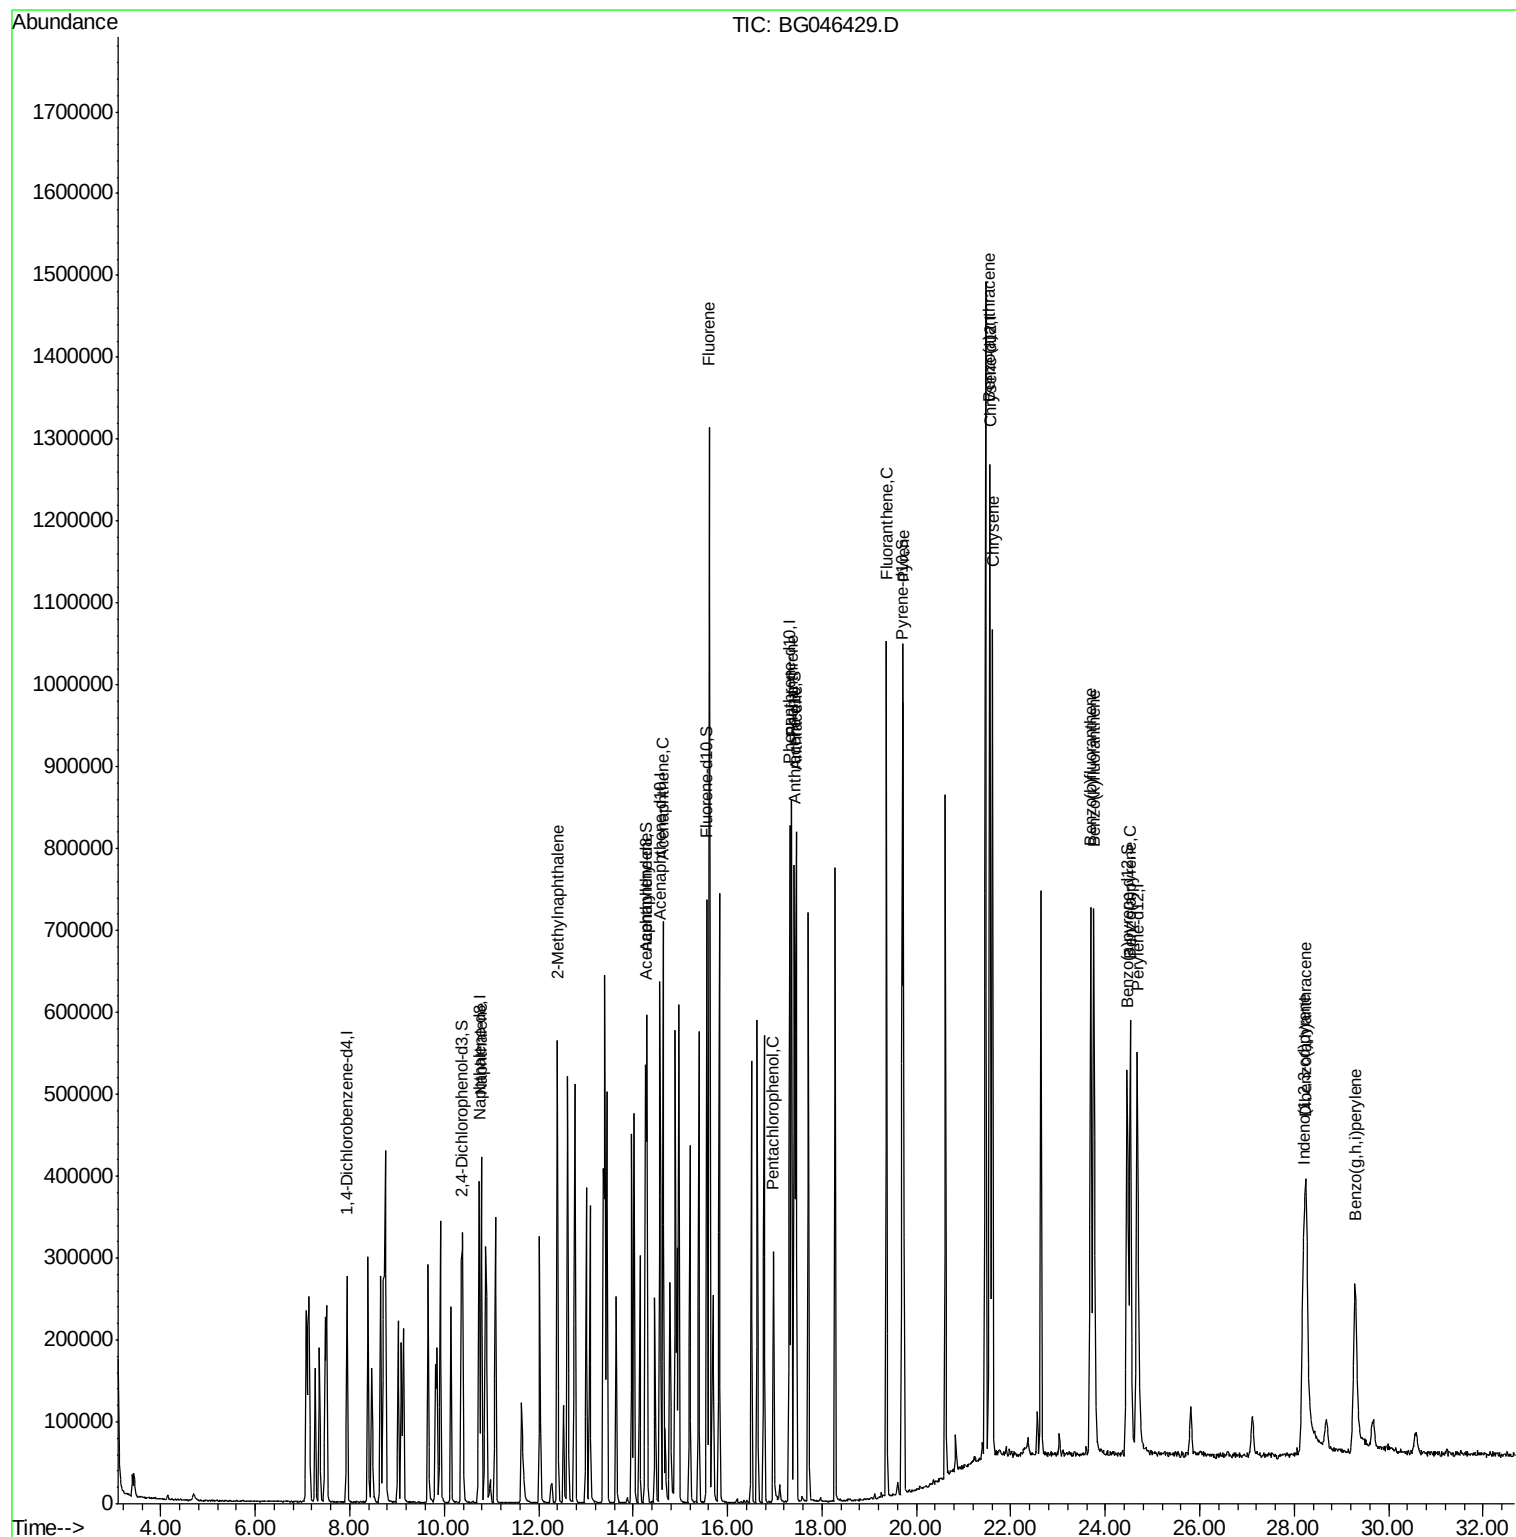

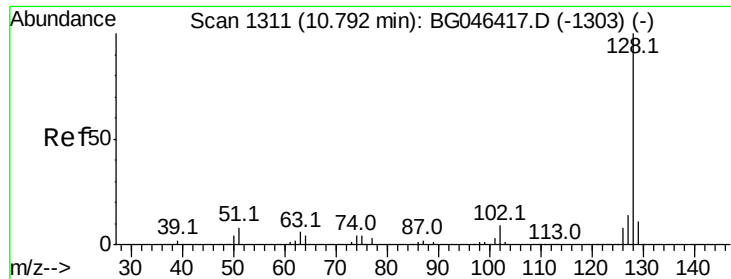

#4

Naphthalene

Concen: 19.523 ng/ul

RT: 10.79 min Scan# 1310

Delta R.T. -0.01 min

Lab File: BG046429.D

Acq: 22 Aug 2020 1:28

Instrument :

BNA_G

ClientSampleId :


Tot Ion:128 Resp: 364541

Ion Ratio Lower Upper

128 100

129 11.3 9.0 13.6




127 13.7 10.9 16.3



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

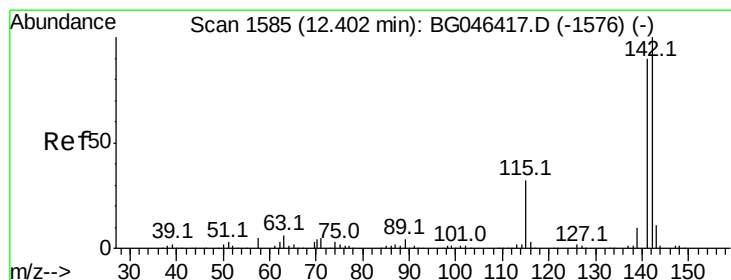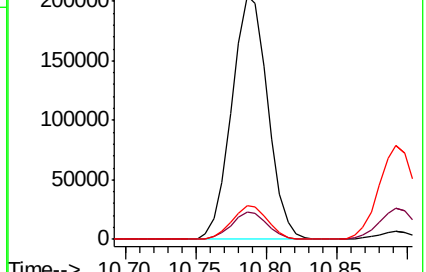

#5

2-Methylnaphthalene

Concen: 19.791 ng/ul

RT: 12.40 min Scan# 1584

Delta R.T. -0.01 min

Lab File: BG046429.D


Acq: 22 Aug 2020 1:28

Tgt Ion:142 Resp: 281716

Ion Ratio Lower Upper



142 100


141 91.5 72.5 108.7



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

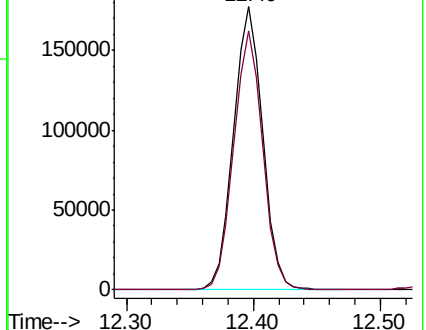







#8
Acenaphthylene
Concen: 19.959 ng/ul
RT: 14.29 min Scan# 1907
Delta R.T. 0.00 min
Lab File: BG046429.D
Acq: 22 Aug 2020 1:28

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
151	20.6	16.5	24.7
153	12.5	11.0	16.6

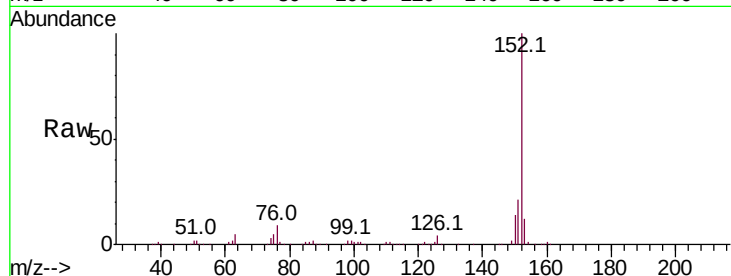


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 151.00 (150.70 to 151.70): E
Ion 153.00 (152.70 to 153.70): E


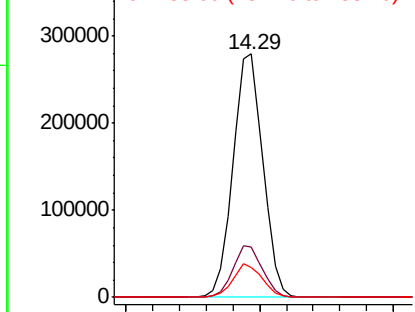



#9
Acenaphthene
Concen: 19.526 ng/ul
RT: 14.63 min Scan# 1965
Delta R.T. -0.01 min
Lab File: BG046429.D
Acq: 22 Aug 2020 1:28

Tgt Ion	Ratio	Lower	Upper
153	100		
152	46.8	37.2	55.8
154	86.3	67.8	101.6



Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E




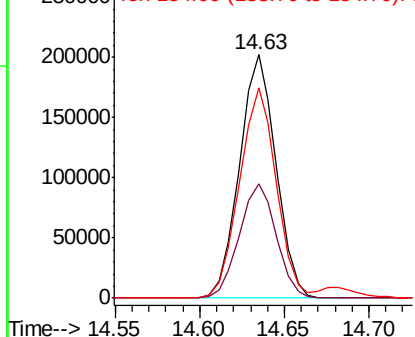


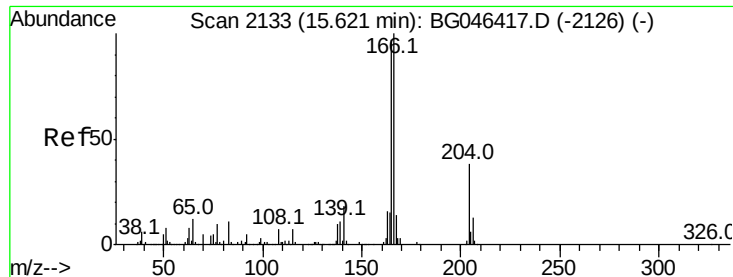

#11
Fluorene
Concen: 19.330 ng/ul
RT: 15.62 min Scan# 2132
Delta R.T. -0.01 min
Lab File: BG046429.D
Acq: 22 Aug 2020 1:28




Instrument :
BNA_G
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
166	100		
165	95.9	75.9	113.9
167	14.6	10.7	16.1

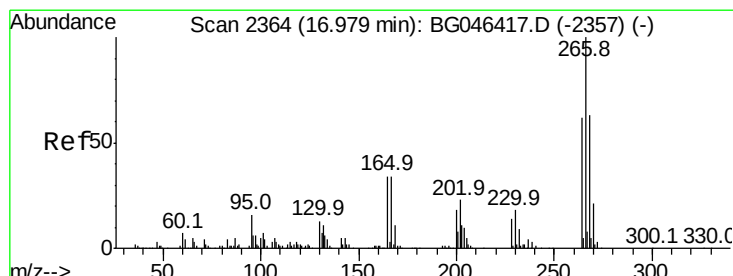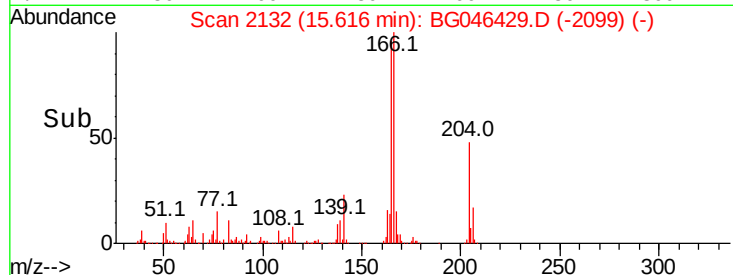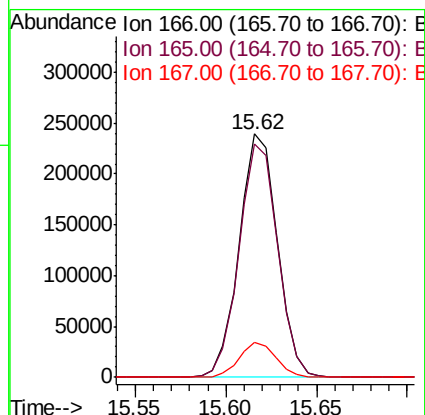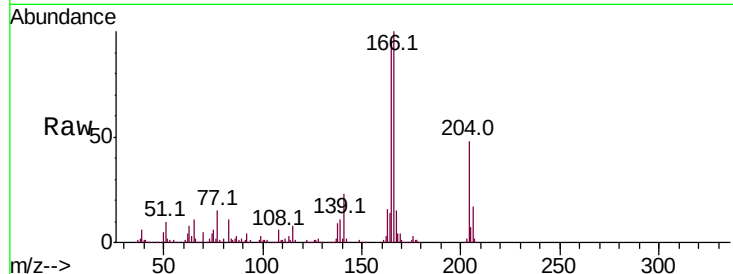

#13
Pentachlorophenol
Concen: 17.223 ng/ul
RT: 16.97 min Scan# 2363
Delta R.T. -0.01 min
Lab File: BG046429.D
Acq: 22 Aug 2020 1:28

Tgt Ion	Ratio	Lower	Upper
266	100		
264	60.8	50.2	75.2
268	63.8	49.7	74.5

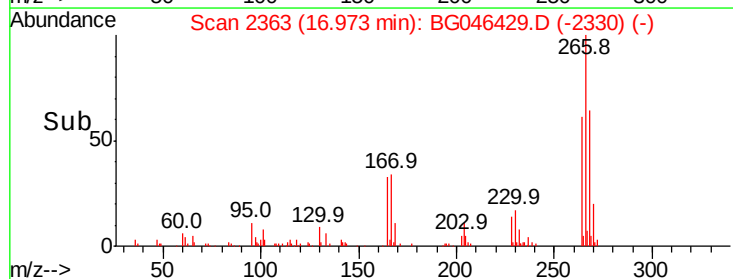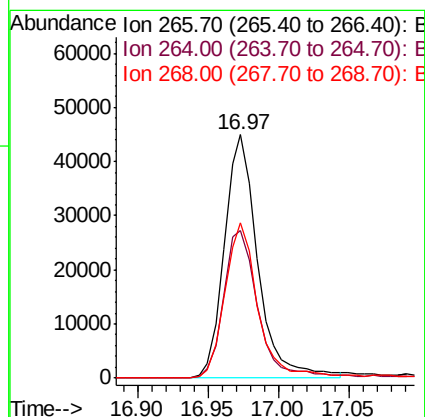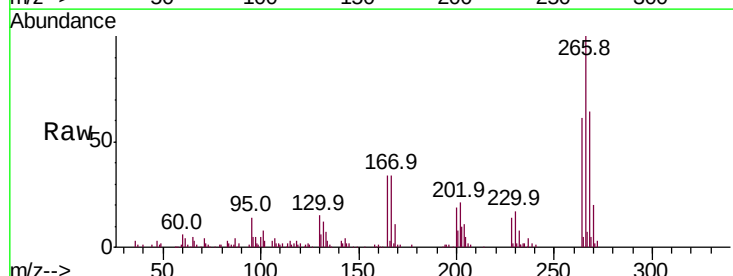







#14
Phenanthrene
Concen: 19.423 ng/ul
RT: 17.35 min Scan# 2428
Delta R.T. -0.01 min
Lab File: BG046429.D
Acq: 22 Aug 2020 1:28

Instrument :
BNA_G
ClientSampled :

Tot Ion	Ratio	Lower	Upper
178	100		
179	15.8	12.8	19.2
176	19.9	15.8	23.8

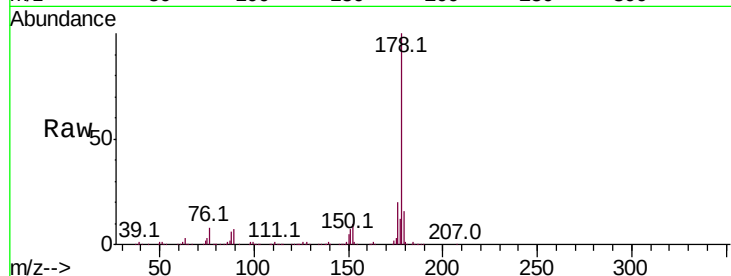


Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E


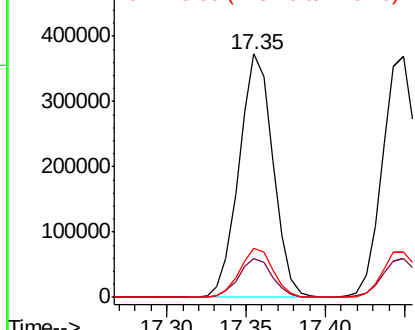



#16
Anthracene
Concen: 19.493 ng/ul
RT: 17.45 min Scan# 2444
Delta R.T. 0.00 min
Lab File: BG046429.D
Acq: 22 Aug 2020 1:28

Tgt Ion	Ratio	Lower	Upper
178	100		
179	15.9	13.2	19.8
176	18.9	15.2	22.8



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E



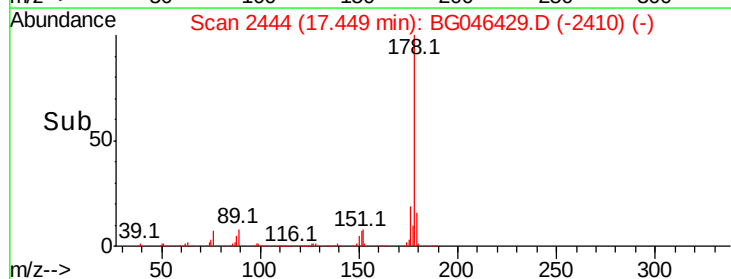
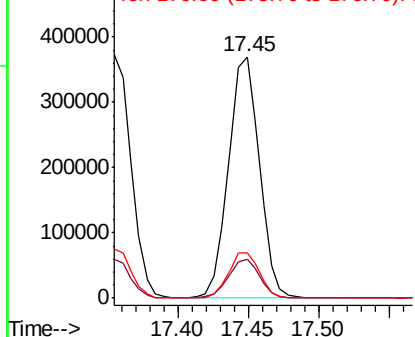


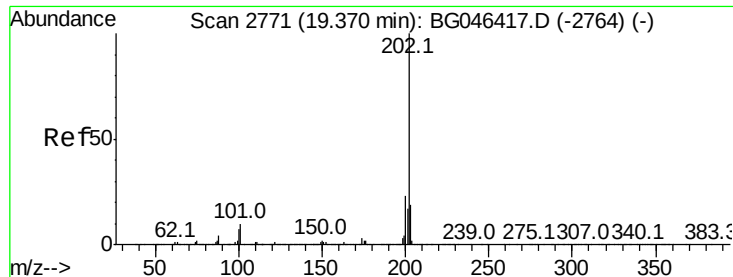

#17
 Fluoranthene
 Concen: 21.050 ng/ul
 RT: 19.36 min Scan# 2770
 Delta R.T. -0.01 min
 Lab File: BG046429.D
 Acq: 22 Aug 2020 1:28




Instrument :
 BNA_G
 ClientSampleId :


Tot Ion:	202	Resp:	670730
Ion	Ratio	Lower	Upper
202	100		
101	9.3	7.8	11.6
100	7.5	5.9	8.9

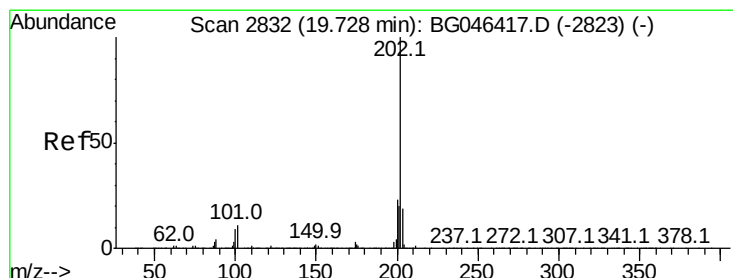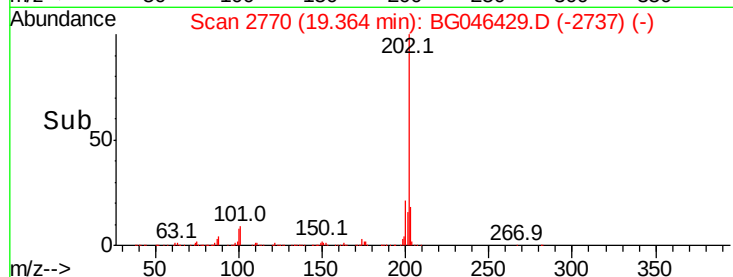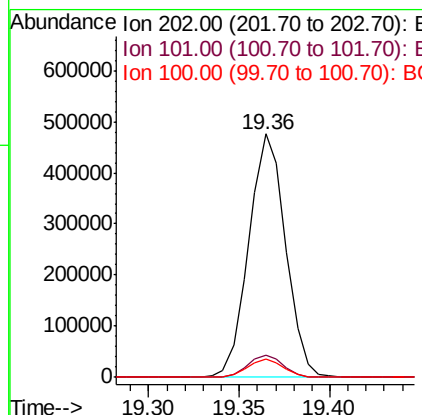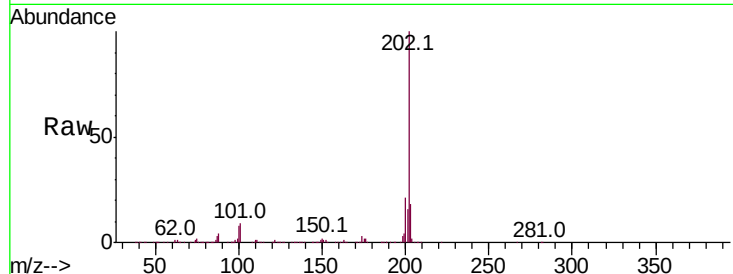

#20
 Pyrene
 Concen: 19.846 ng/ul
 RT: 19.73 min Scan# 2832
 Delta R.T. 0.00 min
 Lab File: BG046429.D
 Acq: 22 Aug 2020 1:28

Tgt Ion:	202	Resp:	670511
Ion	Ratio	Lower	Upper
202	100		
101	10.7	8.9	13.3
100	8.6	7.9	11.9

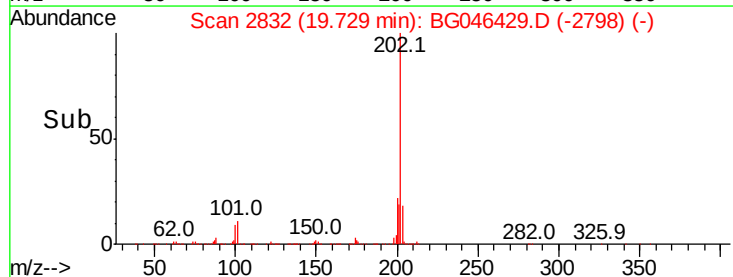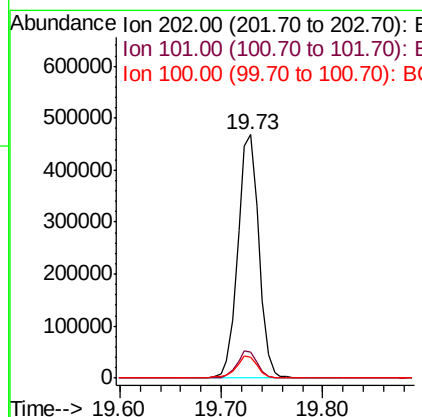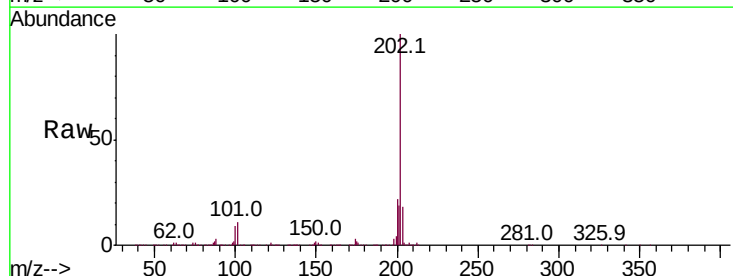



#21

Benzo(a)anthracene

Concen: 19.806 ng/ul

RT: 21.54 min Scan# 3141

Delta R.T. -0.01 min

Lab File: BG046429.D

Acq: 22 Aug 2020 1:28

Instrument :

BNA_G

ClientSampleId :


Tot Ion:228 Resp: 663283

Ion	Ratio	Lower	Upper
228	100		
229	20.9	16.6	25.0
226	28.1	22.6	33.8

228 100

229 20.9 16.6 25.0

226 28.1 22.6 33.8






Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

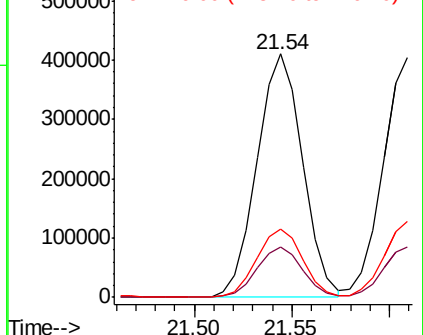

#22

Chrysene

Concen: 19.794 ng/ul

RT: 21.61 min Scan# 3152

Delta R.T. -0.01 min

Lab File: BG046429.D

Acq: 22 Aug 2020 1:28


Tgt Ion:228 Resp: 640815

Ion	Ratio	Lower	Upper
228	100		
226	31.7	25.5	38.3
229	21.2	17.0	25.4

228 100

226 31.7 25.5 38.3

229 21.2 17.0 25.4






Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E



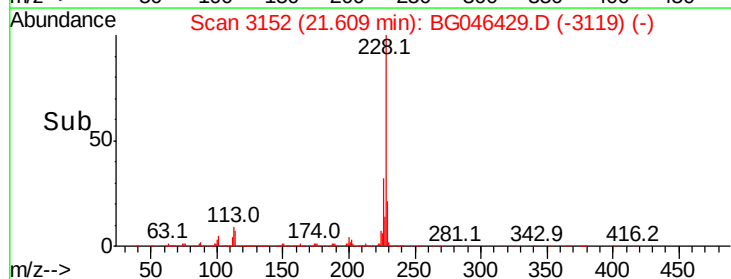
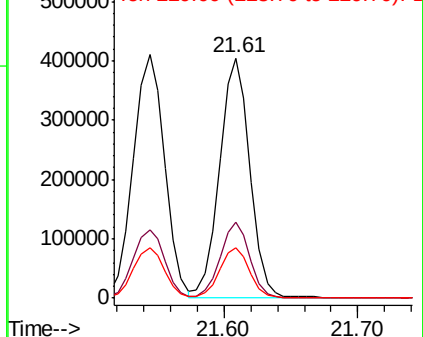


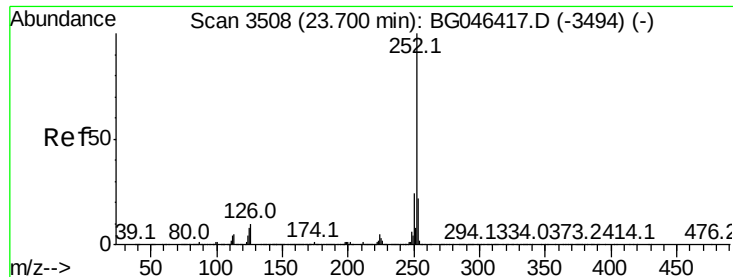

#24
Benzo(b)fluoranthene
Concen: 20.341 ng/ul
RT: 23.69 min Scan# 3507
Delta R.T. -0.01 min
Lab File: BG046429.D
Acq: 22 Aug 2020 1:28




Instrument :
BNA_G
ClientSampleId :


Tot Ion:	252	Resp:	689688
Ion	Ratio	Lower	Upper
252	100		
253	23.4	17.8	26.6
125	7.8	6.4	9.6

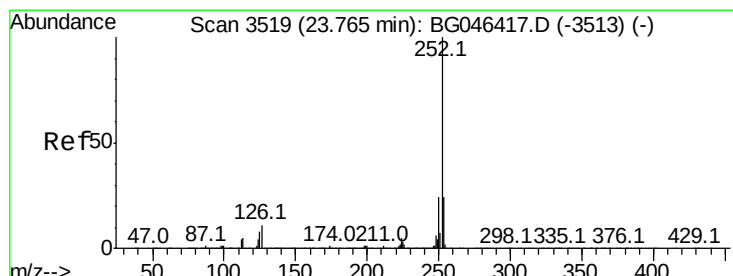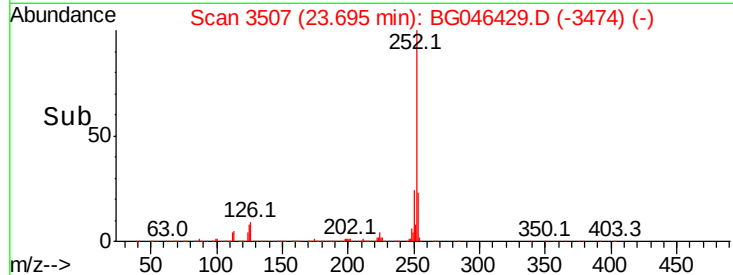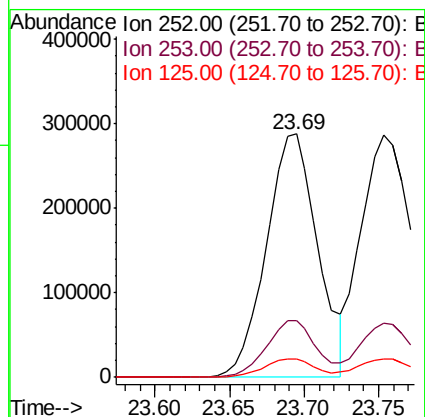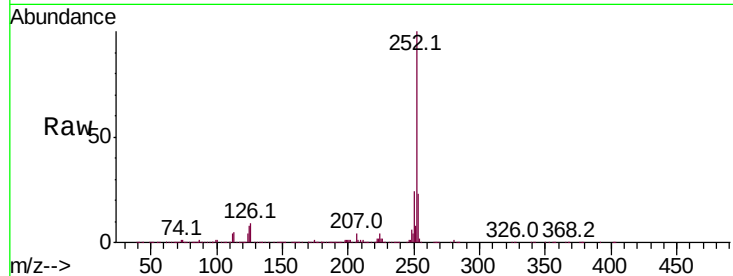

#25
Benzo(k)fluoranthene
Concen: 20.038 ng/ul
RT: 23.75 min Scan# 3517
Delta R.T. -0.01 min
Lab File: BG046429.D
Acq: 22 Aug 2020 1:28

Tgt Ion:	252	Resp:	673971
Ion	Ratio	Lower	Upper
252	100		
253	22.4	18.5	27.7
125	7.6	6.2	9.2


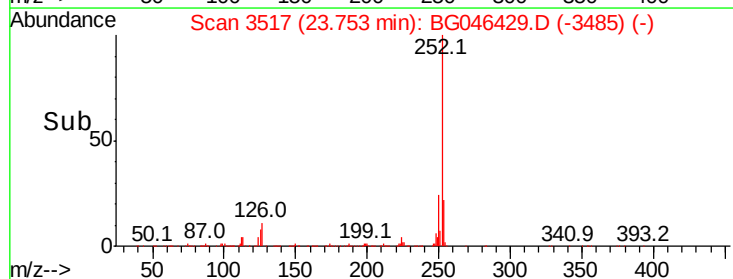
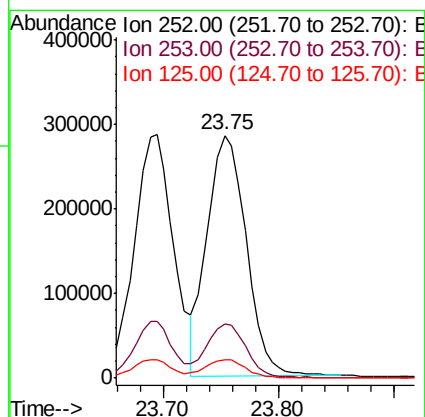
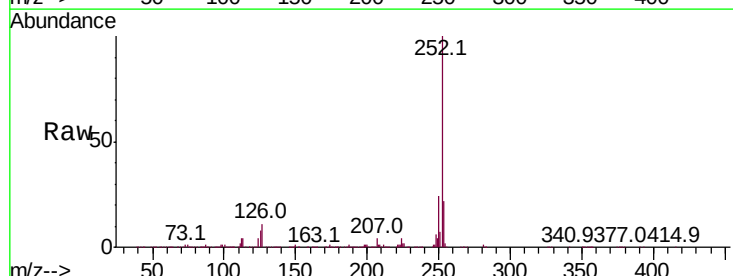


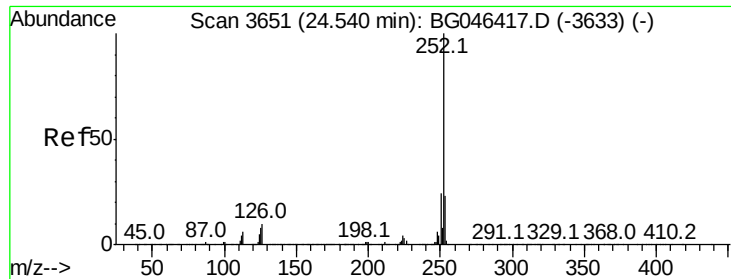

#27
Benzo(a)pyrene
Concen: 19.198 ng/ul
RT: 24.53 min Scan# 3649
Delta R.T. -0.01 min
Lab File: BG046429.D
Acq: 22 Aug 2020 1:28




Instrument :
BNA_G
ClientSampled :


Tot Ion:	252	Resp:	597611
Ion	Ratio	Lower	Upper
252	100		
253	22.2	17.8	26.8
125	8.9	7.1	10.7

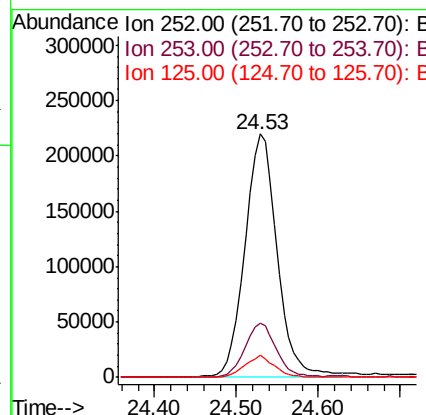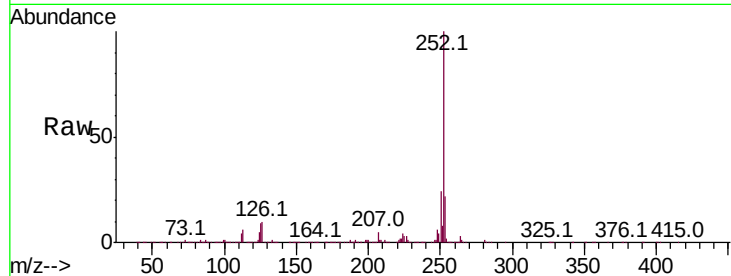

#28
Indeno(1,2,3-cd)pyrene
Concen: 16.093 ng/ul
RT: 28.20 min Scan# 4273
Delta R.T. -0.01 min
Lab File: BG046429.D
Acq: 22 Aug 2020 1:28

Tgt Ion:	276	Resp:	627234
Ion	Ratio	Lower	Upper
276	100		
138	15.4	13.2	19.8
277	23.8	19.9	29.9

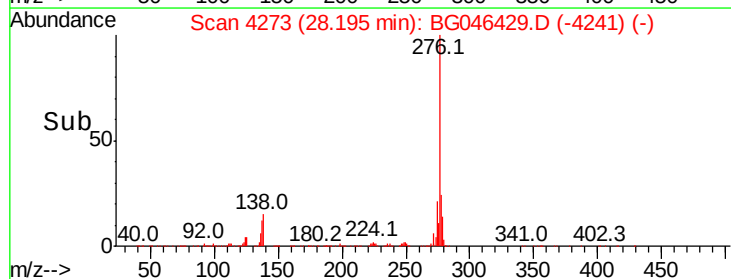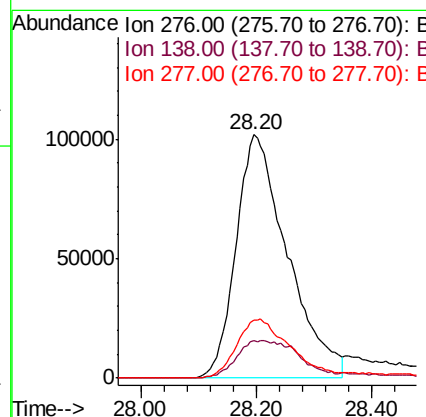

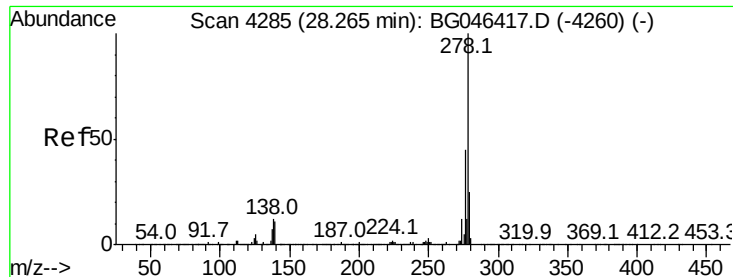

#29

Dibenzo(a,h)anthracene

Concen: 17.515 ng/ul

RT: 28.25 min Scan# 4283

Delta R.T. -0.01 min

Lab File: BG046429.D

Acq: 22 Aug 2020 1:28

Instrument :

BNA_G

ClientSampled :


Tot Ion:278 Resp: 553512

Ion Ratio Lower Upper

278 100

139 11.5 9.8 14.8

279 25.4 19.7 29.5



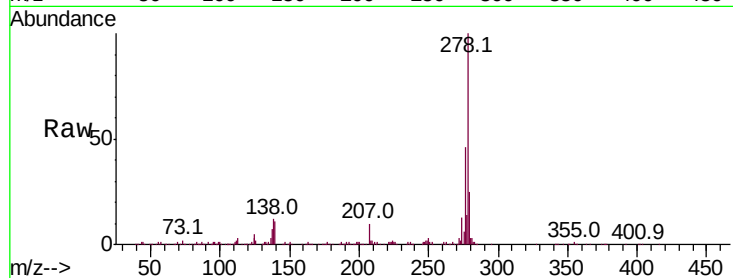


Abundance

Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

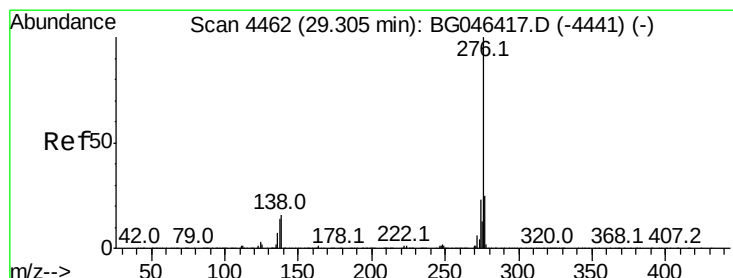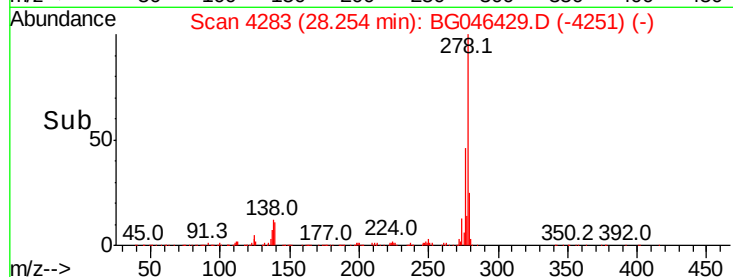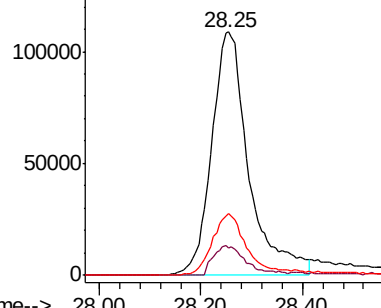

#30

Benzo(g,h,i)perylene

Concen: 14.464 ng/ul

RT: 29.29 min Scan# 4459

Delta R.T. -0.02 min

Lab File: BG046429.D

Acq: 22 Aug 2020 1:28


Tgt Ion:276 Resp: 471797

Ion Ratio Lower Upper

276 100

138 16.9 12.9 19.3

277 23.5 19.4 29.0

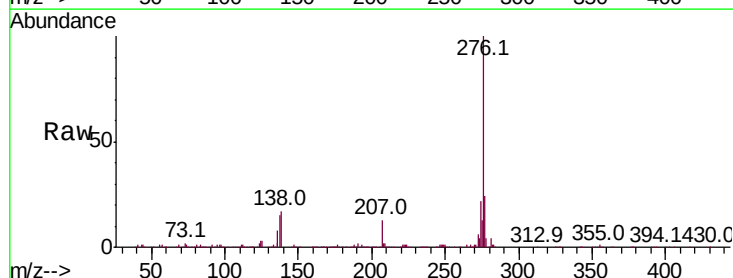

Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

