

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081920\
 Data File : BG046430.D
 Acq On : 22 Aug 2020 2:48
 Operator : CG/JU
 Sample : L3649-08
 Misc :
 ALS Vial : 94 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BFMX5

Quant Time: Aug 22 04:32:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG081320PAH.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 22 00:58:34 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.94	152	93788	20.00	ng/ul	0.00
2) Naphthalene-d8	10.74	136	391700	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.57	164	261923	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.31	188	573792	20.00	ng/ul	0.00
18) Chrysene-d12	21.56	240	542068	20.00	ng/ul	0.00
23) Perylene-d12	24.68	264	570761	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 2,4-Dichlorophenol-d3	10.36	165	136978	20.31	ng/ul	0.00
7) Acenaphthylene-d8	14.26	160	518558	21.51	ng/ul	0.00
10) Fluorene-d10	15.56	176	406330	22.00	ng/ul	0.00
15) Anthracene-d10	17.41	188	575694	21.64	ng/ul	0.00
19) Pyrene-d10	19.70	212	613102	21.97	ng/ul	0.00
26) Benzo(a)pyrene-d12	24.47	264	668403	21.46	ng/ul	0.00
Target Compounds				Qvalue		
9) Acenaphthene	14.63	153	33183	1.896	ng/ul	96
14) Phenanthrene	17.36	178	268802	8.515	ng/ul	100
16) Anthracene	17.44	178	139225	4.371	ng/ul	100
17) Fluoranthene	19.36	202	554199	15.745	ng/ul	99
20) Pyrene	19.73	202	637382	17.913	ng/ul	98
21) Benzo(a)anthracene	21.54	228	789078	22.373	ng/ul	95
22) Chrysene	21.54	228	784363	23.006	ng/ul	94
24) Benzo(b)fluoranthene	23.70	252	1014612	26.882	ng/ul	97
25) Benzo(k)fluoranthene	23.70	252	1014612	27.099	ng/ul	98
27) Benzo(a)pyrene	24.54	252	885009	25.541	ng/ul	95
28) Indeno(1,2,3-cd)pyrene	28.21	276	566519	13.057	ng/ul	97
29) Dibenzo(a,h)anthracene	28.25	278	181581	5.162	ng/ul#	88
30) Benzo(a,h,i)perylene	29.31	276	417154	11.488	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081920\
Data File : BG046430.D
Acq On : 22 Aug 2020 2:48
Operator : CG/JU
Sample : L3649-08
Misc :
ALS Vial : 94 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BFMX5

Quant Time: Aug 22 04:32:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG081320PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 22 00:58:34 2020
Response via : Initial Calibration

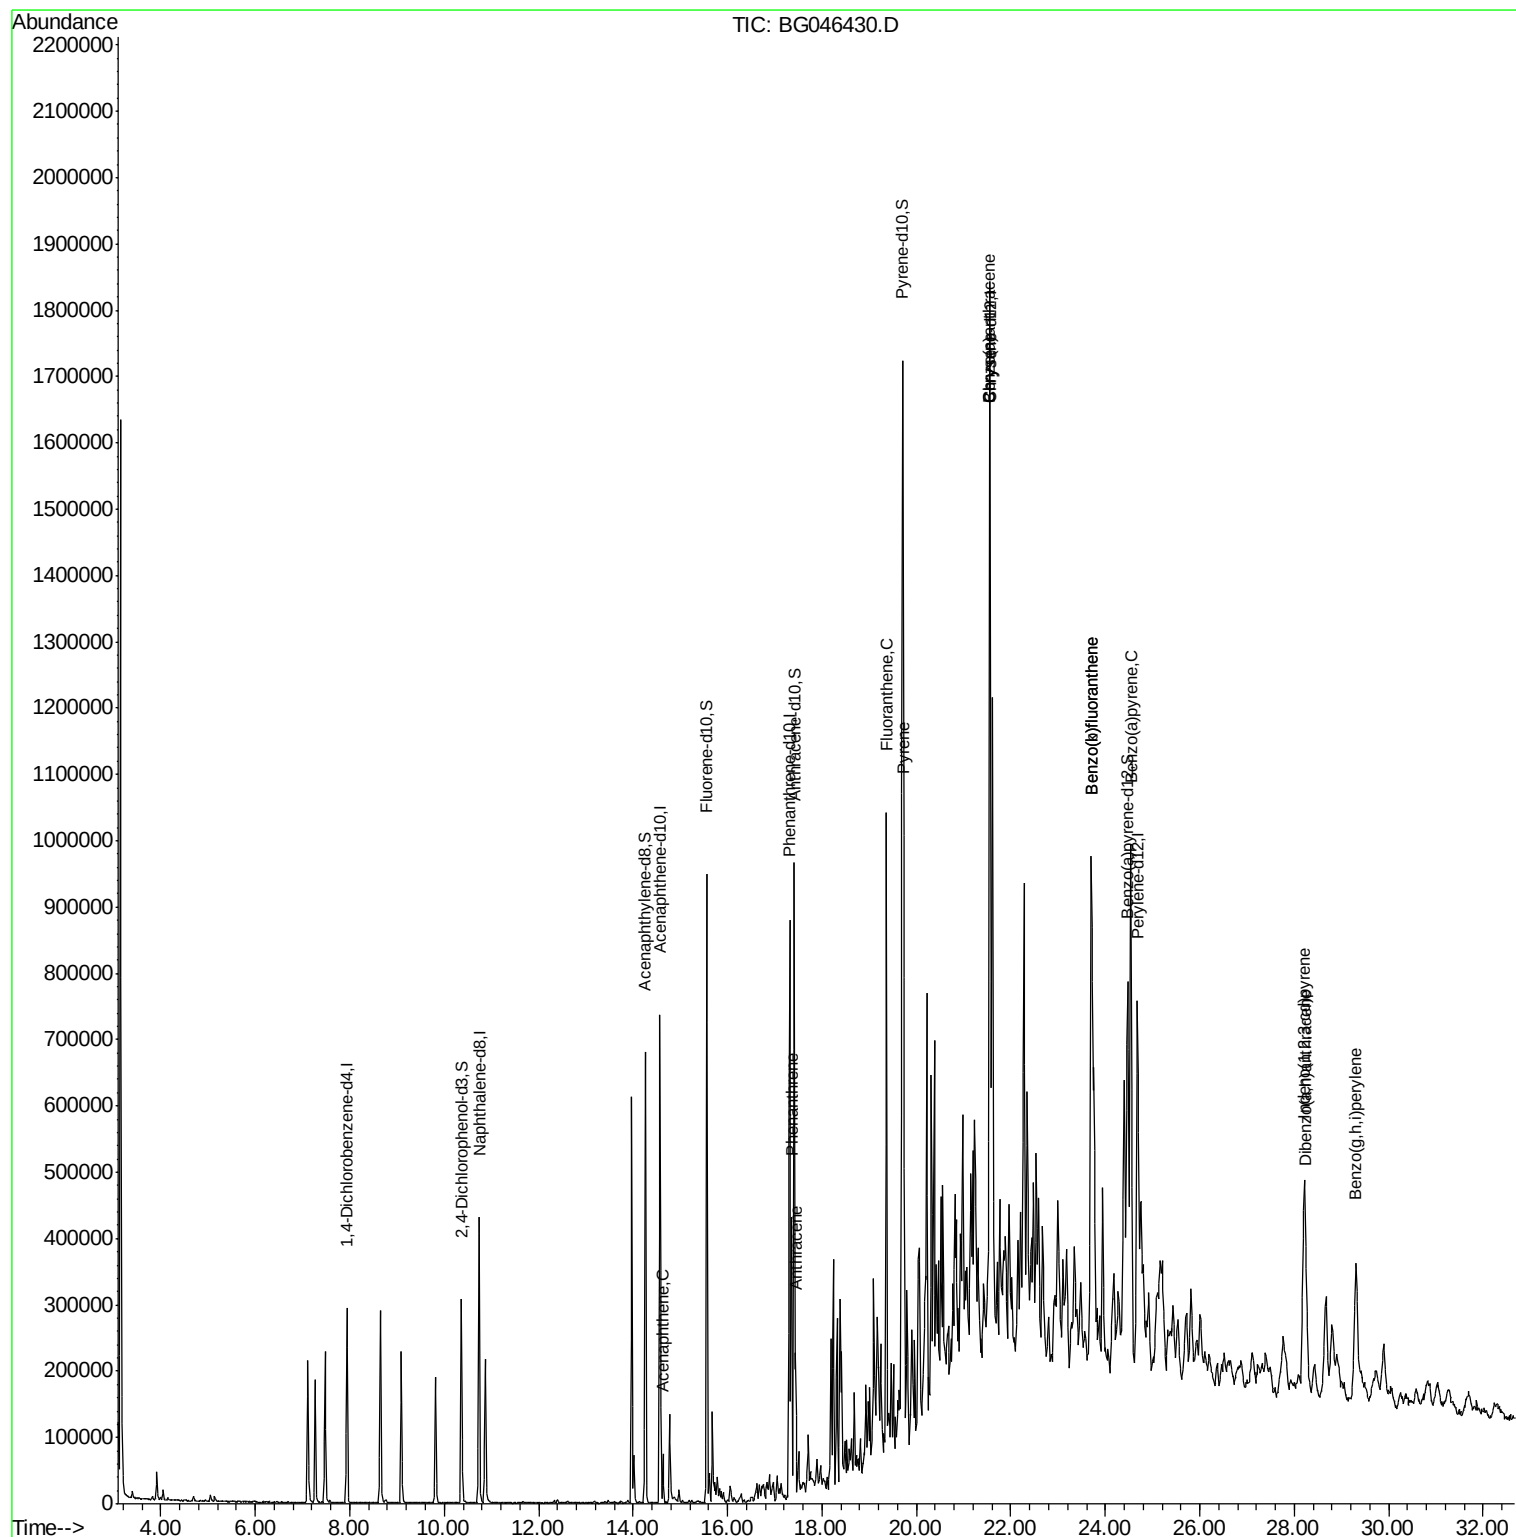

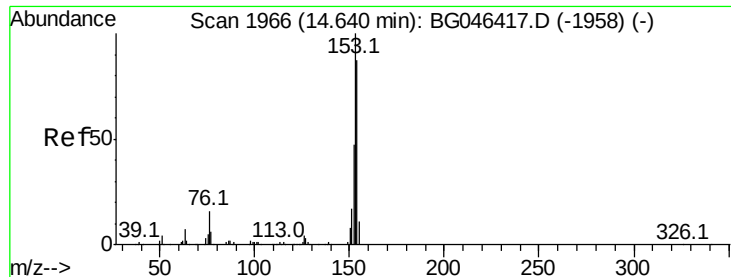

#9

Acenaphthene

Concen: 1.896 ng/ul

RT: 14.63 min Scan# 1965

Delta R.T. -0.01 min

Lab File: BG046430.D

Acq: 22 Aug 2020 2:48

Instrument :

BNA_G

ClientSampleId :

BFMX5


Tot Ion:153 Resp: 33183

Ion Ratio Lower Upper

153 100

152 47.5 37.2 55.8

154 80.3 67.8 101.6



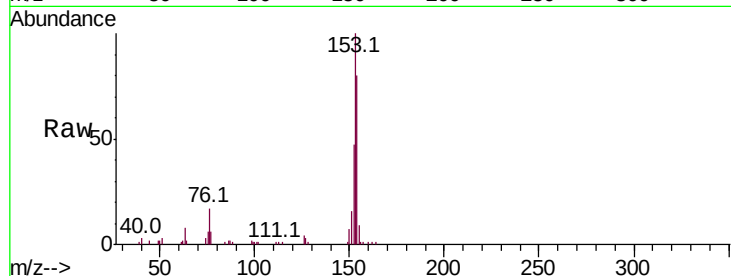


Abundance

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

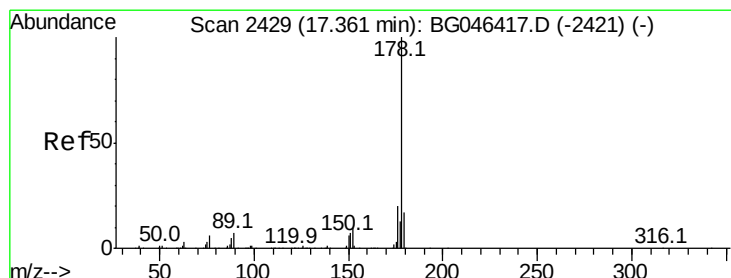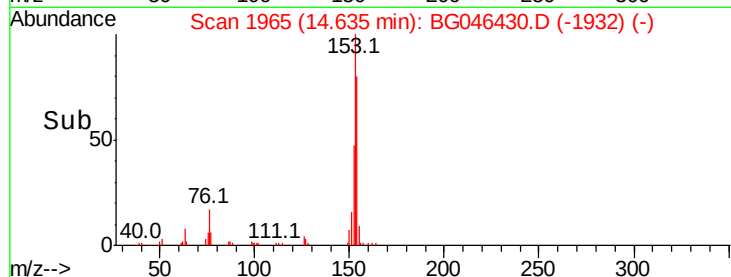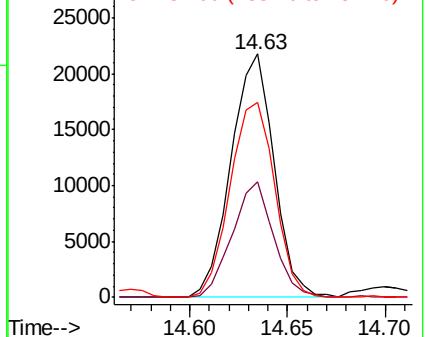

#14

Phenanthrene

Concen: 8.515 ng/ul

RT: 17.36 min Scan# 2428

Delta R.T. -0.01 min

Lab File: BG046430.D

Acq: 22 Aug 2020 2:48


Tgt Ion:178 Resp: 268802

Ion Ratio Lower Upper

178 100

179 15.8 12.8 19.2

176 19.6 15.8 23.8


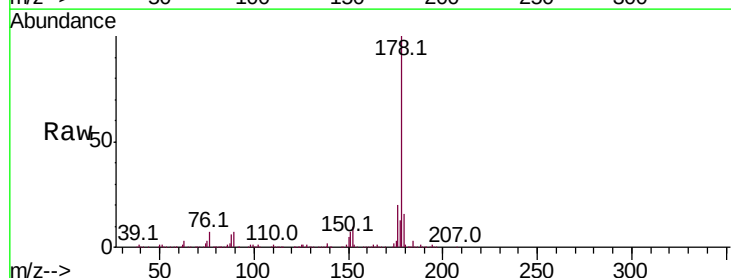



Abundance

Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E



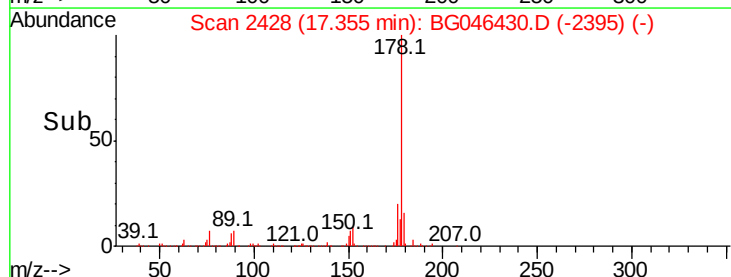
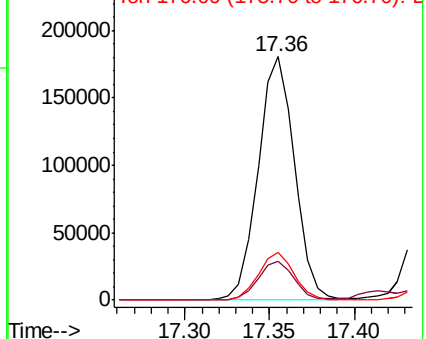


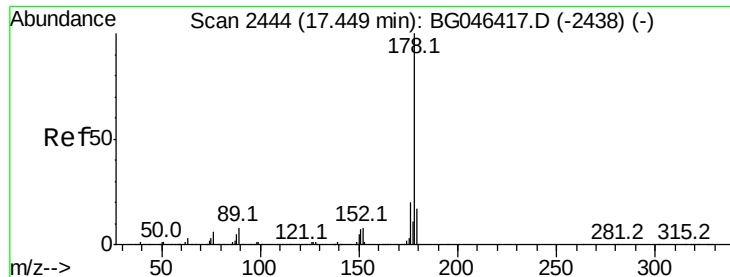

#16
 Anthracene
 Concen: 4.371 ng/ul
 RT: 17.44 min Scan# 2443
 Delta R.T. -0.01 min
 Lab File: BG046430.D
 Acq: 22 Aug 2020 2:48




Instrument :
 BNA_G
 ClientSampleId :
 BFMX5


Tot Ion	Ratio	Lower	Upper
178	100		
179	16.6	13.2	19.8
176	19.3	15.2	22.8

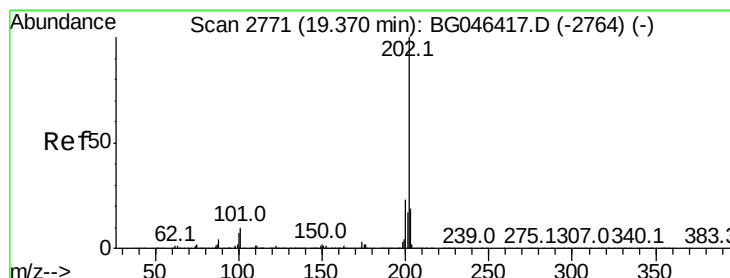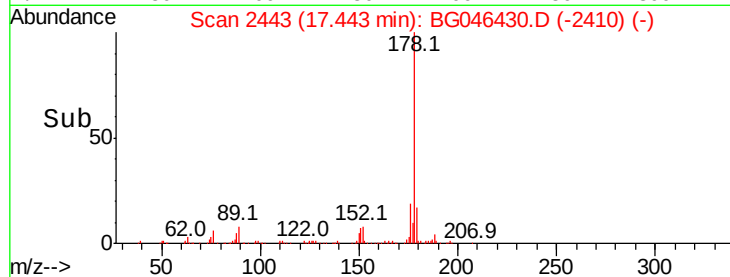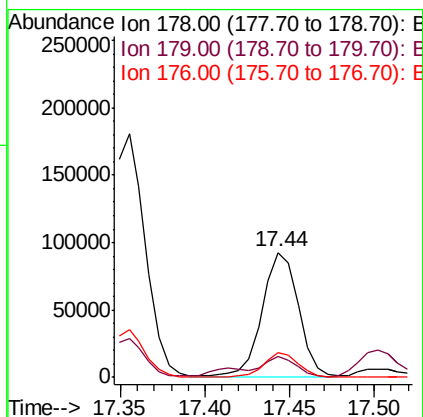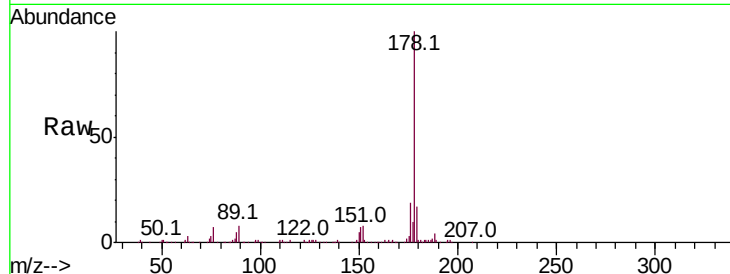

#17
 Fluoranthene
 Concen: 15.745 ng/ul
 RT: 19.36 min Scan# 2770
 Delta R.T. -0.01 min
 Lab File: BG046430.D
 Acq: 22 Aug 2020 2:48

Tgt Ion	Ratio	Lower	Upper
202	100		
101	9.3	7.8	11.6
100	7.2	5.9	8.9

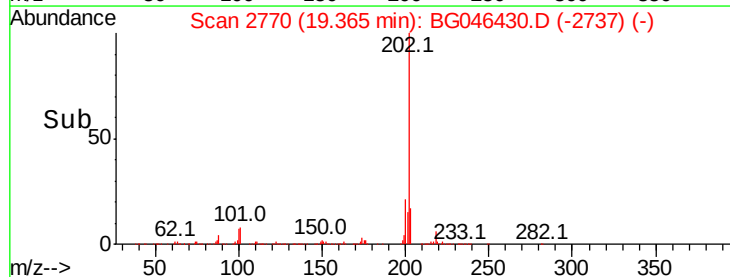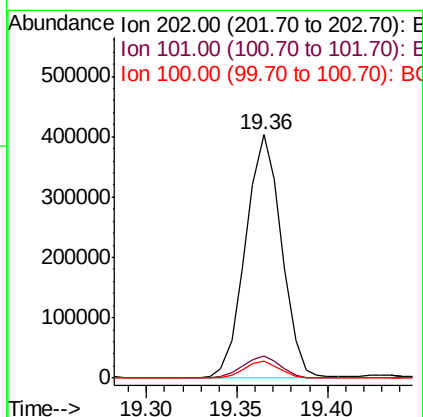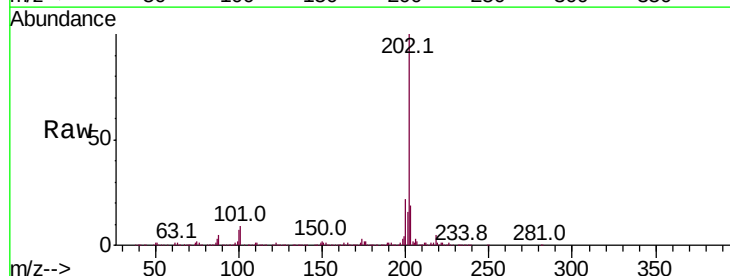

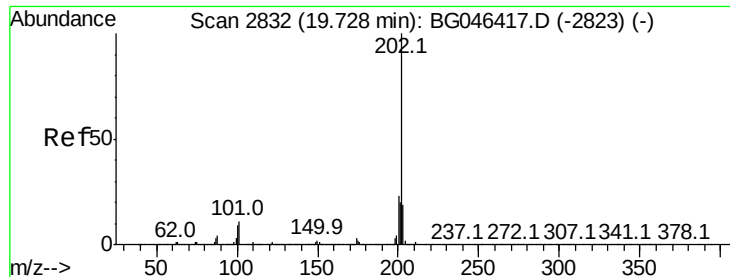

#20

Pvrene

Concen: 17.913 ng/ul

RT: 19.73 min Scan# 2832

Delta R.T. 0.00 min

Lab File: BG046430.D

Acq: 22 Aug 2020 2:48

Instrument :

BNA_G

ClientSampleId :

BFMX5


Tot Ion:202 Resp: 637382

Ion Ratio Lower Upper

202 100

101 10.6 8.9 13.3




100 9.1 7.9 11.9

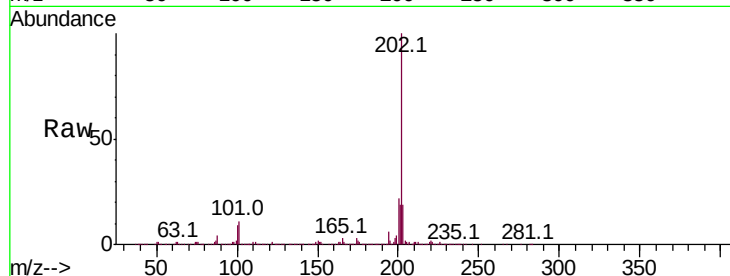

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

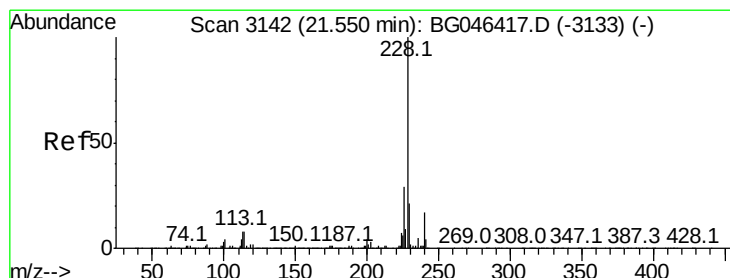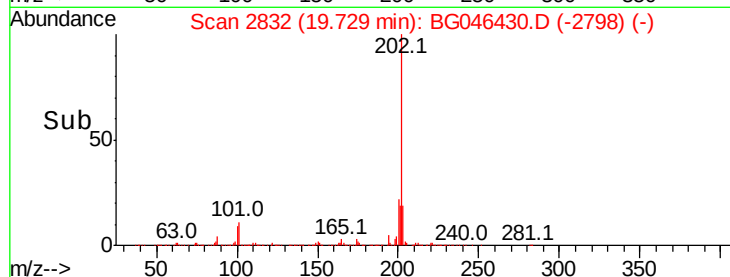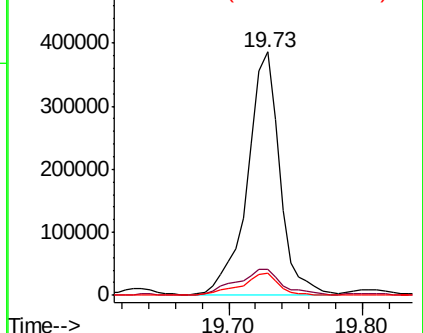

#21

Benzo(a)anthracene

Concen: 22.373 ng/ul

RT: 21.54 min Scan# 3141

Delta R.T. -0.01 min

Lab File: BG046430.D

Acq: 22 Aug 2020 2:48


Tgt Ion:228 Resp: 789078

Ion Ratio Lower Upper

228 100

229 24.7 16.6 25.0



226 29.4 22.6 33.8

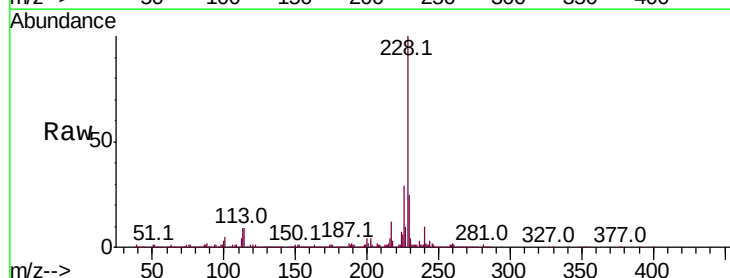


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

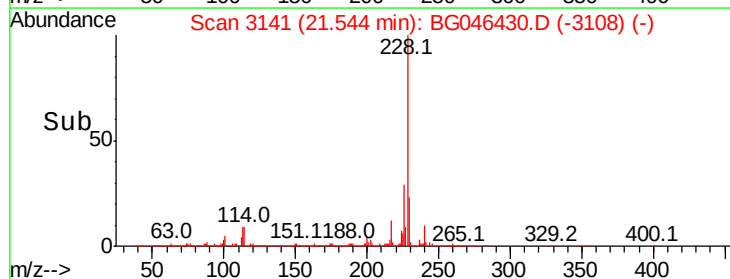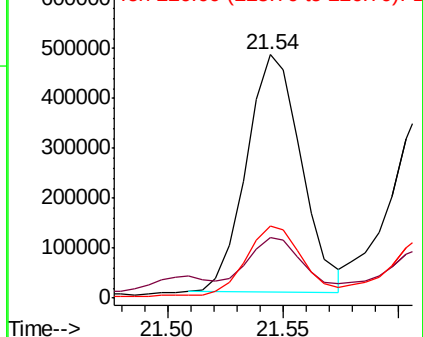

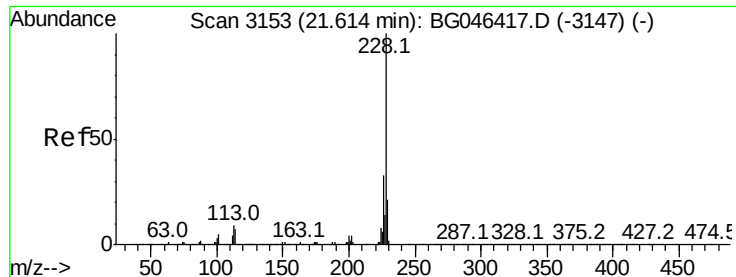

#22

Chrysene

Concen: 23.006 ng/ul

RT: 21.54 min Scan# 3141

Delta R.T. -0.07 min

Lab File: BG046430.D

Acq: 22 Aug 2020 2:48

Instrument :

BNA_G

ClientSampleId :

BFMX5


Tot Ion:228 Resp: 784363

Ion Ratio Lower Upper

228 100

226 29.4 25.5 38.3




229 24.7 17.0 25.4

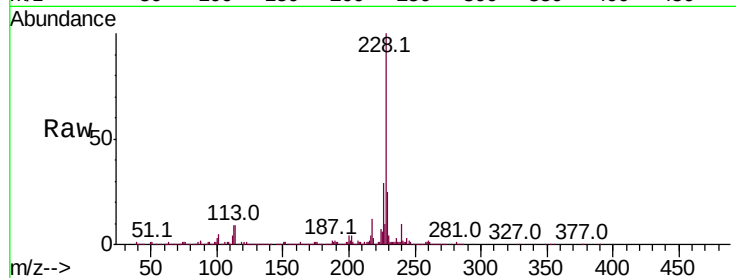

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

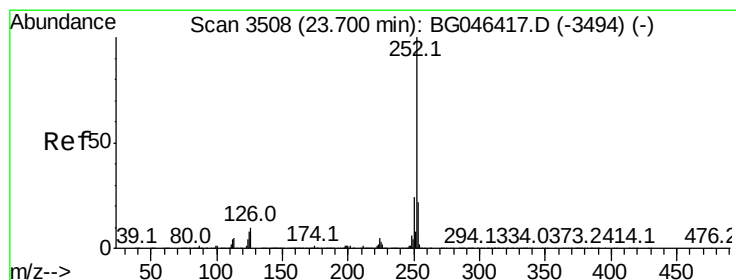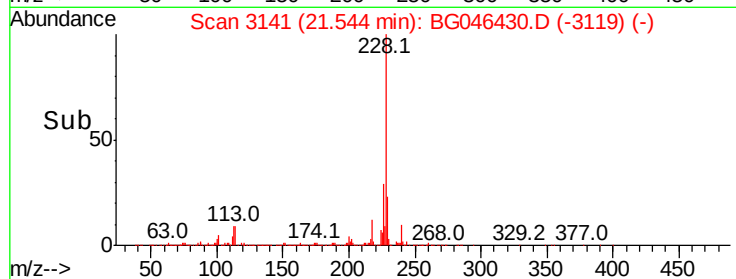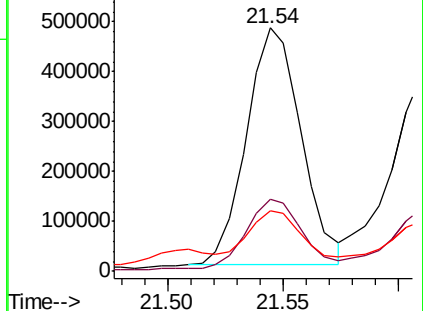

#24

Benzo(b)fluoranthene

Concen: 26.882 ng/ul

RT: 23.70 min Scan# 3508

Delta R.T. 0.00 min

Lab File: BG046430.D

Acq: 22 Aug 2020 2:48


Tgt Ion:252 Resp: 1014612

Ion Ratio Lower Upper

252 100

253 24.0 17.8 26.6



125 8.2 6.4 9.6

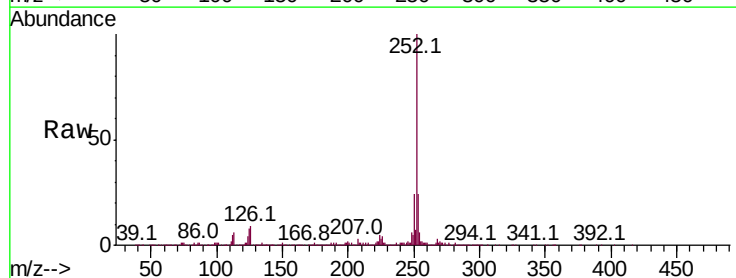


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



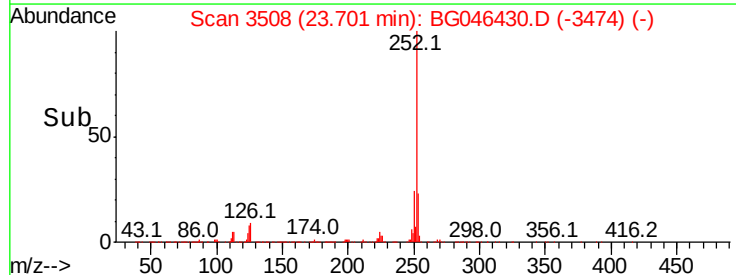
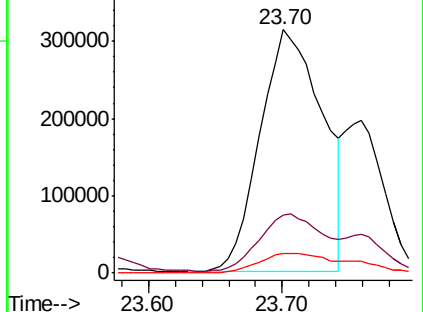


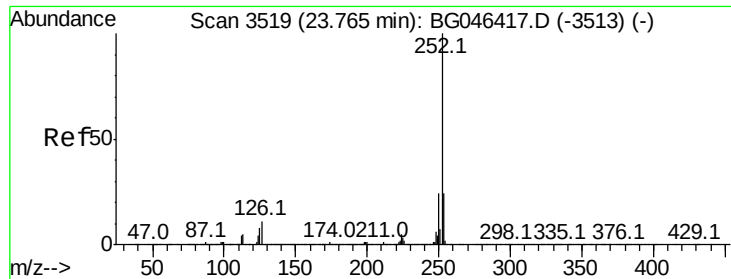

#25
Benzo(k)fluoranthene
Concen: 27.099 ng/ul
RT: 23.70 min Scan# 3508
Delta R.T. -0.06 min
Lab File: BG046430.D
Acq: 22 Aug 2020 2:48




Instrument :
BNA_G
ClientSampleId :
BFMX5


Tot Ion:252 Resp: 1014612
Ion Ratio Lower Upper
252 100
253 24.0 18.5 27.7
125 8.2 6.2 9.2

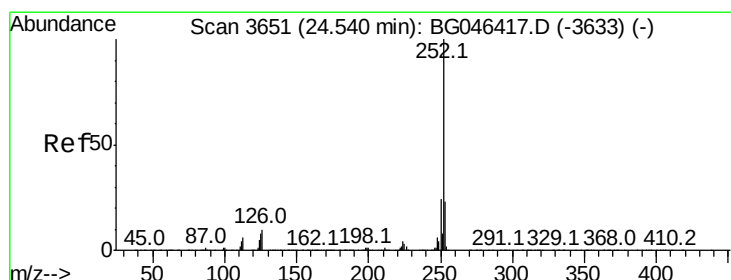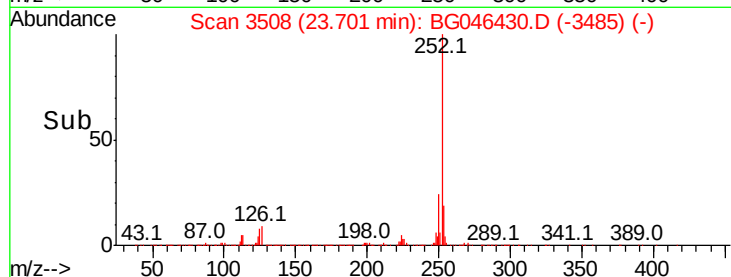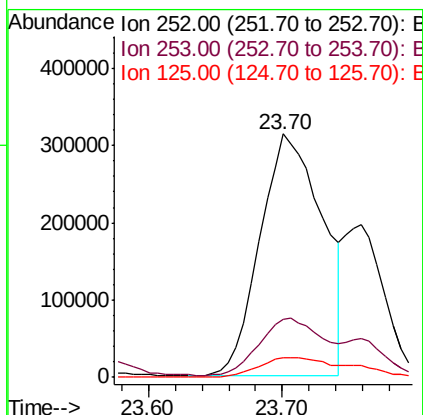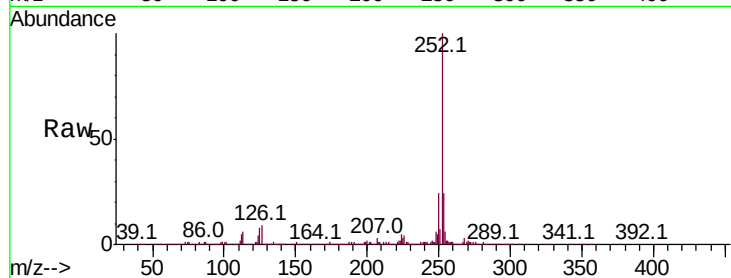

#27
Benzo(a)pyrene
Concen: 25.541 ng/ul
RT: 24.54 min Scan# 3651
Delta R.T. 0.00 min
Lab File: BG046430.D
Acq: 22 Aug 2020 2:48

Tgt Ion:252 Resp: 885009
Ion Ratio Lower Upper
252 100
253 25.1 17.8 26.8
125 8.3 7.1 10.7

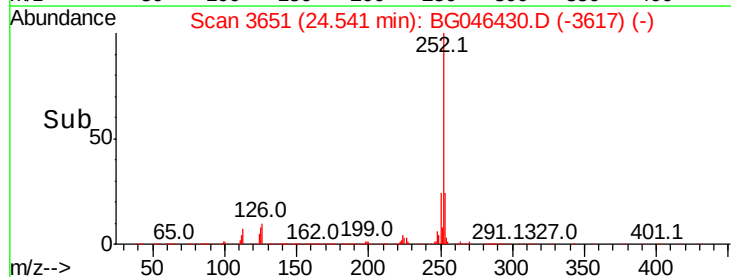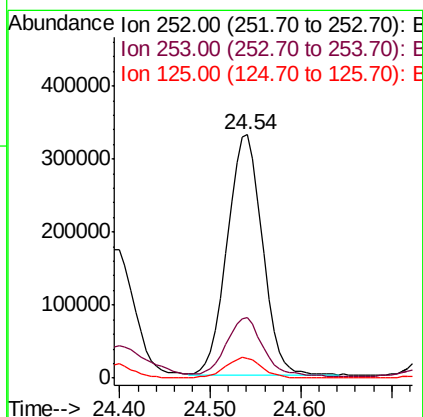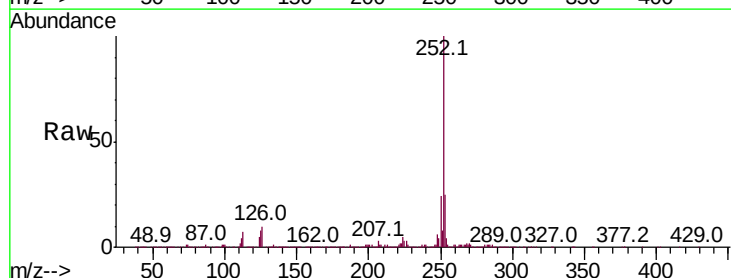




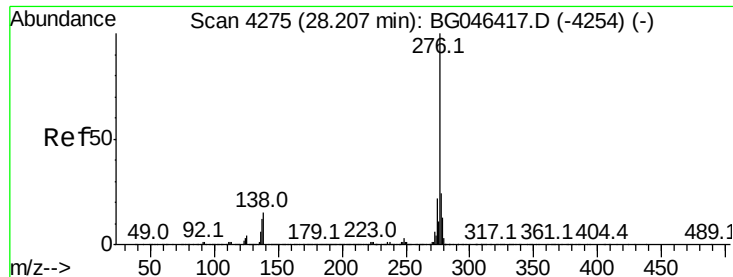


#28

Indeno(1,2,3-cd)pyrene
Concen: 13.057 ng/ul
RT: 28.21 min Scan# 4276
Delta R.T. 0.01 min
Lab File: BG046430.D
Acq: 22 Aug 2020 2:48

Instrument :
BNA_G
ClientSampleId :
BFMX5




Tot Ion:276	Resp:	566519
Ion Ratio	Lower	Upper
276	100	
138	15.6	13.2 19.8
277	26.4	19.9 29.9

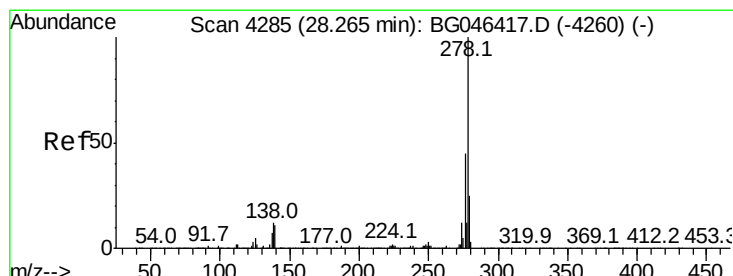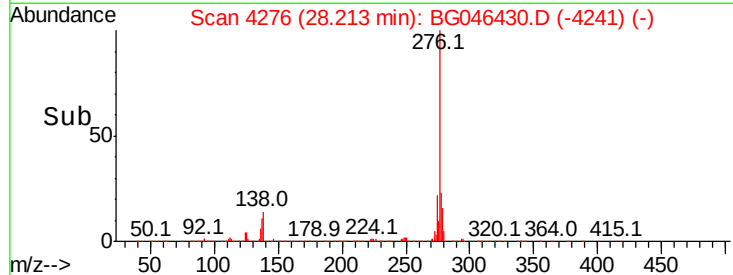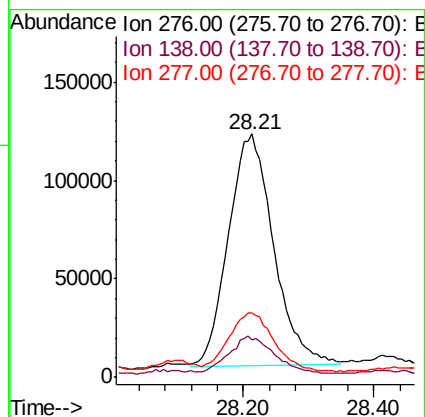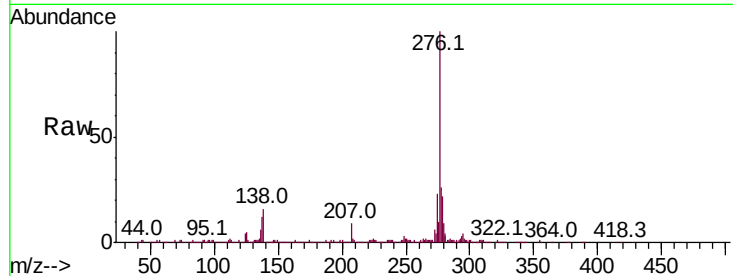


#29

Dibenzo(a,h)anthracene
Concen: 5.162 ng/ul
RT: 28.25 min Scan# 4282
Delta R.T. -0.02 min
Lab File: BG046430.D
Acq: 22 Aug 2020 2:48

Tgt Ion:278	Resp:	181581
Ion Ratio	Lower	Upper
278	100	
139	13.5	9.8 14.8
279	32.9	19.7 29.5#

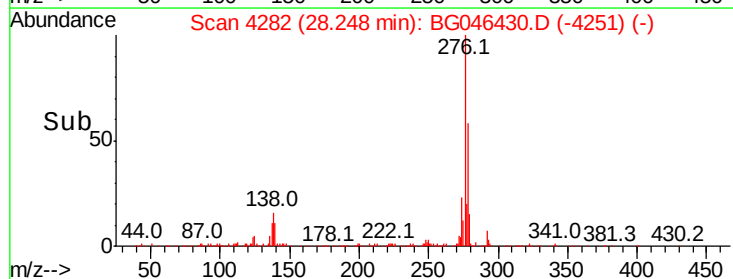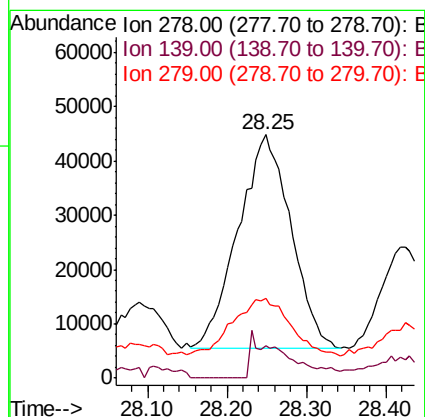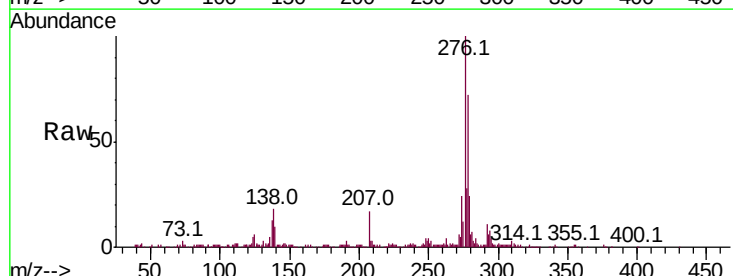

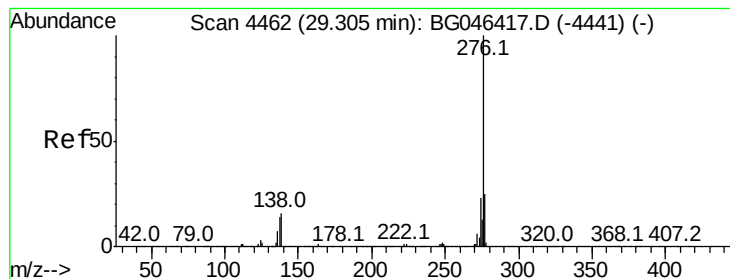

#30

Benzo(a,h,i)perylene

Concen: 11.488 ng/ul

RT: 29.31 min Scan# 4463

Delta R.T. 0.01 min

Lab File: BG046430.D

Acq: 22 Aug 2020 2:48

Instrument :

BNA_G

ClientSampleId :

BFMX5


Tot Ion:276 Resp: 417154

Ion Ratio Lower Upper

276 100

138 15.5 12.9 19.3

277 25.3 19.4 29.0

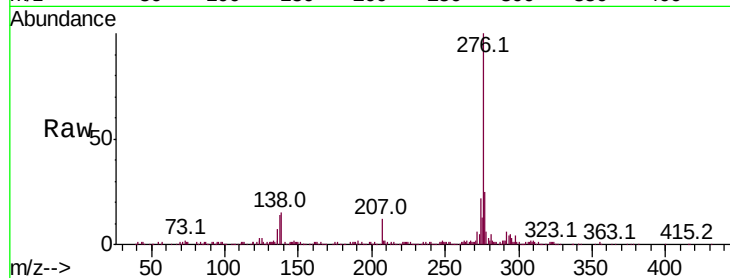

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

