

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081920\
 Data File : BG046432.D
 Acq On : 22 Aug 2020 4:09
 Operator : CG/JU
 Sample : L3649-15
 Misc :
 ALS Vial : 96 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BFMV2

Quant Time: Aug 22 06:56:56 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG081320PAH.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 22 04:33:16 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.94	152	94927	20.00	ng/ul	0.00
2) Naphthalene-d8	10.74	136	390237	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.57	164	258557	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.31	188	579951	20.00	ng/ul	0.00
18) Chrysene-d12	21.56	240	590341	20.00	ng/ul	0.00
23) Perylene-d12	24.67	264	583515	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 2,4-Dichlorophenol-d3	10.36	165	179039	26.65	ng/ul	0.00
7) Acenaphthylene-d8	14.26	160	660827	27.77	ng/ul	0.00
10) Fluorene-d10	15.56	176	491975	26.98	ng/ul	0.00
15) Anthracene-d10	17.41	188	696229	25.90	ng/ul	0.00
19) Pyrene-d10	19.70	212	829863	27.31	ng/ul	0.00
26) Benzo(a)pyrene-d12	24.46	264	909016	28.55	ng/ul	0.00
Target Compounds				Qvalue		
17) Fluoranthene	19.36	202	48142	1.353	ng/ul	98
20) Pyrene	19.73	202	45610	1.177	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081920\
Data File : BG046432.D
Acq On : 22 Aug 2020 4:09
Operator : CG/JU
Sample : L3649-15
Misc :
ALS Vial : 96 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BFMY2

Quant Time: Aug 22 06:56:56 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG081320PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 22 04:33:16 2020
Response via : Initial Calibration




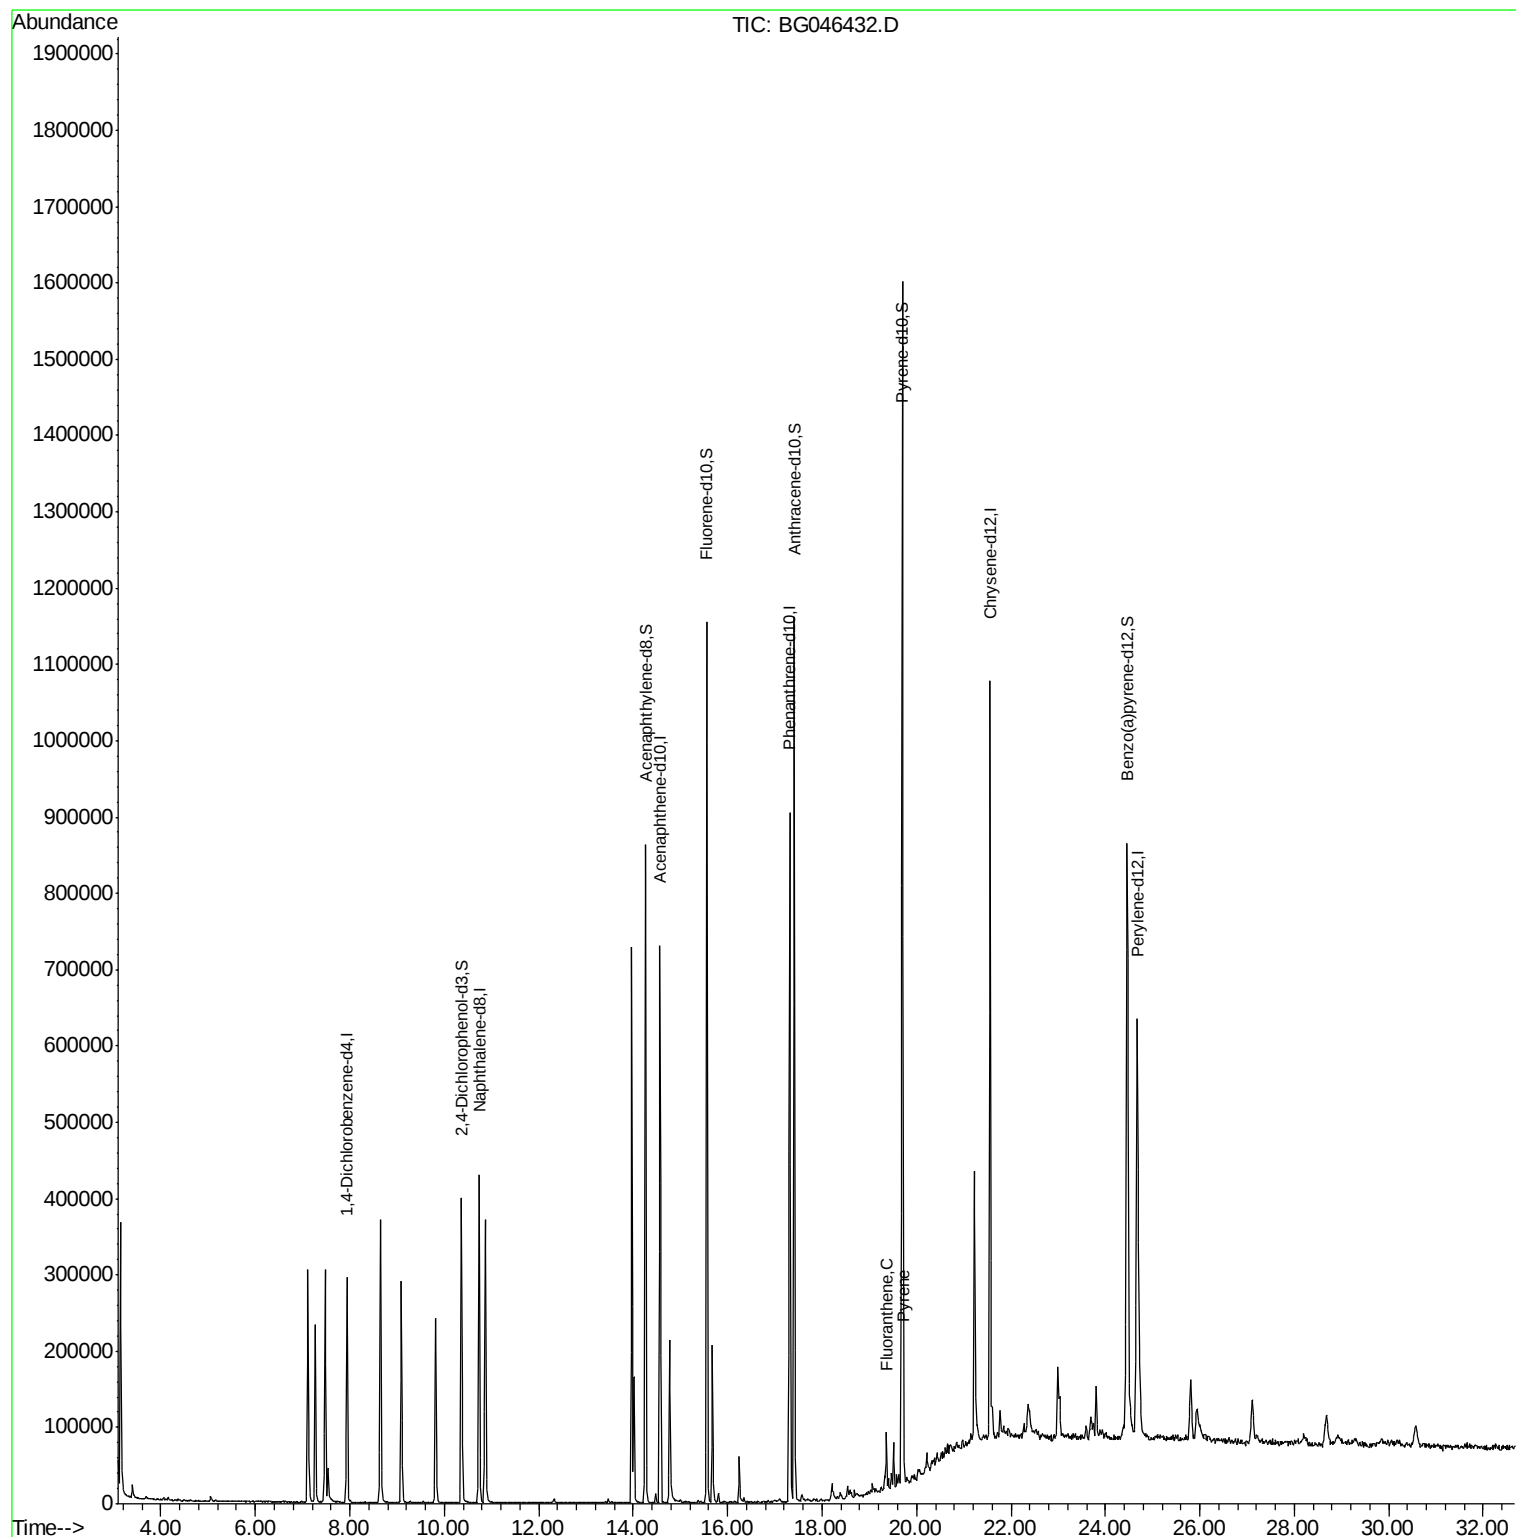


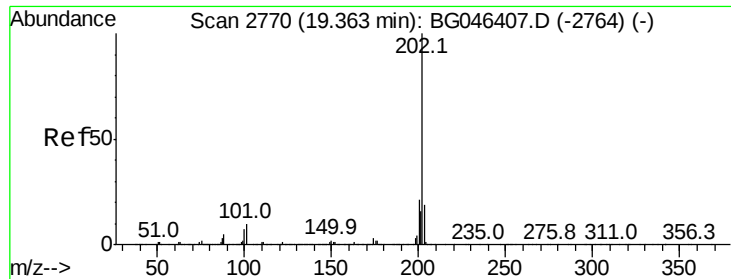

#17
 Fluoranthene
 Concen: 1.353 ng/ul
 RT: 19.36 min Scan# 2770
 Delta R.T. -0.00 min
 Lab File: BG046432.D
 Acq: 22 Aug 2020 4:09

Instrument :
 BNA_G
 ClientSampleId :
 BFMY2

Tot Ion:	202	Resp:	48142
Ion Ratio	Lower	Upper	
202	100		
101	8.7	7.8	11.6
100	6.8	5.9	8.9

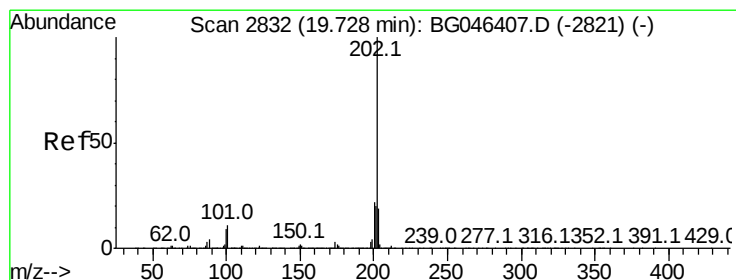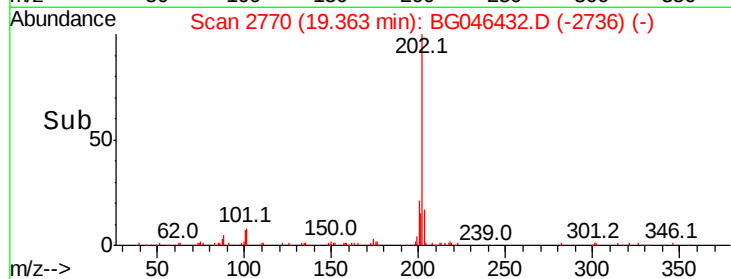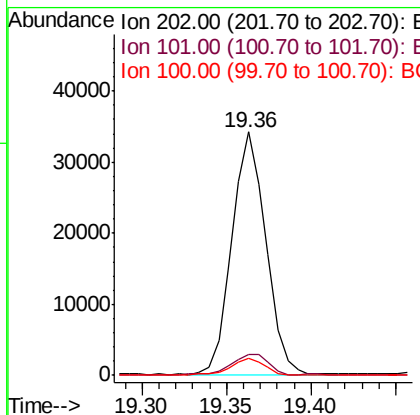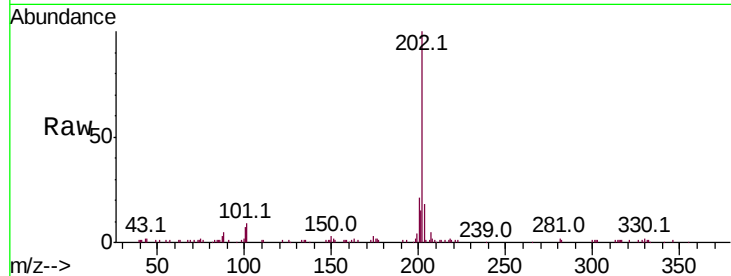

#20
 Pyrene
 Concen: 1.177 ng/ul
 RT: 19.73 min Scan# 2832
 Delta R.T. -0.00 min
 Lab File: BG046432.D
 Acq: 22 Aug 2020 4:09

Tgt Ion:	202	Resp:	45610
Ion Ratio	Lower	Upper	
202	100		
101	10.6	8.9	13.3
100	8.6	7.9	11.9

