
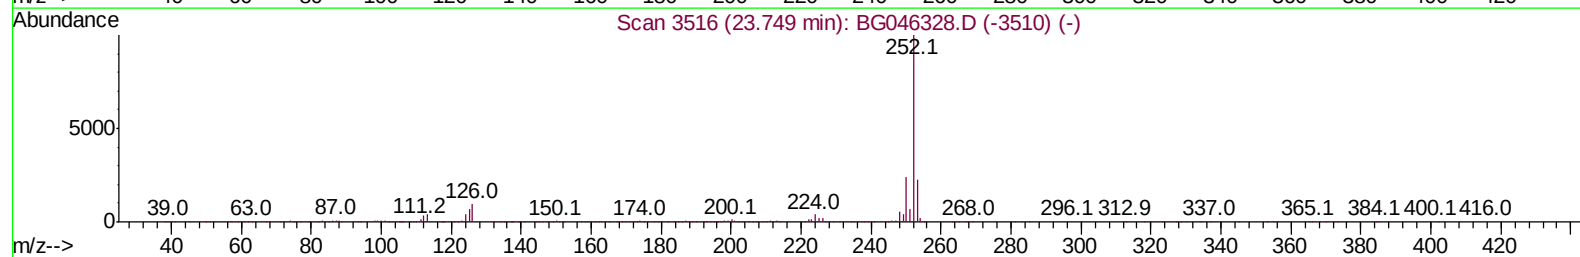
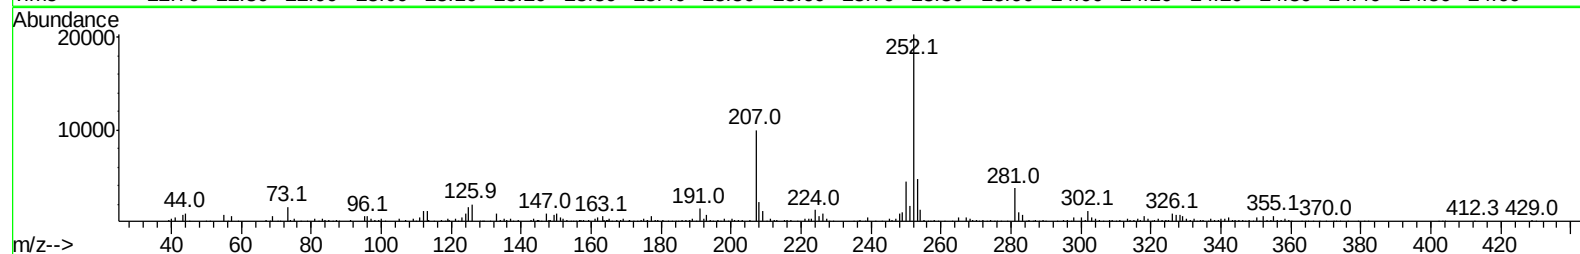


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG081920\
Data File : BG046349.D
Acq On : 19 Aug 2020 16:04
Operator : CG/JU
Sample : L3633-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Aug 19 16:39:53 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG081320PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 19 11:06:56 2020
Response via : Initial Calibration

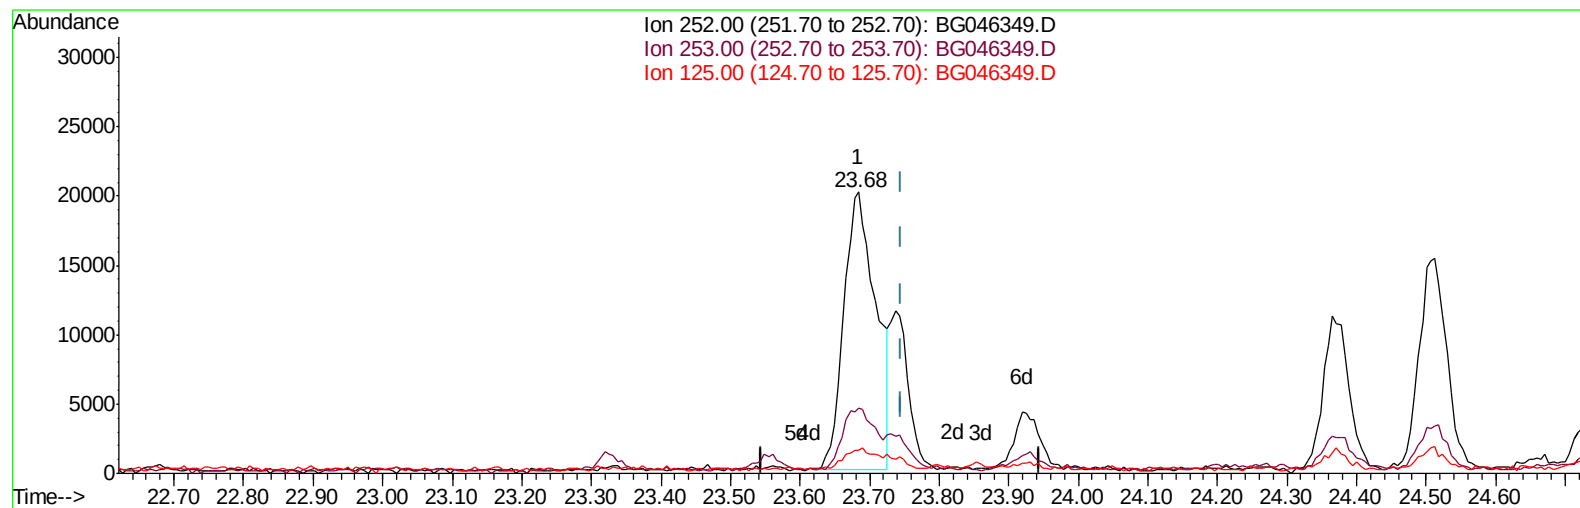

TIC: BG046349.D

(25) Benzo(k)fluoranthene




23.684min (-0.061) 1.52ng/ul

response 64635

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	23.19
125.00	7.70	8.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG081920\
Data File : BG046349.D
Acq On : 19 Aug 2020 16:04
Operator : CG/JU
Sample : L3633-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Aug 19 16:39:53 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG081320PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 19 11:06:56 2020
Response via : Initial Calibration

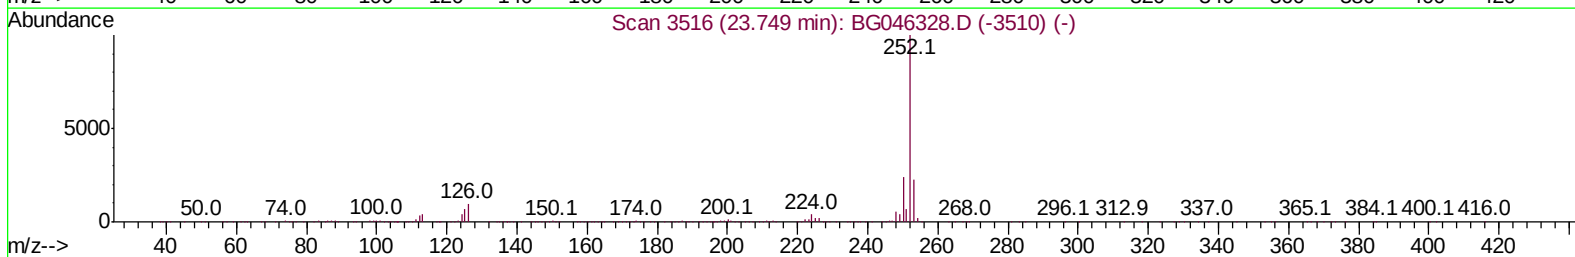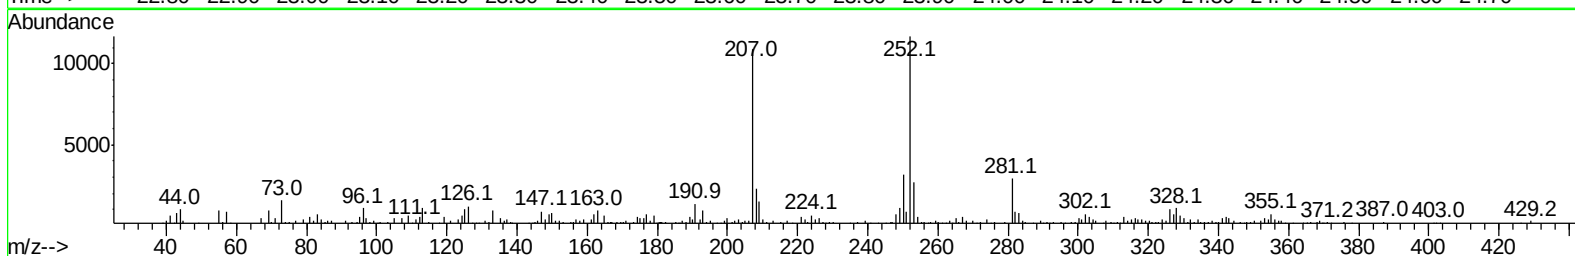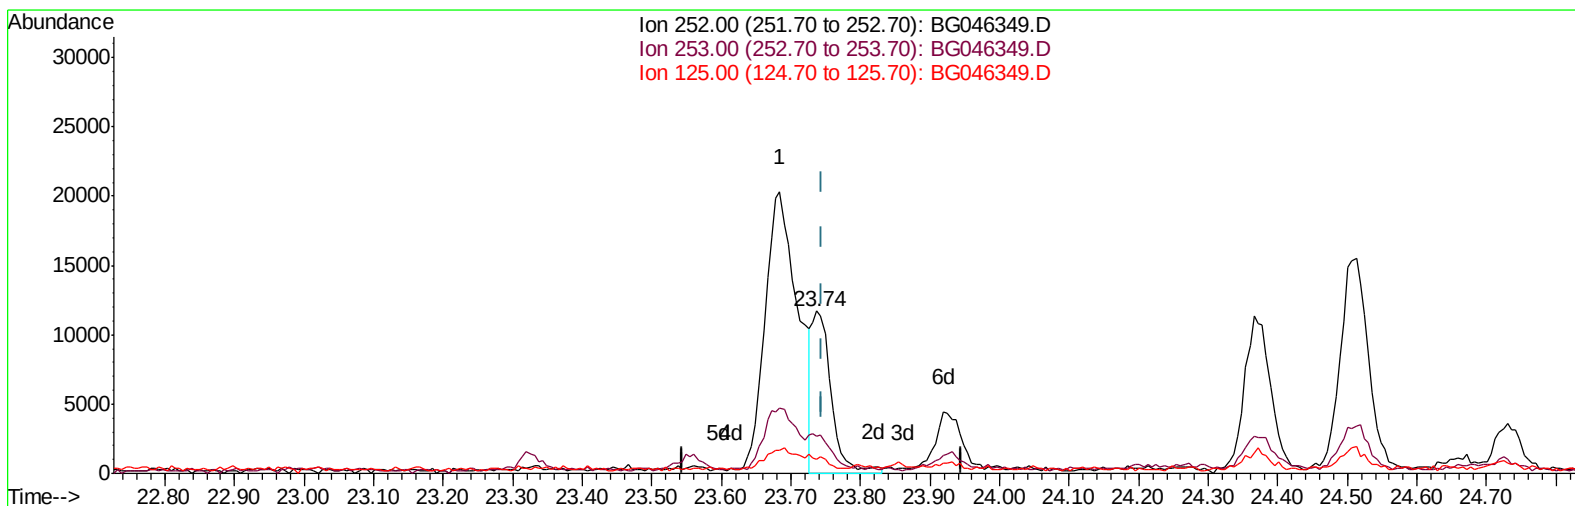

TIC: BG046349.D

(25) Benzo(k)fluoranthene

23.737min (-0.008) 0.53ng/ul m

response 22705

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	23.19
125.00	7.70	9.04
0.00	0.00	0.00