

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081924\
 Data File : BG062461.D
 Acq On : 19 Aug 2024 12:49
 Operator : MA/JU
 Sample : PB162773BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK773

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062461.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.406	16	20	25	rVB	17521	23623	1.16%	0.117%
2	3.811	84	89	104	rBV	219681	360772	17.71%	1.784%
3	4.134	142	144	145	rBV2	2367	2316	0.11%	0.011%
4	4.152	145	147	153	rVB4	7541	9899	0.49%	0.049%
5	4.334	175	178	180	rBV4	2730	3073	0.15%	0.015%
6	4.669	233	235	239	rVB4	1613	2125	0.10%	0.011%
7	7.101	640	649	660	rBV	267482	451580	22.17%	2.233%
8	7.271	671	678	690	rVB	203223	334289	16.41%	1.653%
9	7.477	704	713	720	rBV	212061	347967	17.08%	1.721%
10	7.941	785	792	804	rVB	210872	364833	17.91%	1.804%
11	8.640	904	911	922	rBV	287227	483923	23.75%	2.393%
12	9.092	981	988	996	rBV	210617	370027	18.16%	1.830%
13	9.815	1103	1111	1122	rBV	162374	284616	13.97%	1.408%
14	10.355	1196	1203	1213	rBV	286501	486898	23.90%	2.408%
15	10.737	1261	1268	1276	rVB	351479	615456	30.21%	3.044%
16	10.866	1281	1290	1301	rBV	293841	512516	25.16%	2.535%
17	12.323	1533	1538	1544	rBV3	3625	6480	0.32%	0.032%
18	13.974	1812	1819	1828	rBV	619795	909543	44.65%	4.498%
19	14.256	1859	1867	1878	rBV	665877	1047426	51.42%	5.180%
20	14.567	1913	1920	1928	rBV	659466	1011341	49.64%	5.002%
21	14.749	1944	1951	1966	rBV	302283	486817	23.90%	2.408%
22	15.554	2082	2088	2098	rBV	908423	1396544	68.55%	6.907%
23	15.666	2101	2107	2116	rBV	257116	365600	17.95%	1.808%
24	15.795	2124	2129	2137	rVB4	3659	5658	0.28%	0.028%
25	16.335	2217	2221	2225	rBV2	2856	4530	0.22%	0.022%
26	17.305	2378	2386	2396	rBV	895445	1356360	66.58%	6.708%
27	17.405	2396	2403	2413	rBV2	1114638	1624934	79.76%	8.036%
28	17.598	2432	2436	2438	rBV2	1739	2158	0.11%	0.011%
29	17.980	2497	2501	2505	rVB3	2346	2754	0.14%	0.014%
30	18.198	2534	2538	2546	rBV5	3773	7818	0.38%	0.039%
31	18.274	2548	2551	2554	rVB3	1764	2631	0.13%	0.013%
32	19.067	2681	2686	2688	rBV2	1538	2588	0.13%	0.013%
33	19.255	2714	2718	2725	rBV3	16001	24250	1.19%	0.120%
34	19.325	2725	2730	2738	rVV2	13742	20663	1.01%	0.102%
35	19.390	2738	2741	2745	rVV4	2021	2433	0.12%	0.012%
36	19.472	2750	2755	2756	rBV3	1717	2417	0.12%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081924\
 Data File : BG062461.D
 Acq On : 19 Aug 2024 12:49
 Operator : MA/JU
 Sample : PB162773BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK773

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
 Title : SVOA CALIBRATION

37	19.625	2776	2781	2784	rBV4	8190	9825	0.48%	0.049%
38	19.690	2786	2792	2797	rBV	1446501	2037157	100.00%	10.075%
39	19.972	2838	2840	2842	rBV3	1900	2070	0.10%	0.010%
40	20.171	2872	2874	2877	rVB4	2823	2299	0.11%	0.011%
41	20.236	2883	2885	2890	rVB6	2672	3662	0.18%	0.018%
42	21.229	3050	3054	3059	rVB4	12577	16009	0.79%	0.079%
43	21.446	3089	3091	3092	rBV2	4739	4377	0.21%	0.022%
44	21.546	3101	3108	3116	rBV2	929035	1456809	71.51%	7.205%
45	21.757	3140	3144	3149	rBV5	15125	22938	1.13%	0.113%
46	22.351	3240	3245	3251	rVB4	15346	25155	1.23%	0.124%
47	23.015	3354	3358	3364	rVB5	17074	30238	1.48%	0.150%
48	23.784	3485	3489	3497	rVB4	22039	42777	2.10%	0.212%
49	24.166	3552	3554	3556	rBV3	4513	4618	0.23%	0.023%
50	24.424	3586	3598	3609	rBV2	736982	1922000	94.35%	9.505%
51	24.630	3623	3633	3651	rVB	576254	1625359	79.79%	8.038%
52	25.776	3821	3828	3837	rVB7	22443	68073	3.34%	0.337%
53	27.056	4043	4046	4047	rBV3	8178	9692	0.48%	0.048%




Sum of corrected areas: 20219916

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081924\
Data File : BG062461.D
Acq On : 19 Aug 2024 12:49
Operator : MA/JU
Sample : PB162773BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK773

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

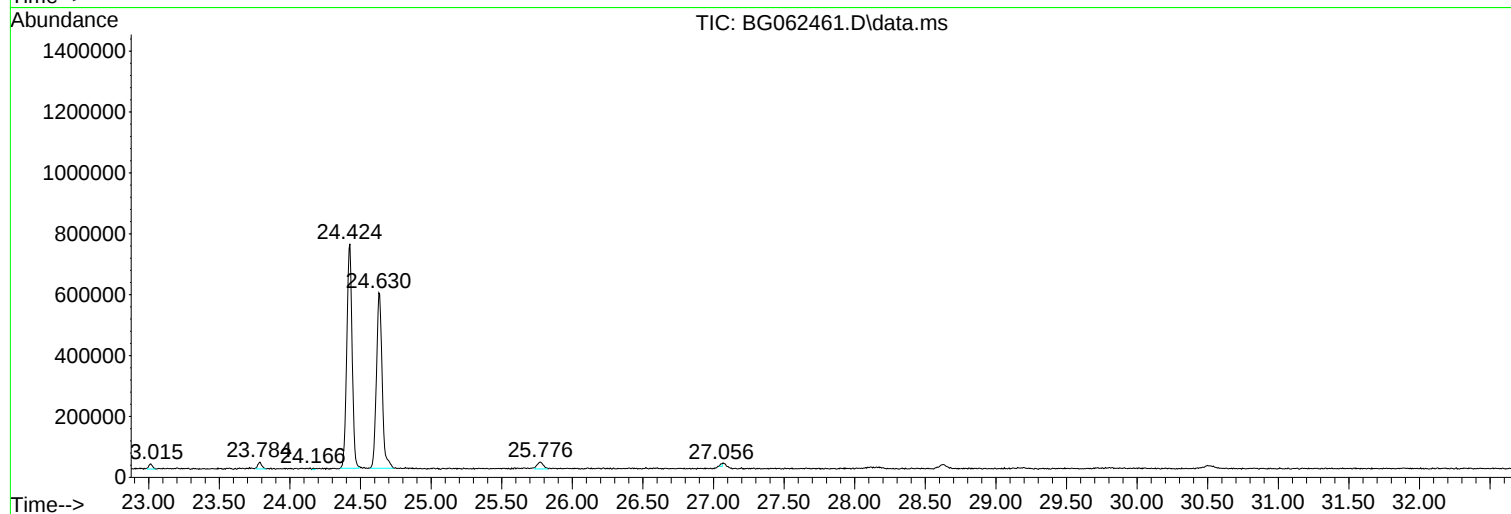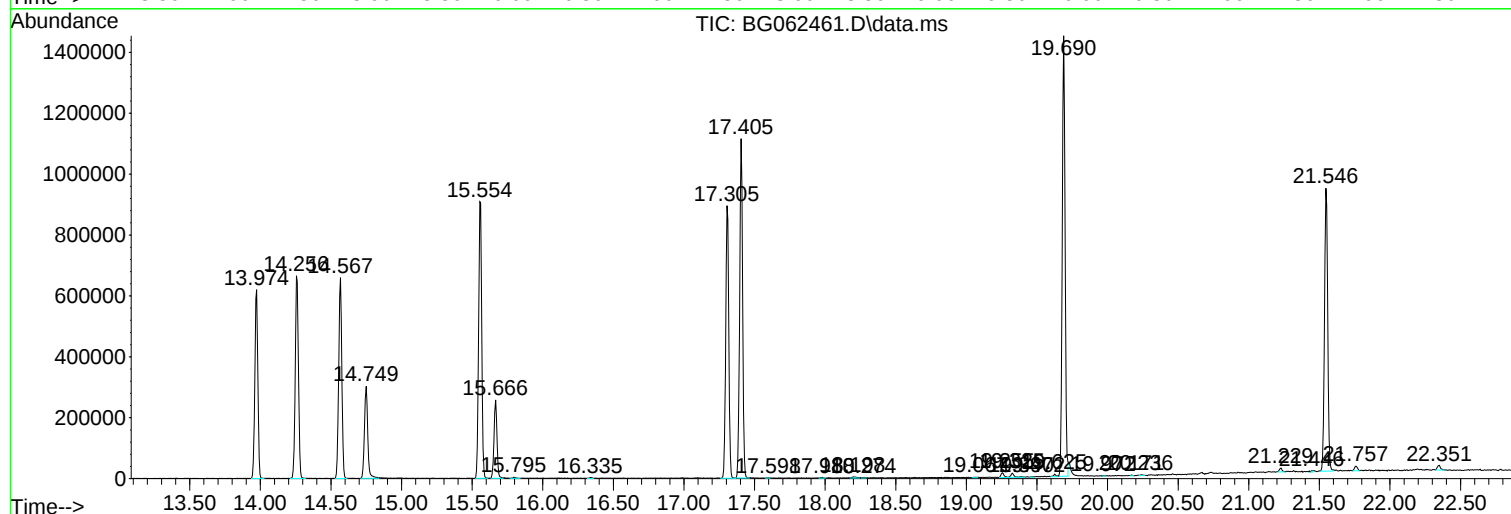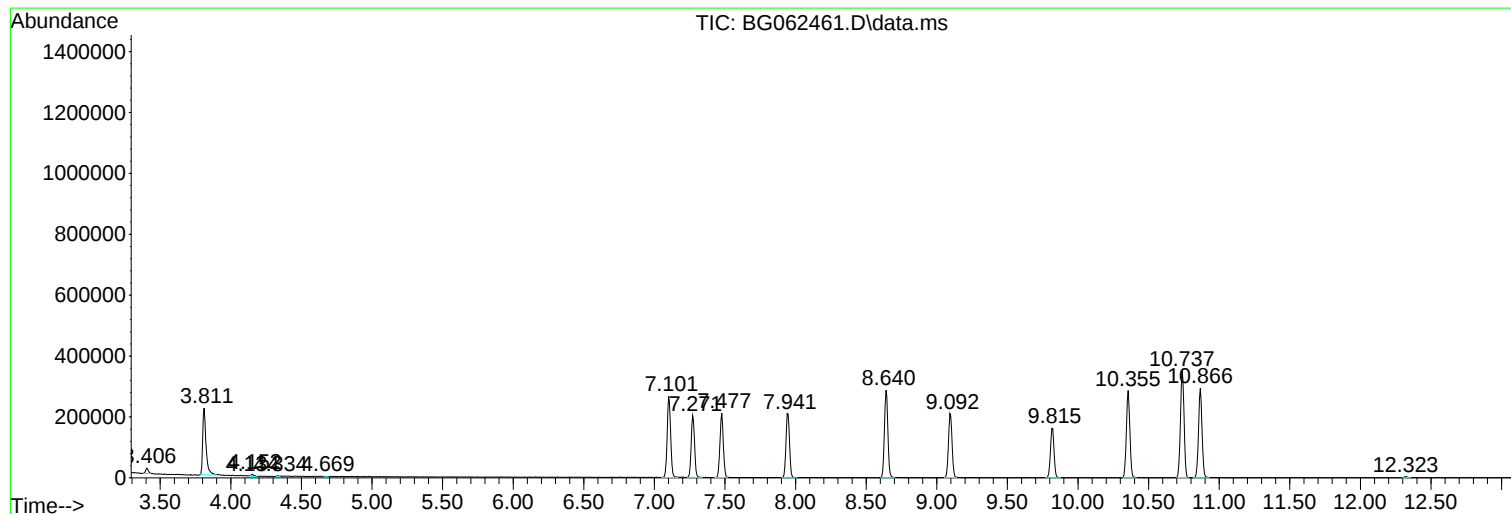

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081924\
Data File : BG062461.D
Acq On : 19 Aug 2024 12:49
Operator : MA/JU
Sample : PB162773BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK773

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081924\
Data File : BG062461.D
Acq On : 19 Aug 2024 12:49
Operator : MA/JU
Sample : PB162773BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK773

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc