

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081924\
 Data File : BG062466.D
 Acq On : 19 Aug 2024 16:31
 Operator : MA/JU
 Sample : PB162773BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK773

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062466.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.410	17	21	28	rVB2	17424	27102	1.29%	0.133%
2	3.810	85	89	103	rBV	199477	330646	15.75%	1.625%
3	4.151	145	147	154	rVB3	5348	6735	0.32%	0.033%
4	4.274	166	168	172	rVB4	2486	2813	0.13%	0.014%
5	7.099	642	649	660	rBV	222394	377195	17.97%	1.853%
6	7.270	670	678	687	rBV	170247	276788	13.19%	1.360%
7	7.475	706	713	723	rVB	203327	340620	16.23%	1.674%
8	7.945	785	793	801	rVB	214720	361488	17.22%	1.776%
9	8.639	904	911	919	rBV	276653	460098	21.92%	2.261%
10	9.097	981	989	996	rBV	204183	363546	17.32%	1.786%
11	9.813	1104	1111	1119	rBV	164826	289260	13.78%	1.421%
12	10.354	1195	1203	1211	rBV	265838	467316	22.27%	2.296%
13	10.736	1258	1268	1278	rVB	322942	566798	27.01%	2.785%
14	10.865	1282	1290	1298	rBV	268931	482911	23.01%	2.373%
15	12.316	1531	1537	1543	rBV	4220	7543	0.36%	0.037%
16	13.967	1811	1818	1827	rBV	605716	861911	41.07%	4.235%
17	14.255	1860	1867	1879	rVB	632225	994974	47.41%	4.889%
18	14.560	1911	1919	1928	rBV	615926	971687	46.30%	4.774%
19	14.748	1944	1951	1962	rBV	294201	483441	23.04%	2.375%
20	15.553	2081	2088	2095	rBV	900099	1355473	64.59%	6.660%
21	15.664	2100	2107	2119	rBV	253083	391326	18.65%	1.923%
22	15.794	2126	2129	2136	rVB2	2954	4423	0.21%	0.022%
23	16.334	2218	2221	2227	rVB3	2930	3357	0.16%	0.016%
24	17.303	2379	2386	2395	rBV	923441	1329255	63.34%	6.531%
25	17.403	2395	2403	2414	rBV	1057722	1590941	75.81%	7.817%
26	17.973	2497	2500	2503	rVB3	2074	2720	0.13%	0.013%
27	18.208	2535	2540	2546	rVB4	2767	5396	0.26%	0.027%
28	18.261	2546	2549	2552	rBV3	1741	2644	0.13%	0.013%
29	19.254	2713	2718	2722	rBV2	15505	22043	1.05%	0.108%
30	19.318	2724	2729	2733	rBV	11983	17884	0.85%	0.088%
31	19.624	2777	2781	2783	rBV4	6078	6359	0.30%	0.031%
32	19.682	2785	2791	2797	rBV	1365548	2031815	96.81%	9.983%
33	20.464	2918	2924	2925	rBV6	3387	5654	0.27%	0.028%
34	20.658	2955	2957	2962	rBV5	7072	9092	0.43%	0.045%
35	20.728	2967	2969	2971	rBV2	3548	3050	0.15%	0.015%
36	21.222	3051	3053	3057	rVB5	7932	7626	0.36%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081924\
Data File : BG062466.D
Acq On : 19 Aug 2024 16:31
Operator : MA/JU
Sample : PB162773BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK773

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Title : SVOA CALIBRATION

37	21.545	3100	3108	3119	rBV	985996	1588433	75.69%	7.804%
38	21.750	3140	3143	3149	rVB4	9369	14019	0.67%	0.069%
39	22.338	3241	3243	3249	rVB2	17391	23265	1.11%	0.114%
40	23.002	3350	3356	3366	rBV2	23138	48304	2.30%	0.237%
41	23.777	3483	3488	3496	rVB4	27409	57232	2.73%	0.281%
42	24.411	3586	3596	3607	rBV2	800611	2098690	100.00%	10.311%
43	24.623	3621	3632	3651	rVB	640458	1816383	86.55%	8.924%
44	25.762	3818	3826	3837	rVB2	36882	104777	4.99%	0.515%
45	27.043	4037	4044	4056	rVB4	32753	109228	5.20%	0.537%
46	30.433	4619	4621	4622	rBV2	5737	4859	0.23%	0.024%
47	30.474	4622	4628	4630	rVV6	13353	26213	1.25%	0.129%




Sum of corrected areas: 20353333

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081924\
Data File : BG062466.D
Acq On : 19 Aug 2024 16:31
Operator : MA/JU
Sample : PB162773BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK773

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

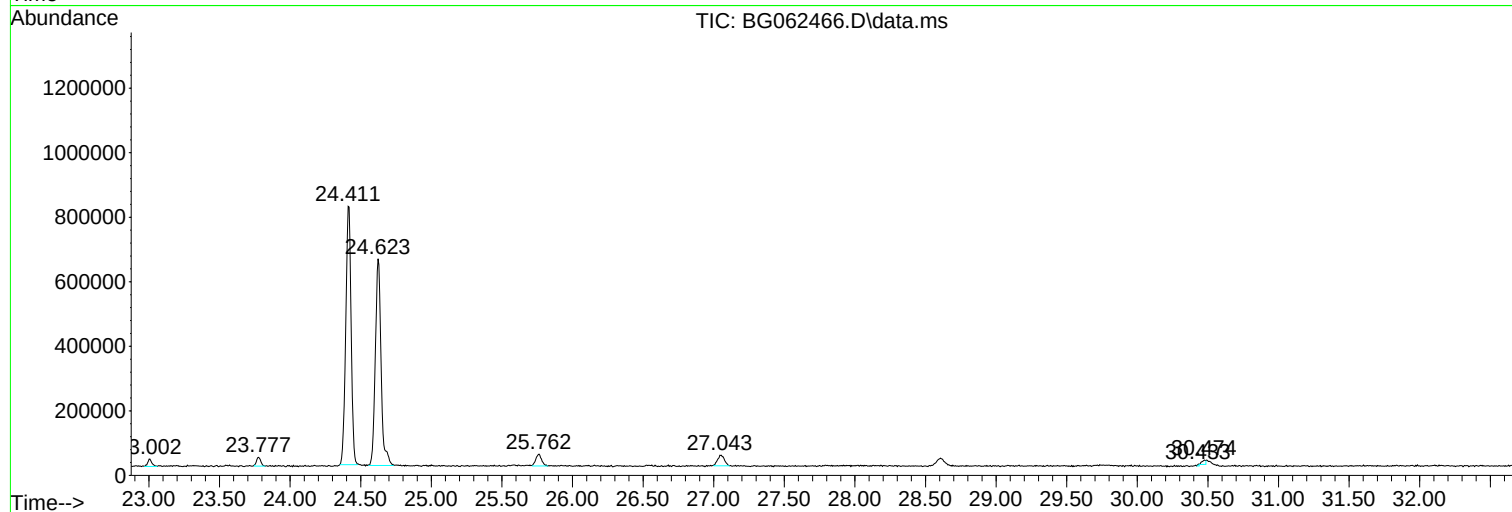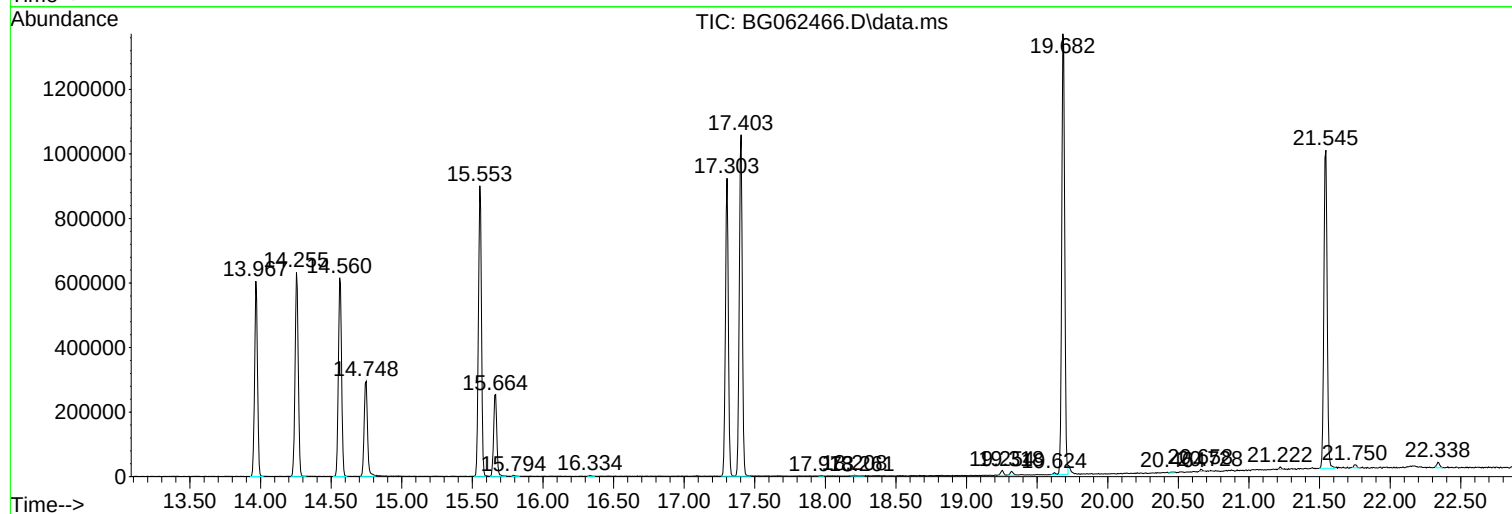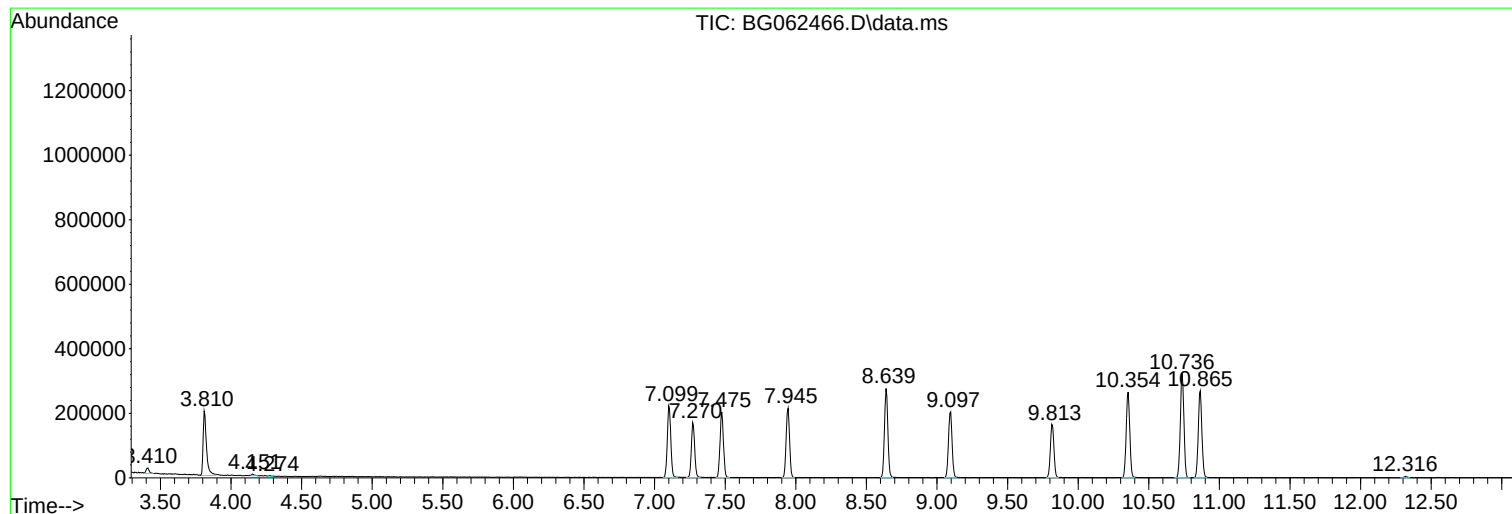

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081924\
Data File : BG062466.D
Acq On : 19 Aug 2024 16:31
Operator : MA/JU
Sample : PB162773BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK773

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG081924\
Data File : BG062466.D
Acq On : 19 Aug 2024 16:31
Operator : MA/JU
Sample : PB162773BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK773

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc