

Data Path : Z:\HPCHEM1\BNA\_G\DATA\BG082016\  
 Data File : BG023812.D  
 Acq On : 20 Aug 2016 11:33  
 Operator : UM/SJ  
 Sample : H4496-10  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 JHPT7

Manual Integrations  
 APPROVED

sohil  
 8/22/2016 3:53:28 PM

Quant Time: Aug 22 04:17:05 2016  
 Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\SOM02.2-EPA-BG081816.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Mon Aug 22 03:42:09 2016  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|---------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 8.09  | 152  | 117839   | 20.00 | ng/ul | 0.00     |
| 18) Naphthalene-d8        | 10.93 | 136  | 487110   | 20.00 | ng/ul | 0.00     |
| 35) Acenaphthene-d10      | 14.77 | 164  | 314382   | 20.00 | ng/ul | 0.00     |
| 61) Phenanthrene-d10      | 17.53 | 188  | 737136m  | 20.00 | ng/ul | 0.00     |
| 75) Chrysene-d12          | 21.85 | 240  | 795116m  | 20.00 | ng/ul | 0.00     |
| 83) Perylene-d12          | 25.24 | 264  | 763425   | 20.00 | ng/ul | 0.02     |

## System Monitoring Compounds

|                                |       |     |         |       |       |      |
|--------------------------------|-------|-----|---------|-------|-------|------|
| 3) 1,4-Dioxane-d8              | 3.47  | 96  | 13771   | 5.30  | ng/uL | 0.00 |
| 5) Phenol-d5                   | 7.25  | 99  | 296346  | 26.82 | ng/ul | 0.00 |
| 7) Bis-(2-Chloroethyl)ether-d  | 7.41  | 67  | 203304  | 26.85 | ng/ul | 0.00 |
| 9) 2-Chlorophenol-d4           | 7.62  | 132 | 209725  | 26.74 | ng/ul | 0.00 |
| 13) 4-Methylphenol-d8          | 8.81  | 113 | 226915  | 26.26 | ng/ul | 0.00 |
| 19) Nitrobenzene-d5            | 9.27  | 128 | 110339  | 28.04 | ng/ul | 0.00 |
| 22) 2-Nitrophenol-d4           | 10.00 | 143 | 126285  | 28.15 | ng/ul | 0.00 |
| 26) 2,4-Dichlorophenol-d3      | 10.56 | 165 | 213213  | 26.28 | ng/ul | 0.00 |
| 29) 4-Chloroaniline-d4         | 11.07 | 131 | 300175  | 30.24 | ng/ul | 0.00 |
| 43) Dimethylphthalate-d6       | 14.16 | 166 | 739624  | 28.38 | ng/ul | 0.00 |
| 46) Acenaphthylene-d8          | 14.46 | 160 | 837889  | 28.39 | ng/ul | 0.00 |
| 51) 4-Nitrophenol-d4           | 14.99 | 143 | 94567m  | 22.45 | ng/ul | 0.00 |
| 57) Fluorene-d10               | 15.76 | 176 | 644193  | 28.31 | ng/ul | 0.00 |
| 62) 4,6-Dinitro-2-methylphenol | 15.90 | 200 | 90904m  | 19.45 | ng/ul | 0.00 |
| 70) Anthracene-d10             | 17.64 | 188 | 964794m | 28.39 | ng/ul | 0.00 |
| 76) Pyrene-d10                 | 19.93 | 212 | 1103213 | 28.92 | ng/ul | 0.00 |
| 87) Benzo(a)pyrene-d12         | 25.00 | 264 | 1032596 | 29.54 | ng/ul | 0.00 |

| Target Compounds      |       |     |        |       |        | Qvalue |
|-----------------------|-------|-----|--------|-------|--------|--------|
| 6) Phenol             | 7.28  | 94  | 29247  | 2.58  | ng/ul# | 67     |
| 44) Dimethylphthalate | 14.21 | 163 | 526283 | 20.19 | ng/ul  | 98     |

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA\_G\DATA\BG082016\  
Data File : BG023812.D  
Acq On : 20 Aug 2016 11:33  
Operator : UM/SJ  
Sample : H4496-10  
Misc :  
ALS Vial : 12 Sample Multiplier: 1


Instrument :  
BNA\_G  
ClientSampleId :  
JHPT7

Manual Integrations  
APPROVED

sohil  
8/22/2016 3:53:28 PM

Quant Time: Aug 22 04:17:05 2016  
Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\SOM02.2-EPA-BG081816.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Mon Aug 22 03:42:09 2016  
Response via : Initial Calibration

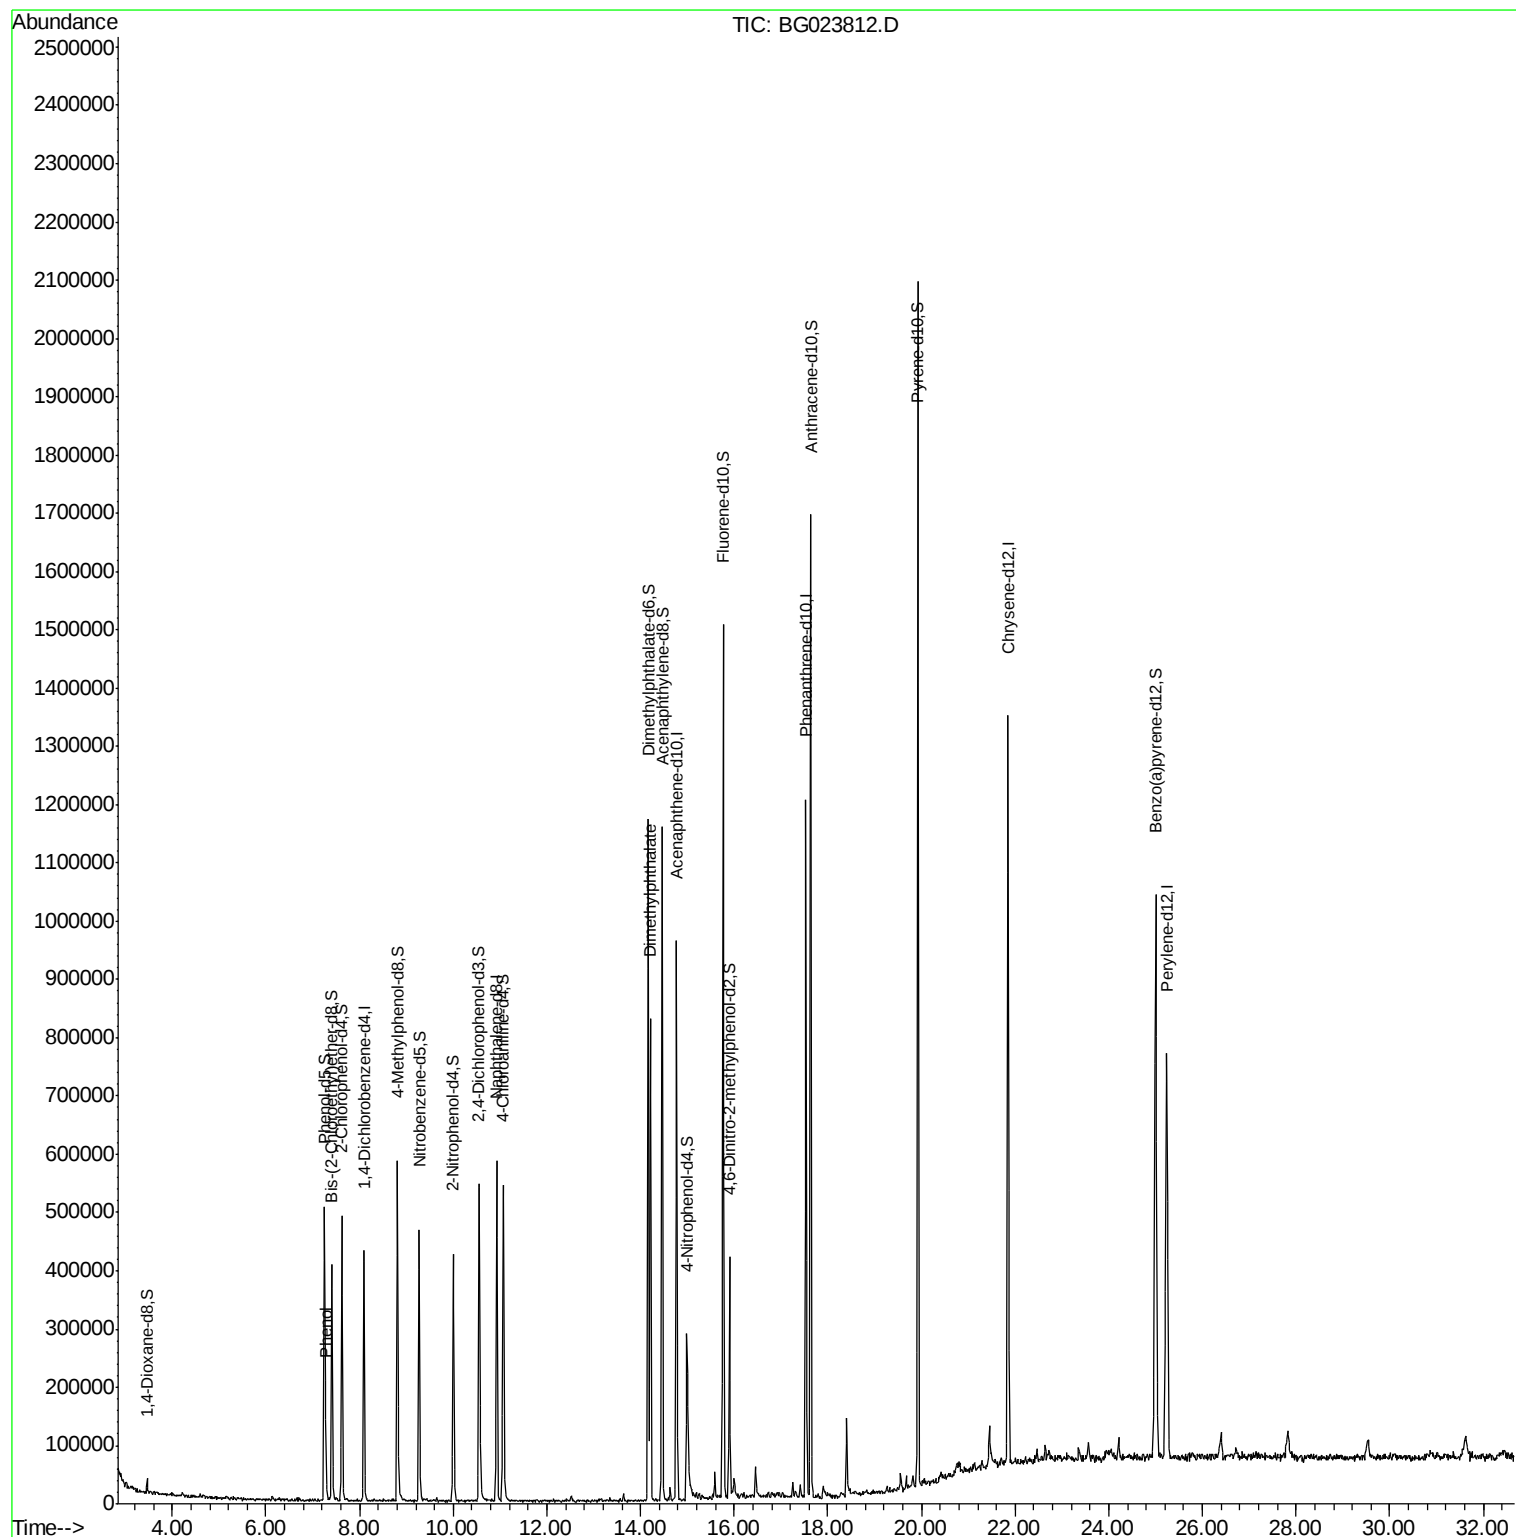

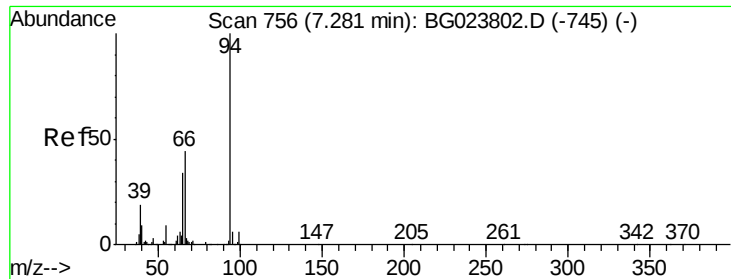

#6

Phenol

Concen: 2.58 ng/ul

RT: 7.28 min Scan# 756

Delta R.T. -0.00 min

Lab File: BG023812.D

Acq: 20 Aug 2016 11:33

Instrument :

BNA\_G





ClientSampled :

JHPT7

|           |       |       |       |
|-----------|-------|-------|-------|
| Tgt Ion:  | 94    | Resp: | 29247 |
| Ion Ratio | Lower | Upper |       |
| 94        | 100   |       |       |
| 65        | 28.1  | 16.8  | 25.2# |
| 66        | 52.9  | 22.6  | 33.8# |

Manual Integrations  
APPROVED

sohil  
8/22/2016 3:53:28 PM

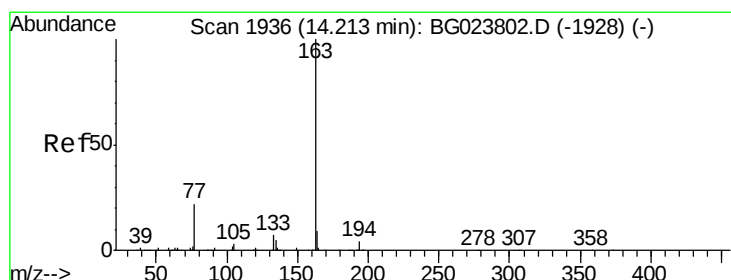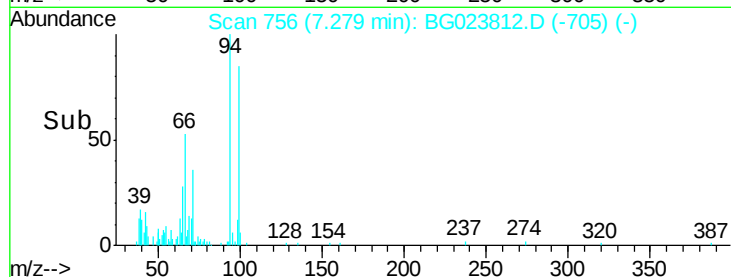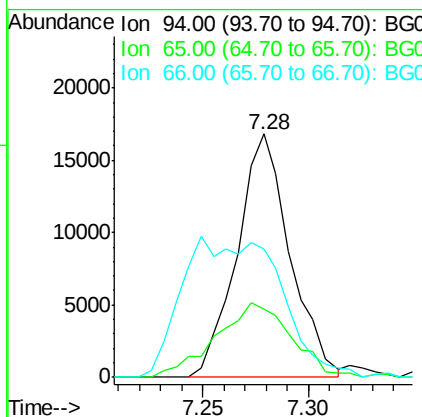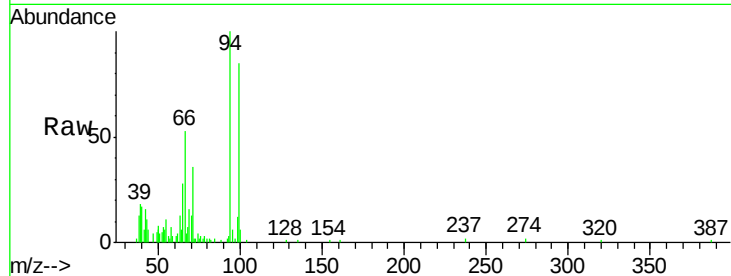

#44

Dimethylphthalate

Concen: 20.19 ng/ul

RT: 14.21 min Scan# 1936

Delta R.T. -0.00 min

Lab File: BG023812.D

Acq: 20 Aug 2016 11:33

|           |       |       |        |
|-----------|-------|-------|--------|
| Tgt Ion:  | 163   | Resp: | 526283 |
| Ion Ratio | Lower | Upper |        |
| 163       | 100   |       |        |
| 194       | 4.1   | 3.4   | 5.2    |
| 164       | 10.1  | 8.8   | 13.2   |

