

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082021\
 Data File : BG049908.D
 Acq On : 20 Aug 2021 12:57
 Operator : CG/JU
 Sample : PB138389BL
 Misc : SFAM-MDL-WATER-02
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK389

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG049908.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.346	49	52	57	rVB3	5300	6207	0.74%	0.076%
2	3.593	92	94	98	rVB2	1514	1300	0.15%	0.016%
3	3.769	121	124	140	rBV	65867	133123	15.81%	1.635%
4	4.109	175	182	186	rBV4	4137	7027	0.83%	0.086%
5	4.386	227	229	235	rVB2	818	1106	0.13%	0.014%
6	4.626	268	270	273	rBV	1825	1622	0.19%	0.020%
7	4.656	273	275	278	rVB2	1309	1264	0.15%	0.016%
8	4.791	296	298	300	rBV	1282	1115	0.13%	0.014%
9	4.897	314	316	319	rVB2	1684	1470	0.17%	0.018%
10	5.913	487	489	494	rBV	840	1114	0.13%	0.014%
11	6.342	558	562	566	rVB	1002	1424	0.17%	0.017%
12	7.147	693	699	712	rBV	107684	202502	24.05%	2.487%
13	7.305	719	726	733	rBV	76470	131955	15.67%	1.620%
14	7.511	755	761	768	rBV	109039	193567	22.99%	2.377%
15	7.981	835	841	849	rBV2	86945	146636	17.42%	1.801%
16	8.186	874	876	881	rBV	884	1302	0.15%	0.016%
17	8.697	955	963	971	rBV	134134	246134	29.24%	3.023%
18	9.038	1020	1021	1024	rBV	940	1130	0.13%	0.014%
19	9.156	1034	1041	1048	rBV	115363	205447	24.40%	2.523%
20	9.884	1158	1165	1175	rVB	102778	190425	22.62%	2.338%
21	10.430	1251	1258	1268	rBV	133866	248552	29.52%	3.052%
22	10.800	1313	1321	1332	rVB	116421	215398	25.58%	2.645%
23	10.941	1337	1345	1353	rBV	136072	254590	30.24%	3.126%
24	11.341	1409	1413	1414	rBV	837	1105	0.13%	0.014%
25	11.435	1427	1429	1434	rBV2	1195	1905	0.23%	0.023%
26	11.652	1462	1466	1468	rVB	1105	1161	0.14%	0.014%
27	11.682	1468	1471	1473	rBV	1355	1134	0.13%	0.014%
28	14.043	1864	1873	1880	rBV	293263	448357	53.26%	5.506%
29	14.337	1916	1923	1932	rBV	296991	472731	56.15%	5.805%
30	14.642	1967	1975	1983	rVB	204886	314924	37.41%	3.867%
31	14.854	2005	2011	2026	rBV3	95739	196539	23.34%	2.414%
32	15.635	2137	2144	2151	rVB	399842	599722	71.23%	7.365%
33	15.758	2160	2165	2172	rBV	129070	202251	24.02%	2.484%
34	15.876	2180	2185	2189	rVB4	3910	5502	0.65%	0.068%
35	16.305	2256	2258	2261	rBV	1186	1194	0.14%	0.015%
36	16.845	2346	2350	2354	rBV	656	1291	0.15%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082021\
 Data File : BG049908.D
 Acq On : 20 Aug 2021 12:57
 Operator : CG/JU
 Sample : PB138389BL
 Misc : SFAM-MDL-WATER-02
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK389

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

37	17.174	2401	2406	2407	rBV	1162	1739	0.21%	0.021%
38	17.392	2436	2443	2449	rBV	272496	407259	48.37%	5.001%
39	17.491	2452	2460	2467	rVV	453555	687717	81.69%	8.445%
40	17.715	2494	2498	2501	rBV	1011	1214	0.14%	0.015%
41	17.938	2531	2536	2540	rBV	1057	1641	0.19%	0.020%
42	18.149	2569	2572	2575	rBV	811	1288	0.15%	0.016%
43	18.243	2586	2588	2592	rVB	973	1268	0.15%	0.016%
44	19.348	2772	2776	2779	rBV2	3799	4559	0.54%	0.056%
45	19.418	2784	2788	2791	rVB2	5362	6811	0.81%	0.084%
46	19.571	2811	2814	2817	rBV3	1490	2327	0.28%	0.029%
47	19.618	2817	2822	2825	rVB2	2231	3529	0.42%	0.043%
48	19.659	2825	2829	2830	rBV3	2264	3012	0.36%	0.037%
49	19.782	2841	2850	2858	rBV	576738	841902	100.00%	10.339%
50	20.123	2907	2908	2912	rBV4	1927	2467	0.29%	0.030%
51	20.317	2939	2941	2944	rBV3	2127	1926	0.23%	0.024%
52	20.423	2957	2959	2960	rBV2	1891	1623	0.19%	0.020%
53	20.476	2967	2968	2970	rBV2	2319	1644	0.20%	0.020%
54	20.916	3042	3043	3046	rVB3	2564	1947	0.23%	0.024%
55	20.946	3046	3048	3050	rBV3	2346	2138	0.25%	0.026%
56	21.662	3164	3170	3177	rBV2	292875	464457	55.17%	5.704%
57	24.676	3673	3683	3694	rVB2	271372	754204	89.58%	9.262%
58	24.893	3711	3720	3732	rVB2	159631	465241	55.26%	5.713%
59	25.011	3738	3740	3741	rBV2	3507	2015	0.24%	0.025%
60	25.451	3813	3815	3816	rBV	4373	3835	0.46%	0.047%
61	26.215	3943	3945	3948	rBV4	4298	3986	0.47%	0.049%
62	27.307	4129	4131	4132	rBV2	2967	1517	0.18%	0.019%
63	27.366	4137	4141	4142	rBV4	7122	7655	0.91%	0.094%
64	29.364	4479	4481	4483	rVB2	5458	3153	0.37%	0.039%
65	29.381	4483	4484	4486	rBV2	3915	3080	0.37%	0.038%
66	29.475	4498	4500	4503	rBV3	4016	4278	0.51%	0.053%
67	29.704	4537	4539	4541	rBV3	4132	3293	0.39%	0.040%
68	30.462	4666	4668	4670	rBV3	3328	2985	0.35%	0.037%
69	32.177	4958	4960	4965	rVB5	3822	5327	0.63%	0.065%


Sum of corrected areas: 8143263

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082021\
Data File : BG049908.D
Acq On : 20 Aug 2021 12:57
Operator : CG/JU
Sample : PB138389BL
Misc : SFAM-MDL-WATER-02
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK389

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

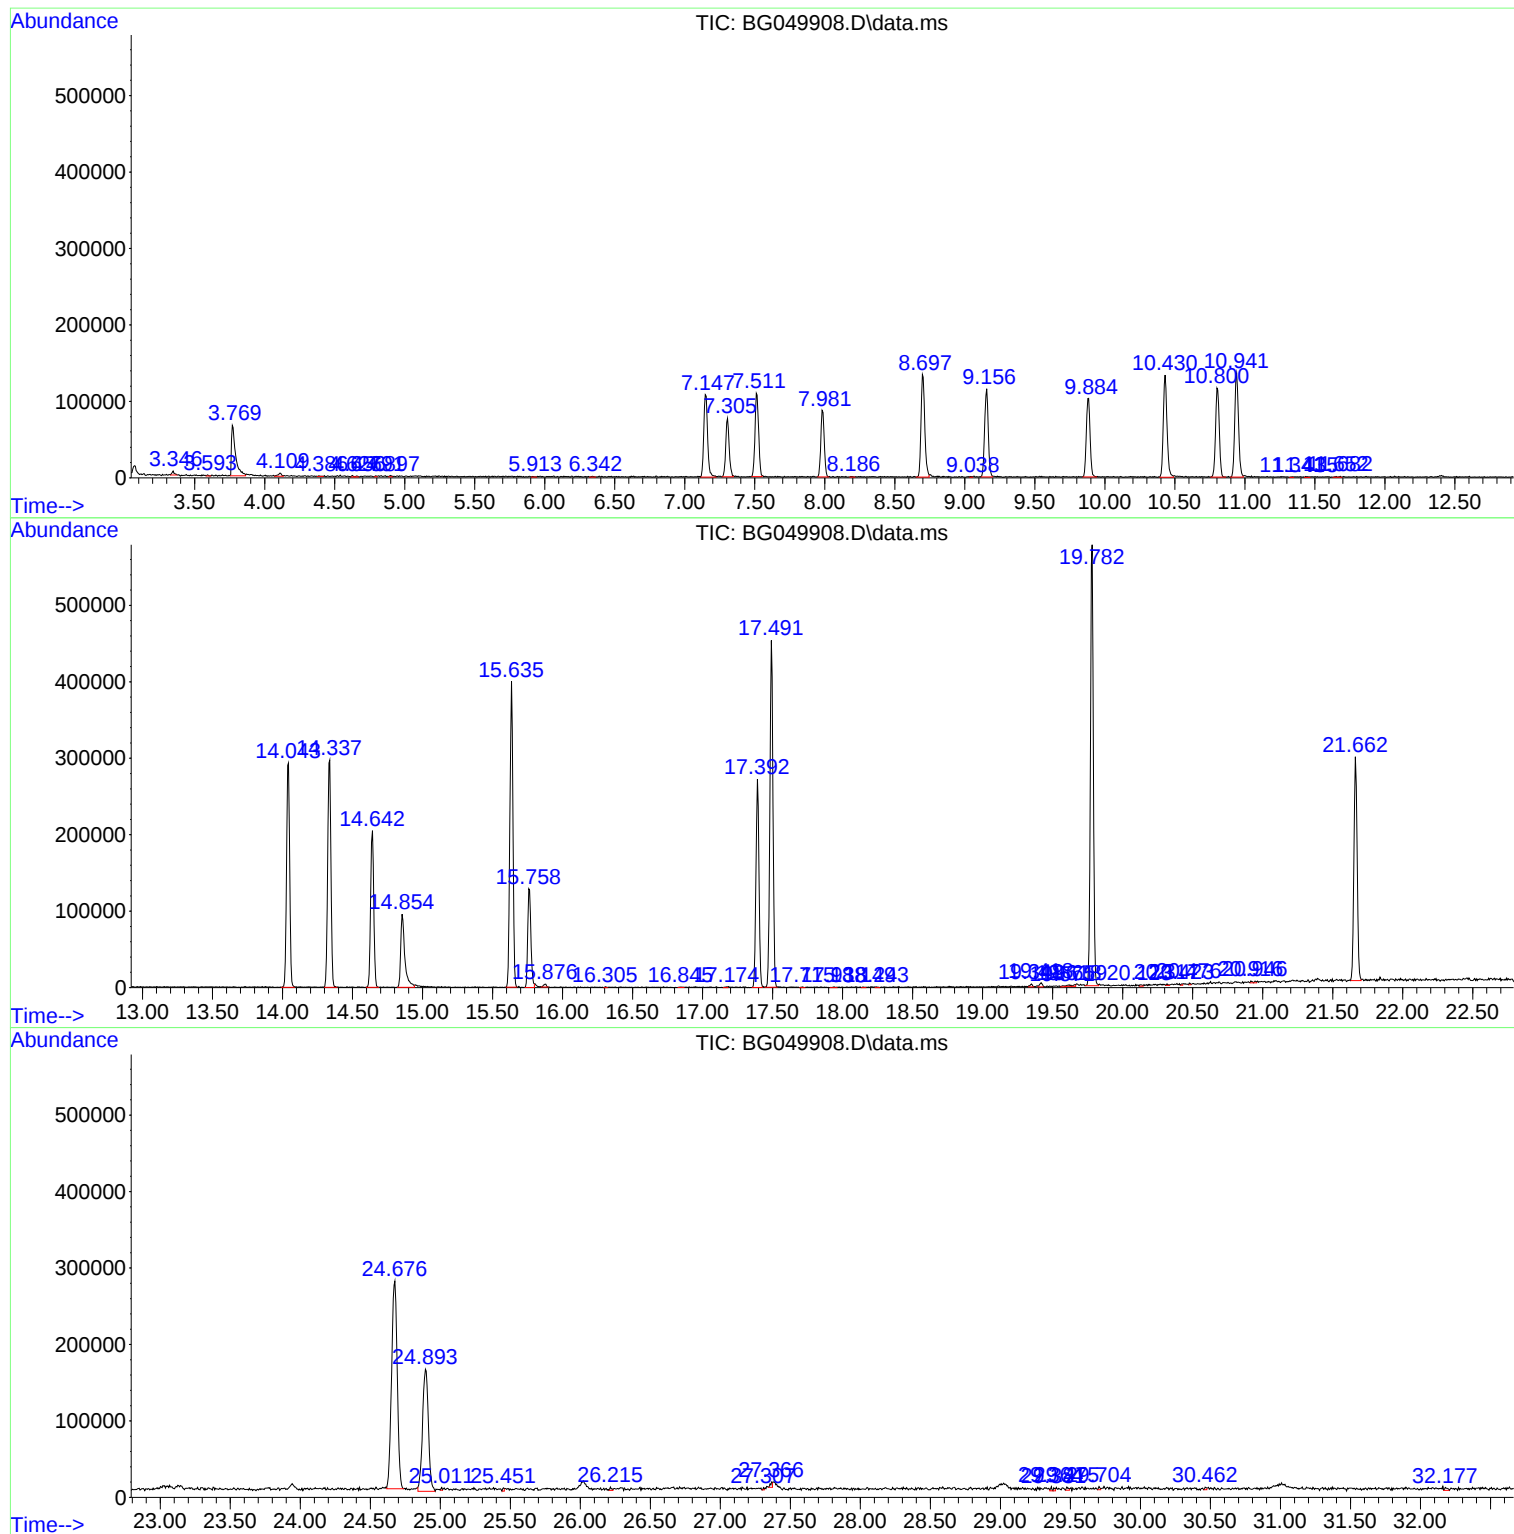

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082021\
Data File : BG049908.D
Acq On : 20 Aug 2021 12:57
Operator : CG/JU
Sample : PB138389BL
Misc : SFAM-MDL-WATER-02
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK389

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082021\
Data File : BG049908.D
Acq On : 20 Aug 2021 12:57
Operator : CG/JU
Sample : PB138389BL
Misc : SFAM-MDL-WATER-02
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK389

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
