

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082021\
 Data File : BG049911.D
 Acq On : 20 Aug 2021 15:53
 Operator : CG/JU
 Sample : PB138425BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK425

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

Signal : TIC: BG049911.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.339	49	51	60	rVB5	7445	12737	1.52%	0.156%
2	3.480	73	75	76	rBV2	1929	1677	0.20%	0.021%
3	3.515	79	81	83	rBV2	1855	1921	0.23%	0.024%
4	3.768	121	124	145	rBV	68172	140655	16.84%	1.723%
5	4.196	195	197	201	rBV2	1206	1159	0.14%	0.014%
6	4.496	246	248	250	rBV2	1242	1197	0.14%	0.015%
7	4.531	252	254	257	rVB2	1547	1211	0.14%	0.015%
8	4.954	323	326	330	rBV3	923	1824	0.22%	0.022%
9	5.330	386	390	393	rBV3	1045	1394	0.17%	0.017%
10	5.430	405	407	409	rBV2	1842	1451	0.17%	0.018%
11	5.612	435	438	439	rBV	1471	1224	0.15%	0.015%
12	5.906	486	488	491	rBV2	1089	1153	0.14%	0.014%
13	6.217	539	541	543	rVB2	1421	1294	0.15%	0.016%
14	6.452	578	581	582	rBV2	1386	1099	0.13%	0.013%
15	6.852	647	649	653	rVB2	1157	1250	0.15%	0.015%
16	7.069	683	686	688	rBV	882	1110	0.13%	0.014%
17	7.145	692	699	708	rVV	113318	204209	24.44%	2.501%
18	7.245	715	716	720	rBV2	1252	1374	0.16%	0.017%
19	7.304	720	726	739	rVB	73786	131168	15.70%	1.606%
20	7.386	739	740	745	rBV	1103	1567	0.19%	0.019%
21	7.510	754	761	770	rBV	112568	198267	23.73%	2.428%
22	7.979	834	841	851	rVB	88896	150860	18.06%	1.847%
23	8.485	924	927	929	rBV	1057	1100	0.13%	0.013%
24	8.696	954	963	976	rBV2	140616	248319	29.72%	3.041%
25	9.148	1034	1040	1049	rBV	113769	204187	24.44%	2.501%
26	9.442	1087	1090	1092	rBV	1496	1437	0.17%	0.018%
27	9.877	1157	1164	1172	rBV2	103763	189629	22.70%	2.322%
28	10.423	1251	1257	1267	rBV2	134755	251983	30.16%	3.086%
29	10.552	1275	1279	1281	rVB	1230	1460	0.17%	0.018%
30	10.799	1313	1321	1328	rBV	119135	212073	25.38%	2.597%
31	10.940	1337	1345	1354	rBV	132993	253161	30.30%	3.100%
32	11.469	1434	1435	1438	rVB	1711	1115	0.13%	0.014%
33	11.510	1438	1442	1444	rBV2	951	1573	0.19%	0.019%
34	11.862	1500	1502	1507	rVB	1247	1851	0.22%	0.023%
35	12.391	1587	1592	1594	rBV3	2514	4140	0.50%	0.051%
36	12.890	1675	1677	1681	rVB2	1031	1217	0.15%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082021\
 Data File : BG049911.D
 Acq On : 20 Aug 2021 15:53
 Operator : CG/JU
 Sample : PB138425BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK425

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

37	13.425	1764	1768	1771	rBV2	765	1168	0.14%	0.014%
38	13.590	1794	1796	1800	rBV	960	1560	0.19%	0.019%
39	13.819	1830	1835	1837	rBV2	706	1393	0.17%	0.017%
40	14.036	1865	1872	1881	rBV	299653	443479	53.08%	5.431%

41	14.330	1915	1922	1931	rVB	295145	469108	56.15%	5.745%
42	14.635	1968	1974	1982	rVB2	204891	312037	37.35%	3.821%
43	14.853	2005	2011	2026	rBV	97737	199509	23.88%	2.443%
44	15.134	2055	2059	2063	rVB	870	1372	0.16%	0.017%
45	15.628	2137	2143	2152	rBV	376003	594063	71.11%	7.275%

46	15.757	2159	2165	2172	rBV	125802	200033	23.94%	2.450%
47	15.875	2180	2185	2189	rVB3	4040	5541	0.66%	0.068%
48	16.204	2240	2241	2246	rBV	910	1138	0.14%	0.014%
49	17.390	2436	2443	2449	rVB	264696	398303	47.67%	4.878%
50	17.490	2453	2460	2466	rBV2	441490	675008	80.79%	8.266%

51	17.602	2477	2479	2482	rBV2	1303	1184	0.14%	0.014%
52	18.430	2618	2620	2624	rVB	1210	1362	0.16%	0.017%
53	18.894	2695	2699	2700	rBV	1319	1520	0.18%	0.019%
54	19.029	2719	2722	2726	rBV2	948	1438	0.17%	0.018%
55	19.346	2770	2776	2783	rVB5	2844	4866	0.58%	0.060%

56	19.417	2783	2788	2791	rBV	5895	8014	0.96%	0.098%
57	19.511	2800	2804	2805	rBV2	1179	1187	0.14%	0.015%
58	19.552	2809	2811	2813	rBV2	1149	1192	0.14%	0.015%
59	19.587	2813	2817	2818	rBV2	1805	2029	0.24%	0.025%
60	19.646	2825	2827	2828	rBV2	1659	1579	0.19%	0.019%

61	19.717	2837	2839	2842	rVB2	2279	2365	0.28%	0.029%
62	19.775	2843	2849	2856	rVB	570306	835472	100.00%	10.231%
63	20.075	2897	2900	2904	rVB3	1440	1993	0.24%	0.024%
64	20.192	2917	2920	2921	rBV2	1698	1717	0.21%	0.021%
65	20.351	2946	2947	2949	rBV2	1628	1236	0.15%	0.015%

66	20.374	2949	2951	2954	rVB4	2141	1581	0.19%	0.019%
67	20.468	2965	2967	2970	rBV3	2074	2198	0.26%	0.027%
68	20.515	2972	2975	2979	rBV3	1733	3203	0.38%	0.039%
69	20.639	2995	2996	2998	rBV	2319	1188	0.14%	0.015%
70	20.674	3000	3002	3005	rBV4	2296	2632	0.32%	0.032%

71	20.786	3019	3021	3023	rBV2	2738	2101	0.25%	0.026%
72	20.821	3025	3027	3029	rVB2	3002	1897	0.23%	0.023%
73	20.950	3047	3049	3053	rVB4	2974	2976	0.36%	0.036%
74	21.097	3072	3074	3075	rBV2	2669	2244	0.27%	0.027%
75	21.661	3163	3170	3179	rBV	294440	472886	56.60%	5.791%

76	22.149	3251	3253	3256	rBV4	3305	3483	0.42%	0.043%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082021\
 Data File : BG049911.D
 Acq On : 20 Aug 2021 15:53
 Operator : CG/JU
 Sample : PB138425BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK425

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
 Title : SVOA CALIBRATION

77	24.216	3603	3605	3607	rVB3	3355	2755	0.33%	0.034%
78	24.240	3607	3609	3613	rBV5	3873	4683	0.56%	0.057%
79	24.434	3640	3642	3643	rBV2	3511	2418	0.29%	0.030%
80	24.669	3672	3682	3693	rVB	278407	762980	91.32%	9.344%
81	24.886	3709	3719	3730	rVB2	168095	465630	55.73%	5.702%
82	25.256	3780	3782	3785	rBV4	3283	3339	0.40%	0.041%
83	25.403	3805	3807	3809	rBV2	3490	2822	0.34%	0.035%
84	25.526	3827	3828	3829	rBV	3937	2161	0.26%	0.026%
85	26.008	3906	3910	3911	rBV4	6524	9240	1.11%	0.113%
86	26.349	3966	3968	3971	rBV3	2708	2470	0.30%	0.030%
87	26.572	4004	4006	4007	rVB2	3957	1663	0.20%	0.020%
88	30.067	4599	4601	4604	rBV4	3612	2984	0.36%	0.037%
89	30.619	4693	4695	4696	rBV2	3530	2275	0.27%	0.028%




Sum of corrected areas: 8165721

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082021\
Data File : BG049911.D
Acq On : 20 Aug 2021 15:53
Operator : CG/JU
Sample : PB138425BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK425

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

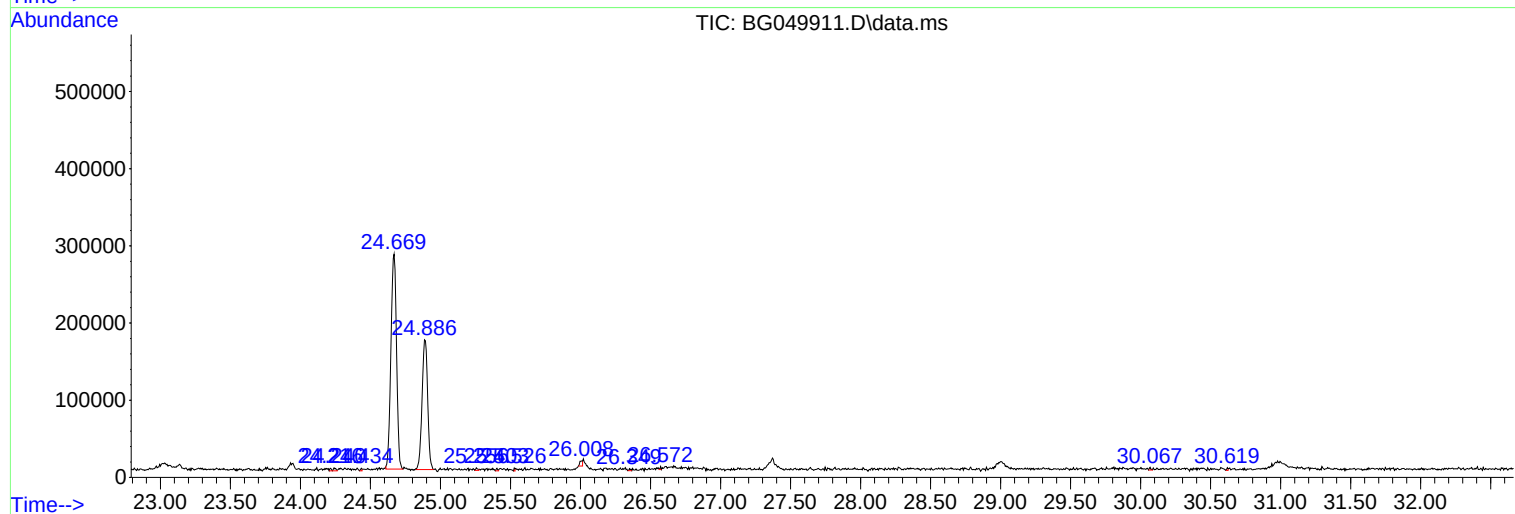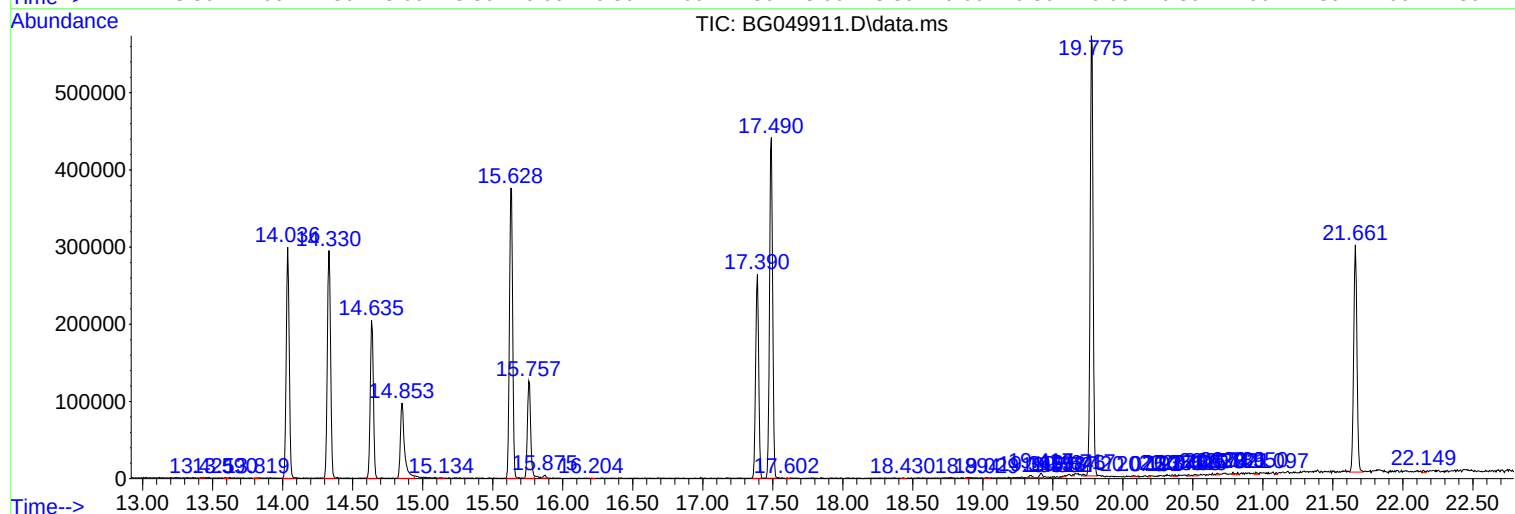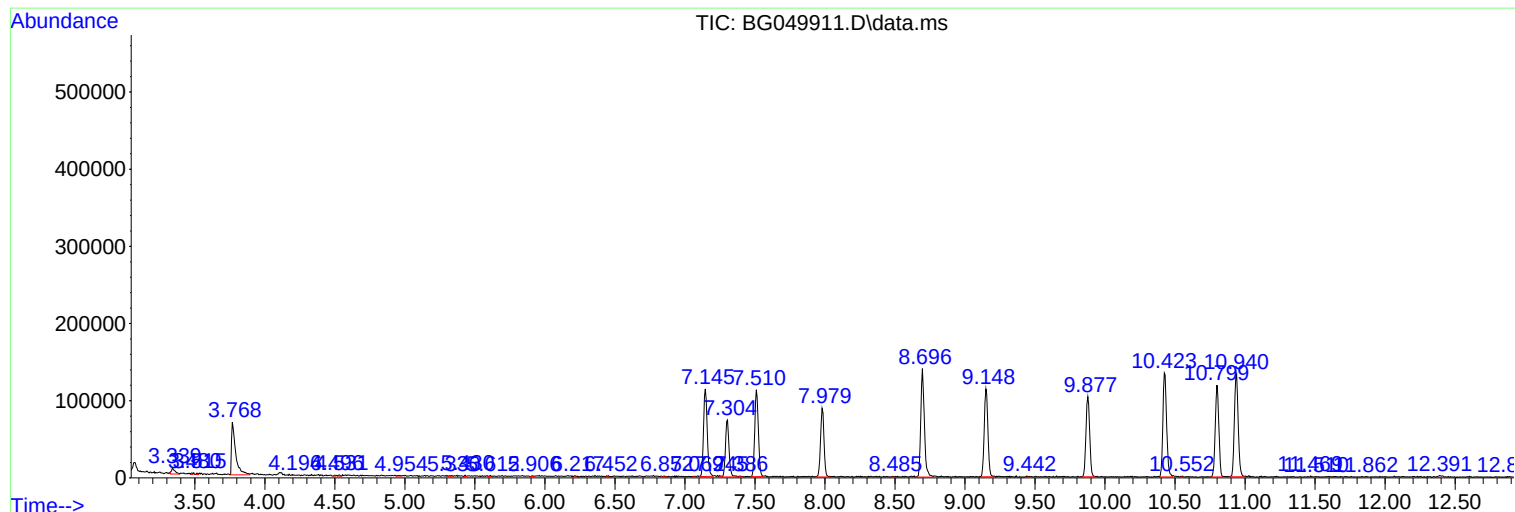

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082021\
Data File : BG049911.D
Acq On : 20 Aug 2021 15:53
Operator : CG/JU
Sample : PB138425BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK425

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082021\
Data File : BG049911.D
Acq On : 20 Aug 2021 15:53
Operator : CG/JU
Sample : PB138425BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK425

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG081921.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
