
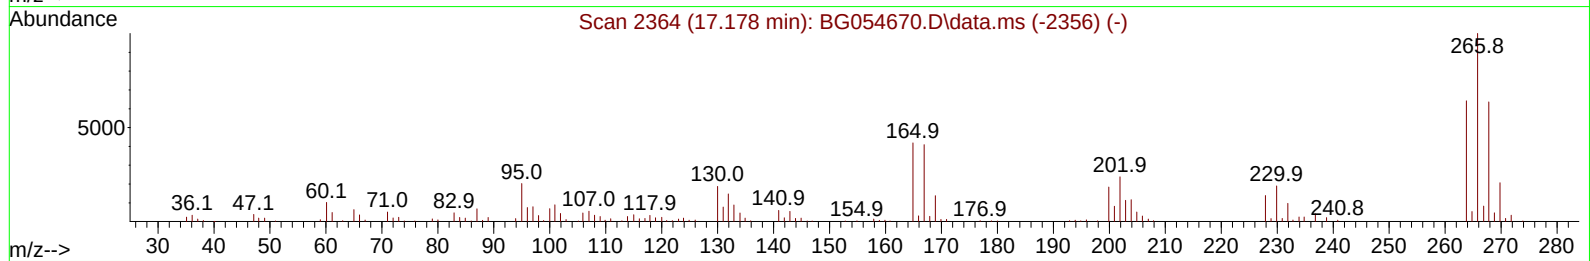
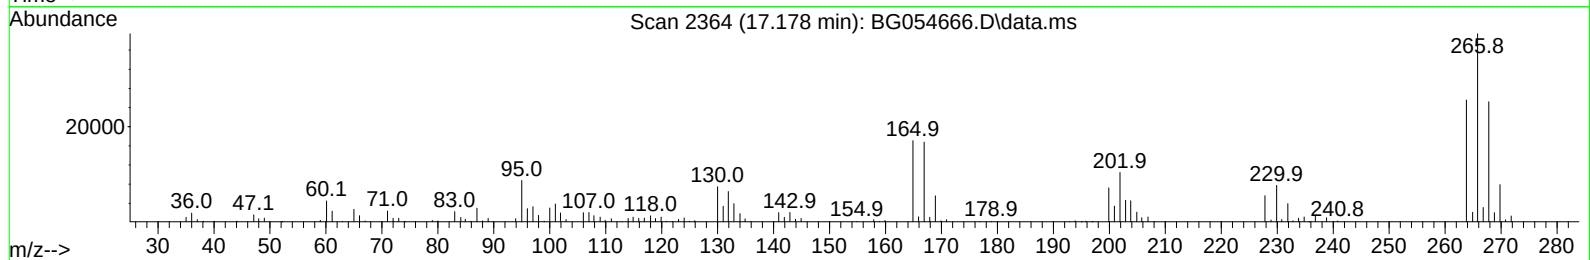


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082022\
Data File : BG054666.D
Acq On : 19 Aug 2022 16:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 05:53:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 22 00:08:53 2022
Response via : Initial Calibration

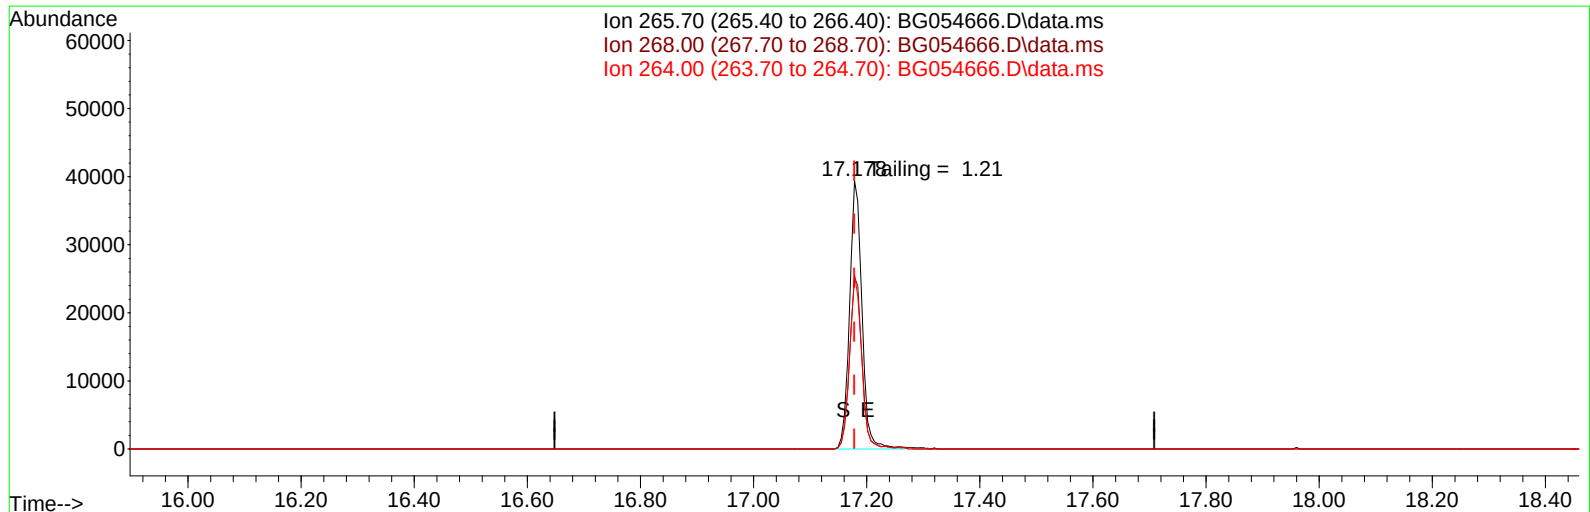

TIC: BG054666.D\data.ms

(70) Pentachlorophenol (C)




17.178min (+ 0.000) 45613.01 ng

response 59821

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.99
264.00	64.20	64.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082022\
Data File : BG054666.D
Acq On : 19 Aug 2022 16:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 22 05:53:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 22 00:08:53 2022
Response via : Initial Calibration

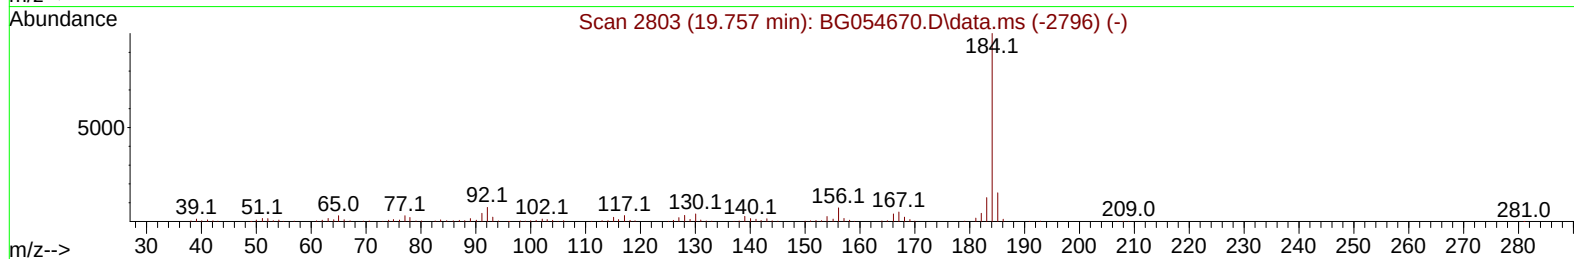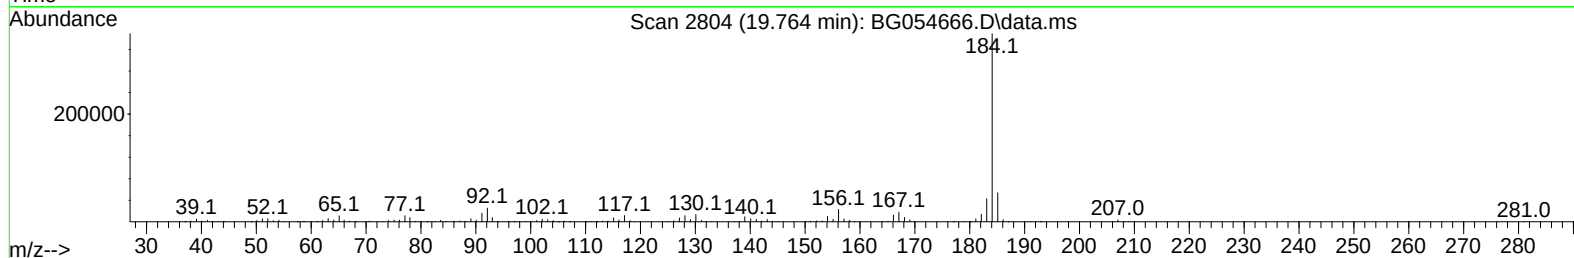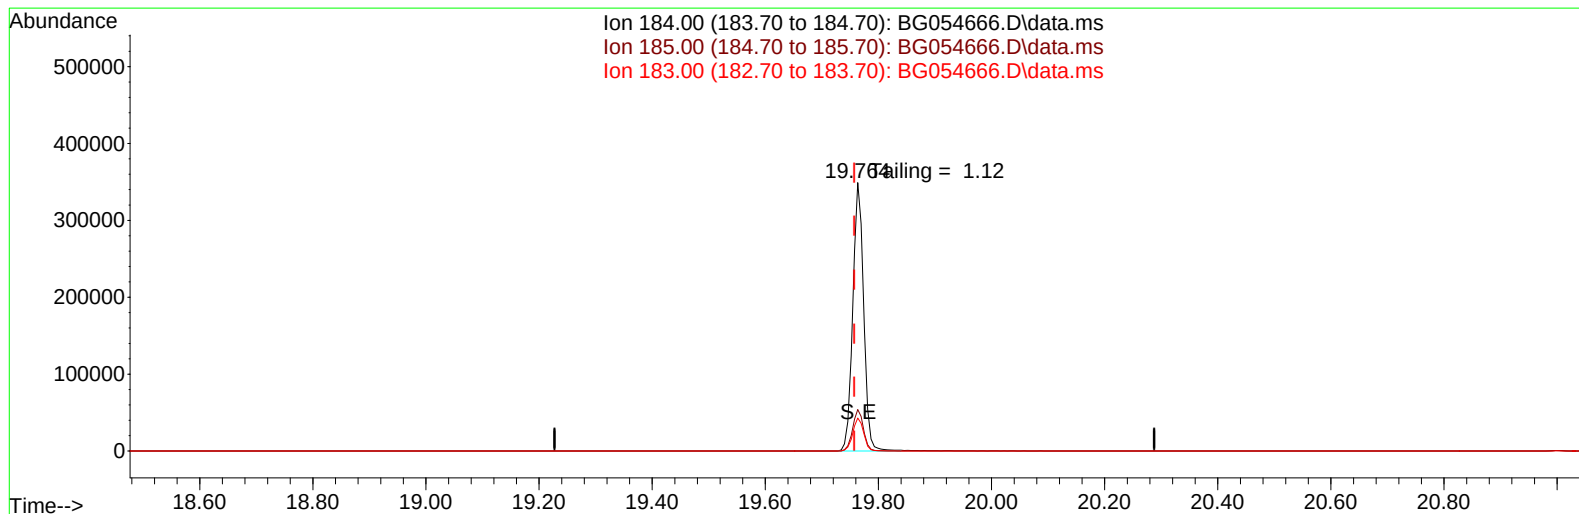

TIC: BG054666.D\data.ms

(77) Benzidine**19.764min (+ 0.006) 88156.77 ng****response 469409**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	15.45
183.00	12.60	12.29
0.00	0.00	0.00