
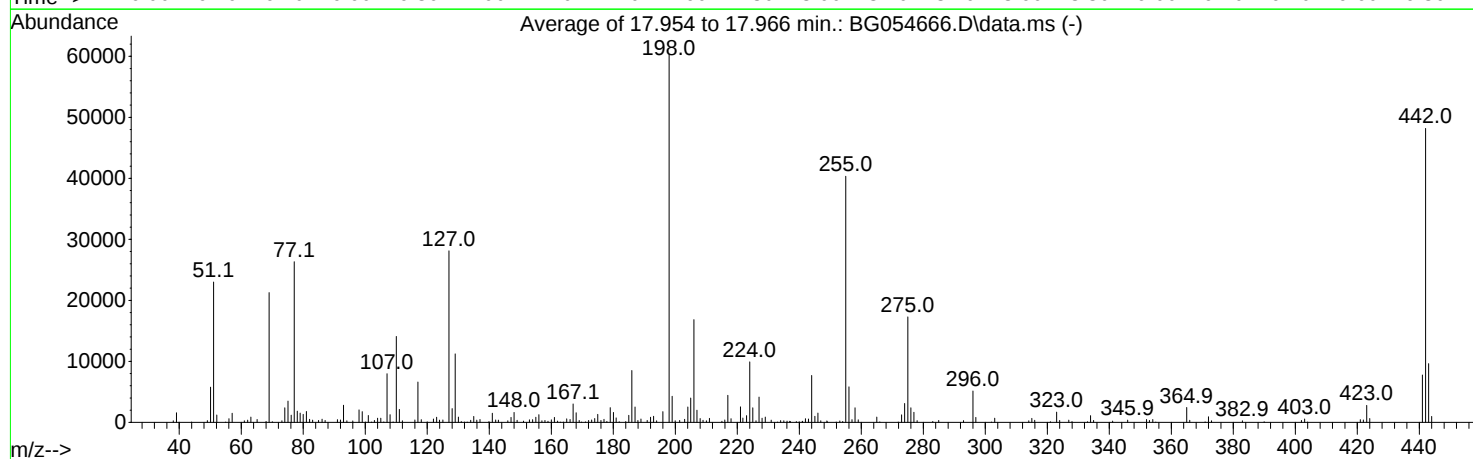


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082022\
 Data File : BG054666.D
 Acq On : 19 Aug 2022 16:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 22 00:08:53 2022

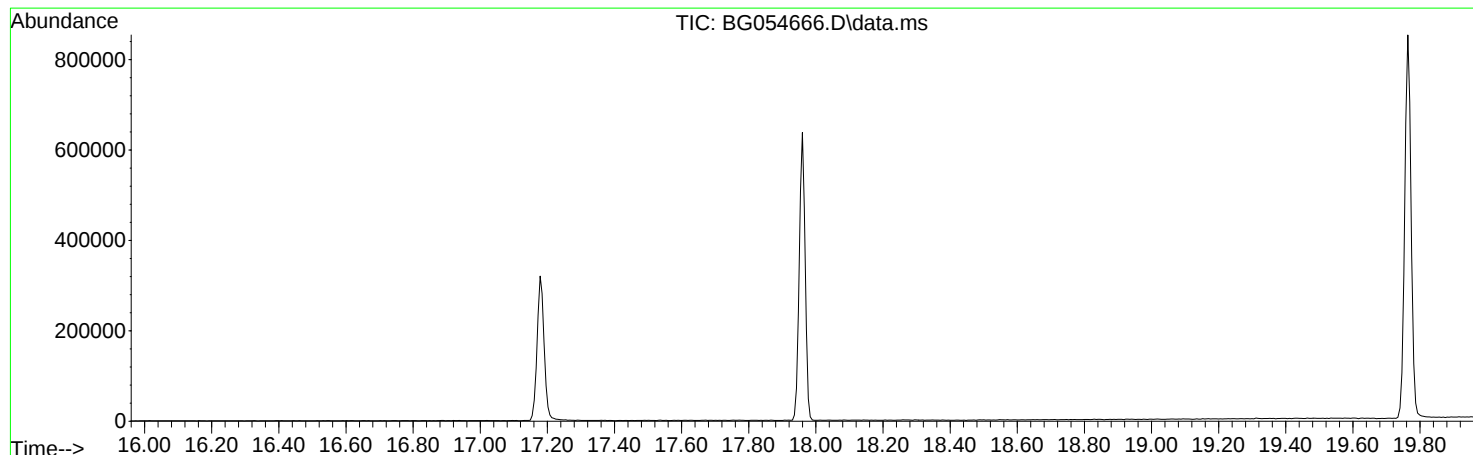

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	23008	PASS
68	69	0.00	2	0.8	171	PASS
69	198	0.00	100	35.3	21276	PASS
70	69	0.00	2	0.5	110	PASS
127	198	10	80	46.6	28115	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	60301	PASS
199	198	5	9	7.1	4273	PASS
275	198	10	60	28.7	17298	PASS
365	198	1	100	4.1	2447	PASS
441	198	0.01	100	12.9	7761	PASS
442	442	50	100	100.0	48184	PASS
443	442	15	24	20.0	9629	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/20/2022	BNA_G	<u>BG054666.D</u>
Compound Name	Response	Retention Time
DDT	191480	21.003
DDD	2982	20.551
DDE	0	20.002
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2982	194462	1.53

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082022\
Data File : BG054666.D
Acq On : 19 Aug 2022 16:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 22 05:53:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 22 00:08:53 2022
Response via : Initial Calibration

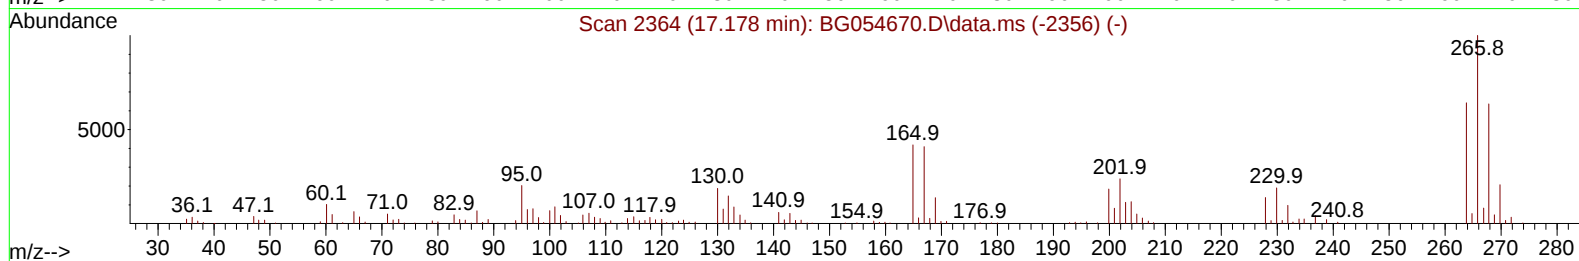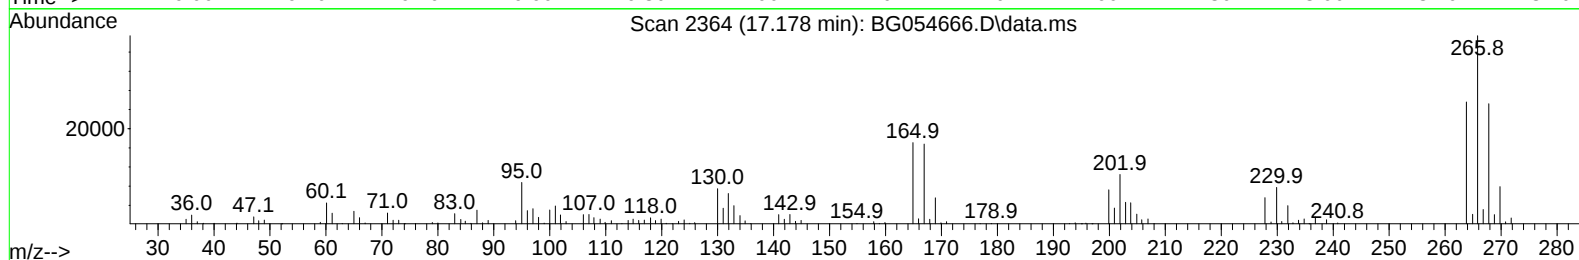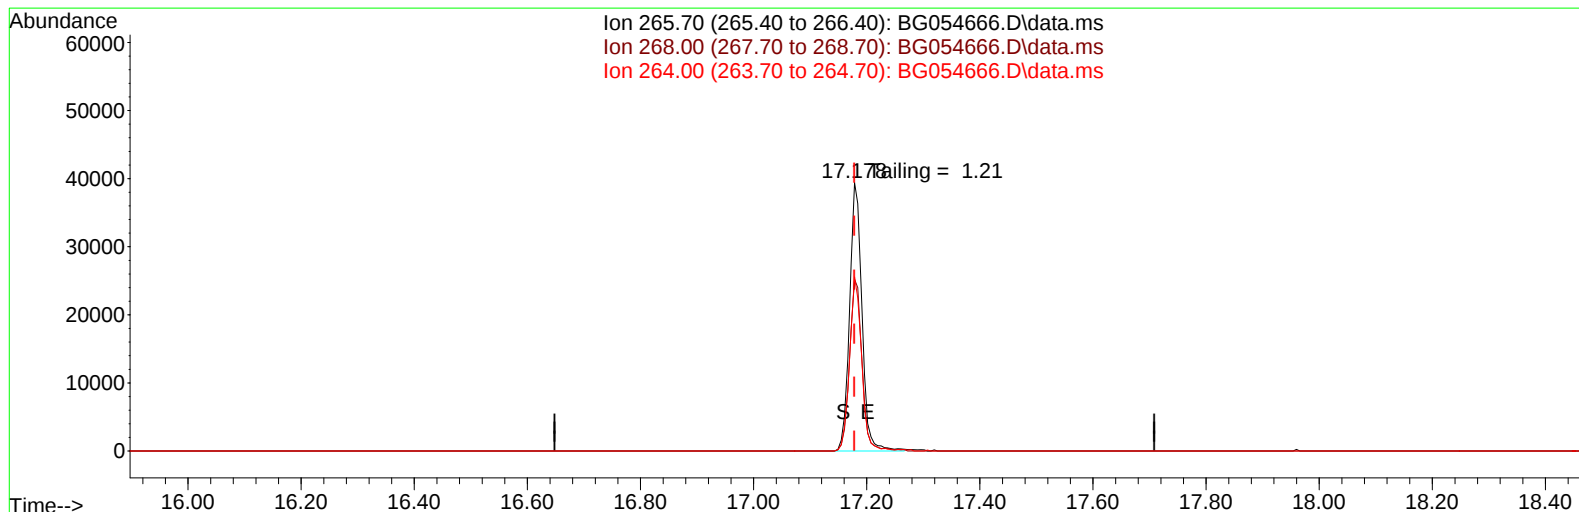

TIC: BG054666.D\data.ms

(70) Pentachlorophenol (C)

17.178min (+ 0.000) 45613.01 ng




response 59821

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.99
264.00	64.20	64.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082022\
Data File : BG054666.D
Acq On : 19 Aug 2022 16:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 22 05:53:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 22 00:08:53 2022
Response via : Initial Calibration

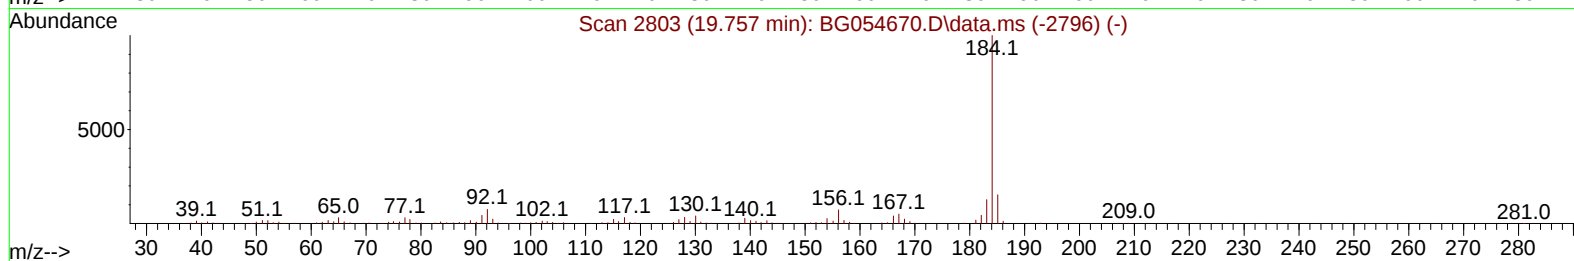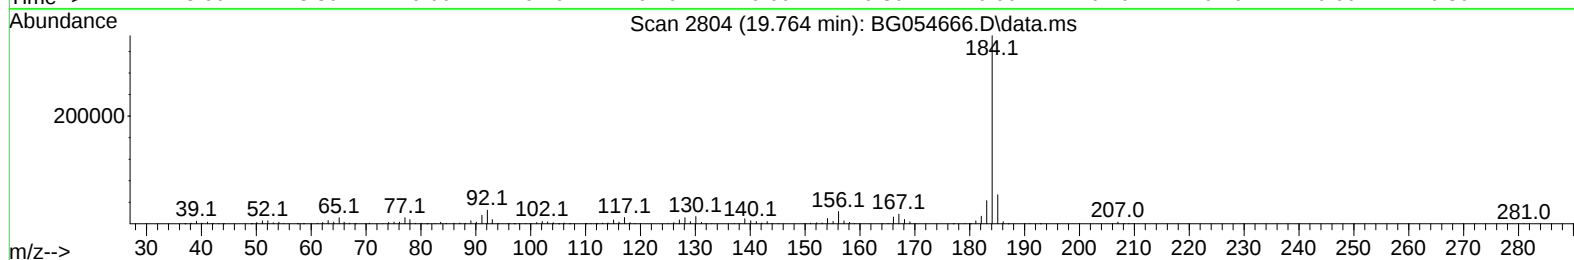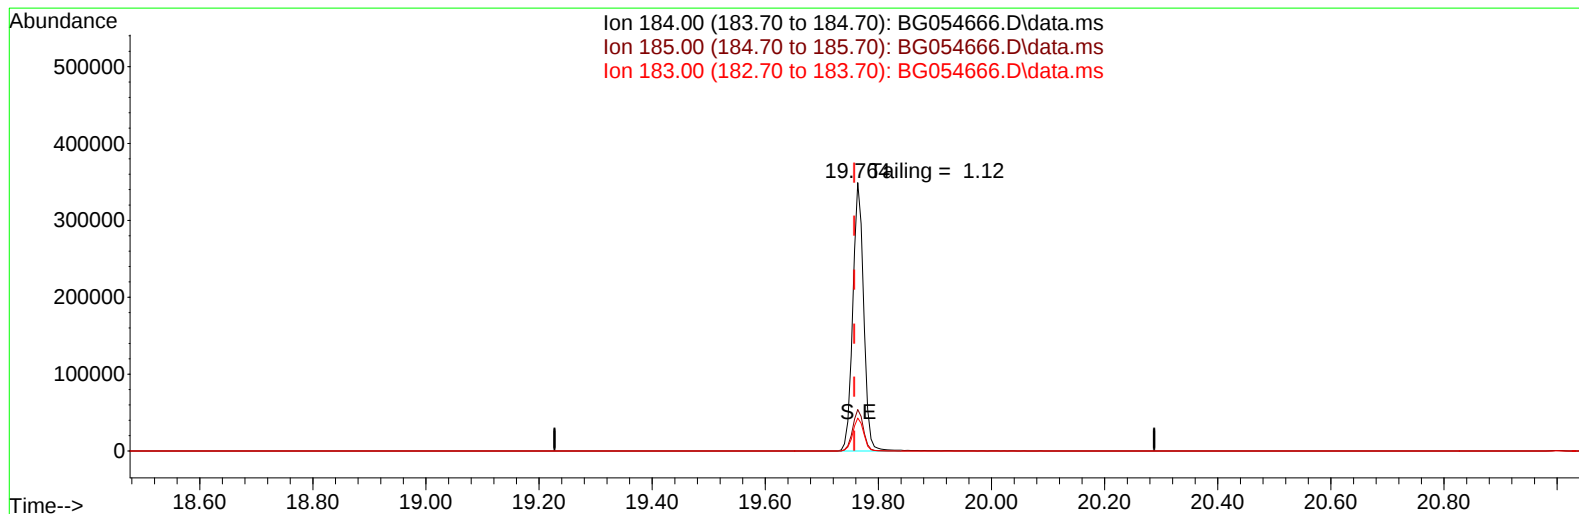

TIC: BG054666.D\data.ms

(77) Benzidine

19.764min (+ 0.006) 88156.77 ng

response 469409

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	15.45
183.00	12.60	12.29
0.00	0.00	0.00