

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082024\
 Data File : BG062471.D
 Acq On : 20 Aug 2024 10:27
 Operator : MA/JU
 Sample : PB162773BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK773

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062471.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	16	20	26	rVB3	16102	21697	1.16%	0.119%
2	3.811	85	89	100	rBV	210461	343033	18.34%	1.881%
3	4.151	143	147	150	rVB5	2590	3778	0.20%	0.021%
4	4.439	194	196	201	rBV2	1499	1986	0.11%	0.011%
5	4.627	222	228	229	rBV5	1168	2078	0.11%	0.011%
6	4.751	247	249	252	rVB3	1951	1976	0.11%	0.011%
7	7.100	641	649	659	rBV	231216	394753	21.11%	2.164%
8	7.271	670	678	689	rBV	168572	275411	14.73%	1.510%
9	7.476	705	713	722	rBV	206046	351991	18.82%	1.930%
10	7.940	785	792	802	rVB	177554	304105	16.26%	1.667%
11	8.639	903	911	919	rBV	296825	501075	26.79%	2.747%
12	9.098	980	989	999	rBV	209749	372290	19.91%	2.041%
13	9.814	1104	1111	1120	rVB	173310	304957	16.31%	1.672%
14	10.355	1195	1203	1215	rBV	293984	517725	27.68%	2.838%
15	10.737	1259	1268	1277	rBV	285702	501445	26.81%	2.749%
16	10.866	1282	1290	1299	rBV	278671	504411	26.97%	2.765%
17	12.317	1531	1537	1543	rBV3	3702	6338	0.34%	0.035%
18	13.968	1812	1818	1828	rVB	581873	834655	44.63%	4.576%
19	14.255	1860	1867	1876	rBV	655309	1011928	54.11%	5.547%
20	14.567	1912	1920	1927	rVB	521757	815847	43.62%	4.473%
21	14.749	1943	1951	1963	rBV	281905	460082	24.60%	2.522%
22	15.554	2080	2088	2097	rBV	898724	1354147	72.40%	7.424%
23	15.665	2100	2107	2116	rBV	243642	360436	19.27%	1.976%
24	15.794	2123	2129	2135	rVB3	2946	4391	0.23%	0.024%
25	16.341	2216	2222	2225	rBV3	2611	4029	0.22%	0.022%
26	17.304	2379	2386	2394	rBV	713416	1043259	55.78%	5.719%
27	17.404	2396	2403	2417	rVB	1039881	1523905	81.48%	8.354%
28	19.084	2687	2689	2693	rVB2	2112	2295	0.12%	0.013%
29	19.254	2713	2718	2724	rBV3	13033	20948	1.12%	0.115%
30	19.325	2726	2730	2734	rVV	11295	16019	0.86%	0.088%
31	19.390	2737	2741	2745	rVB3	2643	3557	0.19%	0.019%
32	19.625	2776	2781	2785	rBV4	6371	10627	0.57%	0.058%
33	19.689	2785	2792	2806	rVB	1274462	1836652	98.20%	10.069%
34	19.930	2829	2833	2835	rBV4	2261	3373	0.18%	0.018%
35	20.083	2857	2859	2863	rBV3	2092	2415	0.13%	0.013%
36	20.159	2870	2872	2874	rBV3	2311	2132	0.11%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082024\
Data File : BG062471.D
Acq On : 20 Aug 2024 10:27
Operator : MA/JU
Sample : PB162773BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK773

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Title : SVOA CALIBRATION

37	20.189	2874	2877	2878	rVV3	1935	2047	0.11%	0.011%
38	20.300	2893	2896	2897	rBV3	2341	2026	0.11%	0.011%
39	20.488	2926	2928	2929	rBV2	2435	1969	0.11%	0.011%
40	20.606	2946	2948	2950	rBV2	2861	2585	0.14%	0.014%
41	20.664	2955	2958	2962	rVB5	6657	8370	0.45%	0.046%
42	21.029	3018	3020	3023	rBV4	4535	6419	0.34%	0.035%
43	21.546	3101	3108	3116	rBV	717390	1154725	61.74%	6.330%
44	22.339	3241	3243	3251	rVB7	11801	17558	0.94%	0.096%
45	23.002	3354	3356	3364	rVB2	16344	26357	1.41%	0.144%
46	23.778	3483	3488	3496	rVB3	25081	46328	2.48%	0.254%
47	24.418	3586	3597	3607	rBV2	698388	1870301	100.00%	10.253%
48	24.624	3623	3632	3641	rBV	440896	1216357	65.04%	6.668%
49	25.763	3820	3826	3836	rVB5	28653	81656	4.37%	0.448%
50	27.062	4040	4047	4059	rVB6	26006	84739	4.53%	0.465%




Sum of corrected areas: 18241183

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082024\
Data File : BG062471.D
Acq On : 20 Aug 2024 10:27
Operator : MA/JU
Sample : PB162773BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK773

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

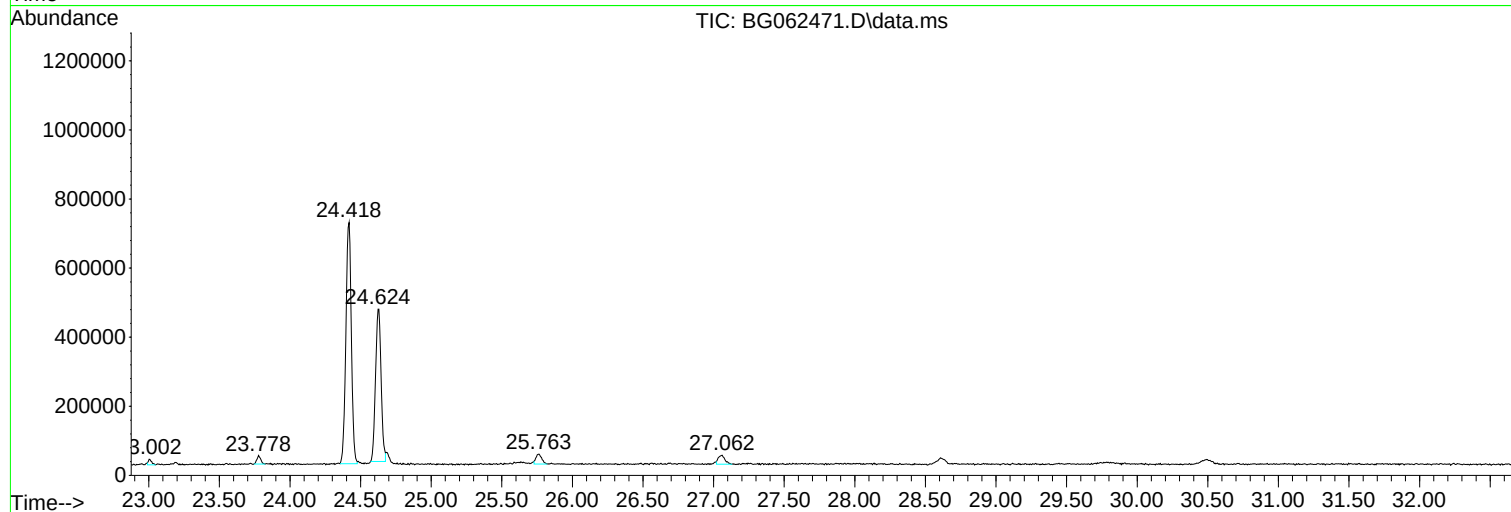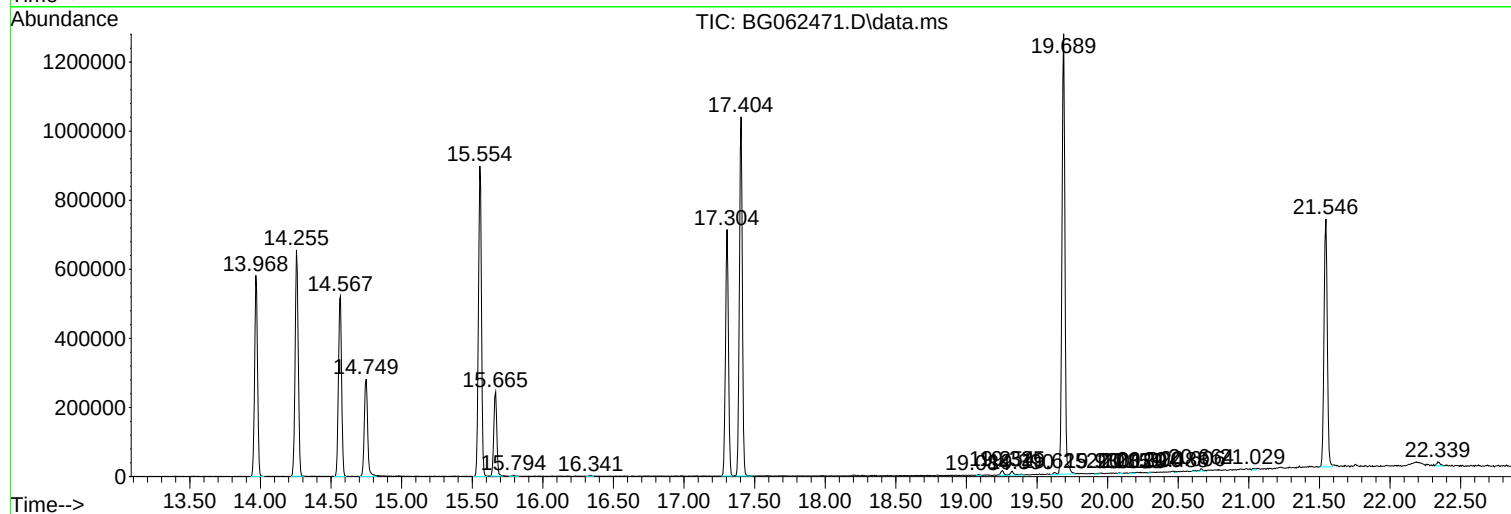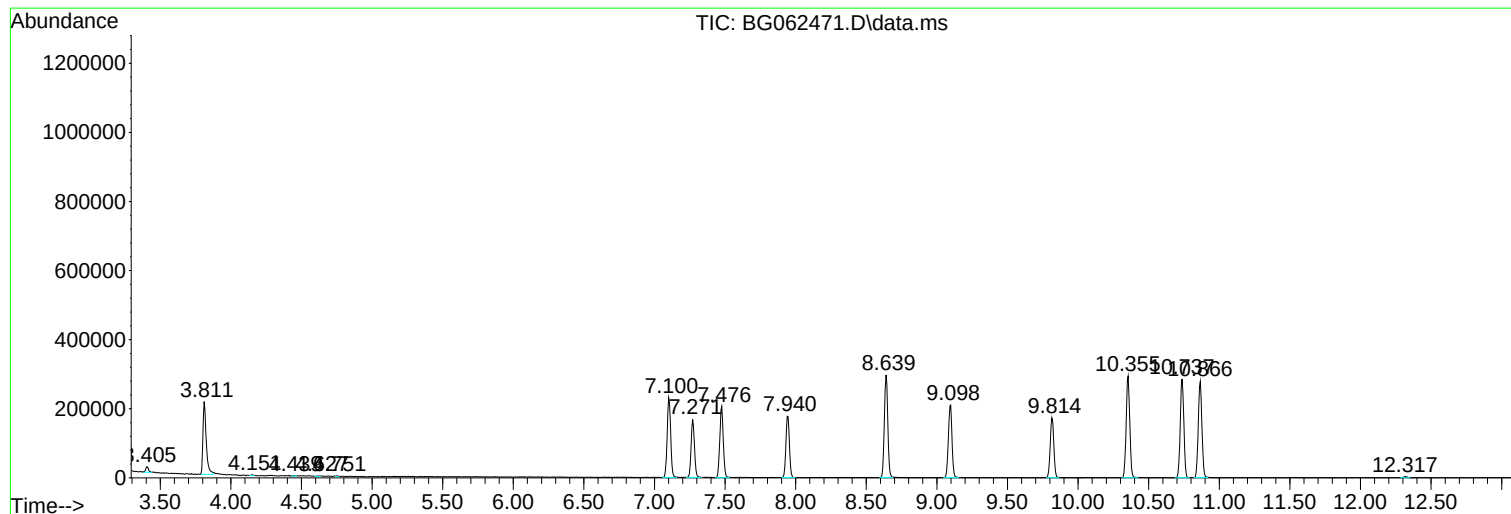

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082024\
Data File : BG062471.D
Acq On : 20 Aug 2024 10:27
Operator : MA/JU
Sample : PB162773BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK773

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082024\
Data File : BG062471.D
Acq On : 20 Aug 2024 10:27
Operator : MA/JU
Sample : PB162773BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK773

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------