

Data Path : Z:\HPCHEM1\BNA G\DATA\BG082117\
 Data File : BG028386.D
 Acq On : 21 Aug 2017 12:03
 Operator : SJ/JU
 Sample : PB101455BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK55

Quant Time: Aug 22 01:39:46 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 22 01:38:44 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.34	152	34244	20.00	ng/ul	0.00
18) Naphthalene-d8	11.16	136	156198	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.95	164	116654	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.80	188	561473	20.00	ng/ul	0.10
75) Chrysene-d12	22.03	240	346489	20.00	ng/ul	0.00
83) Perylene-d12	25.53	264	335510	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.82	96	4657	6.33	ng/uL	0.00
5) Phenol-d5	7.50	99	105493	28.05	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.65	67	74464	31.26	ng/ul	0.00
9) 2-Chlorophenol-d4	7.88	132	77357	32.60	ng/ul	0.00
13) 4-Methylphenol-d8	9.04	113	92948	29.57	ng/ul	0.00
19) Nitrobenzene-d5	9.51	128	42837	35.07	ng/ul	0.00
22) 2-Nitrophenol-d4	10.24	143	50555	37.75	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.78	165	94977	34.28	ng/ul	0.00
29) 4-Chloroaniline-d4	11.29	131	93101	30.19	ng/ul	0.00
43) Dimethylphthalate-d6	14.34	166	387505	37.35	ng/ul	0.00
46) Acenaphthylene-d8	14.65	160	410864	35.12	ng/ul	0.00
51) 4-Nitrophenol-d4	15.15	143	51027	30.93	ng/ul	0.00
57) Fluorene-d10	15.94	176	314583	33.80	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.06	200	65365	17.92	ng/ul	0.00
70) Anthracene-d10	17.80	188	561473	20.85	ng/ul	0.00
76) Pyrene-d10	20.07	212	634964	35.74	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.53	264	328988	20.95	ng/ul	0.25

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	9.04	70	2625	1.030	ng/ul# 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG082117\
Data File : BG028386.D
Acq On : 21 Aug 2017 12:03
Operator : SJ/JU
Sample : PB101455BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK55

Quant Time: Aug 22 01:39:46 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 22 01:38:44 2017
Response via : Initial Calibration

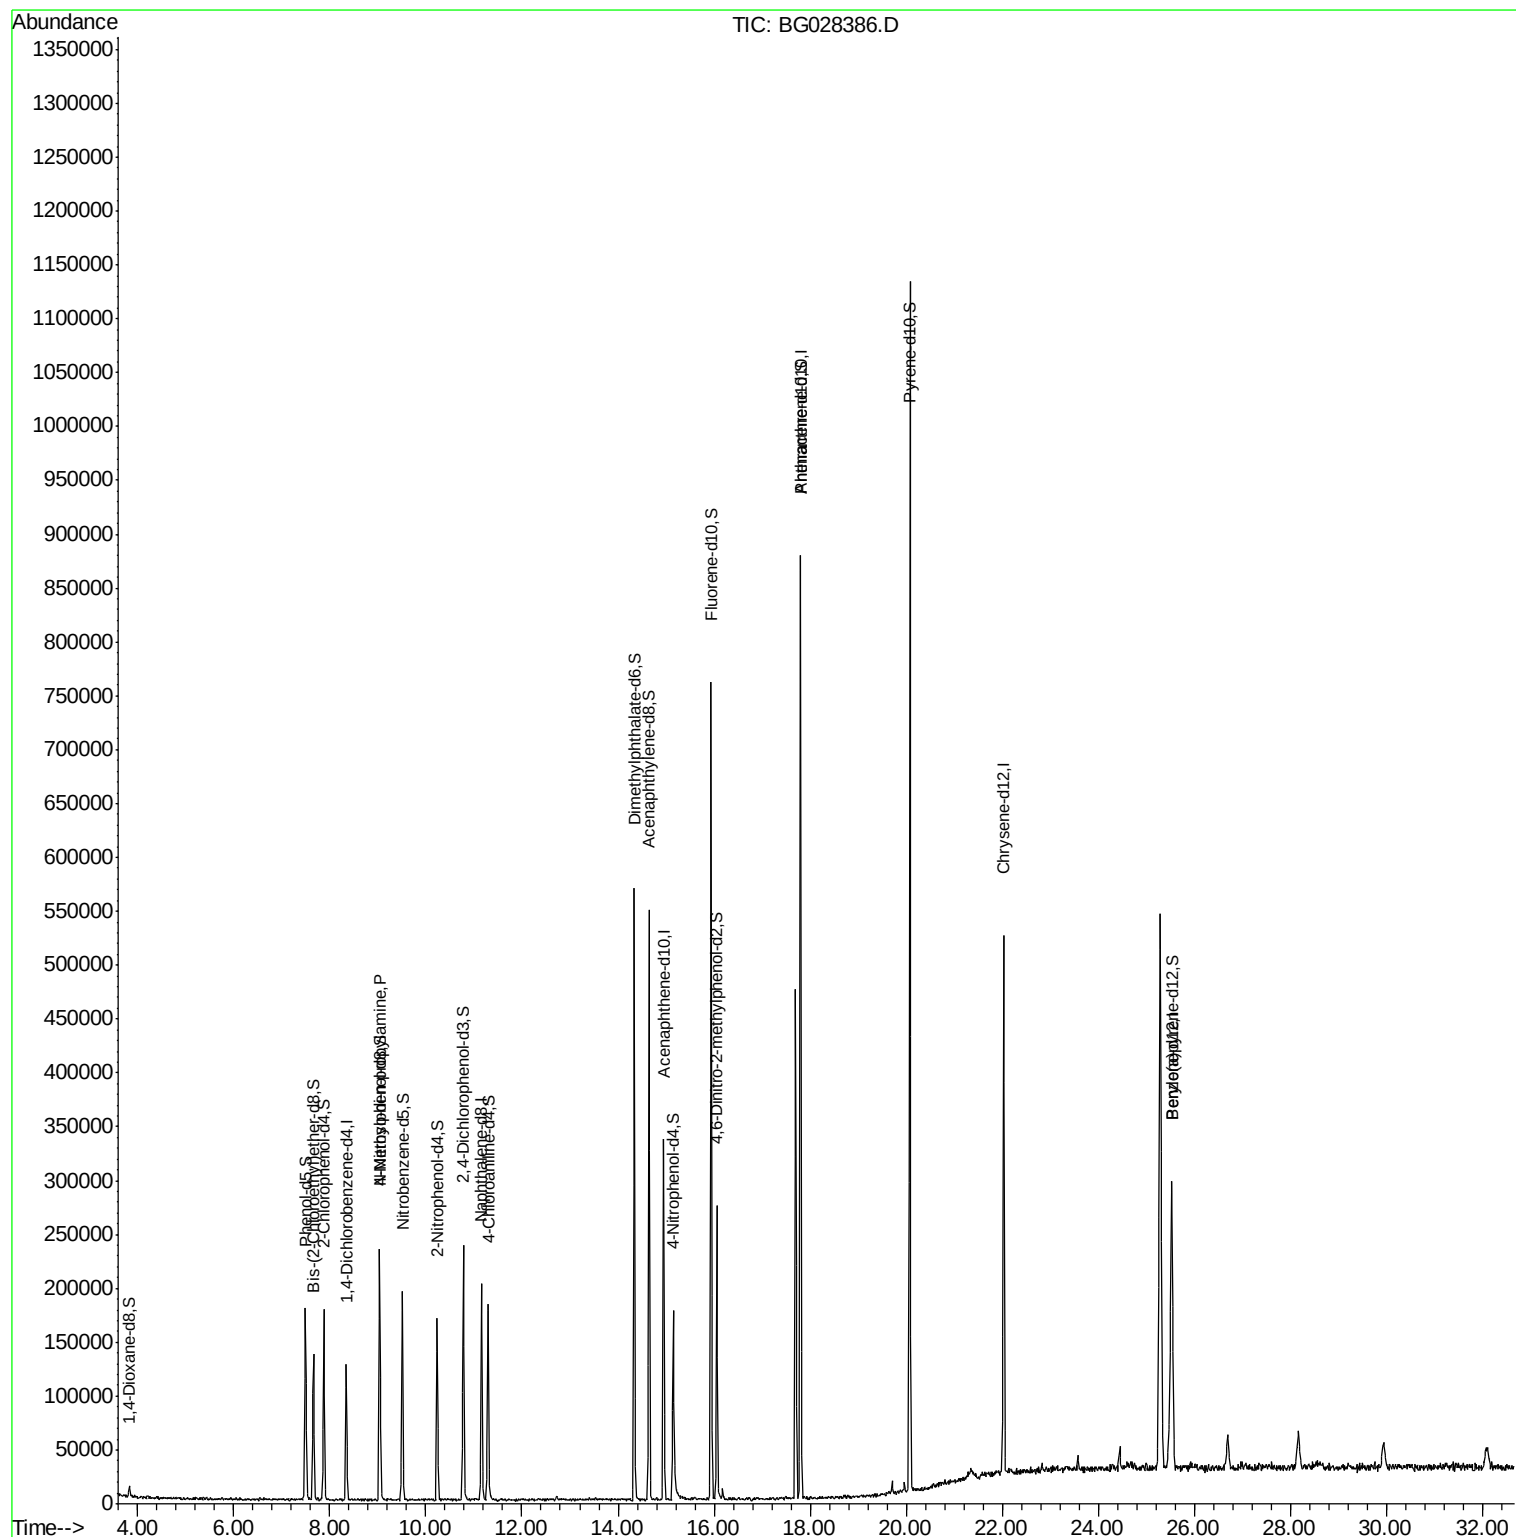

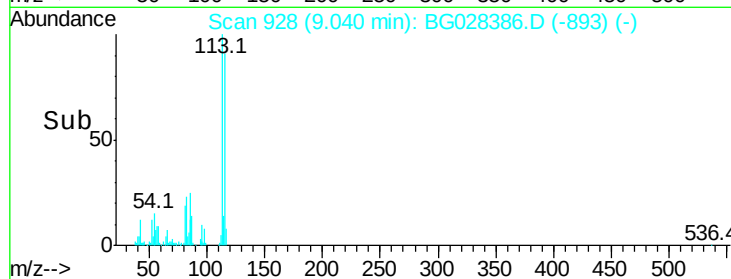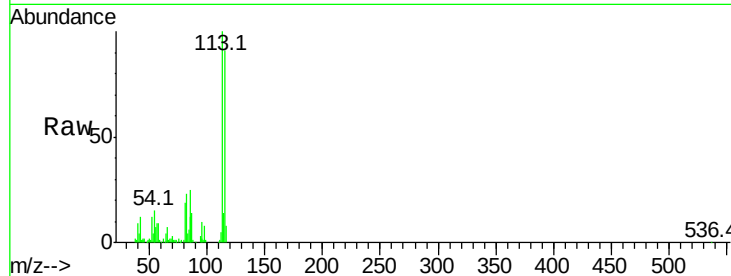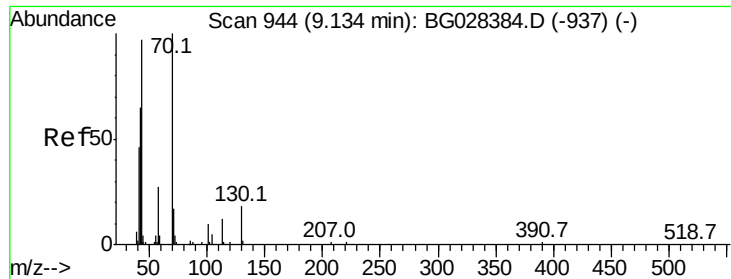

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.030 ng/ul
 RT: 9.04 min Scan# 928
 Delta R.T. -0.09 min
 Lab File: BG028386.D
 Acq: 21 Aug 2017 12:03

Instrument :
 BNA_G
 ClientSampleId :
 SBLK55

Tot Ion:	70	Resp:	2625
Ion	Ratio	Lower	Upper
70	100		
42	358.9	59.0	88.6#
101	0.0	6.6	9.8#
130	0.0	15.6	23.4#

