

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG082117\
 Data File : BG028407.D
 Acq On : 22 Aug 2017 3:17
 Operator : SJ/JU
 Sample : I4827-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 B0AF1

Quant Time: Aug 22 13:59:19 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 22 04:33:26 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.34	152	45062	20.00	ng/ul	0.00
18) Naphthalene-d8	11.16	136	197537	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.95	164	146187	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.70	188	349564	20.00	ng/ul	0.00
75) Chrysene-d12	22.03	240	368769	20.00	ng/ul	0.00
83) Perylene-d12	25.52	264	369067	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.84	96	2218	2.29	ng/uL	0.01
5) Phenol-d5	7.50	99	55951	11.31	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.66	67	36543	11.66	ng/ul	0.00
9) 2-Chlorophenol-d4	7.88	132	40004	12.81	ng/ul	0.00
13) 4-Methylphenol-d8	9.04	113	48418	11.71	ng/ul	0.00
19) Nitrobenzene-d5	9.51	128	22078	14.29	ng/ul	0.00
22) 2-Nitrophenol-d4	10.24	143	25018	14.77	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.79	165	50282	14.35	ng/ul	0.00
29) 4-Chloroaniline-d4	11.29	131	54902	14.08	ng/ul	0.00
43) Dimethylphthalate-d6	14.34	166	203114	15.62	ng/ul	0.00
46) Acenaphthylene-d8	14.65	160	224341	15.30	ng/ul	0.00
51) 4-Nitrophenol-d4	15.15	143	23566	11.40	ng/ul	0.00
57) Fluorene-d10	15.94	176	173953	14.91	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.06	200	30092	13.25	ng/ul	0.00
70) Anthracene-d10	17.80	188	286516	17.09	ng/ul	0.00
76) Pyrene-d10	20.07	212	320877	16.97	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.29	264	294615	17.05	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	14.38	163	53058	4.432 ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG082117\
Data File : BG028407.D
Acq On : 22 Aug 2017 3:17
Operator : SJ/JU
Sample : I4827-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
B0AF1

Quant Time: Aug 22 13:59:19 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 22 04:33:26 2017
Response via : Initial Calibration

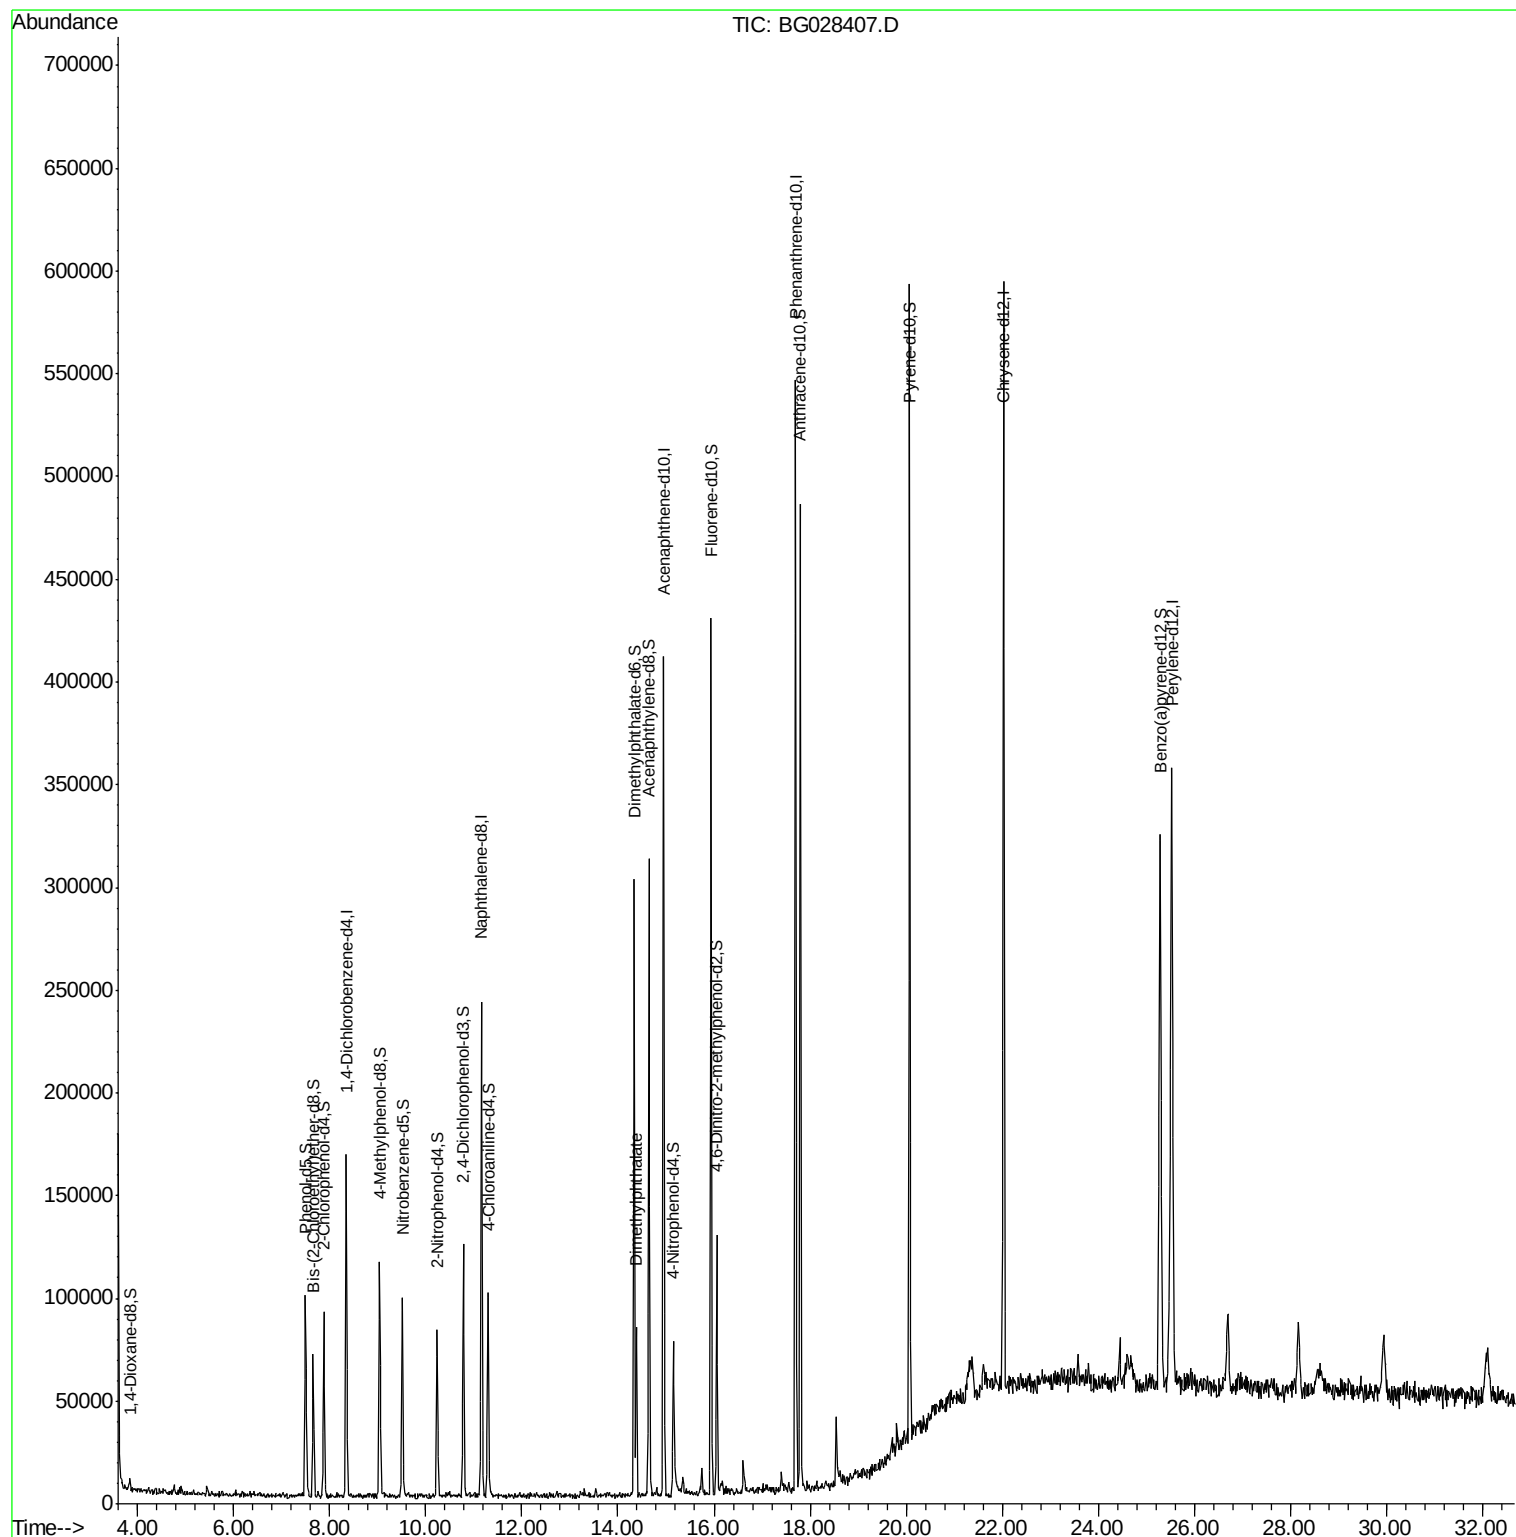

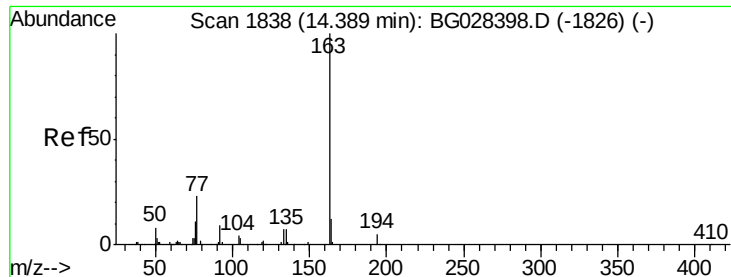

#44

Dimethylphthalate

Concen: 4.432 ng/ul

RT: 14.38 min Scan# 1837

Delta R.T. -0.01 min

Lab File: BG028407.D

Acq: 22 Aug 2017 3:17

Instrument :

BNA_G

ClientSampleId :

B0AF1


Tgt Ion:163 Resp: 53058

Ion Ratio Lower Upper

163 100

194 5.2 3.4 5.0#

164 11.6 9.0 13.4

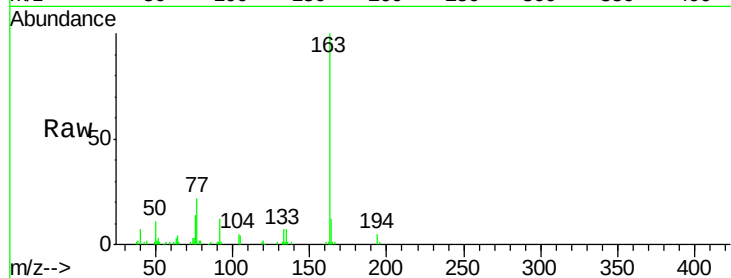

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

