

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082124\
 Data File : BG062510.D
 Acq On : 21 Aug 2024 16:02
 Operator : MA/JU
 Sample : PB162825BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK825

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062510.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.406	16	20	28	rVB	20930	30614	1.52%	0.143%
2	3.811	84	89	106	rBV	254602	422720	21.05%	1.978%
3	4.146	143	146	150	rVB3	4747	5668	0.28%	0.027%
4	7.101	642	649	660	rBV	315826	528356	26.31%	2.472%
5	7.265	669	677	686	rBV	209452	349290	17.39%	1.634%
6	7.471	705	712	721	rBV	282259	467070	23.26%	2.185%
7	7.941	785	792	799	rBV	250233	413917	20.61%	1.937%
8	8.640	903	911	921	rBV	391718	658555	32.79%	3.081%
9	9.092	980	988	999	rBV	282125	490130	24.41%	2.293%
10	9.815	1103	1111	1123	rVB	238735	417675	20.80%	1.954%
11	10.349	1195	1202	1216	rBV	371208	674987	33.61%	3.158%
12	10.731	1260	1267	1275	rBV	385712	693762	34.55%	3.246%
13	10.860	1282	1289	1302	rBV	346316	633258	31.53%	2.963%
14	11.524	1396	1402	1409	rBV3	2217	3954	0.20%	0.018%
15	12.317	1529	1537	1543	rBV3	5015	9729	0.48%	0.046%
16	13.968	1811	1818	1828	rVB	679108	939037	46.76%	4.394%
17	14.256	1860	1867	1878	rVB	753108	1168330	58.18%	5.466%
18	14.561	1912	1919	1927	rBV	649176	1010322	50.31%	4.727%
19	14.749	1944	1951	1966	rBV	304685	482679	24.03%	2.258%
20	15.554	2080	2088	2097	rBV	998741	1493916	74.39%	6.990%
21	15.660	2100	2106	2114	rBV	289085	403650	20.10%	1.889%
22	15.795	2123	2129	2136	rVB4	3730	6445	0.32%	0.030%
23	16.335	2217	2221	2224	rBV3	2644	3819	0.19%	0.018%
24	17.305	2378	2386	2394	rBV	759779	1181219	58.82%	5.527%
25	17.399	2396	2402	2413	rVB	1058404	1588711	79.11%	7.433%
26	17.545	2424	2427	2431	rBV3	1601	2031	0.10%	0.010%
27	17.968	2498	2499	2505	rVB3	1761	2260	0.11%	0.011%
28	18.203	2533	2539	2543	rBV4	2362	5027	0.25%	0.024%
29	18.268	2547	2550	2555	rVB4	1763	3018	0.15%	0.014%
30	18.791	2637	2639	2642	rBV3	1949	2213	0.11%	0.010%
31	19.249	2713	2717	2725	rVB2	15607	22820	1.14%	0.107%
32	19.319	2725	2729	2733	rBV2	12186	18225	0.91%	0.085%
33	19.384	2736	2740	2742	rVB3	2861	3198	0.16%	0.015%
34	19.619	2776	2780	2783	rVV4	6851	7946	0.40%	0.037%
35	19.684	2785	2791	2805	rVB	1369953	1970470	98.12%	9.219%
36	19.813	2811	2813	2815	rVB3	2740	2062	0.10%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082124\
 Data File : BG062510.D
 Acq On : 21 Aug 2024 16:02
 Operator : MA/JU
 Sample : PB162825BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK825

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
 Title : SVOA CALIBRATION

37	19.860	2818	2821	2822	rBV3	2217	2319	0.12%	0.011%
38	20.013	2846	2847	2850	rBV3	2893	2789	0.14%	0.013%
39	20.230	2882	2884	2885	rBV2	2948	2375	0.12%	0.011%
40	20.306	2894	2897	2900	rBV5	2174	3059	0.15%	0.014%
41	20.559	2938	2940	2941	rBV2	3144	2733	0.14%	0.013%
42	20.624	2949	2951	2953	rVB3	3239	2025	0.10%	0.009%
43	20.659	2955	2957	2959	rVB3	7629	6367	0.32%	0.030%
44	20.770	2974	2976	2977	rBV2	4802	3471	0.17%	0.016%
45	21.540	3100	3107	3115	rBV	861445	1355009	67.47%	6.340%
46	21.657	3125	3127	3128	rBV2	5644	4858	0.24%	0.023%
47	22.333	3240	3242	3247	rVB5	15033	17785	0.89%	0.083%
48	23.003	3352	3356	3362	rVB4	21886	36584	1.82%	0.171%
49	23.766	3481	3486	3495	rVB3	32332	63477	3.16%	0.297%
50	24.413	3586	3596	3610	rVB2	777382	2008260	100.00%	9.396%
51	24.624	3621	3632	3650	rVB	521898	1514226	75.40%	7.085%
52	25.746	3817	3823	3832	rVB3	41286	113583	5.66%	0.531%
53	27.038	4035	4043	4053	rBV4	37011	117222	5.84%	0.548%




Sum of corrected areas: 21373225

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082124\
Data File : BG062510.D
Acq On : 21 Aug 2024 16:02
Operator : MA/JU
Sample : PB162825BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK825

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

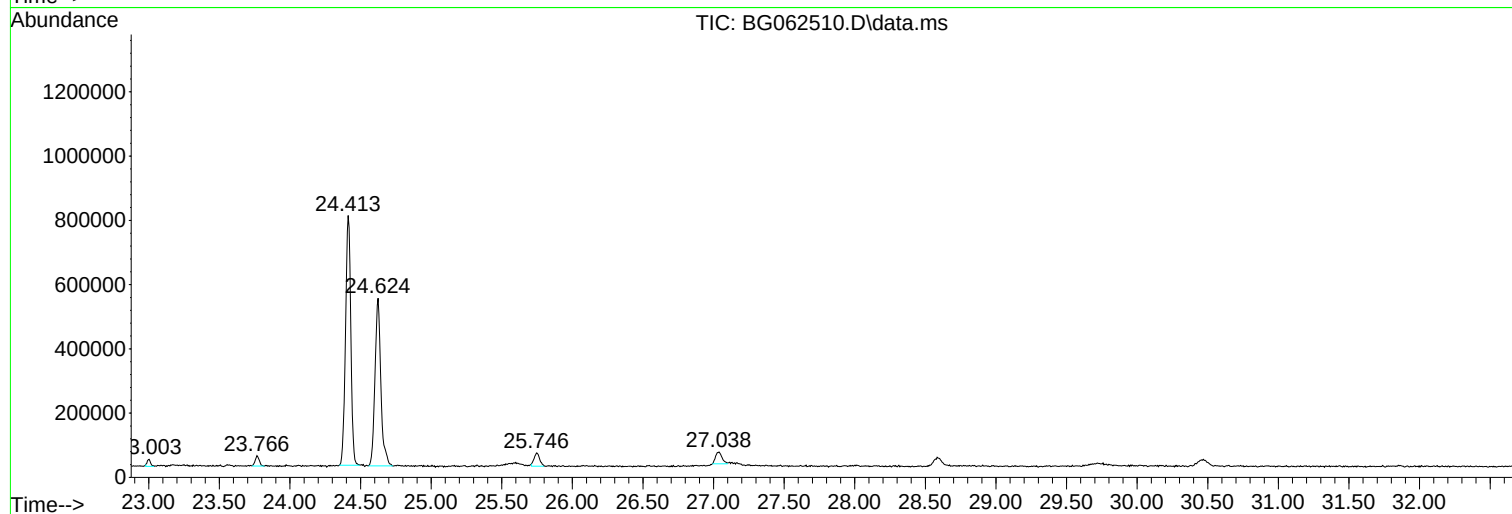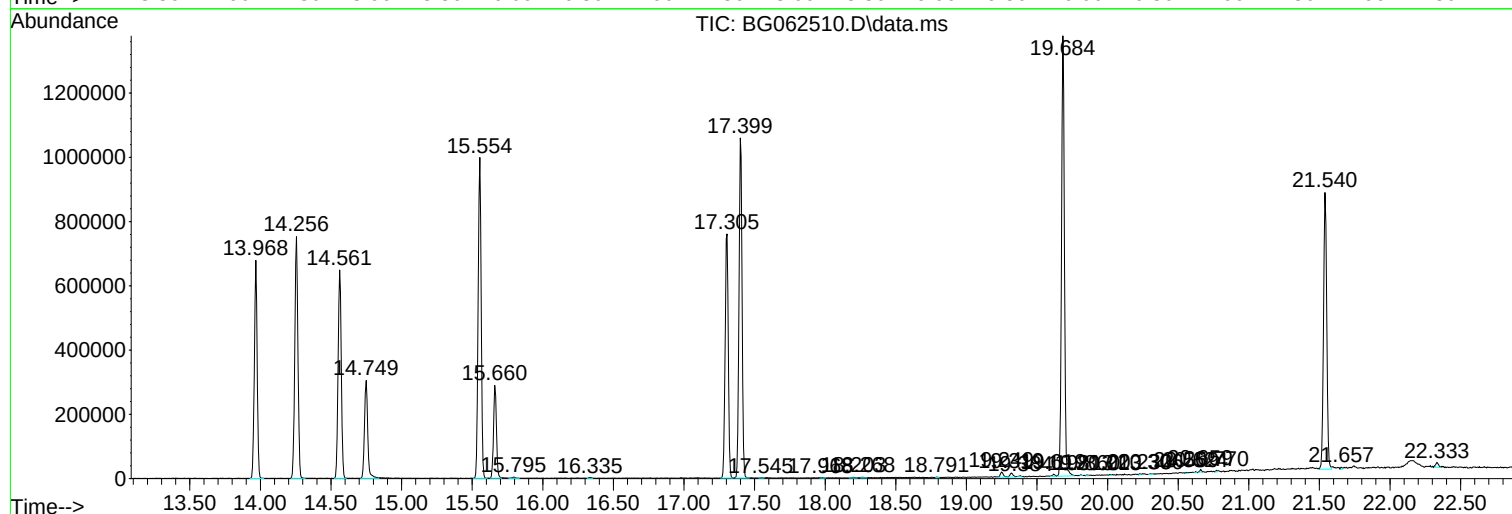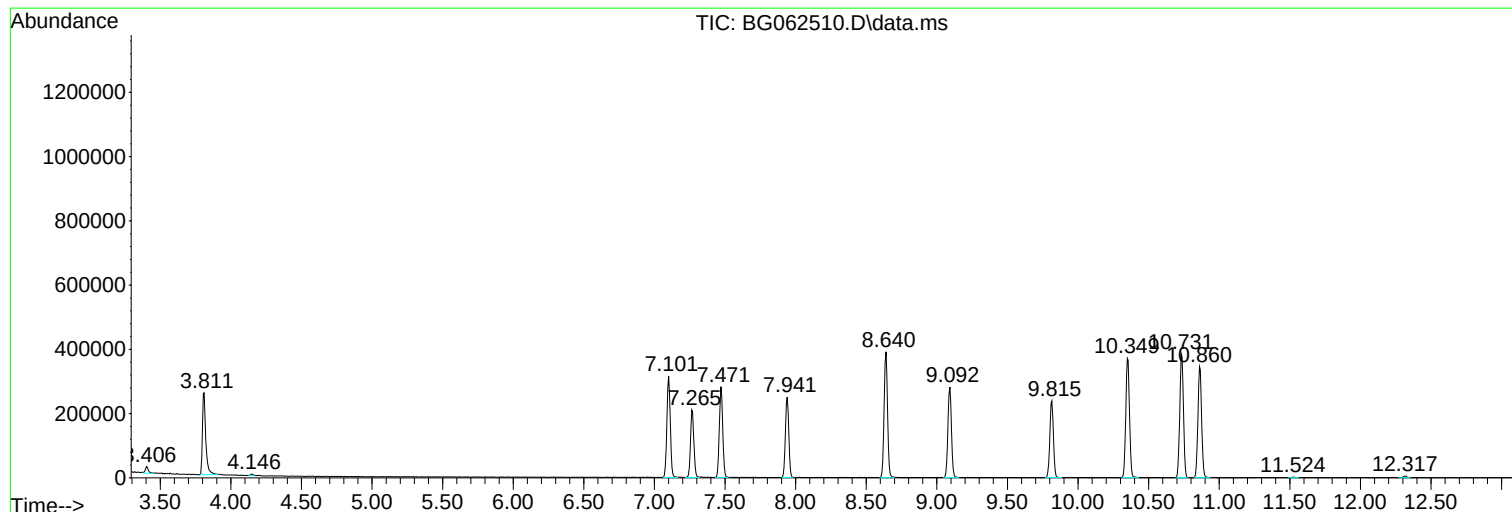

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082124\
Data File : BG062510.D
Acq On : 21 Aug 2024 16:02
Operator : MA/JU
Sample : PB162825BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK825

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082124\
Data File : BG062510.D
Acq On : 21 Aug 2024 16:02
Operator : MA/JU
Sample : PB162825BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK825

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc