

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082124\
 Data File : BG062511.D
 Acq On : 21 Aug 2024 16:43
 Operator : MA/JU
 Sample : P3626-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCYB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062511.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.407	17	20	25	rVB2	6835	8478	0.54%	0.057%
2	3.666	60	64	70	rBV	17269	26769	1.71%	0.179%
3	3.813	84	89	101	rBV	101737	163569	10.45%	1.094%
4	4.148	142	146	150	rVB4	4340	6461	0.41%	0.043%
5	4.306	171	173	176	rVV2	1948	2317	0.15%	0.015%
6	5.052	297	300	305	rVB4	1955	2986	0.19%	0.020%
7	6.027	461	466	470	rBV4	3129	4927	0.31%	0.033%
8	7.102	642	649	659	rBV	151826	268735	17.17%	1.797%
9	7.267	670	677	686	rVB	112772	179502	11.47%	1.200%
10	7.473	705	712	718	rBV	143409	239332	15.29%	1.600%
11	7.537	720	723	728	rVB3	3893	5935	0.38%	0.040%
12	7.942	783	792	799	rBV	265661	451777	28.86%	3.021%
13	8.001	799	802	809	rVB5	2518	4255	0.27%	0.028%
14	8.636	904	910	921	rBV	179443	302850	19.35%	2.025%
15	9.088	979	987	995	rBV	138845	244163	15.60%	1.633%
16	9.534	1060	1063	1069	rBV4	1347	2329	0.15%	0.016%
17	9.652	1076	1083	1089	rBV2	14639	25230	1.61%	0.169%
18	9.811	1101	1110	1119	rBV	112405	199290	12.73%	1.333%
19	10.351	1194	1202	1211	rBV	192836	338411	21.62%	2.263%
20	10.733	1258	1267	1275	rBV	428095	739840	47.27%	4.947%
21	10.862	1282	1289	1299	rBV	188708	347159	22.18%	2.321%
22	11.261	1352	1357	1362	rVV4	6093	9807	0.63%	0.066%
23	11.467	1386	1392	1398	rBV2	29469	55646	3.56%	0.372%
24	12.313	1529	1536	1540	rBV3	2677	5027	0.32%	0.034%
25	13.394	1716	1720	1723	rVB2	1550	1987	0.13%	0.013%
26	13.523	1738	1742	1745	rBV4	1285	1637	0.10%	0.011%
27	13.964	1808	1817	1825	rBV	350181	508687	32.50%	3.401%
28	14.252	1859	1866	1874	rVB	415531	637923	40.76%	4.266%
29	14.463	1899	1902	1907	rVB	1721	2172	0.14%	0.015%
30	14.557	1911	1918	1926	rVB	721910	1137198	72.65%	7.604%
31	14.745	1944	1950	1966	rBV2	141855	270425	17.28%	1.808%
32	14.974	1983	1989	1998	rBV5	3863	6961	0.44%	0.047%
33	15.350	2048	2053	2056	rBV4	2512	4097	0.26%	0.027%
34	15.409	2060	2063	2069	rVV4	2288	3536	0.23%	0.024%
35	15.550	2080	2087	2095	rBV	550422	814085	52.01%	5.444%
36	15.656	2100	2105	2112	rVV	115780	165138	10.55%	1.104%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082124\
 Data File : BG062511.D
 Acq On : 21 Aug 2024 16:43
 Operator : MA/JU
 Sample : P3626-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCYB5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
 Title : SVOA CALIBRATION

37	15.714	2112	2115	2121	rVB4	2497	3834	0.24%	0.026%
38	15.791	2124	2128	2135	rVB4	2303	3966	0.25%	0.027%
39	16.037	2166	2170	2173	rBV3	2459	3026	0.19%	0.020%
40	16.108	2177	2182	2184	rBV4	2250	2958	0.19%	0.020%

41	16.278	2206	2211	2213	rBV3	3018	3610	0.23%	0.024%
42	16.707	2274	2284	2291	rBV4	2542	8072	0.52%	0.054%
43	16.854	2306	2309	2312	rBV3	3026	2769	0.18%	0.019%
44	17.018	2334	2337	2340	rVB2	1899	1905	0.12%	0.013%
45	17.189	2365	2366	2370	rBV3	1802	2353	0.15%	0.016%

46	17.300	2378	2385	2392	rVV	932163	1346251	86.01%	9.002%
47	17.394	2394	2401	2408	rBV	597787	873001	55.77%	5.838%
48	17.482	2412	2416	2420	rVV3	6002	8075	0.52%	0.054%
49	17.547	2423	2427	2430	rBV5	1894	2788	0.18%	0.019%
50	17.576	2430	2432	2435	rVB2	1767	1862	0.12%	0.012%

51	17.806	2466	2471	2474	rBV3	2419	3507	0.22%	0.023%
52	17.970	2496	2499	2505	rVB5	5749	6613	0.42%	0.044%
53	18.070	2509	2516	2521	rBV7	5755	10290	0.66%	0.069%
54	18.129	2523	2526	2529	rBV5	2080	2637	0.17%	0.018%
55	18.187	2532	2536	2551	rBV	39998	74294	4.75%	0.497%

56	18.493	2584	2588	2590	rBV2	2408	2982	0.19%	0.020%
57	18.628	2607	2611	2613	rBV4	1896	2338	0.15%	0.016%
58	19.116	2692	2694	2695	rBV2	1946	1709	0.11%	0.011%
59	19.133	2695	2697	2702	rVB5	3417	5549	0.35%	0.037%
60	19.186	2702	2706	2708	rBV3	1780	2216	0.14%	0.015%

61	19.251	2712	2717	2721	rVB4	8345	11936	0.76%	0.080%
62	19.315	2721	2728	2734	rBV3	10763	23600	1.51%	0.158%
63	19.433	2747	2748	2751	rBV3	2319	2544	0.16%	0.017%
64	19.468	2751	2754	2759	rVV6	6834	11637	0.74%	0.078%
65	19.615	2776	2779	2784	rBV4	8215	12416	0.79%	0.083%

66	19.680	2784	2790	2796	rVV	751169	1042262	66.59%	6.969%
67	19.721	2796	2797	2803	rVB4	14002	18107	1.16%	0.121%
68	19.891	2824	2826	2827	rVB2	2958	1670	0.11%	0.011%
69	20.073	2855	2857	2859	rBV3	1853	2115	0.14%	0.014%
70	20.173	2872	2874	2875	rBV2	2803	1617	0.10%	0.011%

71	20.185	2875	2876	2877	rBV	4180	2569	0.16%	0.017%
72	20.655	2953	2956	2960	rBV6	7203	8195	0.52%	0.055%
73	20.831	2984	2986	2987	rBV2	4226	3323	0.21%	0.022%
74	21.213	3046	3051	3062	rBV2	49905	106453	6.80%	0.712%
75	21.536	3099	3106	3114	rBV2	916412	1457782	93.14%	9.748%

76	22.323	3238	3240	3243	rBV3	6442	6586	0.42%	0.044%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082124\
Data File : BG062511.D
Acq On : 21 Aug 2024 16:43
Operator : MA/JU
Sample : P3626-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCYB5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Title : SVOA CALIBRATION

77	23.169	3380	3384	3391	rVB4	22010	45061	2.88%	0.301%
78	23.633	3461	3463	3465	rBV3	5163	3178	0.20%	0.021%
79	23.762	3481	3485	3491	rVB3	23644	40369	2.58%	0.270%
80	24.403	3584	3594	3605	rBV2	372412	975362	62.31%	6.522%
81	24.614	3620	3630	3647	rVB	571074	1565222	100.00%	10.466%
82	25.742	3815	3822	3828	rVB6	18803	47579	3.04%	0.318%


Sum of corrected areas: 14954829

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082124\
Data File : BG062511.D
Acq On : 21 Aug 2024 16:43
Operator : MA/JU
Sample : P3626-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCYB5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

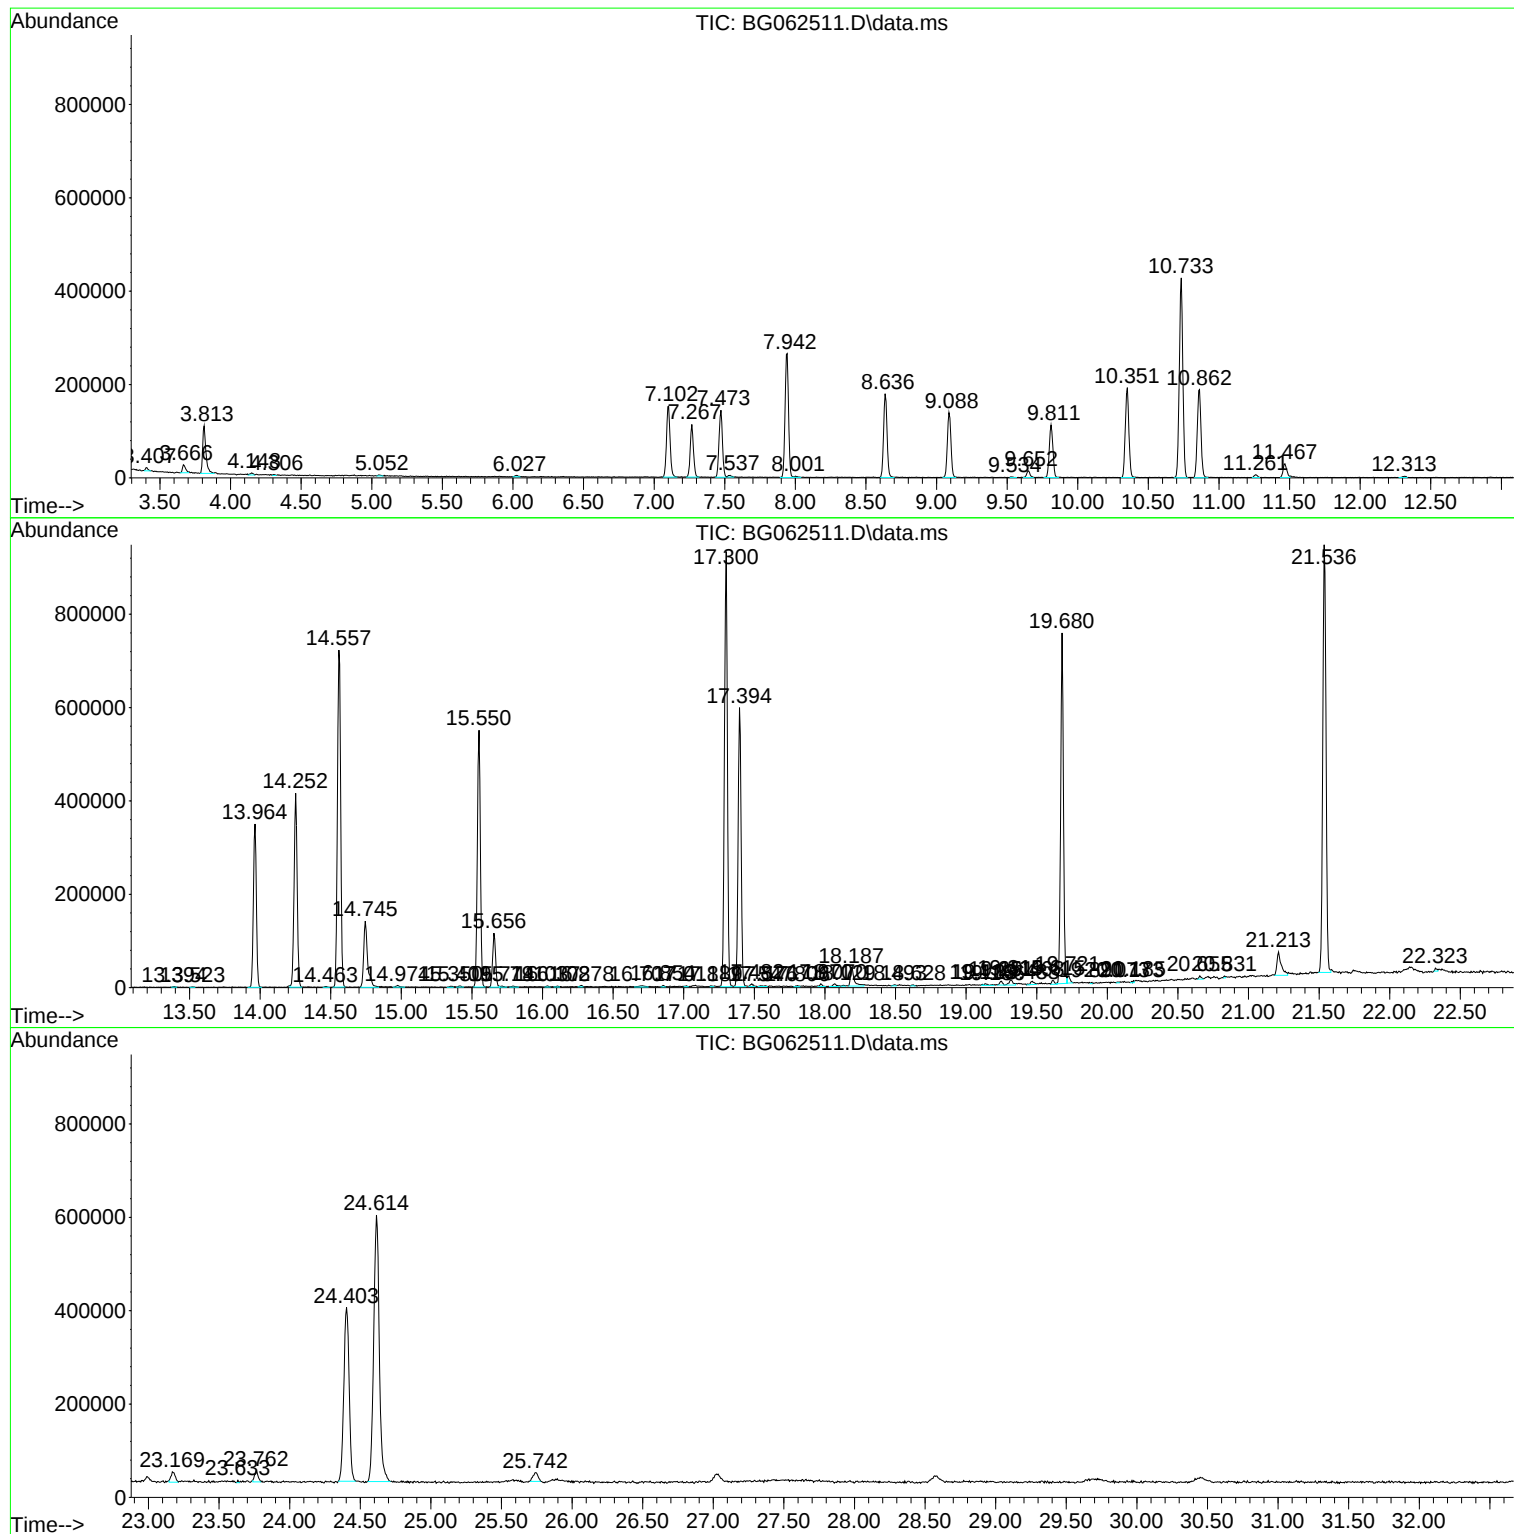

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082124\
Data File : BG062511.D
Acq On : 21 Aug 2024 16:43
Operator : MA/JU
Sample : P3626-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCYB5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082124\
Data File : BG062511.D
Acq On : 21 Aug 2024 16:43
Operator : MA/JU
Sample : P3626-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCYB5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------