
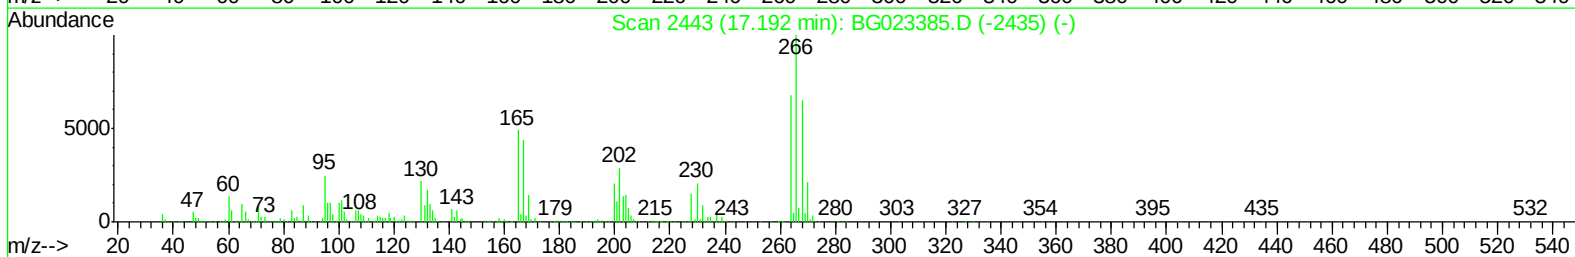
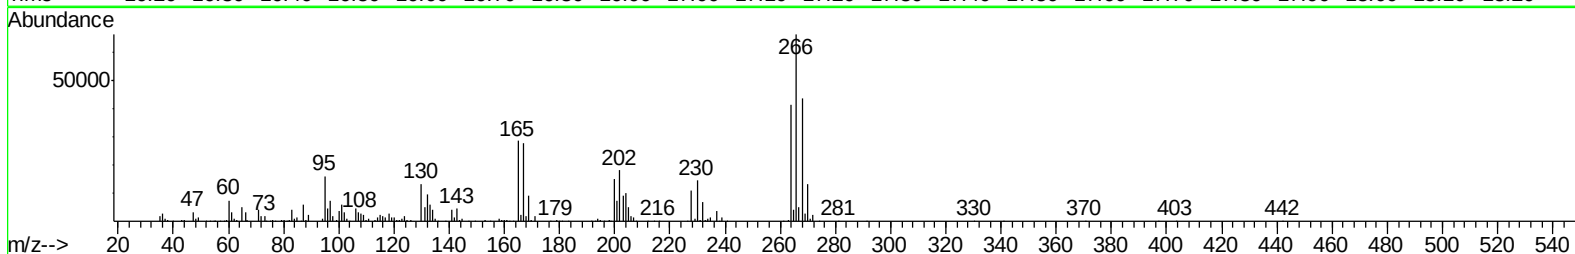


Data Path : Z:\HPCHEM1\BNA_G\Data\BG082216\
Data File : BG023830.D
Acq On : 22 Aug 2016 12:21
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 08:12:24 2016
Quant Method : Z:\HPCHEM1\BNA_G\Methods\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 01 19:22:14 2016
Response via : Initial Calibration

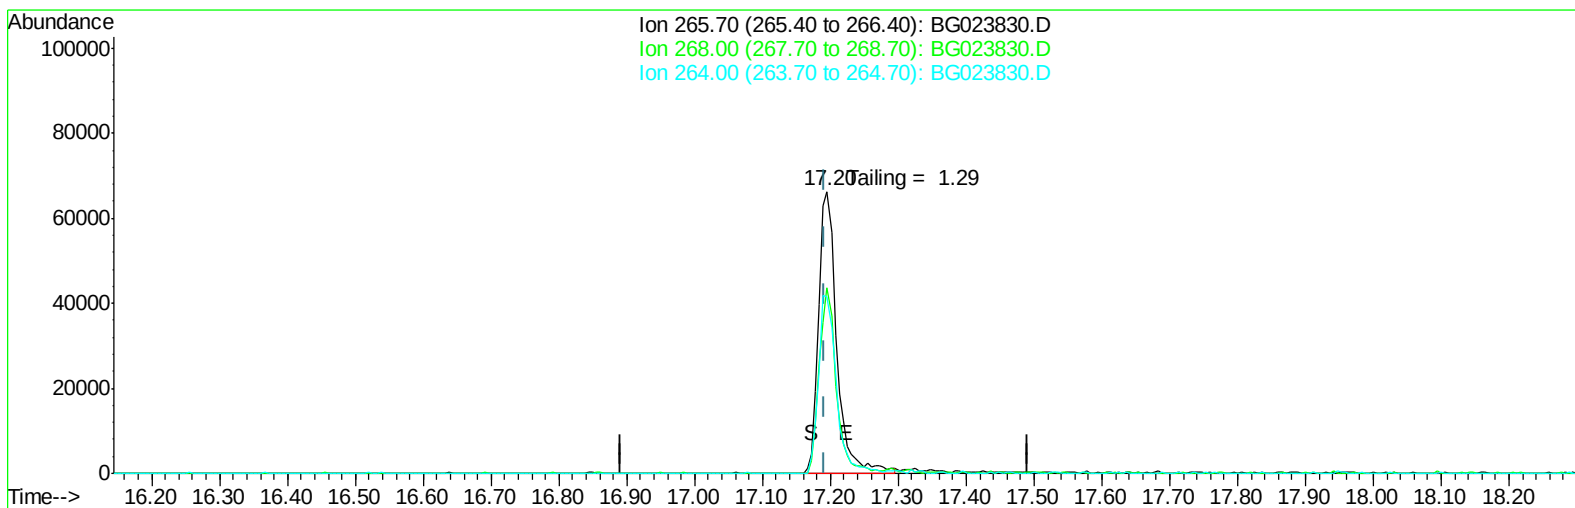

TIC: BG023830.D

(69) Pentachlorophenol (C)




17.196min (+0.003) 1636.03ng

response 121828

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	65.85
264.00	63.20	62.61
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG082216\
Data File : BG023830.D
Acq On : 22 Aug 2016 12:21
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 08:12:24 2016
Quant Method : Z:\HPCHEM1\BNA_G\Methods\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 01 19:22:14 2016
Response via : Initial Calibration

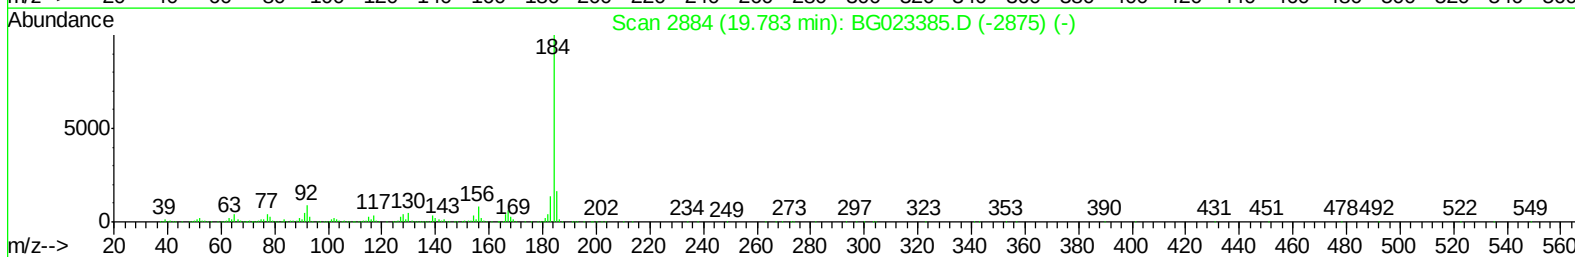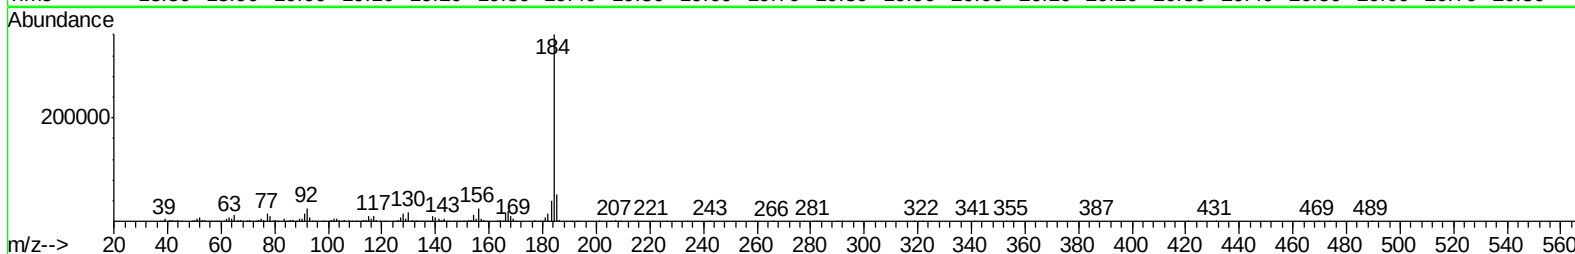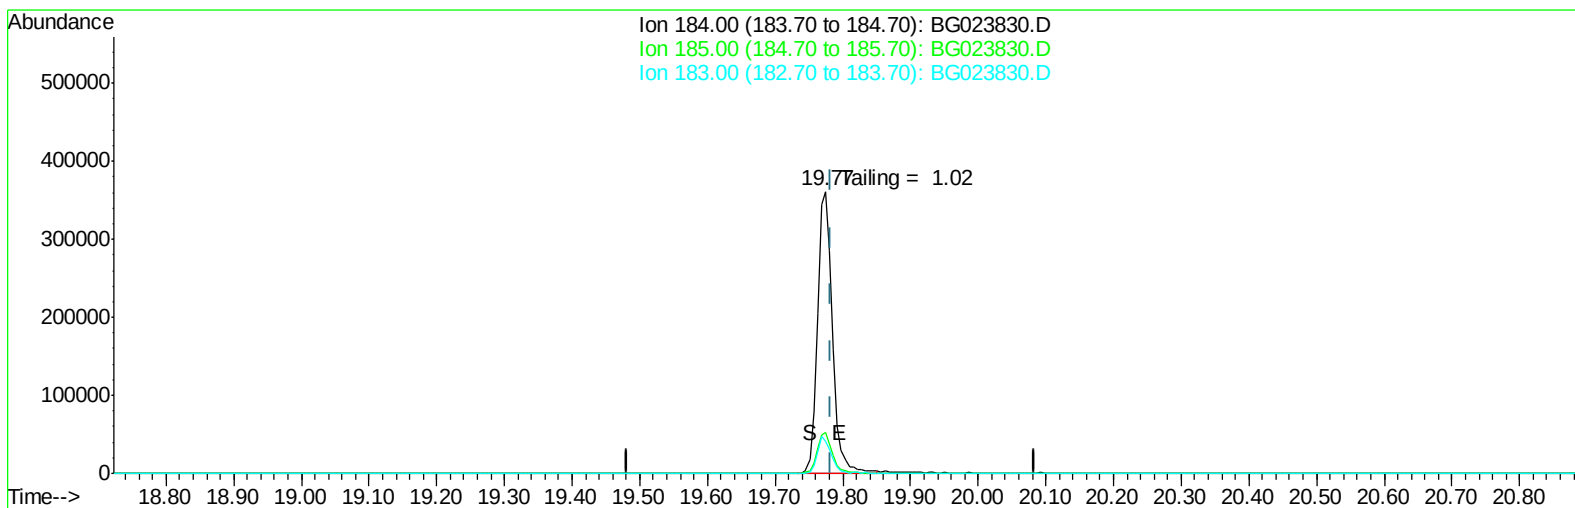

TIC: BG023830.D

(76) Benzidine

19.774min (-0.009) 1635.70ng

response 568739

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.62
183.00	13.40	11.32
0.00	0.00	0.00