


Data Path : Z:\HPCHEM1\BNA G\Data\BG082216\
 Data File : BG023830.D
 Acq On : 22 Aug 2016 12:21
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\Methods\8270-BG080116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 01 19:22:14 2016

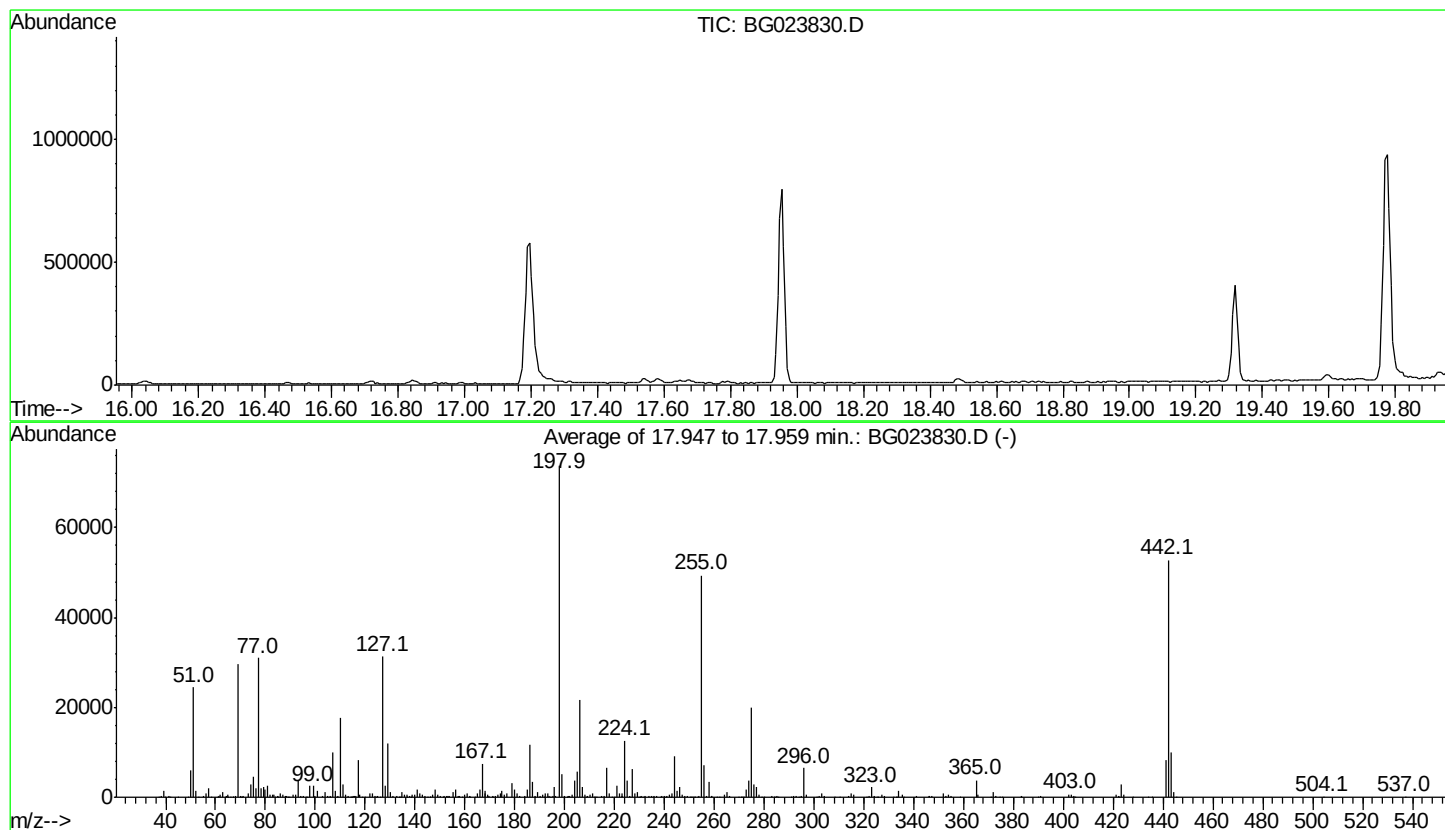

AutoFind: Scans 2572, 2573, 2574; Background Corrected with Scan 2565

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.1	24394	PASS
68	69	0.00	2	0.8	230	PASS
69	198	0.00	100	40.3	29735	PASS
70	69	0.00	2	0.8	225	PASS
127	198	10	80	42.4	31264	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	73805	PASS
199	198	5	9	6.9	5108	PASS
275	198	10	60	27.1	19976	PASS
365	198	1	100	5.0	3716	PASS
441	442	0.01	24	15.6	8247	PASS
442	198	50	100	71.4	52728	PASS
443	442	15	24	19.2	10112	PASS