

Data Path : U:\HPCHEM1\BNA G\DATA\BG082217\
 Data File : BG028417.D
 Acq On : 22 Aug 2017 13:56
 Operator : SJ/JU
 Sample : PB101638BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK38

Quant Time: Aug 23 03:45:04 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 23 02:58:29 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.34	152	33689	20.00	ng/ul	0.00
18) Naphthalene-d8	11.16	136	155116	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.95	164	119976	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.80	188	623660	20.00	ng/ul	0.10
75) Chrysene-d12	22.03	240	334380	20.00	ng/ul	0.00
83) Perylene-d12	25.53	264	325087	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.83	96	4619	6.38	ng/uL	0.00
5) Phenol-d5	7.50	99	114466	30.94	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.65	67	74560	31.82	ng/ul	0.00
9) 2-Chlorophenol-d4	7.88	132	85699	36.72	ng/ul	0.00
13) 4-Methylphenol-d8	9.03	113	101132	32.70	ng/ul	0.00
19) Nitrobenzene-d5	9.51	128	47584	39.23	ng/ul	0.00
22) 2-Nitrophenol-d4	10.23	143	56653	42.60	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.78	165	101975	37.06	ng/ul	0.00
29) 4-Chloroaniline-d4	11.29	131	101594	33.17	ng/ul	0.00
43) Dimethylphthalate-d6	14.34	166	423051	39.64	ng/ul	0.00
46) Acenaphthylene-d8	14.65	160	471037	39.15	ng/ul	0.00
51) 4-Nitrophenol-d4	15.15	143	57411	33.84	ng/ul	0.00
57) Fluorene-d10	15.94	176	367064	38.34	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.06	200	72751	17.96	ng/ul	0.00
70) Anthracene-d10	17.80	188	623660	20.85	ng/ul	0.00
76) Pyrene-d10	20.07	212	682370	39.79	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.29	264	621692	40.85	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	9.03	70	2809	1.121 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : U:\HPCHEM1\BNA G\DATA\BG082217\
Data File : BG028417.D
Acq On : 22 Aug 2017 13:56
Operator : SJ/JU
Sample : PB101638BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK38

Quant Time: Aug 23 03:45:04 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 23 02:58:29 2017
Response via : Initial Calibration

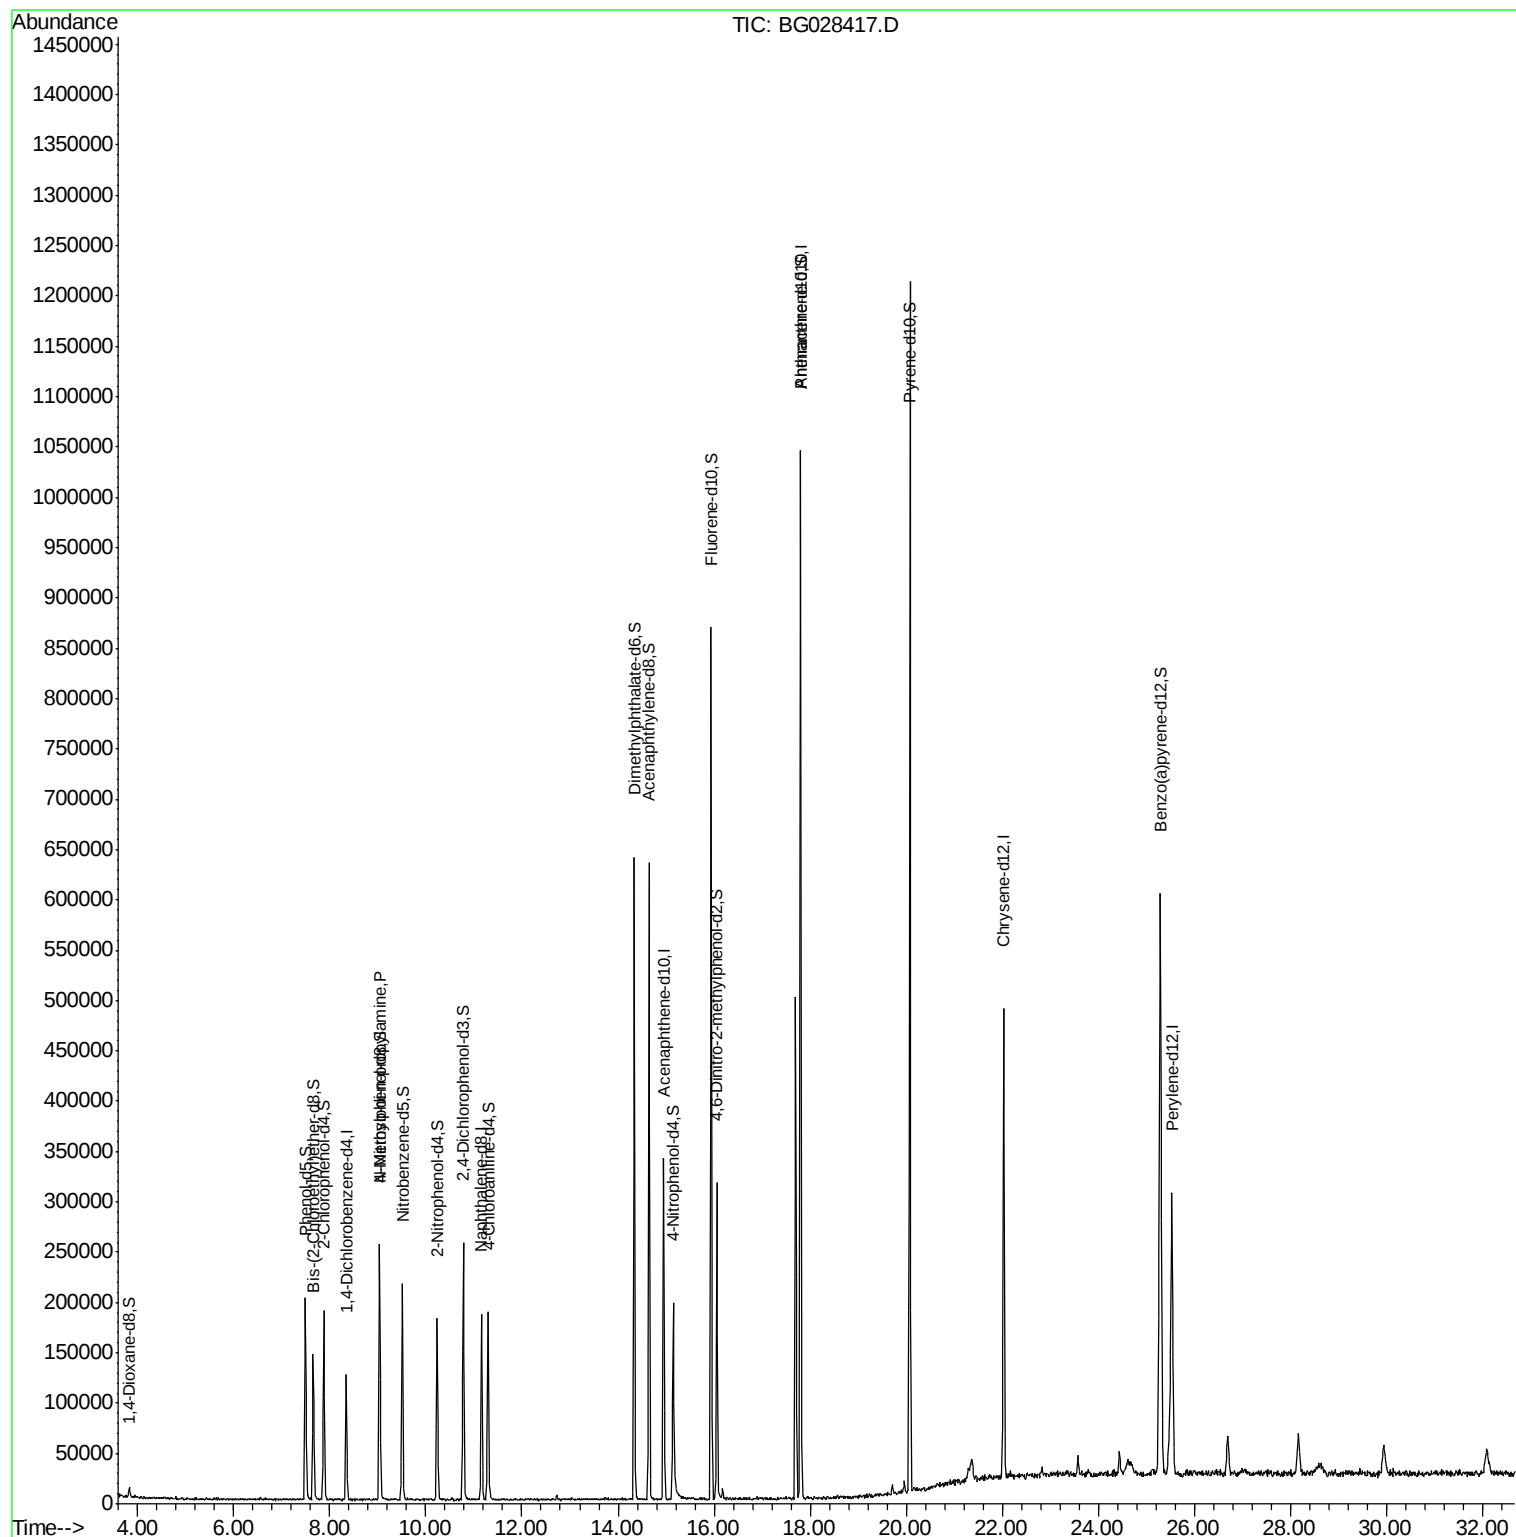

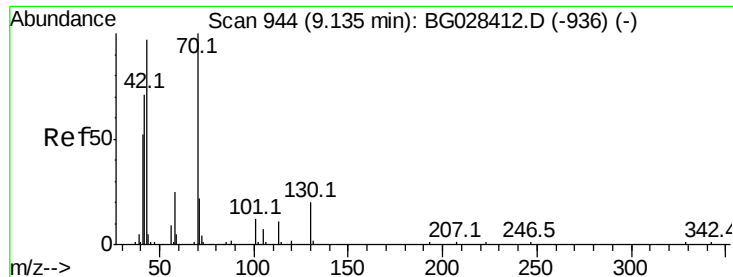

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.121 ng/ul
 RT: 9.03 min Scan# 927
 Delta R.T. -0.10 min
 Lab File: BG028417.D
 Acq: 22 Aug 2017 13:56

Instrument :
 BNA_G
 ClientSampleId :
 SBLK38

Tot Ion	Ratio	Lower	Upper
70	100		
42	347.3	59.0	88.6#
101	0.0	6.6	9.8#
130	0.0	15.6	23.4#

