
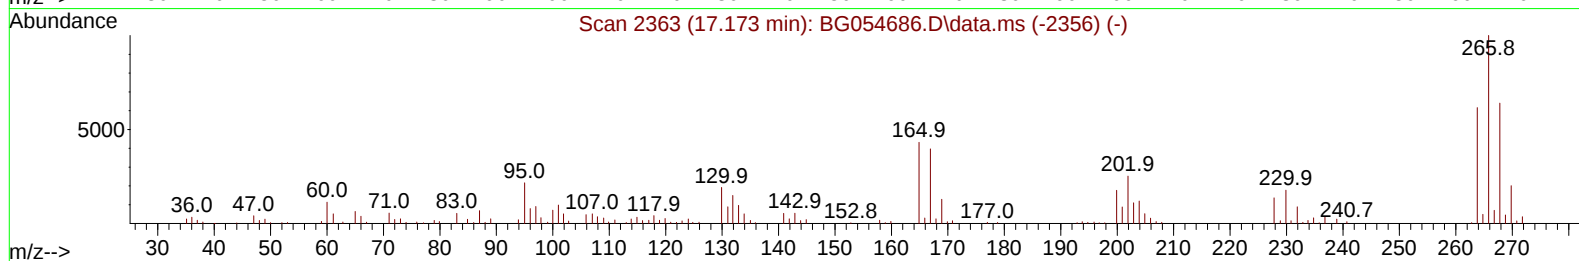
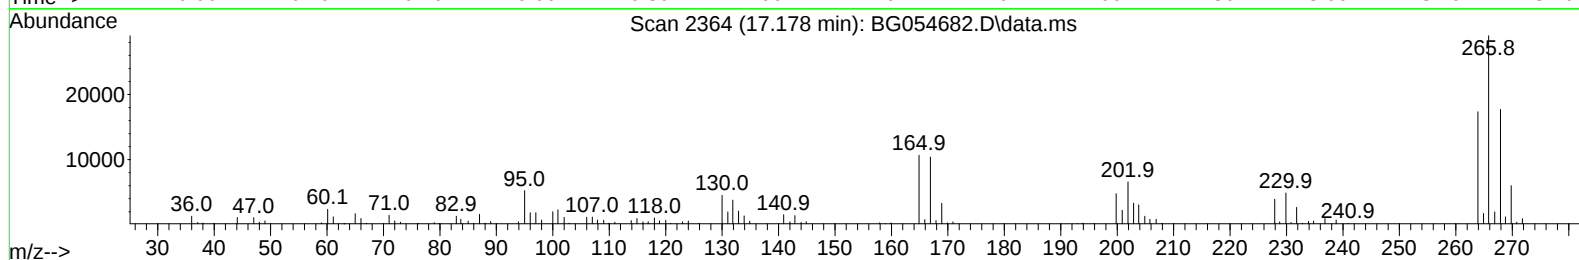


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082222\
Data File : BG054682.D
Acq On : 22 Aug 2022 14:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 06:29:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 23 03:09:46 2022
Response via : Initial Calibration

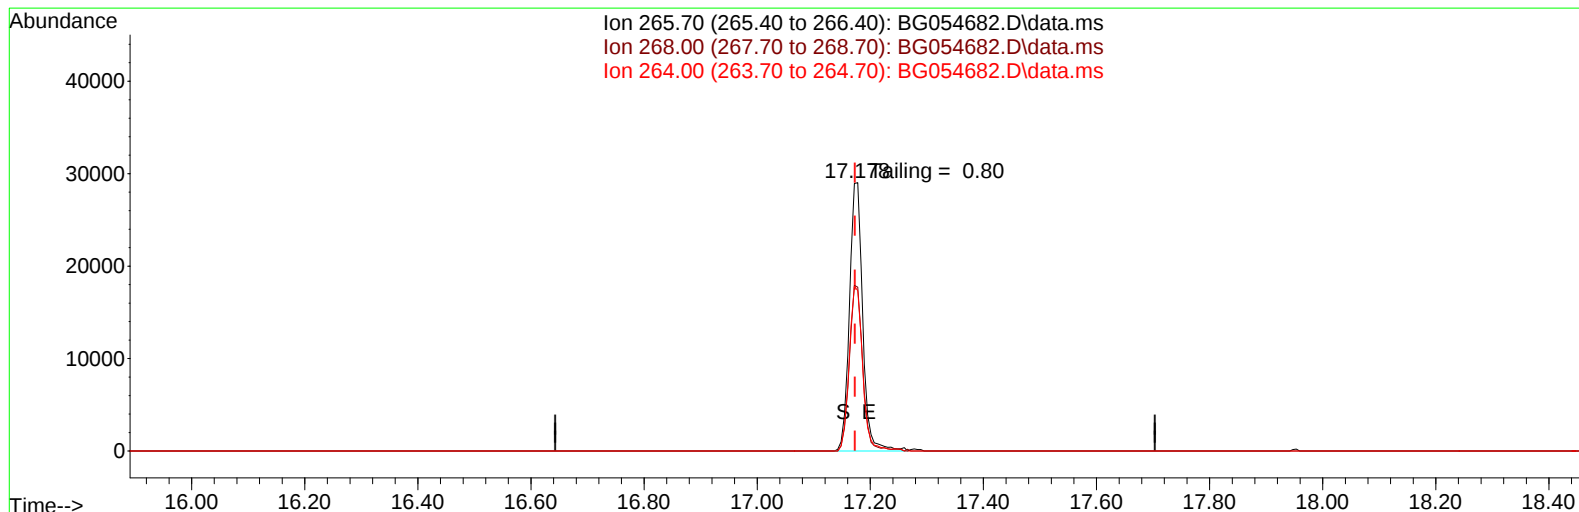

TIC: BG054682.D\data.ms

(70) Pentachlorophenol (C)




17.178min (+ 0.005) 95303.80 ng

response 47314

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	61.04
264.00	61.70	59.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082222\
Data File : BG054682.D
Acq On : 22 Aug 2022 14:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 23 06:29:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 23 03:09:46 2022
Response via : Initial Calibration

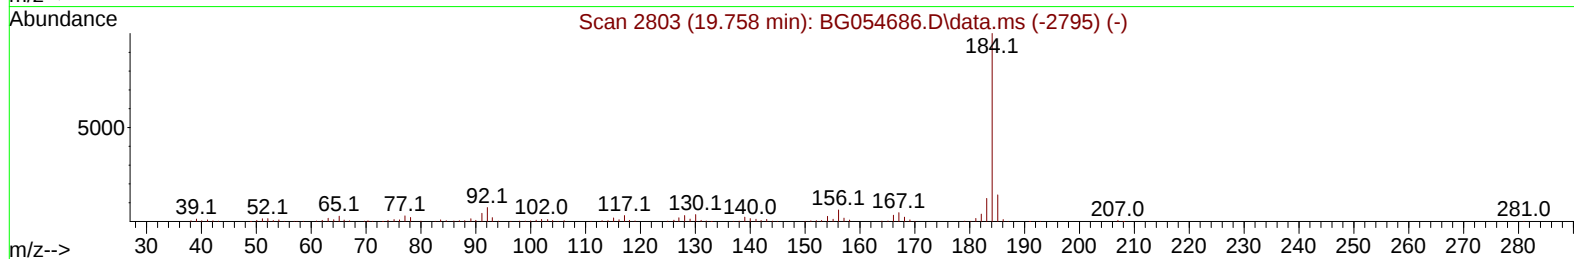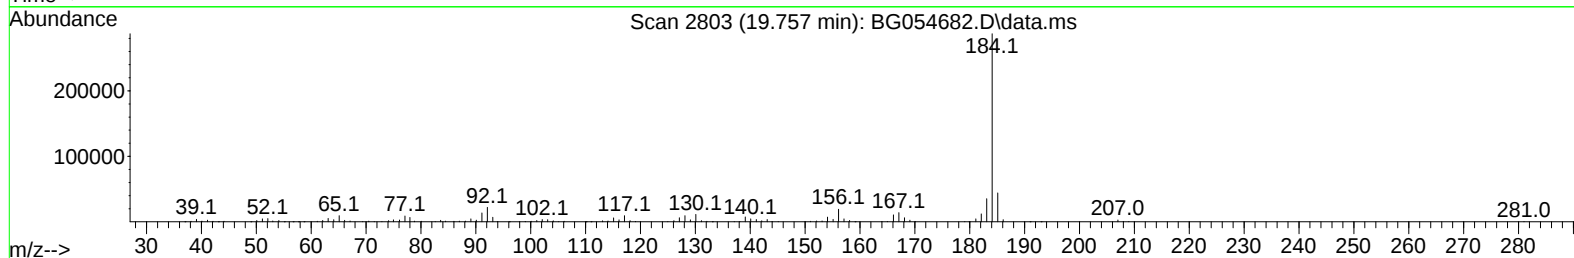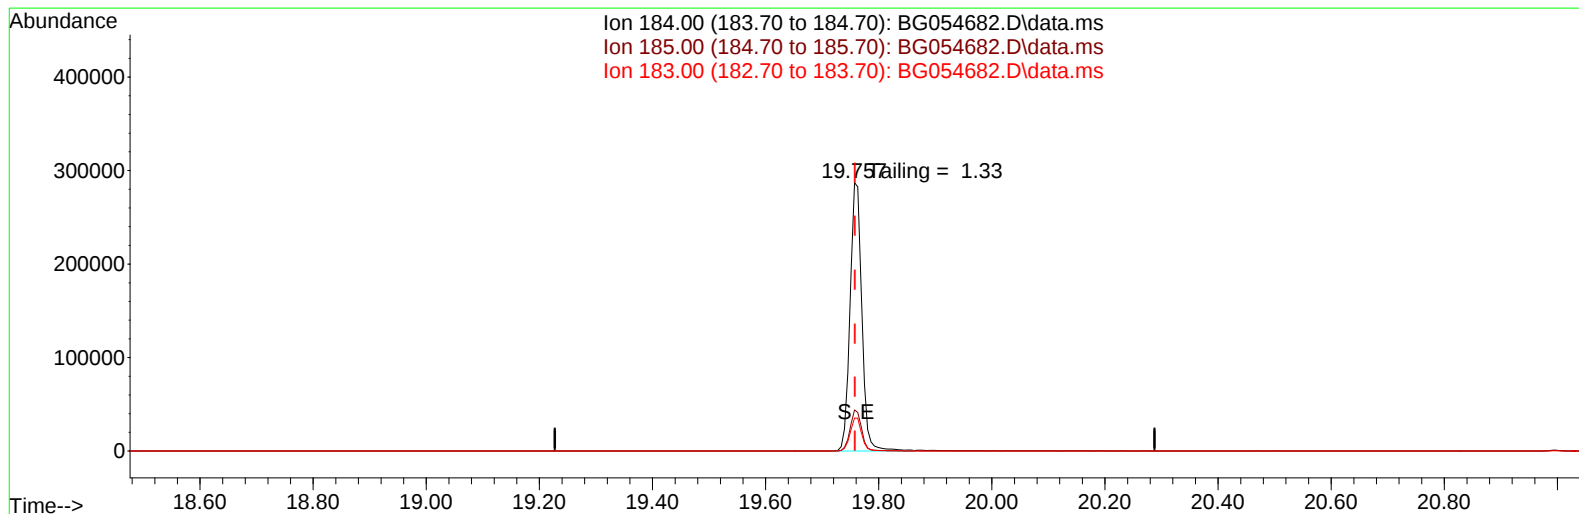

TIC: BG054682.D\data.ms

(77) Benzidine**19.757min (-0.001) 60030.96 ng****response 418394**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	15.33
183.00	12.30	12.32
0.00	0.00	0.00