


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082222\
 Data File : BG054682.D
 Acq On : 22 Aug 2022 14:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 23 03:09:46 2022

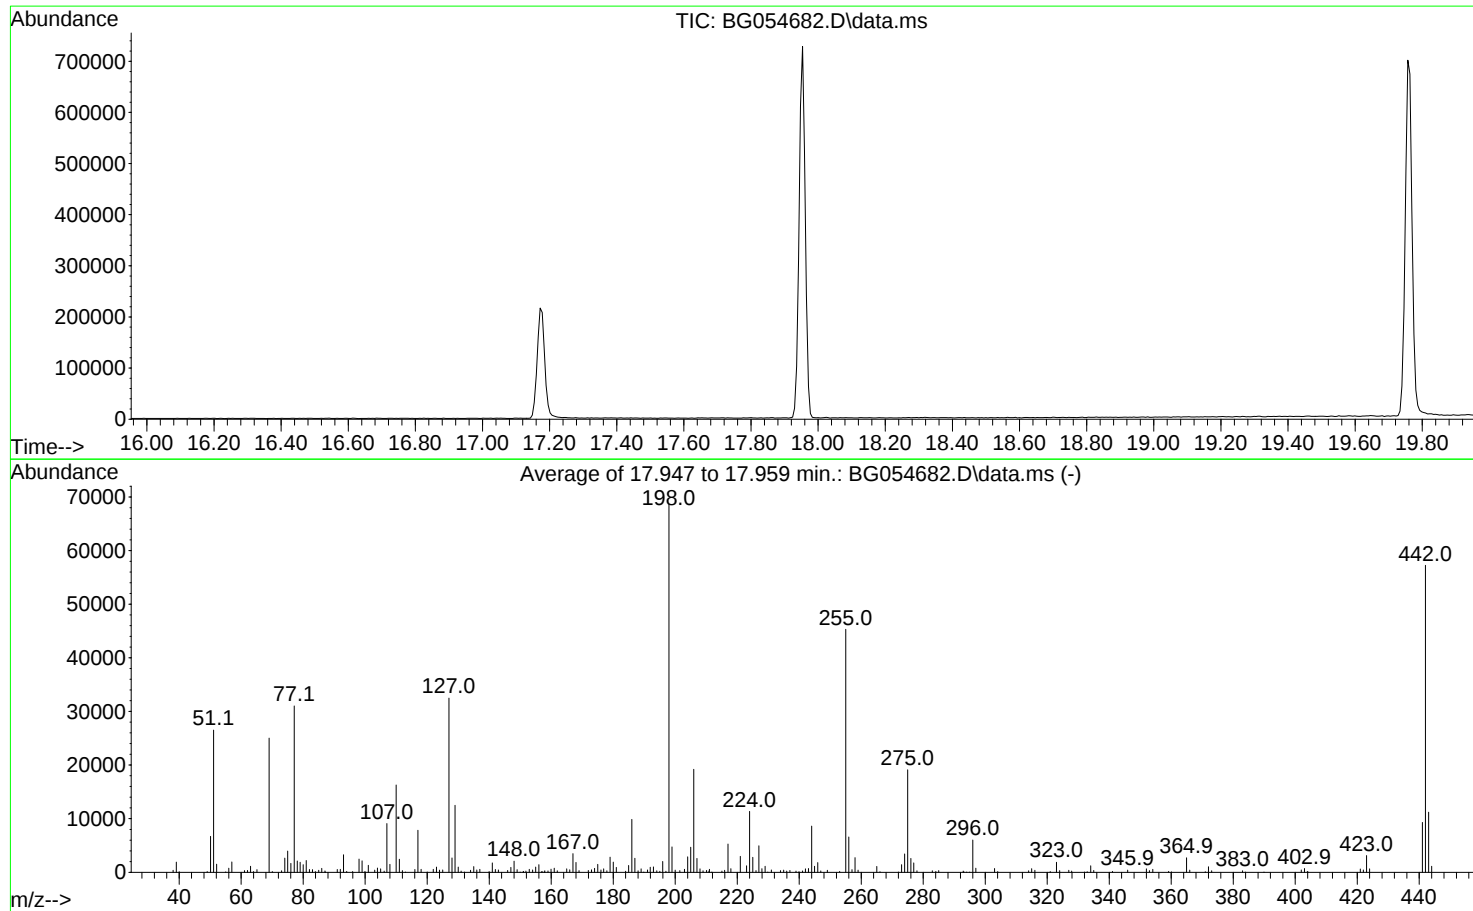




AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	26528	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.5	25016	PASS
70	69	0.00	2	0.5	134	PASS
127	198	10	80	47.4	32501	PASS
197	198	0.00	2	0.3	207	PASS
198	198	100	100	100.0	68624	PASS
199	198	5	9	6.9	4724	PASS
275	198	10	60	27.9	19133	PASS
365	198	1	100	3.9	2688	PASS
441	198	0.01	100	13.6	9309	PASS
442	442	50	100	100.0	57269	PASS
443	442	15	24	19.6	11210	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082222\
Data File : BG054682.D
Acq On : 22 Aug 2022 14:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 23 06:29:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 23 03:09:46 2022
Response via : Initial Calibration

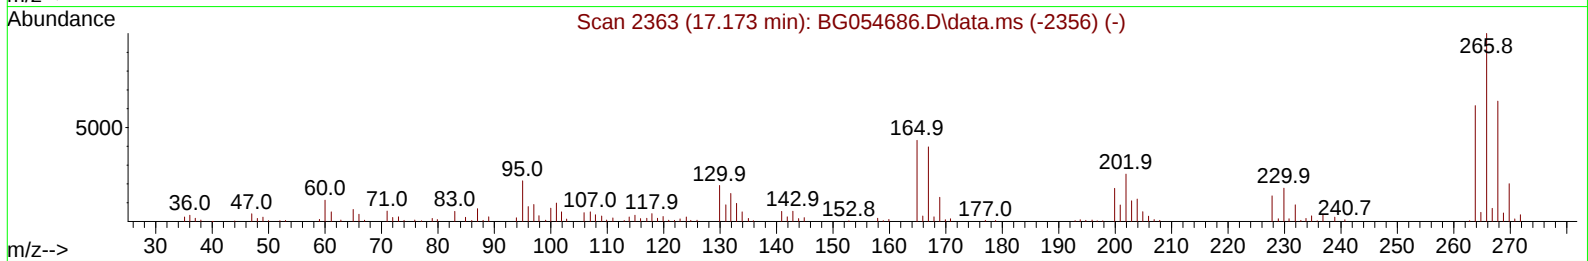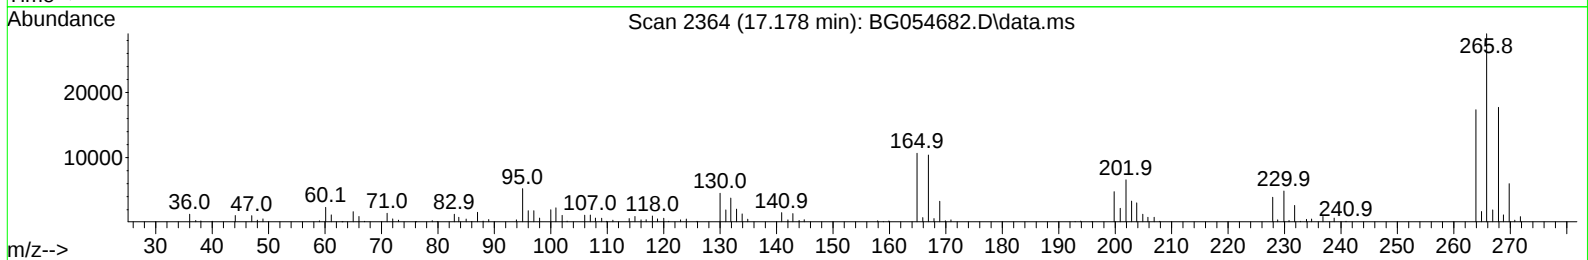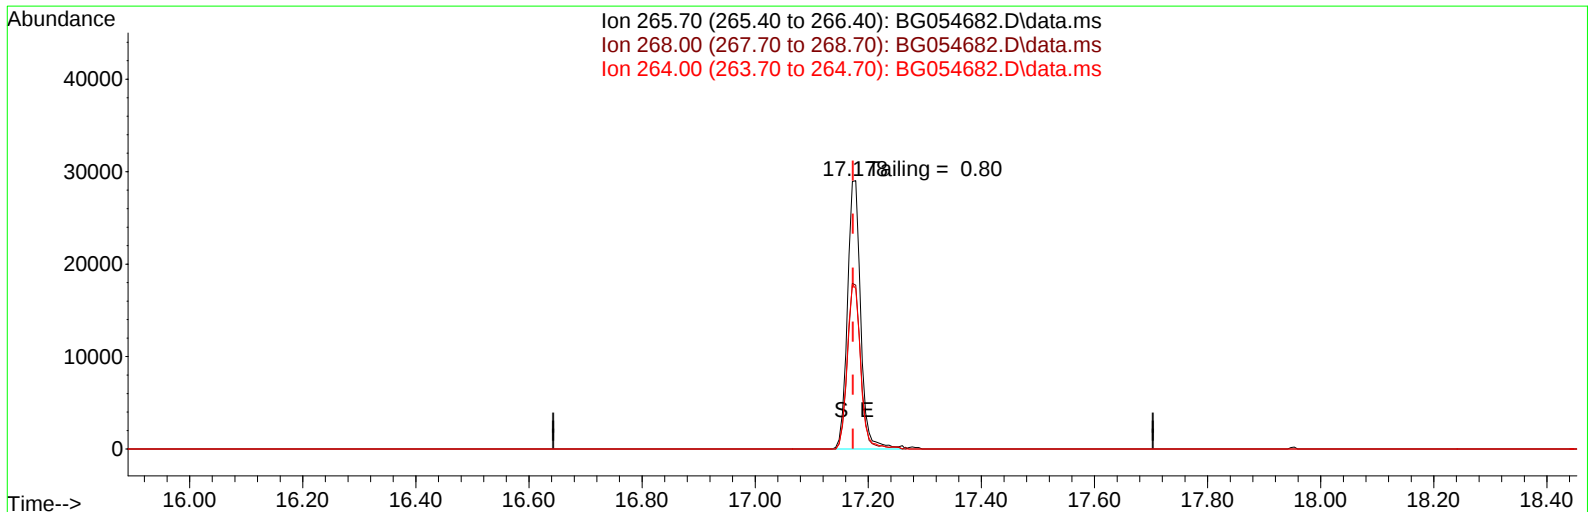

TIC: BG054682.D\data.ms

(70) Pentachlorophenol (C)

17.178min (+ 0.005) 95303.80 ng




response 47314

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	61.04
264.00	61.70	59.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082222\
Data File : BG054682.D
Acq On : 22 Aug 2022 14:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 23 06:29:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG082222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 23 03:09:46 2022
Response via : Initial Calibration

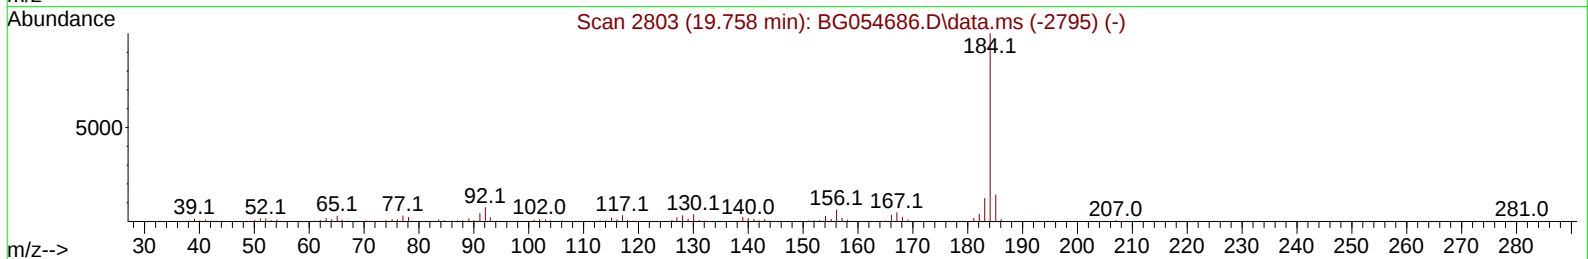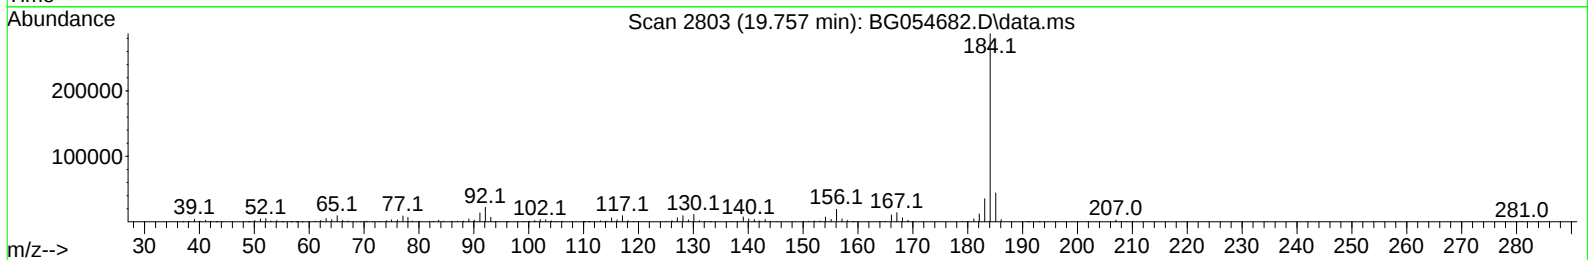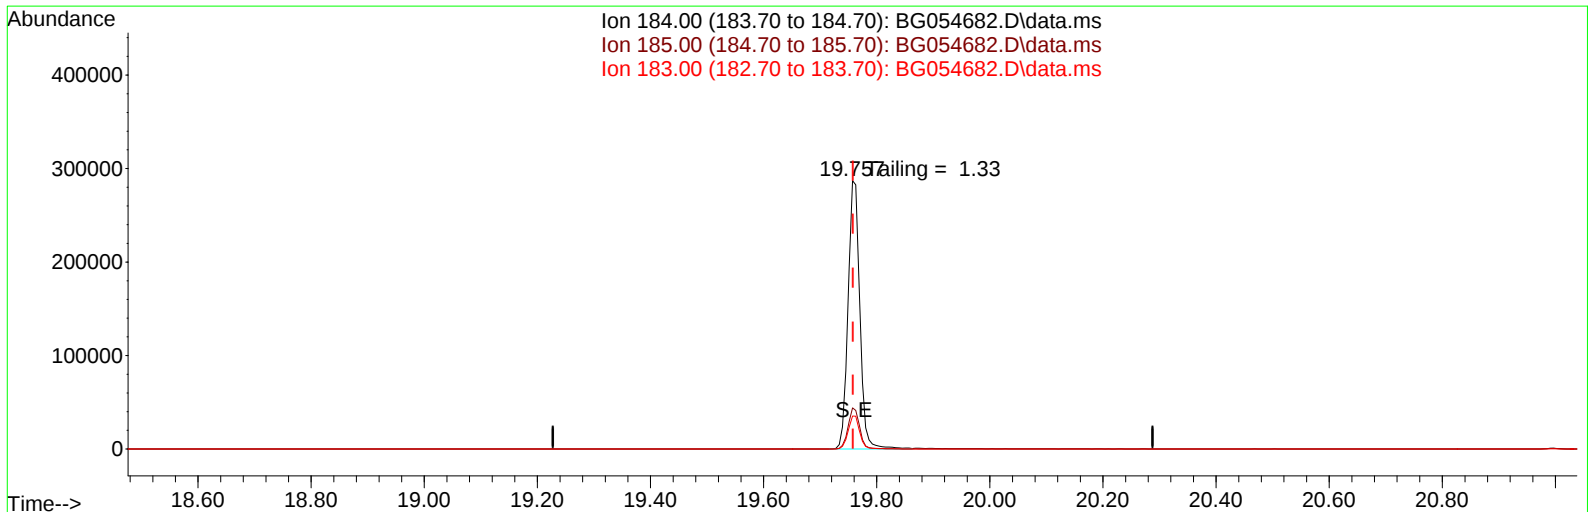

TIC: BG054682.D\data.ms

(77) Benzidine

19.757min (-0.001) 60030.96 ng

response 418394

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	15.33
183.00	12.30	12.32
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/22/2022	BNA_G	BG054682.D
Compound Name	Response	Retention Time
DDT	136385	20.997
DDD	5967	20.544
DDE	1891	20.039
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7858	144243	5.45

Instrument :
BNA_G
ClientSampleId :
DFTPP