

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082224\
 Data File : BG062539.D
 Acq On : 22 Aug 2024 14:02
 Operator : MA/JU
 Sample : P3673-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCXY7

Quant Time: Aug 22 15:34:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 20 23:01:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.941	152	63265	20.000	ng/u1	0.00
20) Naphthalene-d8	10.731	136	278569	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.561	164	220529	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.305	188	488563	20.000	ng/u1	0.00
79) Chrysene-d12	21.552	240	417420	20.000	ng/u1	0.00
88) Perylene-d12	24.642	264	483287	20.000	ng/u1	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	3235	1.941	ng/uL	0.00
4) Pyridine-d5	3.811	84	11507	2.266	ng/u1	0.00
7) Phenol-d5	7.101	99	80581	12.804	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.265	67	47087	11.877	ng/u1	0.00
11) 2-Chlorophenol-d4	7.471	132	59238	13.779	ng/u1	0.00
15) 4-Methylphenol-d8	8.634	113	65621	12.439	ng/u1	0.00
21) Nitrobenzene-d5	9.092	128	28846	16.147	ng/u1	0.00
24) 2-Nitrophenol-d4	9.809	143	31298	17.612	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.349	165	67709	14.959	ng/u1	0.00
31) 4-Chloroaniline-d4	10.860	131	36011	5.017	ng/u1	0.00
46) Dimethylphthalate-d6	13.968	166	222173	12.952	ng/u1	0.00
49) Acenaphthylene-d8	14.256	160	252714	13.306	ng/u1	0.00
54) 4-Nitrophenol-d4	14.749	143	26266	9.598	ng/u1	0.00
60) Fluorene-d10	15.554	176	211191	13.650	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.660	200	28290	12.744	ng/u1	0.00
73) Anthracene-d10	17.404	188	318622	13.576	ng/u1	0.00
81) Pyrene-d10	19.690	212	368722	15.083	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.424	264	355164	13.848	ng/u1	0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.458	149	14614	1.009	ng/u1	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082224\
Data File : BG062539.D
Acq On : 22 Aug 2024 14:02
Operator : MA/JU
Sample : P3673-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCXY7

Quant Time: Aug 22 15:34:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 20 23:01:24 2024
Response via : Initial Calibration

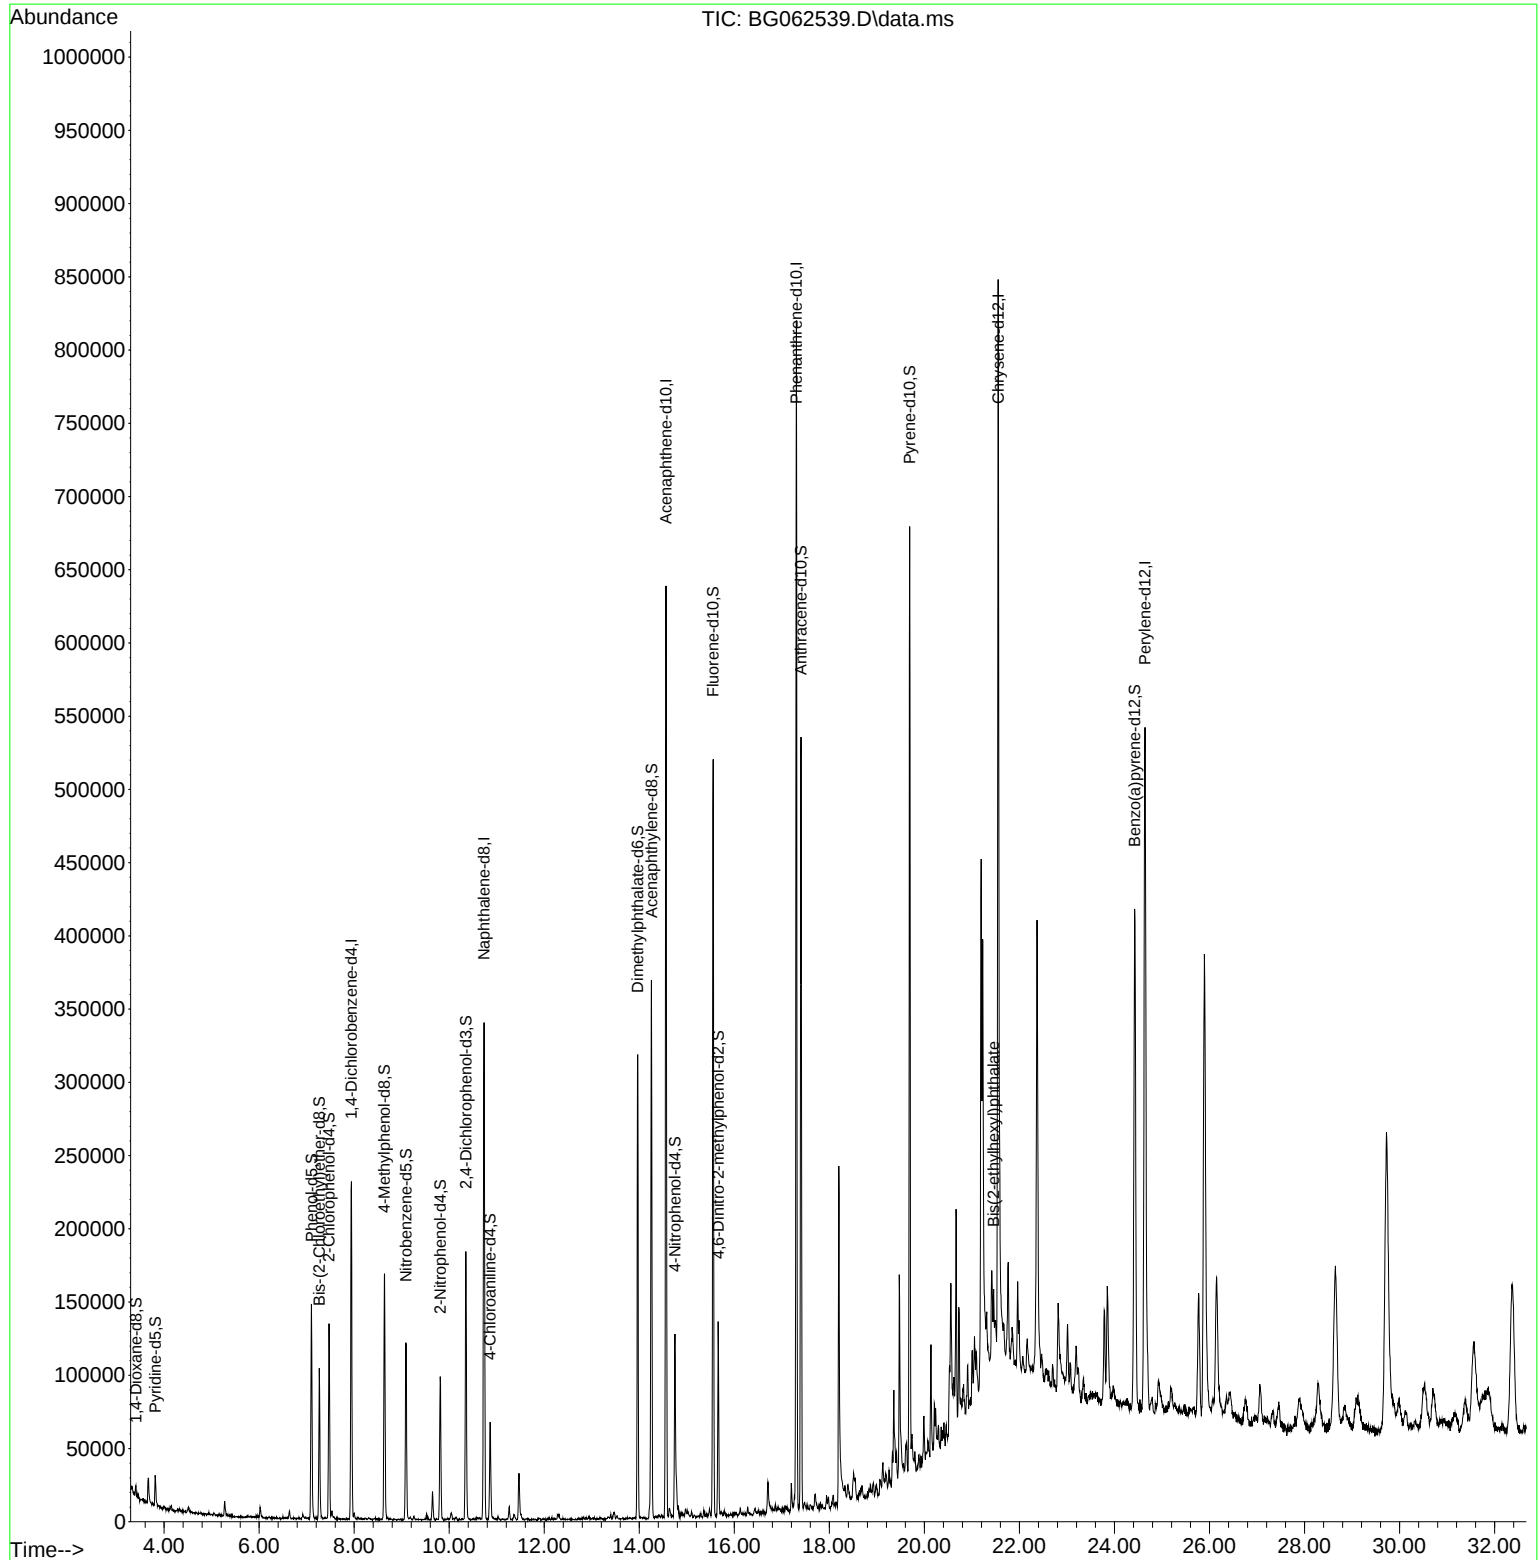

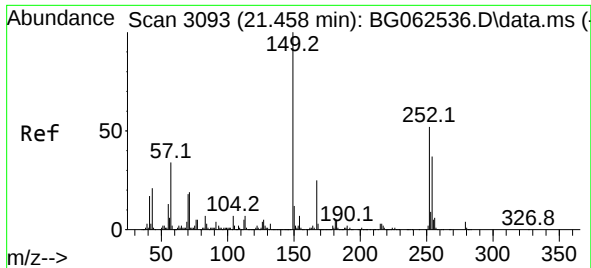

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.009 ng/ul
 RT: 21.458 min Scan# 3093
 Delta R.T. 0.012 min
 Lab File: BG062539.D
 Acq: 22 Aug 2024 14:02

Instrument :
 BNA_G
 ClientSampleId :
 DCXY7

Tgt Ion:149 Resp: 14614
 Ion Ratio Lower Upper
 149 100
 167 31.3 21.2 31.8
 279 3.8 2.7 4.1

