

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082224\
 Data File : BG062543.D
 Acq On : 22 Aug 2024 16:45
 Operator : MA/JU
 Sample : P3673-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCY18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062543.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.399	17	19	23	rVB2	8958	9805	0.63%	0.062%
2	3.663	61	64	69	rBV	16191	21143	1.37%	0.134%
3	3.810	84	89	101	rBV	122151	194492	12.58%	1.229%
4	4.145	144	146	150	rVB3	3509	3288	0.21%	0.021%
5	4.973	285	287	291	rBV4	1422	1861	0.12%	0.012%
6	5.056	297	301	305	rBV3	2756	4077	0.26%	0.026%
7	5.220	326	329	331	rBV4	1162	1627	0.11%	0.010%
8	5.596	390	393	398	rBV4	1068	1601	0.10%	0.010%
9	6.019	461	465	469	rBV	6200	7921	0.51%	0.050%
10	7.100	642	649	661	rVB	164343	278982	18.05%	1.763%
11	7.264	671	677	685	rBV	117302	190208	12.31%	1.202%
12	7.470	705	712	719	rBV	155467	252514	16.34%	1.596%
13	7.529	719	722	731	rVV2	4907	9783	0.63%	0.062%
14	7.599	731	734	738	rVB4	1296	1937	0.13%	0.012%
15	7.934	782	791	798	rBV	287046	487668	31.55%	3.081%
16	7.999	798	802	807	rVB3	4175	6678	0.43%	0.042%
17	8.633	901	910	919	rBV	194576	336358	21.76%	2.125%
18	8.704	919	922	926	rVB2	1323	2271	0.15%	0.014%
19	9.085	978	987	998	rBV	146075	257528	16.66%	1.627%
20	9.362	1030	1034	1038	rBV3	1051	1581	0.10%	0.010%
21	9.520	1055	1061	1066	rBV5	1662	2831	0.18%	0.018%
22	9.644	1077	1082	1088	rBV2	18645	30031	1.94%	0.190%
23	9.808	1103	1110	1121	rBV2	124168	212515	13.75%	1.343%
24	10.349	1194	1202	1210	rBV	192737	334417	21.63%	2.113%
25	10.730	1255	1267	1275	rBV	420680	741435	47.97%	4.685%
26	10.860	1281	1289	1296	rBV	205132	362207	23.43%	2.289%
27	11.259	1354	1357	1365	rVB3	6219	8701	0.56%	0.055%
28	11.465	1386	1392	1399	rBV2	30032	55078	3.56%	0.348%
29	12.305	1531	1535	1541	rBV4	3366	5449	0.35%	0.034%
30	13.391	1714	1720	1725	rVB3	3634	6242	0.40%	0.039%
31	13.538	1741	1745	1749	rVB5	2646	4034	0.26%	0.025%
32	13.732	1775	1778	1784	rBV2	1058	2260	0.15%	0.014%
33	13.961	1811	1817	1825	rVB	380711	550053	35.59%	3.476%
34	14.249	1853	1866	1874	rBV	427437	683136	44.19%	4.316%
35	14.466	1899	1903	1907	rVB2	2079	2837	0.18%	0.018%
36	14.560	1912	1919	1926	rVB	780914	1199003	77.57%	7.576%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082224\
 Data File : BG062543.D
 Acq On : 22 Aug 2024 16:45
 Operator : MA/JU
 Sample : P3673-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCY18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
 Title : SVOA CALIBRATION

37	14.748	1944	1951	1963	rBV3	164886	311535	20.15%	1.968%
38	14.972	1986	1989	1993	rBV4	4703	5923	0.38%	0.037%
39	15.030	1997	1999	2004	rBV3	1181	1996	0.13%	0.013%
40	15.283	2040	2042	2045	rBV2	1426	1703	0.11%	0.011%
41	15.353	2051	2054	2058	rBV	3162	3403	0.22%	0.022%
42	15.412	2062	2064	2068	rBV4	2522	2773	0.18%	0.018%
43	15.547	2080	2087	2095	rBV	586143	895939	57.96%	5.661%
44	15.659	2100	2106	2114	rVV	136456	195499	12.65%	1.235%
45	15.718	2114	2116	2119	rVV3	2263	1913	0.12%	0.012%
46	15.782	2123	2127	2132	rBV4	2173	4700	0.30%	0.030%
47	15.917	2146	2150	2155	rBV3	2359	4058	0.26%	0.026%
48	15.988	2157	2162	2164	rBV4	1313	2213	0.14%	0.014%
49	16.035	2167	2170	2177	rVB3	2476	3700	0.24%	0.023%
50	16.105	2177	2182	2185	rBV4	2171	4213	0.27%	0.027%
51	16.276	2206	2211	2217	rVB3	3245	4898	0.32%	0.031%
52	16.446	2236	2240	2243	rBV4	1283	1581	0.10%	0.010%
53	16.857	2305	2310	2314	rBV3	3513	4123	0.27%	0.026%
54	17.016	2334	2337	2342	rBV2	1732	2528	0.16%	0.016%
55	17.069	2343	2346	2348	rBV3	2682	2766	0.18%	0.017%
56	17.186	2364	2366	2367	rBV	2050	1679	0.11%	0.011%
57	17.304	2378	2386	2395	rBV	995239	1493377	96.61%	9.436%
58	17.398	2396	2402	2412	rVV2	647258	976810	63.19%	6.172%
59	17.486	2412	2417	2422	rVV5	11005	16244	1.05%	0.103%
60	17.551	2425	2428	2429	rVB2	2408	1838	0.12%	0.012%
61	17.674	2446	2449	2452	rBV4	1446	2190	0.14%	0.014%
62	17.973	2497	2500	2506	rVB5	6677	8939	0.58%	0.056%
63	18.085	2513	2519	2521	rBV4	2183	3961	0.26%	0.025%
64	18.197	2534	2538	2546	rBV4	34289	56370	3.65%	0.356%
65	18.508	2587	2591	2594	rBV5	2666	4161	0.27%	0.026%
66	18.537	2594	2596	2601	rVB6	3016	3019	0.20%	0.019%
67	18.949	2664	2666	2670	rBV4	1618	2706	0.18%	0.017%
68	19.001	2672	2675	2680	rVB6	3024	4910	0.32%	0.031%
69	19.072	2681	2687	2688	rBV6	2874	4433	0.29%	0.028%
70	19.142	2696	2699	2703	rVB4	8959	11332	0.73%	0.072%
71	19.178	2703	2705	2708	rVB4	2932	2619	0.17%	0.017%
72	19.219	2708	2712	2713	rBV3	2279	2903	0.19%	0.018%
73	19.254	2713	2718	2723	rBV4	12185	17461	1.13%	0.110%
74	19.325	2726	2730	2733	rVV2	9435	11973	0.77%	0.076%
75	19.354	2733	2735	2737	rVB3	1837	1551	0.10%	0.010%
76	19.383	2737	2740	2748	rVB8	3225	5891	0.38%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082224\
 Data File : BG062543.D
 Acq On : 22 Aug 2024 16:45
 Operator : MA/JU
 Sample : P3673-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCY18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
 Title : SVOA CALIBRATION

77	19.477	2751	2756	2762	rBV10	6729	14638	0.95%	0.092%
78	19.624	2777	2781	2785	rVB4	9535	10935	0.71%	0.069%
79	19.689	2785	2792	2797	rBV	764843	1099202	71.11%	6.945%
80	19.736	2797	2800	2806	rVB5	17373	23841	1.54%	0.151%
81	20.176	2874	2875	2877	rBV2	4221	3859	0.25%	0.024%
82	20.206	2877	2880	2882	rVV4	5328	7540	0.49%	0.048%
83	20.394	2910	2912	2915	rBV4	3330	3439	0.22%	0.022%
84	20.564	2939	2941	2943	rBV2	4792	4168	0.27%	0.026%
85	20.658	2955	2957	2961	rVB5	6326	7018	0.45%	0.044%
86	20.764	2973	2975	2977	rBV2	6842	5605	0.36%	0.035%
87	21.216	3048	3052	3058	rBV2	71168	116017	7.51%	0.733%
88	21.545	3102	3108	3116	rBV2	922322	1470502	95.13%	9.291%
89	22.338	3241	3243	3247	rBV4	9595	11447	0.74%	0.072%
90	23.002	3353	3356	3363	rVB6	15570	26824	1.74%	0.169%
91	23.184	3383	3387	3393	rVB	32656	57569	3.72%	0.364%
92	23.772	3483	3487	3497	rVB5	22458	51421	3.33%	0.325%
93	24.418	3588	3597	3609	rVB2	379311	999546	64.66%	6.316%
94	24.635	3623	3634	3649	rBV2	552983	1545740	100.00%	9.767%
95	27.461	4113	4115	4118	rBV4	6878	5719	0.37%	0.036%


Sum of corrected areas: 15826413

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082224\
Data File : BG062543.D
Acq On : 22 Aug 2024 16:45
Operator : MA/JU
Sample : P3673-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCY18

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

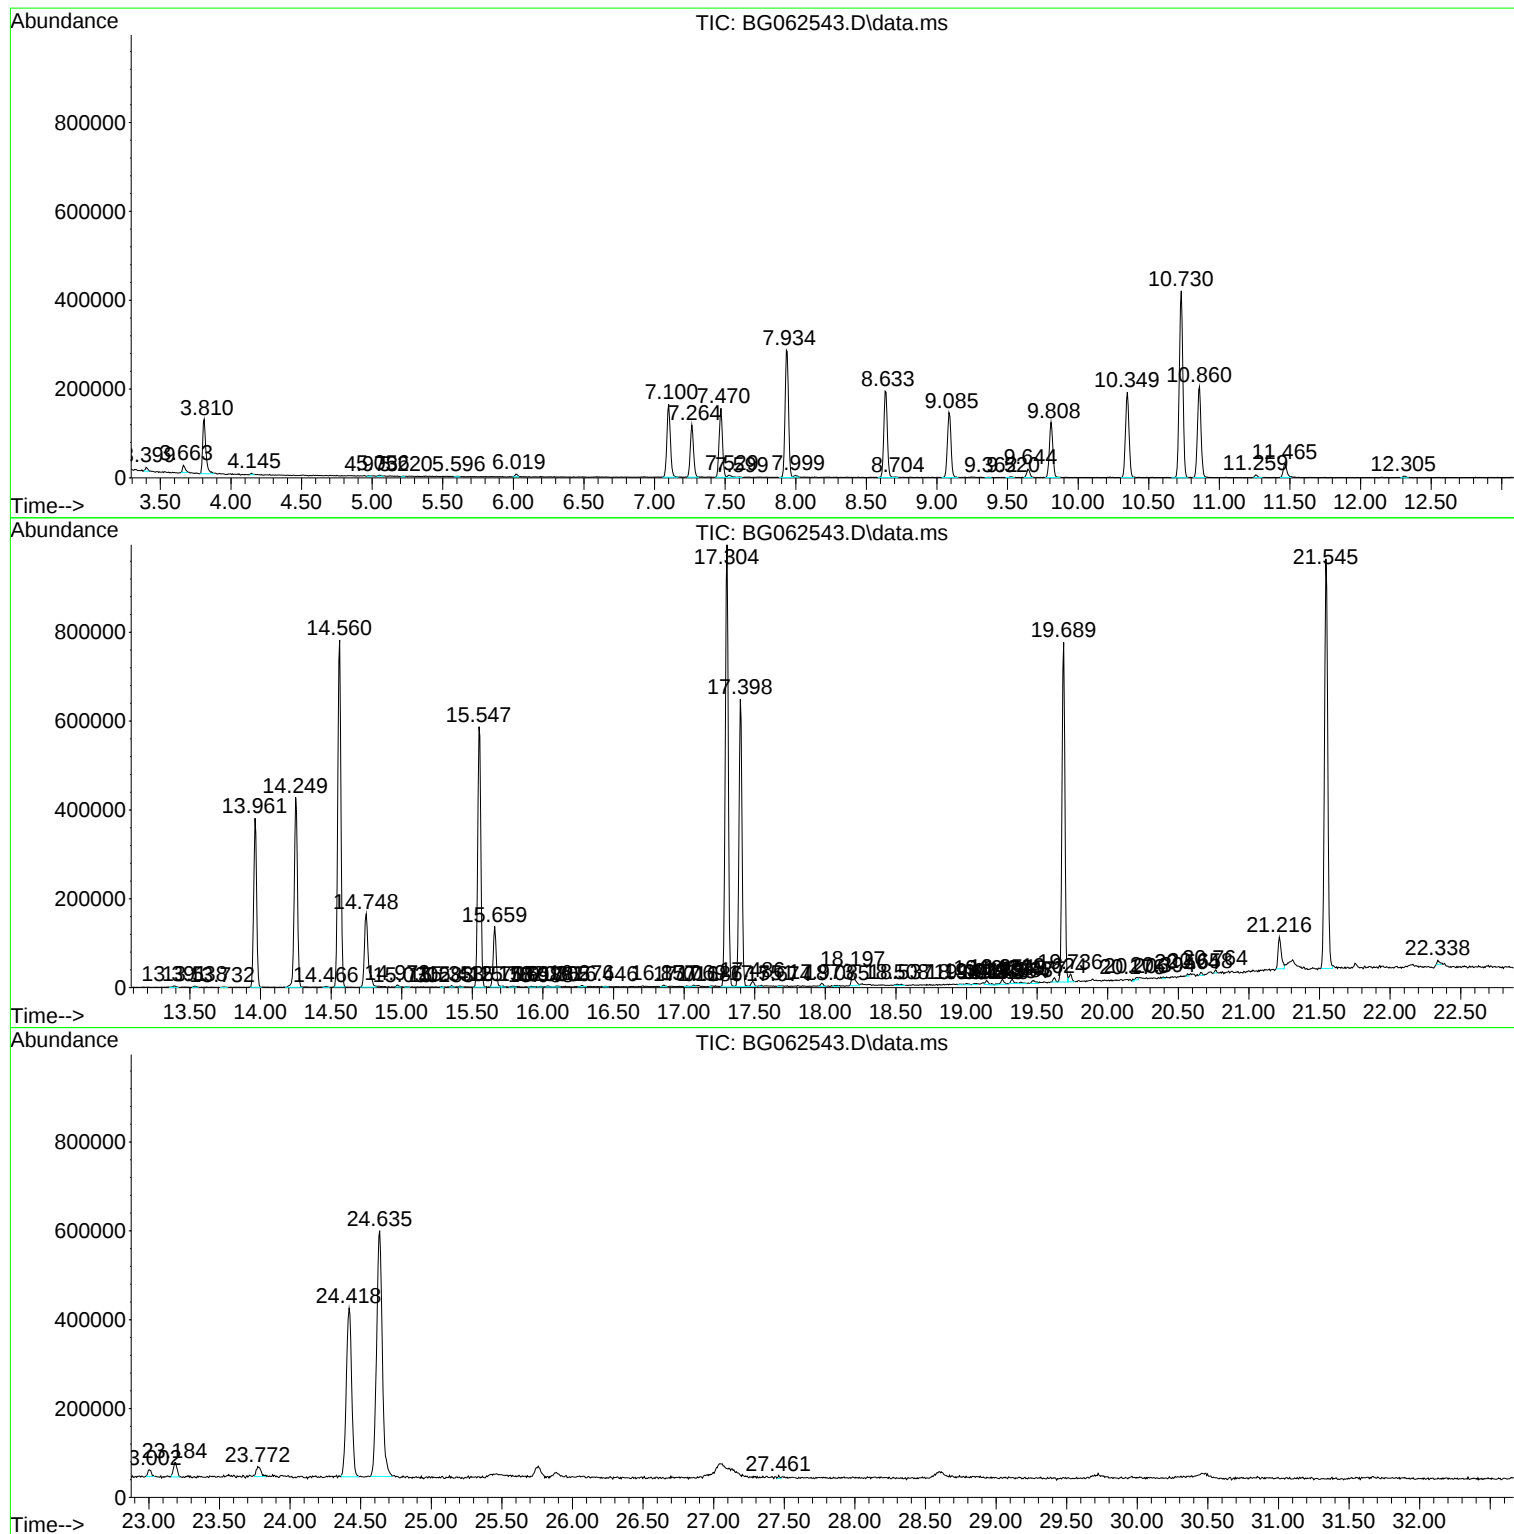

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082224\
Data File : BG062543.D
Acq On : 22 Aug 2024 16:45
Operator : MA/JU
Sample : P3673-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCY18

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG082224\
Data File : BG062543.D
Acq On : 22 Aug 2024 16:45
Operator : MA/JU
Sample : P3673-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCY18

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG081424.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc