
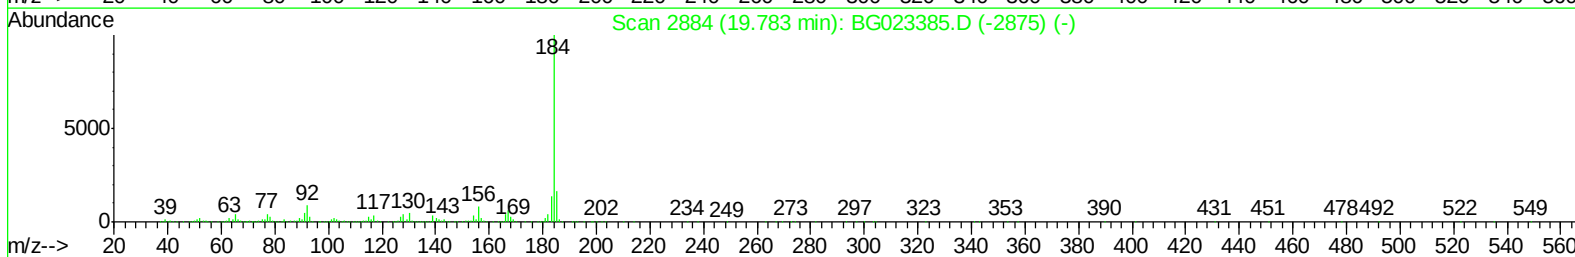
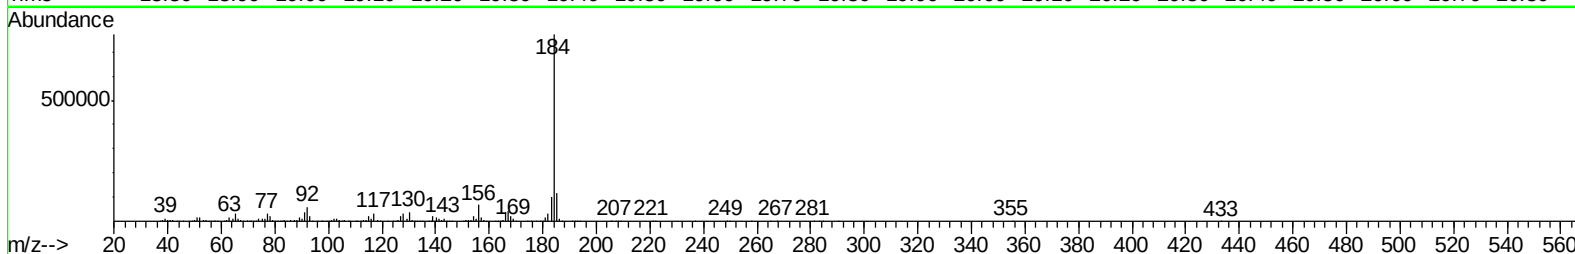


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG082316\
Data File : BG023864.D
Acq On : 23 Aug 2016 21:58
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 08:17:15 2016
Quant Method : Z:\HPCHEM1\BNA_G\Methods\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 01 19:22:14 2016
Response via : Initial Calibration

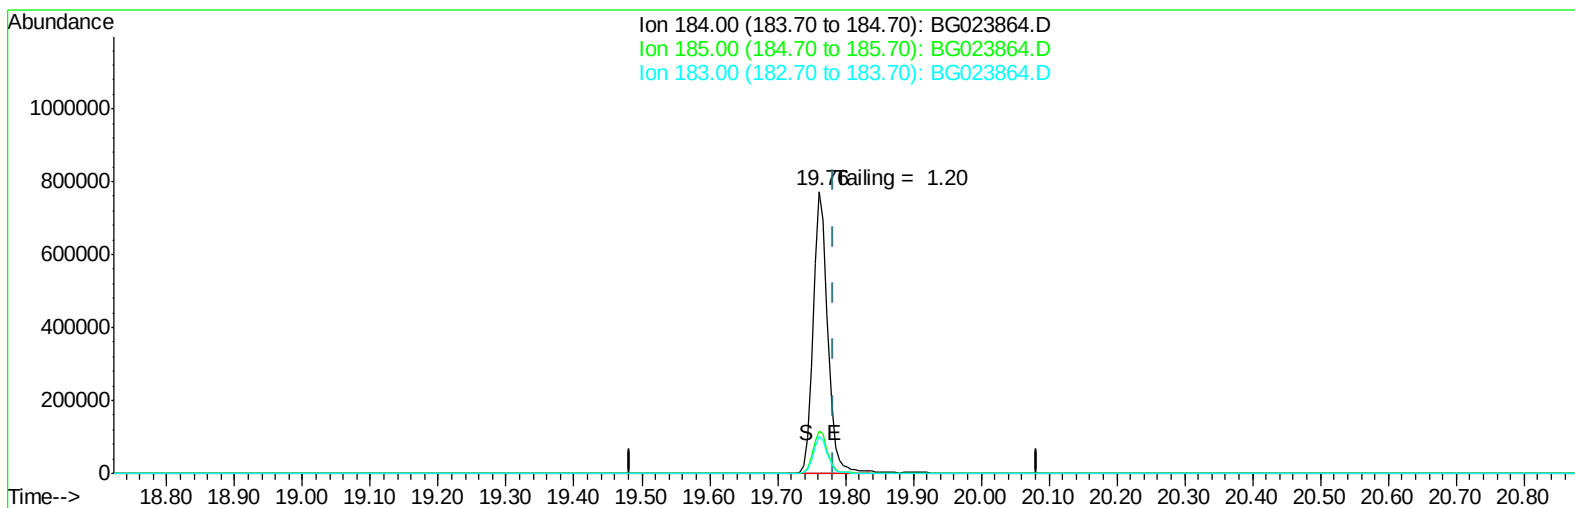

TIC: BG023864.D

(76) Benzidine




19.762min (-0.021) 85755.18ng

response 1160946

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.13
183.00	13.40	12.98
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG082316\
Data File : BG023864.D
Acq On : 23 Aug 2016 21:58
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 08:17:15 2016
Quant Method : Z:\HPCHEM1\BNA_G\Methods\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 01 19:22:14 2016
Response via : Initial Calibration

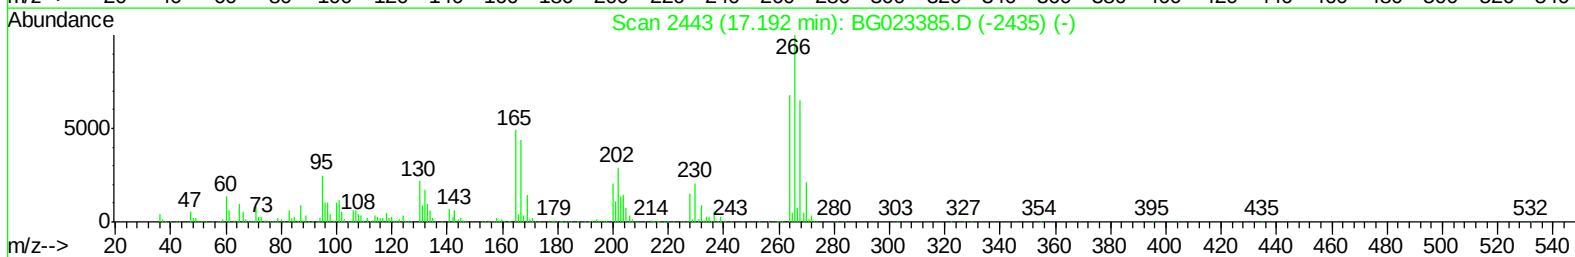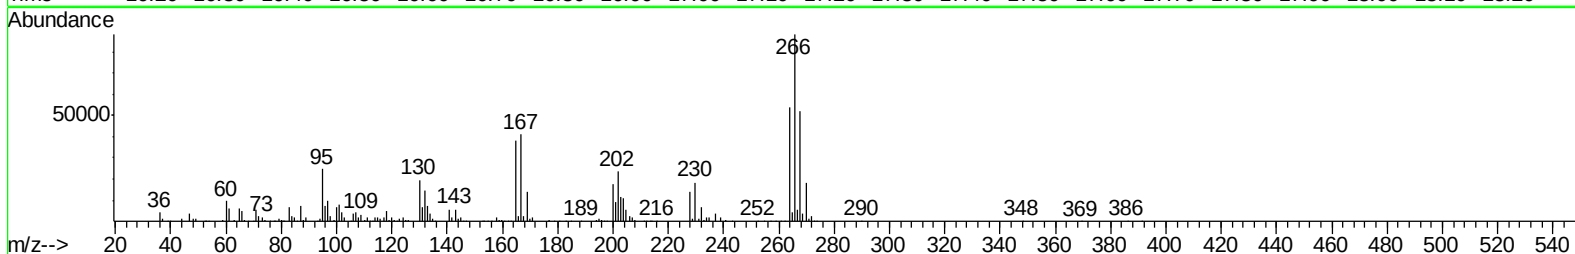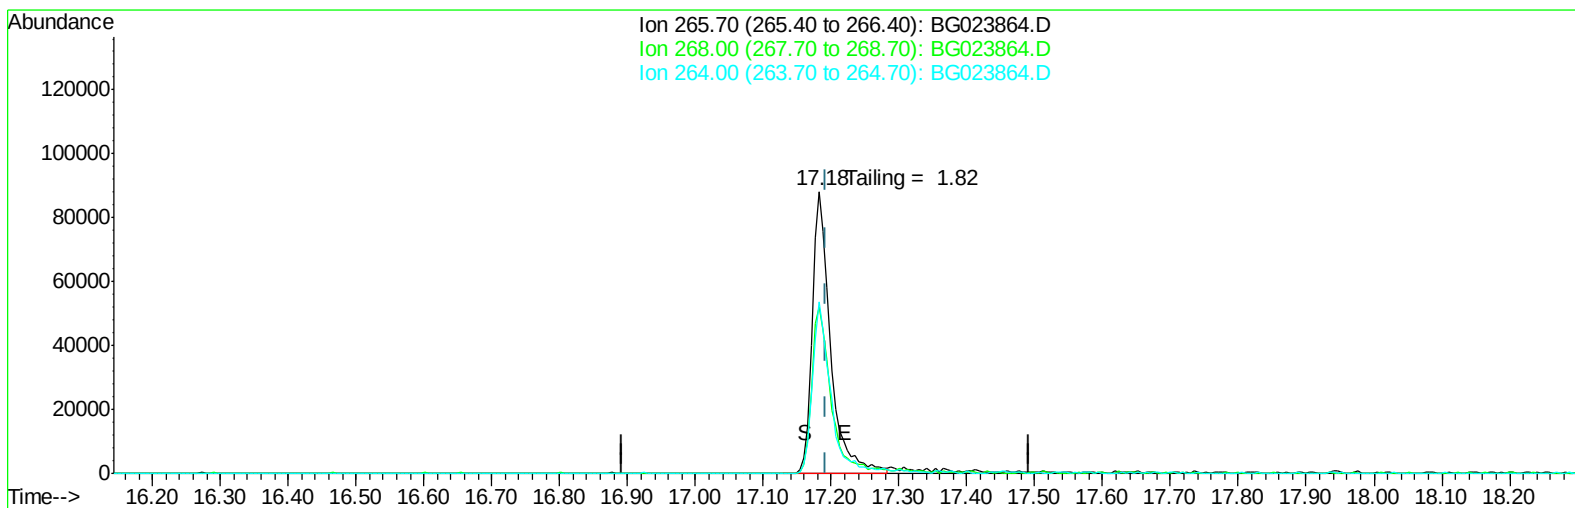

TIC: BG023864.D

(69) Pentachlorophenol (C)

17.183min (-0.010) 76161.21ng

response 167022

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	59.00
264.00	63.20	60.81
0.00	0.00	0.00