

Data Path : Z:\HPCHEM1\BNA G\DATA\BG082316\
 Data File : BG023853.D
 Acq On : 23 Aug 2016 15:01
 Operator : UM/SJ
 Sample : H4528-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 VITALEFILL-MCMPH3-2

Quant Time: Aug 24 01:38:37 2016
 Quant Method : Z:\HPCHEM1\BNA G\Methods\8270-BG080116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 01 19:22:14 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.09	152	103035	20.00	ng	-0.03
21) Naphthalene-d8	10.93	136	431045	20.00	ng	-0.03
38) Acenaphthene-d10	14.76	164	267627	20.00	ng	-0.02
63) Phenanthrene-d10	17.53	188	650702	20.00	ng	-0.01
75) Chrysene-d12	21.84	240	704827	20.00	ng	-0.02
86) Perylene-d12	25.21	264	695121	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	608993	99.49	ng	-0.03
7) Phenol-d6	7.24	99	865850	90.82	ng	-0.03
23) Nitrobenzene-d5	9.27	82	584601	67.43	ng	-0.03
41) 2,4,6-Tribromophenol	16.26	330	339693	86.78	ng	-0.02
44) 2-Fluorobiphenyl	13.38	172	1096490	69.10	ng	-0.02
78) Terphenyl-d14	20.13	244	1613897	67.78	ng	-0.02
Target Compounds						Qvalue
49) Dimethylphthalate	14.20	163	311555	15.17	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG082316\
Data File : BG023853.D
Acq On : 23 Aug 2016 15:01
Operator : UM/SJ
Sample : H4528-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
VITALEFILL-MCMPH3-2

Quant Time: Aug 24 01:38:37 2016
Quant Method : Z:\HPCHEM1\BNA G\Methods\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 01 19:22:14 2016
Response via : Initial Calibration

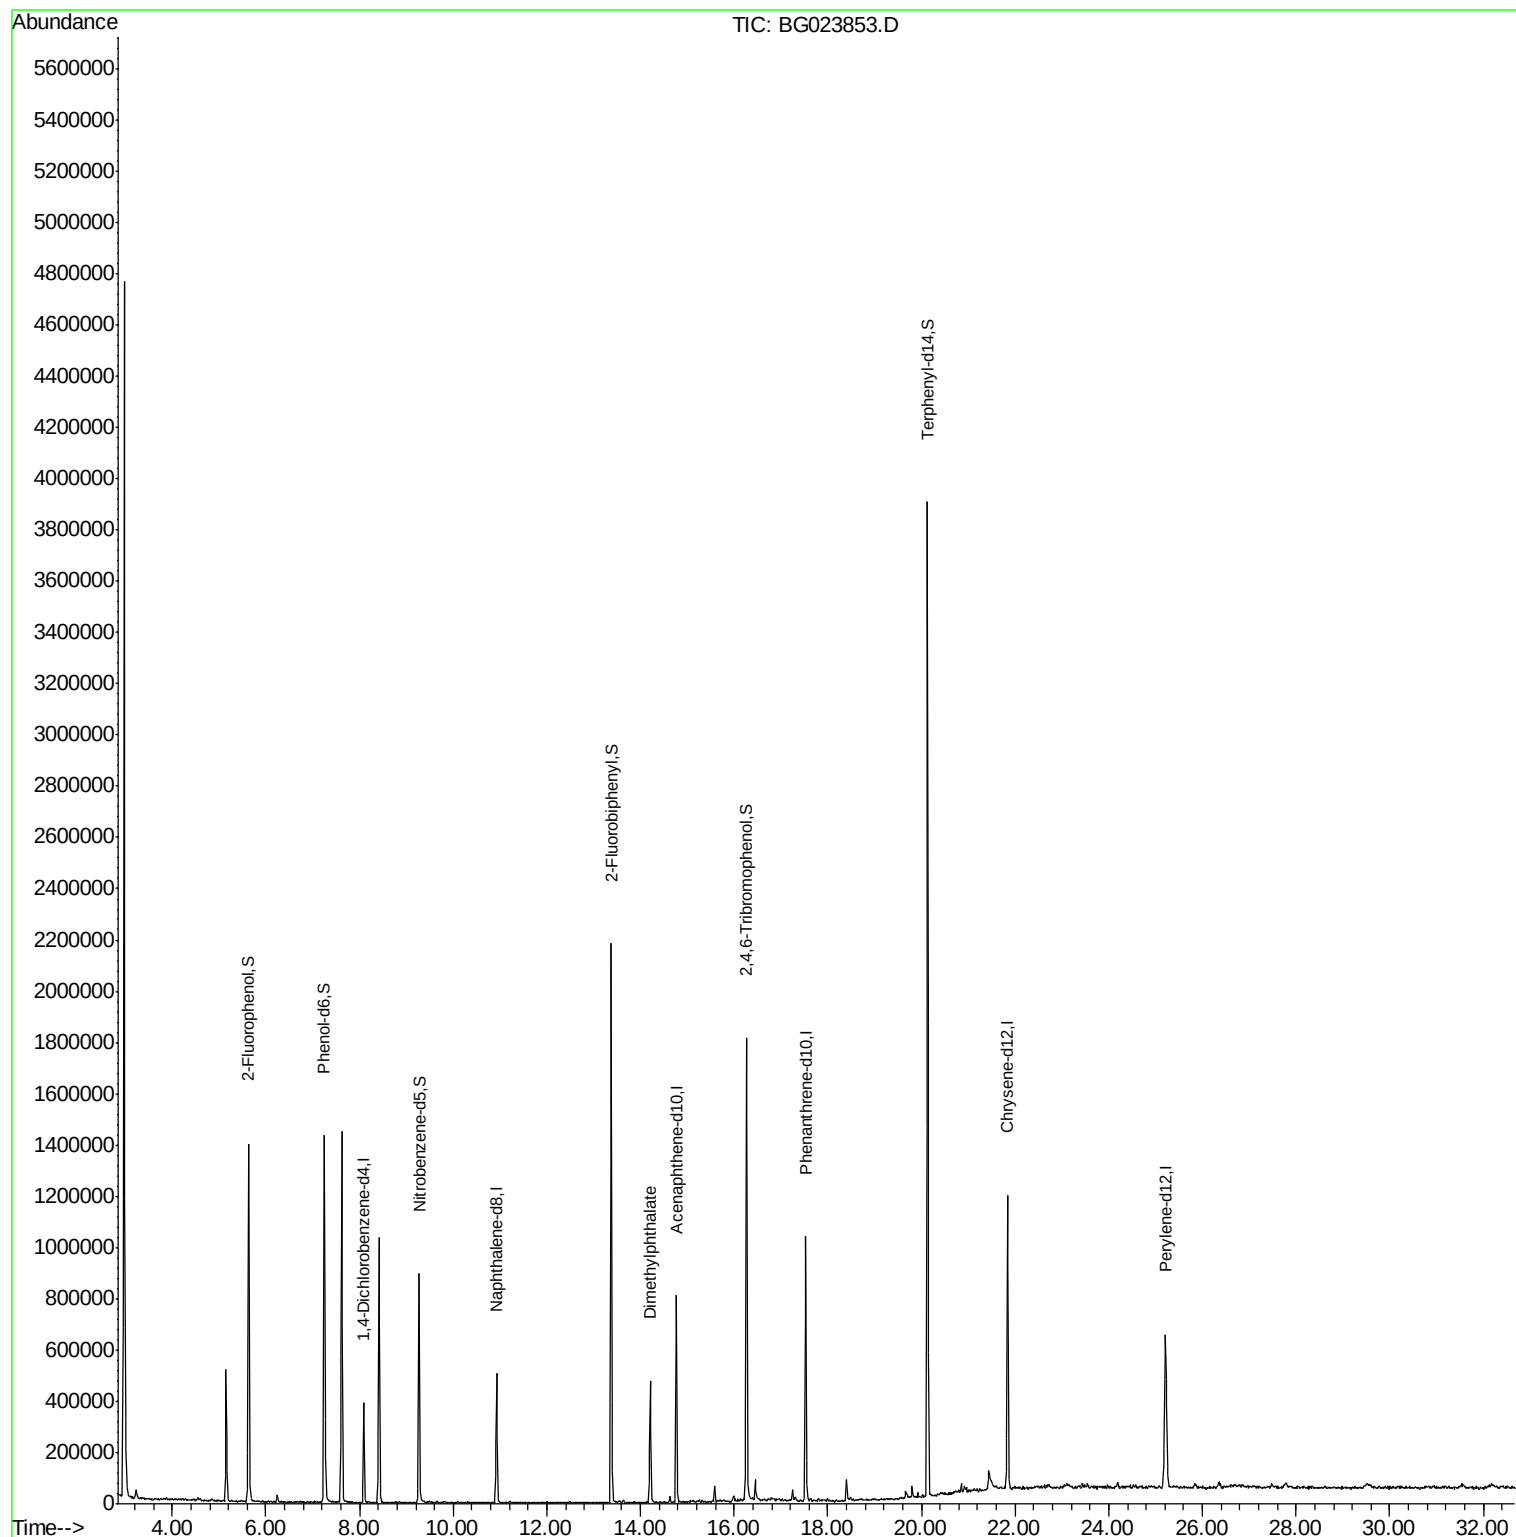

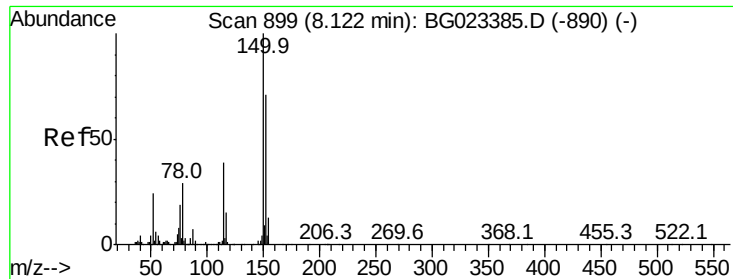

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.09 min Scan# 894

Delta R.T. -0.03 min

Lab File: BG023853.D

Acq: 23 Aug 2016 15:01

Instrument :

BNA_G

ClientSampleId :

VITALEFILL-MCMPH3-2


Tot Ion:152 Resp: 103035

Ion Ratio Lower Upper

152 100

150 159.8 144.7 217.1


115 60.2 64.0 96.0#

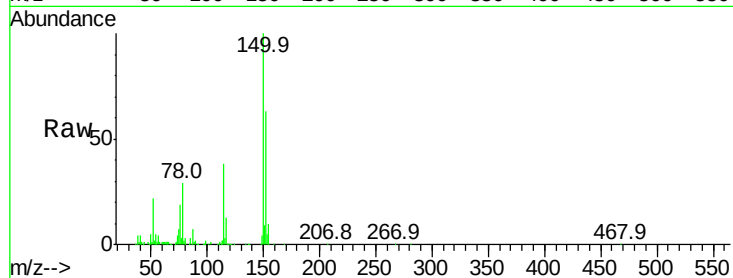



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

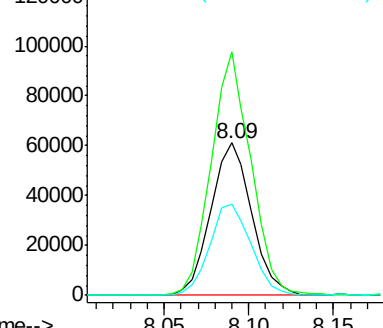

Time-->

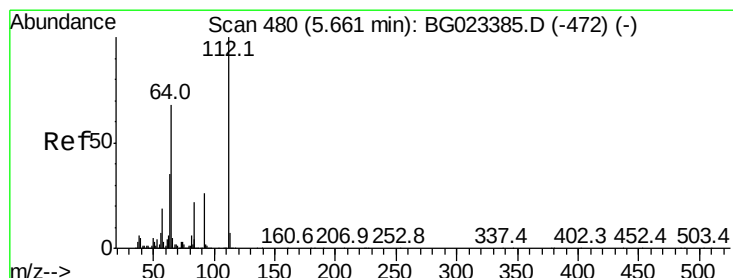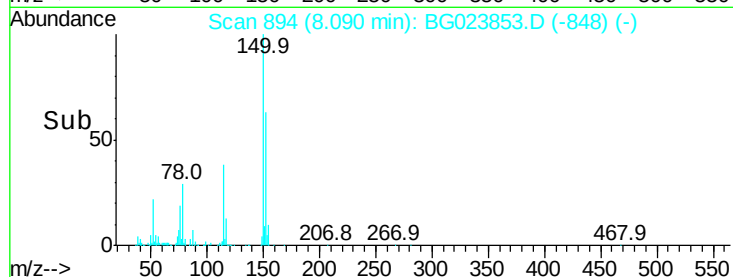

#5

2-Fluorophenol

Concen: 99.49 ng

RT: 5.63 min Scan# 476

Delta R.T. -0.03 min

Lab File: BG023853.D

Acq: 23 Aug 2016 15:01


Tgt Ion:112 Resp: 608993

Ion Ratio Lower Upper

112 100

64 69.3 59.0 88.4


63 35.8 37.8 56.8#

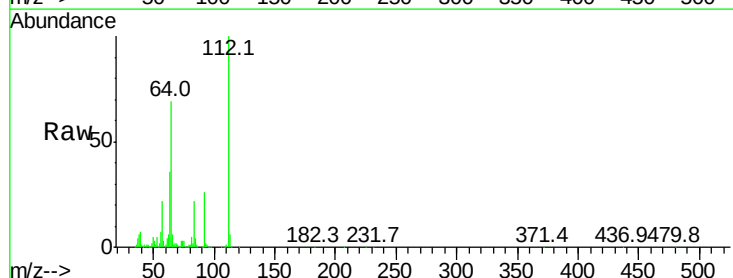


Abundance Ion 112.00 (111.70 to 112.70): E


Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

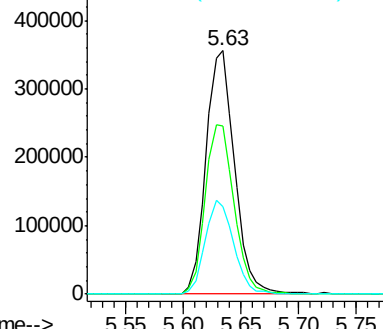

Time-->

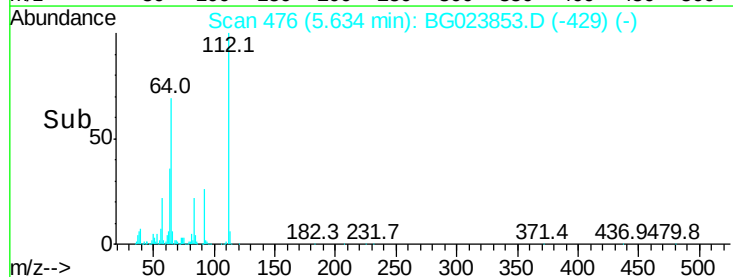

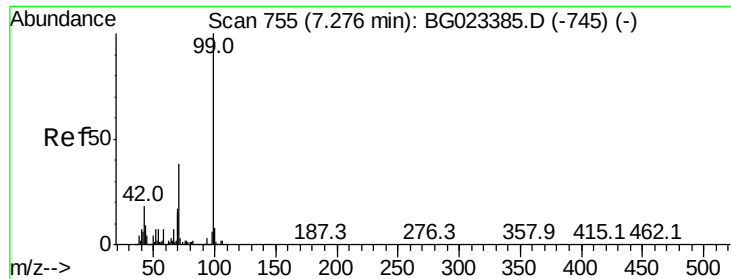

#7

Phenol-d6

Concen: 90.82 ng

RT: 7.24 min Scan# 750

Delta R.T. -0.03 min

Lab File: BG023853.D

Acq: 23 Aug 2016 15:01

Instrument :

BNA_G

ClientSampleId :

VITALEFILL-MCMPH3-2


Tot Ion: 99 Resp: 865850

Ion Ratio Lower Upper




99 100

42 19.4 17.8 26.6

71 40.8 41.5 62.3#

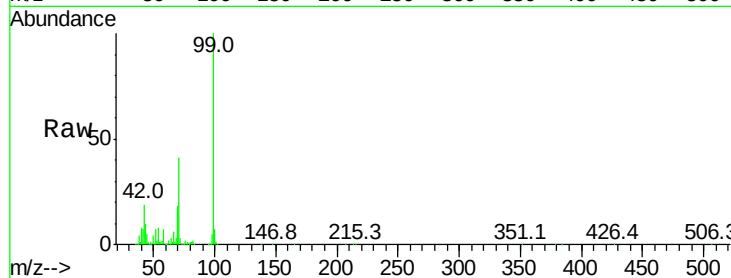

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

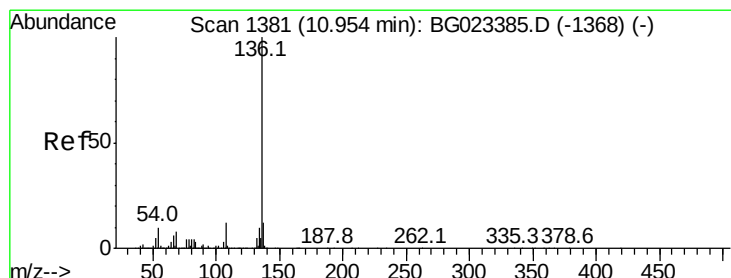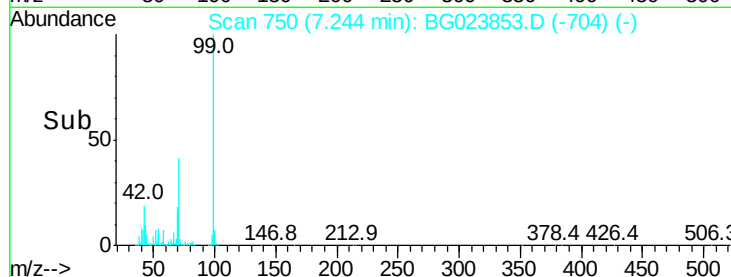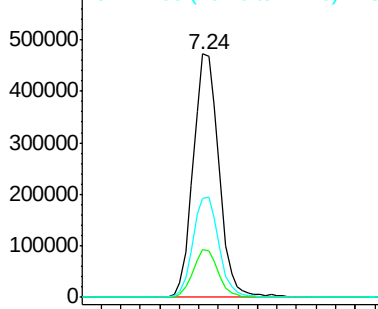

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.93 min Scan# 1377

Delta R.T. -0.03 min

Lab File: BG023853.D

Acq: 23 Aug 2016 15:01

Tgt Ion: 136 Resp: 431045


Ion Ratio Lower Upper

136 100



137 10.7 9.6 14.4


54 9.0 7.3 10.9

68 6.2 5.3 7.9

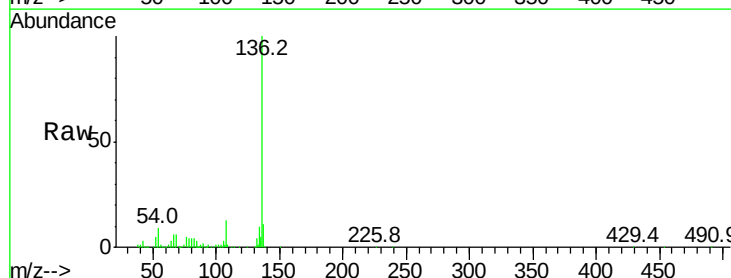

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



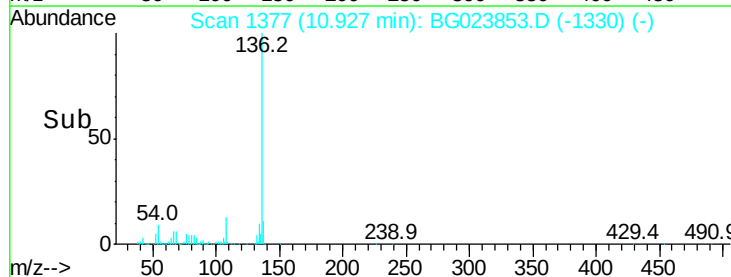
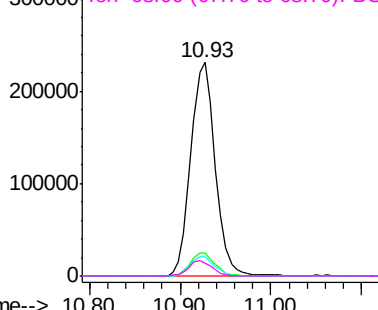


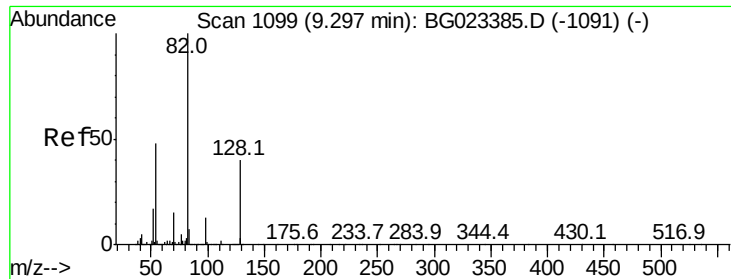

#23
 Nitrobenzene-d5
 Concen: 67.43 ng
 RT: 9.27 min Scan# 1095
 Delta R.T. -0.03 min
 Lab File: BG023853.D
 Acq: 23 Aug 2016 15:01




Instrument :
 BNA_G
 ClientSampleId :
 VITALEFILL-MCMPH3-2


Tot Ion	82	Resp	584601
Ion	Ratio	Lower	Upper
82	100		
128	34.1	24.4	36.6
54	50.8	41.4	62.0

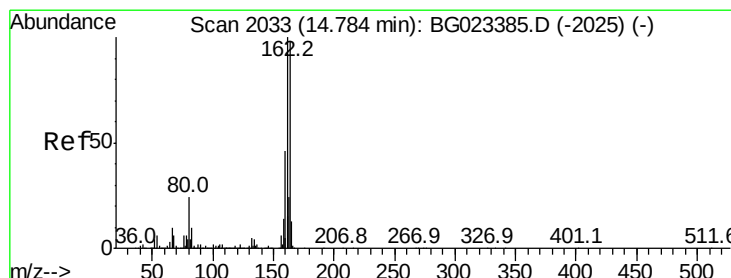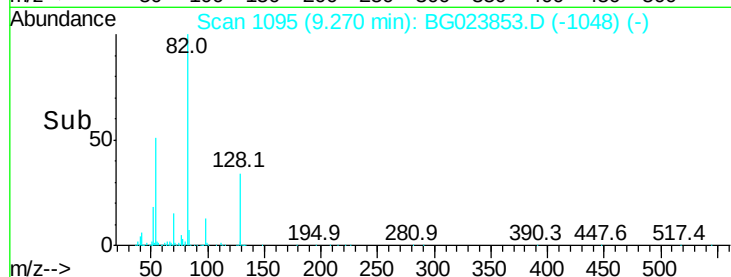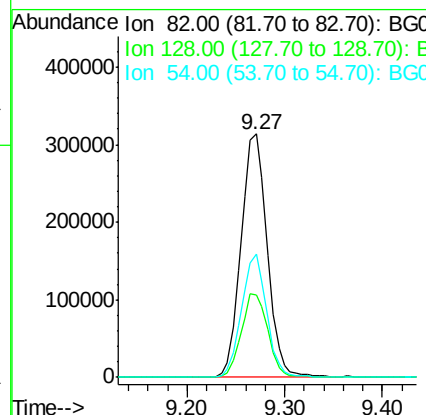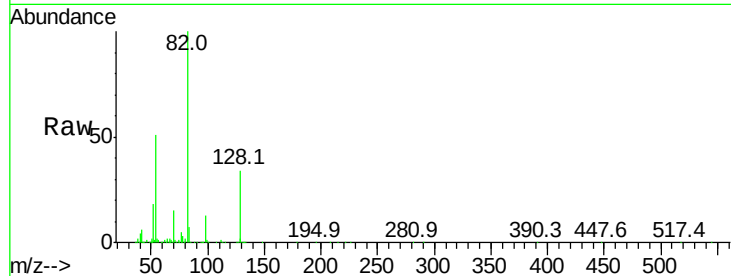

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.76 min Scan# 2030
 Delta R.T. -0.02 min
 Lab File: BG023853.D
 Acq: 23 Aug 2016 15:01

Tgt Ion	164	Resp	267627
Ion	Ratio	Lower	Upper
164	100		
162	102.2	87.7	131.5
160	44.8	37.2	55.8


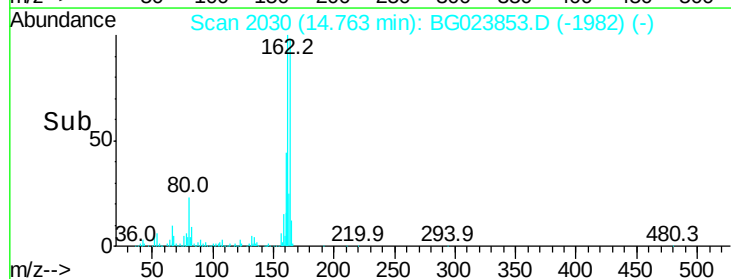
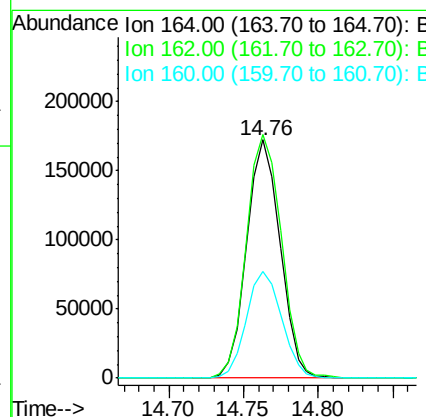
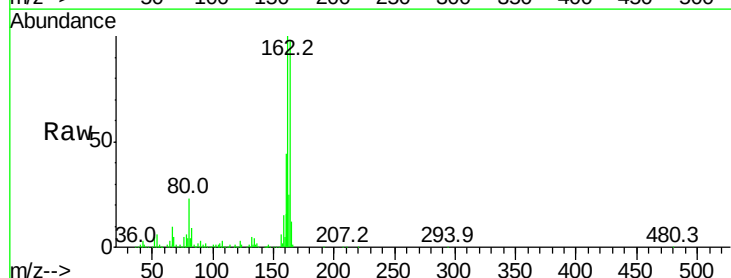


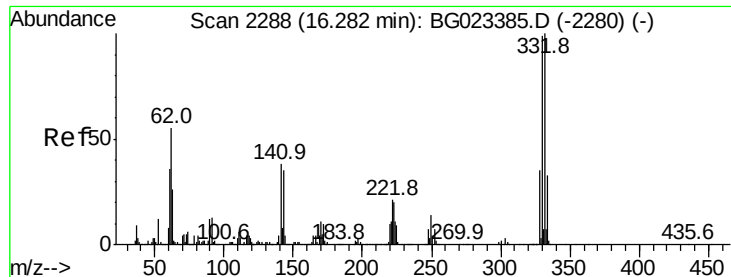

#41
 2,4,6-Tribromophenol
 Concen: 86.78 ng
 RT: 16.26 min Scan# 2285
 Delta R.T. -0.02 min
 Lab File: BG023853.D
 Acq: 23 Aug 2016 15:01




Instrument :
 BNA_G
 ClientSampleId :
 VITALEFILL-MCMPH3-2


Tot Ion:330 Resp: 339693
 Ion Ratio Lower Upper
 330 100
 332 95.6 77.4 116.2
 141 40.5 31.7 47.5

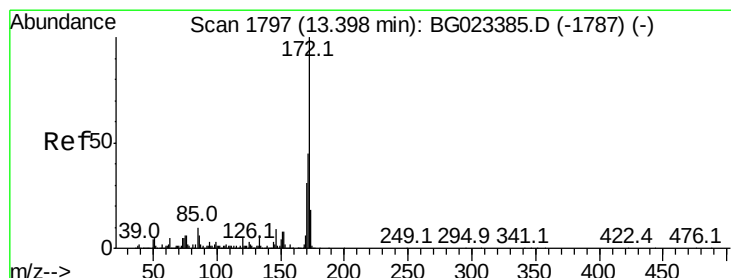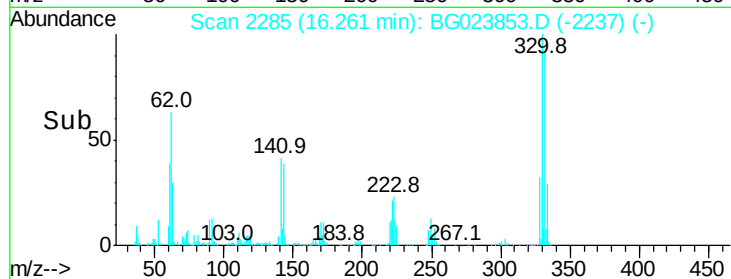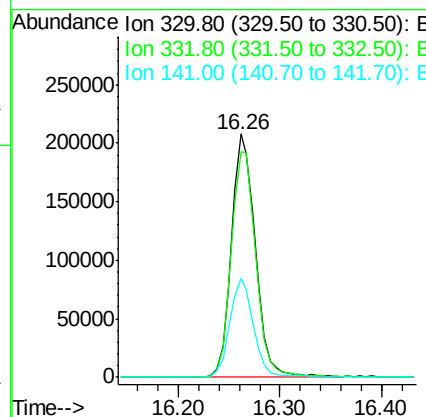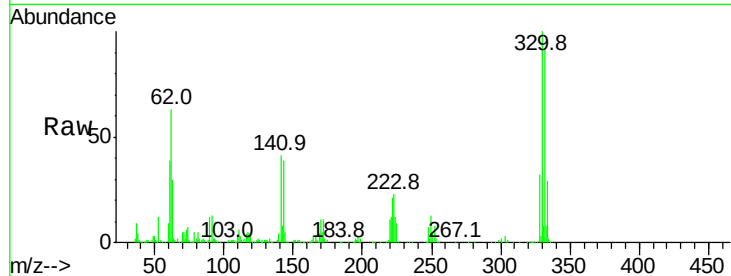

#44
 2-Fluorobiphenyl
 Concen: 69.10 ng
 RT: 13.38 min Scan# 1794
 Delta R.T. -0.02 min
 Lab File: BG023853.D
 Acq: 23 Aug 2016 15:01

Tgt Ion:172 Resp: 1096490
 Ion Ratio Lower Upper
 172 100
 171 36.5 31.6 47.4
 170 24.7 21.3 31.9

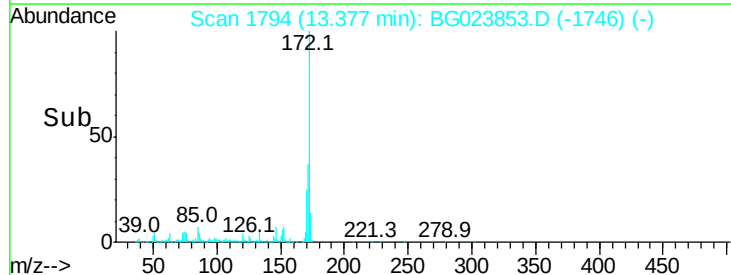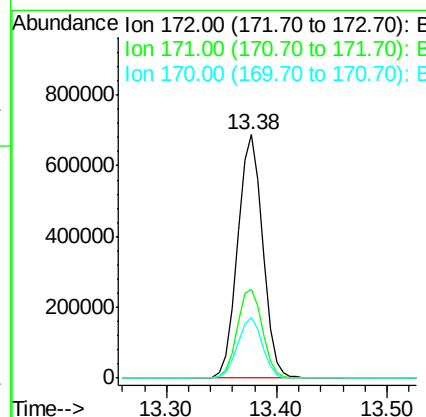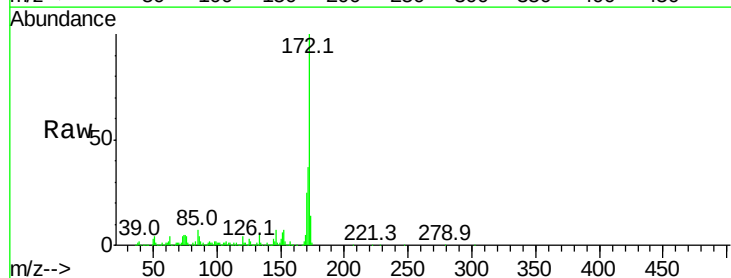

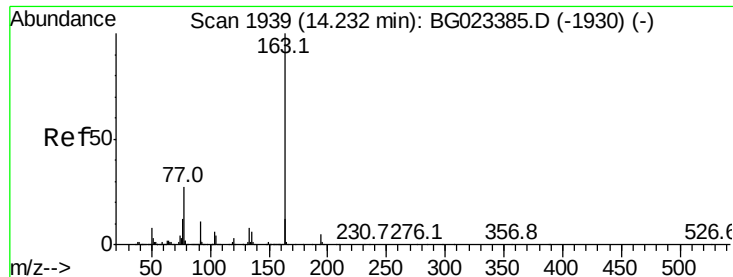

#49

Dimethylphthalate

Concen: 15.17 ng

RT: 14.20 min Scan# 1935

Delta R.T. -0.03 min

Lab File: BG023853.D

Acq: 23 Aug 2016 15:01

Instrument :

BNA_G

ClientSampleId :

VITALEFILL-MCMPH3-2


Tot Ion:163 Resp: 311555

Ion Ratio Lower Upper

163 100

194 4.3 3.6 5.4




164 9.0 8.1 12.1

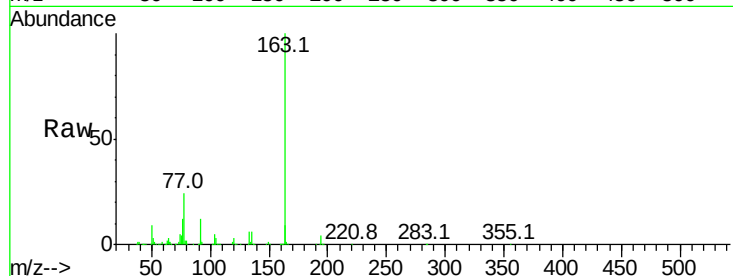

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

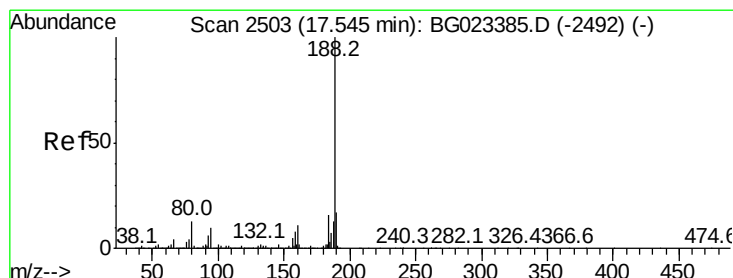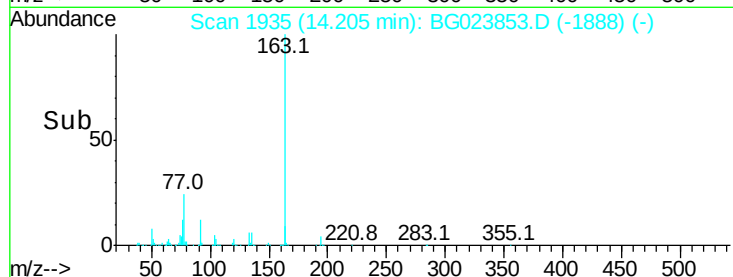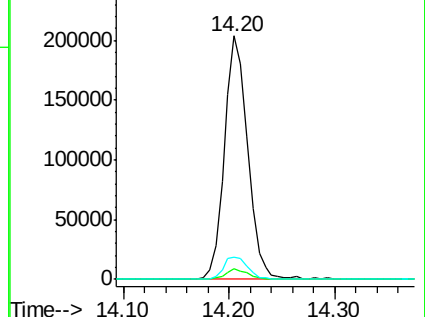

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.53 min Scan# 2501

Delta R.T. -0.01 min

Lab File: BG023853.D

Acq: 23 Aug 2016 15:01


Tgt Ion:188 Resp: 650702

Ion Ratio Lower Upper

188 100

94 7.6 5.2 7.8



80 10.8 7.2 10.8#

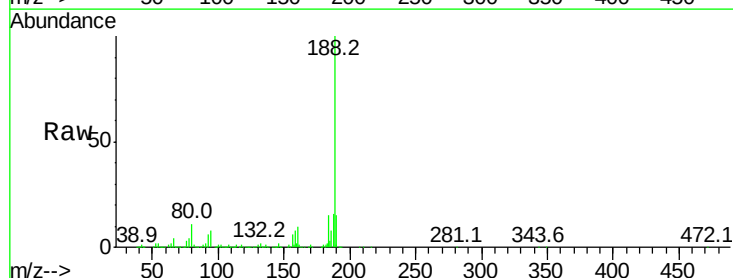


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

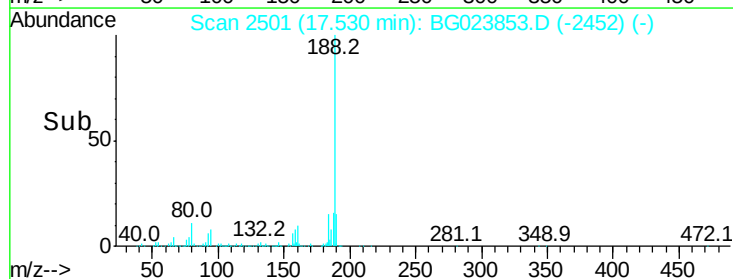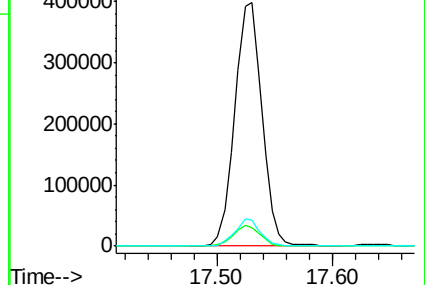

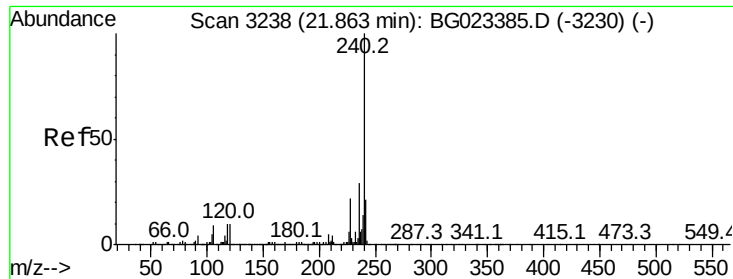

#75

Chrvsene-d12

Concen: 20.00 ng

RT: 21.84 min Scan# 3235

Delta R.T. -0.02 min

Lab File: BG023853.D

Acq: 23 Aug 2016 15:01

Instrument :

BNA_G

ClientSampleId :

VITALEFILL-MCMPH3-2


Tot Ion:240 Resp: 704827

Ion Ratio Lower Upper

240 100

120 7.7 4.1 6.1#




236 25.0 21.1 31.7

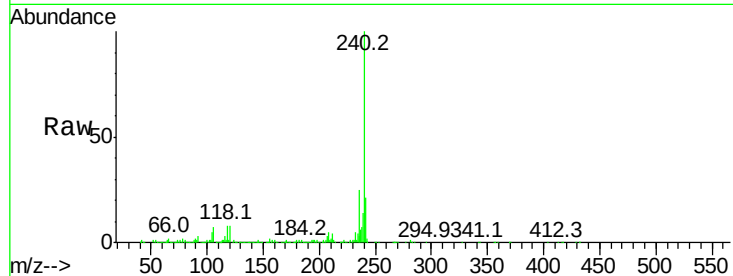

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

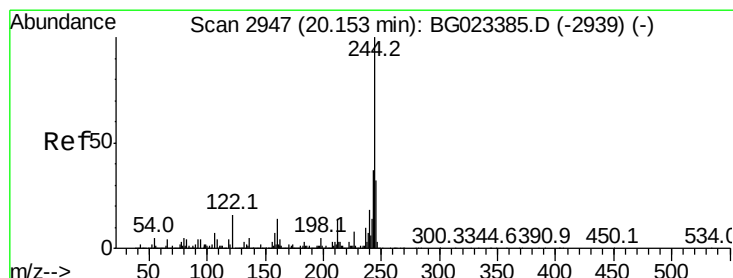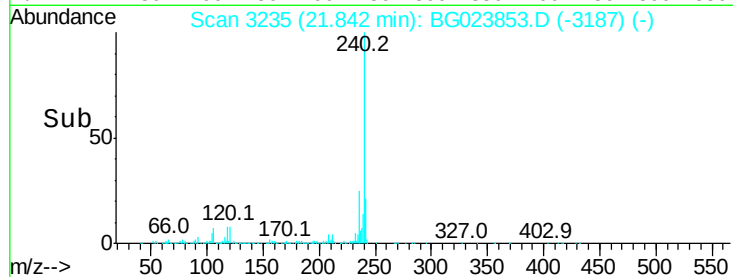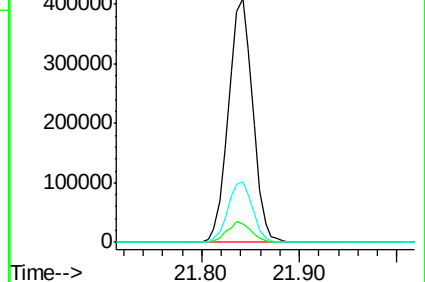

#78

Terphenyl-d14

Concen: 67.78 ng

RT: 20.13 min Scan# 2944

Delta R.T. -0.02 min

Lab File: BG023853.D

Acq: 23 Aug 2016 15:01


Tgt Ion:244 Resp: 1613897

Ion Ratio Lower Upper

244 100

212 9.9 10.8 16.2#



122 10.3 8.0 12.0

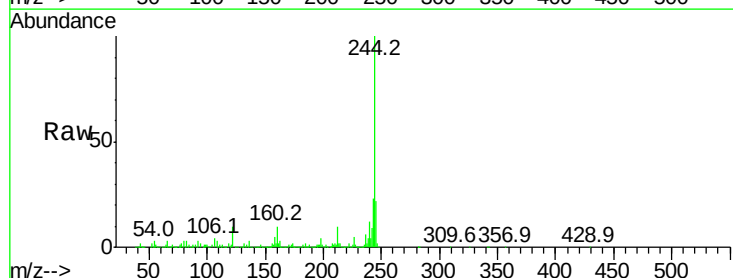


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

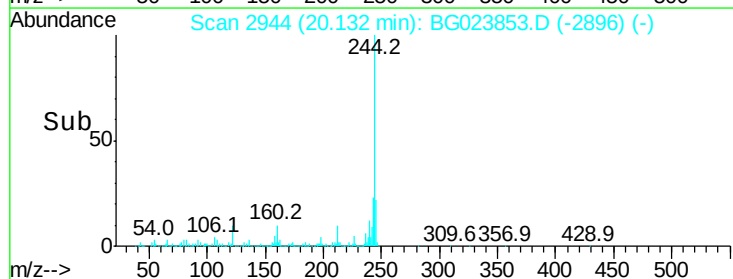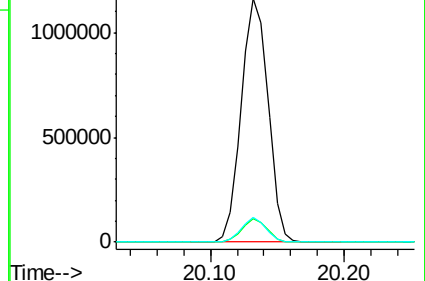

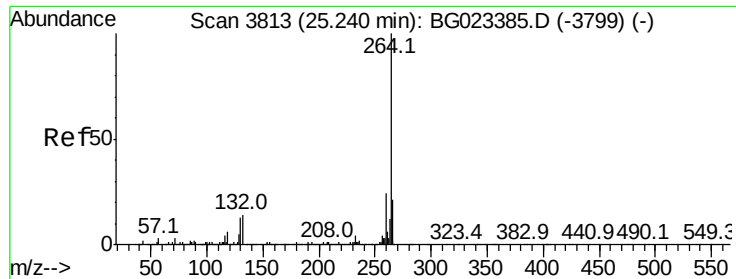

#86

Pervlene-d12

Concen: 20.00 ng

RT: 25.21 min Scan# 3809

Delta R.T. -0.03 min

Lab File: BG023853.D


Acq: 23 Aug 2016 15:01

Instrument :

BNA_G

ClientSampleId :

VITALEFILL-MCMPH3-2

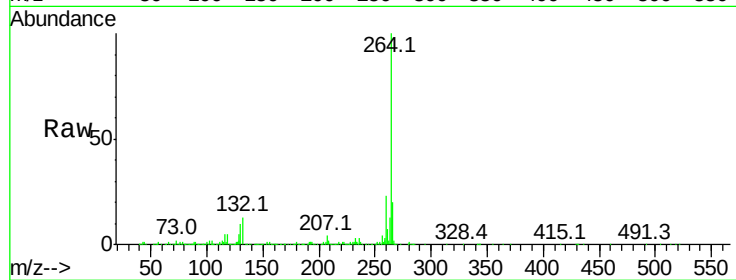


Tot Ion: 264 Resp: 695121

Ion Ratio Lower Upper

264 100

260 23.0 18.4 27.6

265 19.7 18.9 28.3

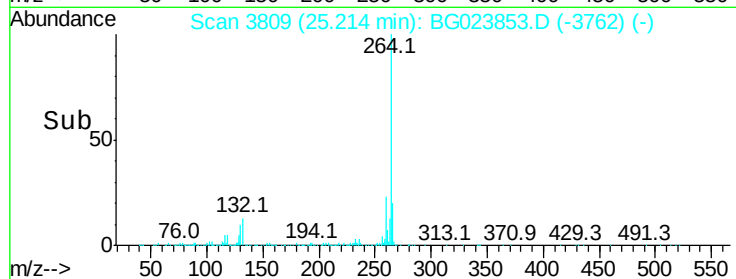

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

