


Data Path : Z:\HPCHEM1\BNA G\Data\BG082316\
 Data File : BG023846.D
 Acq On : 23 Aug 2016 9:49
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\Methods\8270-BG080116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 01 19:22:14 2016

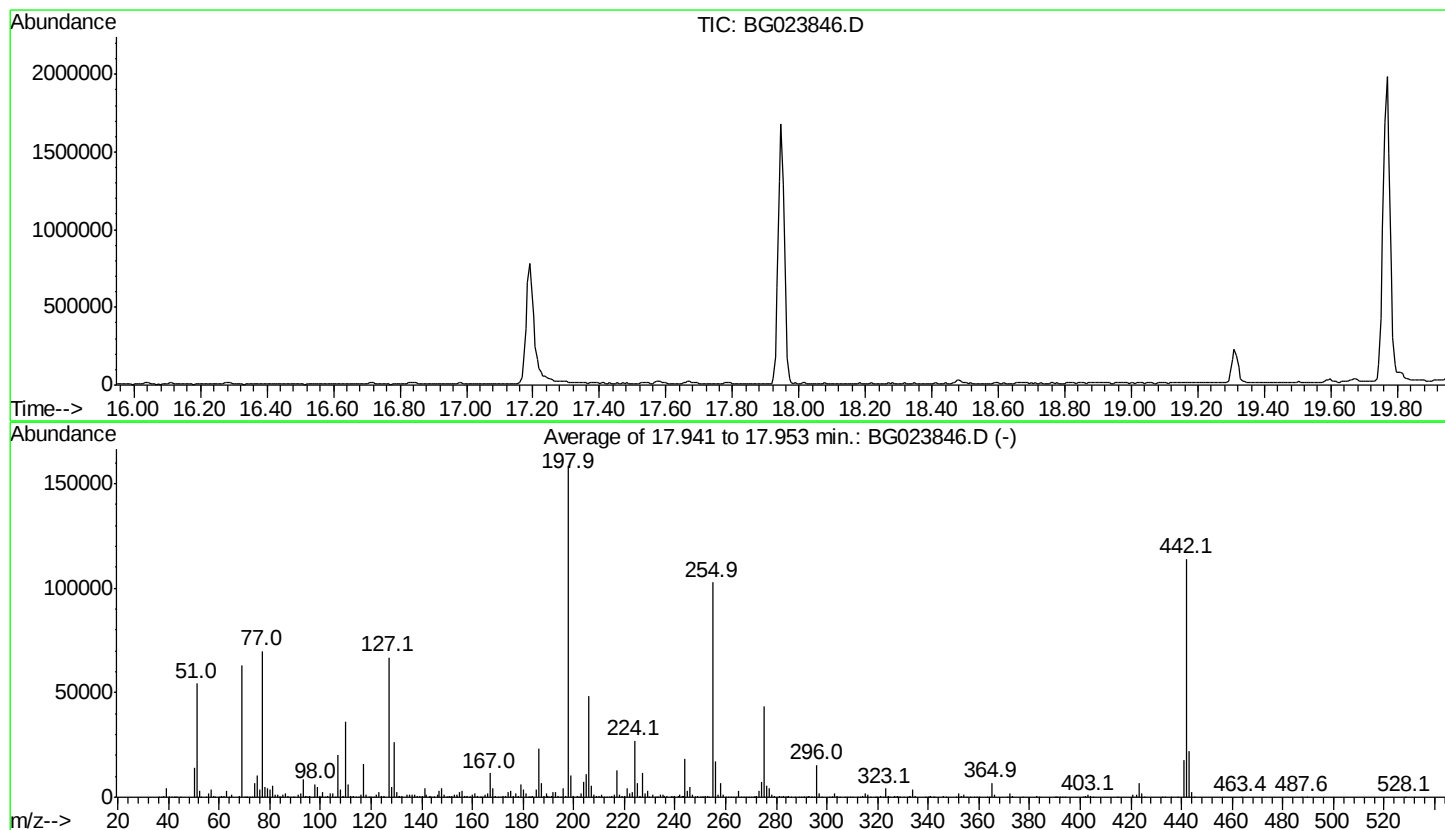

AutoFind: Scans 2571, 2572, 2573; Background Corrected with Scan 2564

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	54330	PASS
68	69	0.00	2	1.2	768	PASS
69	198	0.00	100	39.6	62874	PASS
70	69	0.00	2	0.4	271	PASS
127	198	10	80	42.1	66832	PASS
197	198	0.00	2	0.3	475	PASS
198	198	100	100	100.0	158613	PASS
199	198	5	9	6.5	10344	PASS
275	198	10	60	27.3	43362	PASS
365	198	1	100	4.3	6885	PASS
441	442	0.01	24	15.5	17730	PASS
442	198	50	100	71.9	114106	PASS
443	442	15	24	19.4	22117	PASS